

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
 Data File : BG020173.D
 Acq On : 15 Dec 2015 4:11
 Operator : UM/SJ
 Sample : G4787-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 G9BM7

Quant Time: Dec 15 06:01:50 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 15 05:59:19 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	21026	20.00	ng/ul	0.00
18) Naphthalene-d8	10.92	136	94628	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	70903	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.48	188	186793	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	208152	20.00	ng/ul	0.00
86) Perylene-d12	25.01	264	196196	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	2654	6.97	ng/uL	0.00
5) Phenol-d5	7.25	99	57806	31.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.42	67	37542	33.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	43375	32.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	47716	30.09	ng/ul	0.00
19) Nitrobenzene-d5	9.27	128	24227	32.84	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	28782	35.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	52858	31.79	ng/ul	0.00
29) 4-Chloroaniline-d4	11.05	131	68090	36.46	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	198247	34.57	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	219355	32.87	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	30778	29.92	ng/ul	0.00
58) Fluorene-d10	15.72	176	168644	32.42	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	24823	22.42	ng/ul	0.00
71) Anthracene-d10	17.57	188	272944	31.71	ng/ul	0.00
79) Pyrene-d10	19.85	212	294125	30.32	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	274362	28.04	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.17	163	77137	13.17	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
Data File : BG020173.D
Acq On : 15 Dec 2015 4:11
Operator : UM/SJ
Sample : G4787-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
G9BM7

Quant Time: Dec 15 06:01:50 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 15 05:59:19 2015
Response via : Initial Calibration

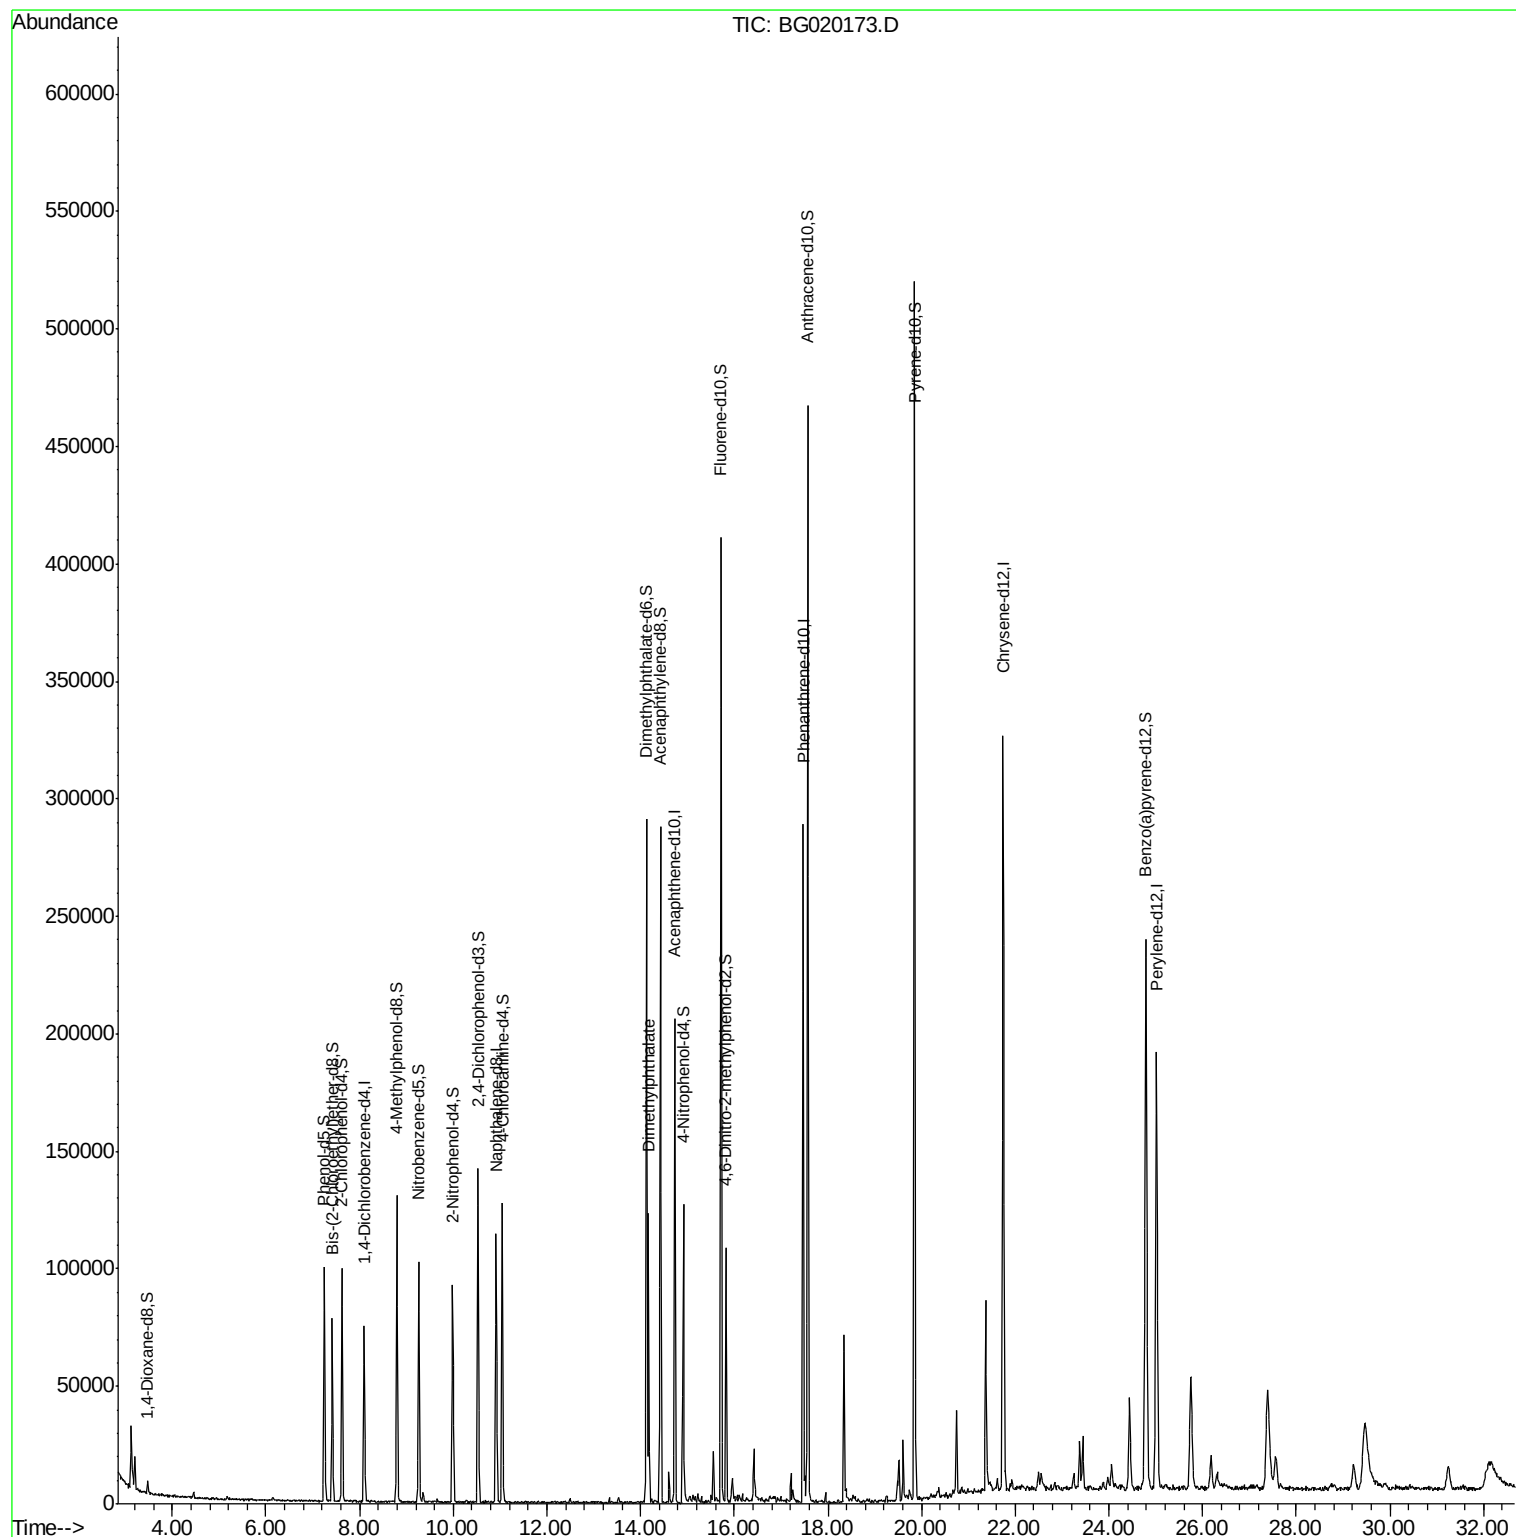

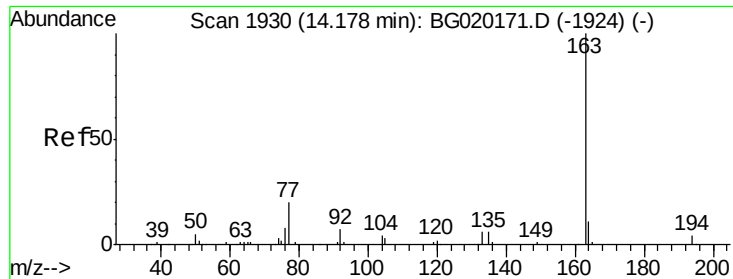

#45

Dimethylphthalate

Concen: 13.17 ng/ul

RT: 14.17 min Scan# 1929

Delta R.T. -0.00 min

Lab File: BG020173.D

Acq: 15 Dec 2015 4:11

Instrument :

BNA_G

ClientSampleId :

G9BM7


Tgt Ion:163 Resp: 77137

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 10.2 7.7 11.5

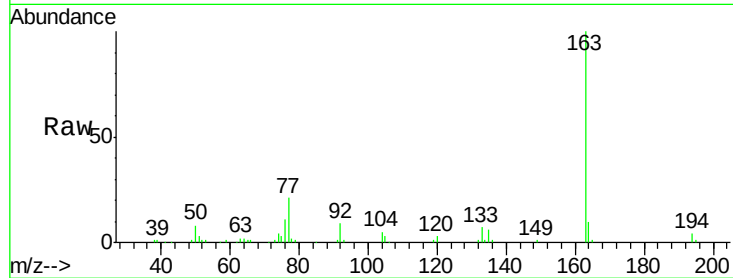

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

