

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
 Data File : BG020151.D
 Acq On : 14 Dec 2015 11:32
 Operator : UM/SJ
 Sample : PB87242BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.126	44	49	57	rVB	16648	31649	3.27%	0.352%
2	3.202	59	62	66	rVB4	4244	5306	0.55%	0.059%
3	3.343	83	86	87	rVB2	1640	1214	0.13%	0.014%
4	3.472	103	108	114	rBV3	6310	8414	0.87%	0.094%
5	4.054	205	207	210	rVB2	1281	1271	0.13%	0.014%
6	4.788	329	332	335	rBV2	656	974	0.10%	0.011%
7	6.486	617	621	624	rVB4	773	984	0.10%	0.011%
8	7.050	713	717	719	rBV3	832	1319	0.14%	0.015%
9	7.244	740	750	759	rBV	114571	193880	20.06%	2.159%
10	7.415	773	779	787	rBV	86295	141588	14.65%	1.577%
11	7.515	793	796	800	rBV3	732	1123	0.12%	0.013%
12	7.626	807	815	822	rBV	113614	187553	19.41%	2.089%
13	7.932	864	867	869	rBV2	791	993	0.10%	0.011%
14	8.096	889	895	903	rBV	76465	131266	13.58%	1.462%
15	8.795	1008	1014	1022	rBV2	156752	260184	26.92%	2.898%
16	9.265	1087	1094	1103	rVB	119348	202360	20.94%	2.254%
17	9.642	1155	1158	1161	rBV2	719	1051	0.11%	0.012%
18	9.988	1211	1217	1225	rVV	101943	178678	18.49%	1.990%
19	10.529	1301	1309	1317	rBV	161985	275783	28.54%	3.071%
20	10.916	1365	1375	1382	rBV	119776	207466	21.47%	2.311%
21	11.046	1390	1397	1407	rBV	160876	286444	29.64%	3.190%
22	11.933	1545	1548	1551	rVB	875	1137	0.12%	0.013%
23	12.497	1638	1644	1649	rBV4	2323	5015	0.52%	0.056%
24	14.130	1913	1922	1929	rBV	346779	490153	50.72%	5.459%
25	14.424	1965	1972	1980	rVB	350544	540083	55.88%	6.015%
26	14.730	2017	2024	2031	rVB2	218548	345014	35.70%	3.843%
27	14.912	2048	2055	2069	rBV2	147808	240153	24.85%	2.675%
28	15.399	2135	2138	2141	rBV2	624	1056	0.11%	0.012%
29	15.717	2186	2192	2199	rBV	482565	732723	75.82%	8.161%
30	15.828	2205	2211	2219	rBV	113103	161484	16.71%	1.799%
31	15.958	2228	2233	2237	rBV2	4279	5965	0.62%	0.066%
32	16.075	2252	2253	2258	rBV3	691	1072	0.11%	0.012%
33	17.474	2484	2491	2499	rVB	304756	460415	47.64%	5.128%
34	17.573	2501	2508	2520	rVB	548511	836394	86.54%	9.315%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
 Data File : BG020151.D
 Acq On : 14 Dec 2015 11:32
 Operator : UM/SJ
 Sample : PB87242BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

35	17.855	2548	2556	2559	rVB4	977	1952	0.20%	0.022%
36	19.489	2828	2834	2838	rBV	5232	7454	0.77%	0.083%
37	19.741	2871	2877	2882	rBV2	4327	5959	0.62%	0.066%
38	19.853	2889	2896	2904	rBV	694190	966435	100.00%	10.764%
39	20.112	2938	2940	2944	rVB2	929	1068	0.11%	0.012%
40	20.752	3044	3049	3052	rBV4	2391	3151	0.33%	0.035%
41	20.858	3066	3067	3069	rBV2	1387	1112	0.12%	0.012%
42	21.005	3090	3092	3094	rBV3	1034	990	0.10%	0.011%
43	21.216	3125	3128	3130	rBV3	1180	1761	0.18%	0.020%
44	21.663	3202	3204	3206	rBV2	1357	1326	0.14%	0.015%
45	21.745	3211	3218	3227	rVB	322553	523411	54.16%	5.829%
46	22.503	3344	3347	3348	rBV2	1455	1560	0.16%	0.017%
47	22.550	3351	3355	3359	rVV5	1422	2197	0.23%	0.024%
48	23.002	3430	3432	3435	rBV4	912	1277	0.13%	0.014%
49	23.243	3469	3473	3480	rBV5	3407	6764	0.70%	0.075%
50	23.331	3485	3488	3491	rBV4	1275	1615	0.17%	0.018%
51	23.690	3547	3549	3552	rVB3	1363	1056	0.11%	0.012%
52	23.866	3576	3579	3588	rVB6	4249	8765	0.91%	0.098%
53	24.060	3609	3612	3618	rVB7	3857	7355	0.76%	0.082%
54	24.318	3654	3656	3659	rBV3	1104	1221	0.13%	0.014%
55	24.418	3671	3673	3674	rVB2	1564	1015	0.11%	0.011%
56	24.448	3674	3678	3683	rBV5	1478	3459	0.36%	0.039%
57	24.553	3694	3696	3699	rBV3	1512	1860	0.19%	0.021%
58	24.683	3716	3718	3720	rBV2	1275	1279	0.13%	0.014%
59	24.788	3724	3736	3750	rVV	335077	929612	96.19%	10.353%
60	24.906	3754	3756	3759	rVV2	1389	1424	0.15%	0.016%
61	25.018	3763	3775	3787	rVB2	177721	495453	51.27%	5.518%
62	26.175	3964	3972	3974	rBV6	5951	12850	1.33%	0.143%
63	26.434	4014	4016	4020	rBV4	1887	2335	0.24%	0.026%
64	26.563	4037	4038	4042	rBV4	1238	1116	0.12%	0.012%
65	26.674	4056	4057	4061	rBV2	1229	1281	0.13%	0.014%
66	27.009	4111	4114	4115	rBV2	1187	1208	0.12%	0.013%
67	27.356	4171	4173	4176	rBV4	1352	1309	0.14%	0.015%
68	27.550	4202	4206	4207	rBV3	4884	4828	0.50%	0.054%
69	27.685	4228	4229	4233	rBV3	1207	1332	0.14%	0.015%
70	28.343	4339	4341	4343	rBV2	965	981	0.10%	0.011%
71	28.414	4351	4353	4357	rBV4	1403	2024	0.21%	0.023%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
Data File : BG020151.D
Acq On : 14 Dec 2015 11:32
Operator : UM/SJ
Sample : PB87242BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK42

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Title : SVOA CALIBRATION

72	28.866	4429	4430	4434	rVB4	1316	1214	0.13%	0.014%
73	28.913	4434	4438	4439	rBV3	1123	1231	0.13%	0.014%
74	29.136	4474	4476	4478	rBV3	1374	1013	0.10%	0.011%
75	29.224	4484	4491	4495	rBV6	3584	9281	0.96%	0.103%
76	29.360	4513	4514	4518	rBV4	1201	1396	0.14%	0.016%
77	29.465	4530	4532	4533	rBV	1328	979	0.10%	0.011%
78	29.536	4540	4544	4545	rBV2	1242	1282	0.13%	0.014%
79	29.918	4607	4609	4611	rVB3	1438	1301	0.13%	0.014%
80	29.941	4611	4613	4615	rBV4	892	1103	0.11%	0.012%
81	30.447	4698	4699	4702	rBV3	1911	1158	0.12%	0.013%
82	30.711	4742	4744	4745	rBV	1191	1078	0.11%	0.012%
83	31.140	4816	4817	4820	rBV2	993	1200	0.12%	0.013%
84	31.193	4823	4826	4827	rBV3	1426	1589	0.16%	0.018%
85	31.786	4925	4927	4928	rVV2	1820	1522	0.16%	0.017%
86	31.816	4931	4932	4935	rVB3	1893	1237	0.13%	0.014%
87	32.338	5019	5021	5025	rBV3	1600	2245	0.23%	0.025%


Sum of corrected areas: 8978788

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
Data File : BG020151.D
Acq On : 14 Dec 2015 11:32
Operator : UM/SJ
Sample : PB87242BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK42

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

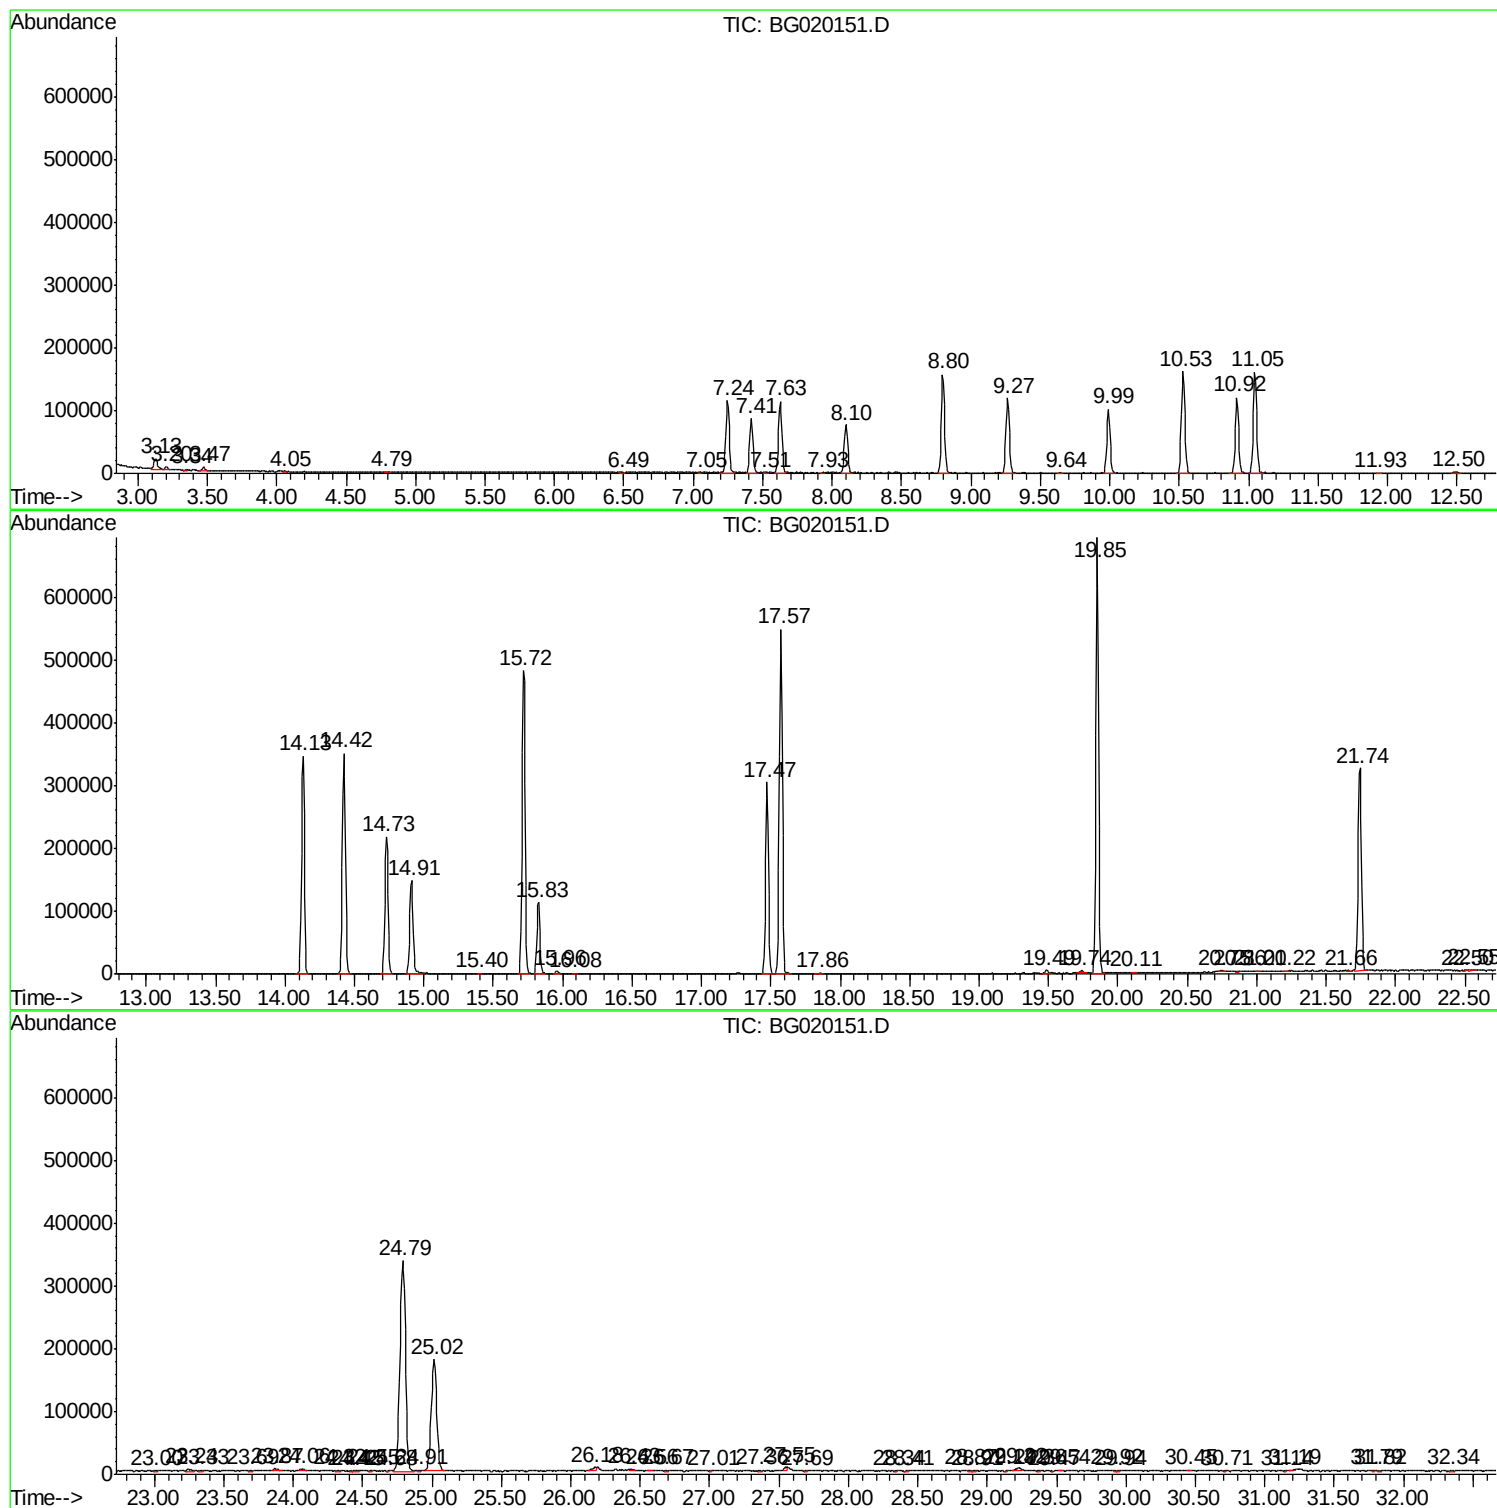

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
Data File : BG020151.D
Acq On : 14 Dec 2015 11:32
Operator : UM/SJ
Sample : PB87242BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK42

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
Data File : BG020151.D
Acq On : 14 Dec 2015 11:32
Operator : UM/SJ
Sample : PB87242BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK42

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc