

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
 Data File : BG020172.D
 Acq On : 15 Dec 2015 3:32
 Operator : UM/SJ
 Sample : PB87250BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.126	44	49	58	rVV	15713	28525	3.25%	0.343%
2	3.202	59	62	65	rVB5	3627	4533	0.52%	0.054%
3	3.355	86	88	91	rBV3	816	1086	0.12%	0.013%
4	3.473	105	108	113	rVB2	5046	7026	0.80%	0.084%
5	4.054	204	207	214	rBV5	1549	2243	0.26%	0.027%
6	4.313	247	251	256	rBV3	798	1599	0.18%	0.019%
7	7.145	731	733	736	rVB	923	1106	0.13%	0.013%
8	7.174	736	738	741	rBV	751	1129	0.13%	0.014%
9	7.251	744	751	761	rVB	99733	169875	19.37%	2.041%
10	7.321	761	763	766	rBV3	856	1091	0.12%	0.013%
11	7.421	774	780	787	rVB	77245	122376	13.95%	1.470%
12	7.627	809	815	823	rVB	99104	163702	18.66%	1.967%
13	8.103	888	896	902	rVB	80170	132420	15.10%	1.591%
14	8.802	1008	1015	1023	rBV	127845	218888	24.96%	2.630%
15	9.266	1084	1094	1102	rVV	99674	174170	19.86%	2.093%
16	9.995	1210	1218	1224	rVV	87659	152147	17.35%	1.828%
17	10.529	1302	1309	1320	rVB	136154	239358	27.29%	2.876%
18	10.917	1368	1375	1383	rVB	117423	206582	23.55%	2.482%
19	11.046	1390	1397	1406	rBB	136774	240900	27.46%	2.895%
20	12.492	1639	1643	1649	rBV3	2325	3524	0.40%	0.042%
21	14.131	1916	1922	1928	rBV	293531	422891	48.21%	5.081%
22	14.425	1964	1972	1979	rBV	314487	476714	54.35%	5.728%
23	14.730	2018	2024	2031	rVB2	216317	345972	39.44%	4.157%
24	14.912	2049	2055	2069	rBV	140381	220924	25.19%	2.655%
25	15.006	2069	2071	2074	rVV3	1369	1615	0.18%	0.019%
26	15.406	2136	2139	2143	rBV3	618	1277	0.15%	0.015%
27	15.717	2185	2192	2201	rVB	420531	644812	73.51%	7.748%
28	15.823	2204	2210	2218	rBV	96767	141744	16.16%	1.703%
29	15.958	2229	2233	2237	rVB	3954	5190	0.59%	0.062%
30	16.669	2351	2354	2357	rBV2	1056	1259	0.14%	0.015%
31	17.262	2452	2455	2458	rVB2	1120	1371	0.16%	0.016%
32	17.474	2485	2491	2500	rVB2	323317	478237	54.52%	5.746%
33	17.574	2500	2508	2515	rBV	497049	753865	85.95%	9.058%
34	18.661	2689	2693	2698	rBV3	567	1079	0.12%	0.013%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
 Data File : BG020172.D
 Acq On : 15 Dec 2015 3:32
 Operator : UM/SJ
 Sample : PB87250BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

35	19.483	2829	2833	2840	rVB	4996	7418	0.85%	0.089%
36	19.736	2873	2876	2879	rBV	3974	4949	0.56%	0.059%
37	19.854	2889	2896	2903	rBV	620779	877121	100.00%	10.539%
38	20.012	2922	2923	2930	rVB3	1032	1312	0.15%	0.016%
39	20.065	2930	2932	2935	rBV2	955	1203	0.14%	0.014%
40	20.747	3044	3048	3053	rVV	5174	7087	0.81%	0.085%
41	20.911	3073	3076	3078	rVB4	1544	1705	0.19%	0.020%
42	20.982	3086	3088	3090	rBV2	1429	1449	0.17%	0.017%
43	21.081	3103	3105	3107	rBV2	1214	1169	0.13%	0.014%
44	21.140	3112	3115	3117	rBV3	1105	1219	0.14%	0.015%
45	21.164	3117	3119	3122	rVB4	1337	1491	0.17%	0.018%
46	21.745	3211	3218	3225	rBV	352712	557055	63.51%	6.694%
47	21.928	3247	3249	3251	rBV3	2580	2158	0.25%	0.026%
48	21.986	3258	3259	3263	rVB4	1351	1306	0.15%	0.016%
49	22.180	3289	3292	3293	rBV3	1125	1056	0.12%	0.013%
50	22.374	3324	3325	3328	rBV2	1323	1439	0.16%	0.017%
51	22.515	3347	3349	3351	rBV2	990	1082	0.12%	0.013%
52	23.244	3470	3473	3478	rVB5	2787	4987	0.57%	0.060%
53	23.355	3490	3492	3494	rBV2	1435	1320	0.15%	0.016%
54	23.438	3505	3506	3510	rBV4	1354	1112	0.13%	0.013%
55	23.778	3561	3564	3567	rBV4	2051	2894	0.33%	0.035%
56	23.866	3576	3579	3580	rBV2	3532	3676	0.42%	0.044%
57	23.878	3580	3581	3588	rVB7	4373	5288	0.60%	0.064%
58	24.019	3602	3605	3607	rBV4	1242	1484	0.17%	0.018%
59	24.066	3610	3613	3619	rVB6	4152	7719	0.88%	0.093%
60	24.472	3681	3682	3685	rBV3	1503	1414	0.16%	0.017%
61	24.795	3725	3737	3750	rBV	304442	839217	95.68%	10.084%
62	25.018	3762	3775	3788	rBV2	191022	536377	61.15%	6.445%
63	25.312	3823	3825	3827	rBV3	1495	1589	0.18%	0.019%
64	25.459	3846	3850	3852	rVB4	1575	2033	0.23%	0.024%
65	25.735	3895	3897	3900	rVB3	1655	1106	0.13%	0.013%
66	25.776	3903	3904	3909	rVB3	1493	1647	0.19%	0.020%
67	25.841	3912	3915	3916	rBV2	1920	1755	0.20%	0.021%
68	26.187	3968	3974	3979	rVB7	4920	11055	1.26%	0.133%
69	26.428	4011	4015	4016	rBV4	1346	1363	0.16%	0.016%
70	26.499	4026	4027	4030	rBV3	1224	1334	0.15%	0.016%
71	26.587	4039	4042	4043	rBV3	1264	1221	0.14%	0.015%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
 Data File : BG020172.D
 Acq On : 15 Dec 2015 3:32
 Operator : UM/SJ
 Sample : PB87250BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

72	26.604	4043	4045	4046	rVV2	1492	1161	0.13%	0.014%
73	26.646	4050	4052	4055	rVB3	1179	1159	0.13%	0.014%
74	27.498	4195	4197	4198	rBV2	1594	1049	0.12%	0.013%
75	27.550	4199	4206	4212	rVV9	5388	15253	1.74%	0.183%
76	27.785	4245	4246	4248	rBV2	1462	1294	0.15%	0.016%
77	27.956	4271	4275	4276	rBV3	1654	1322	0.15%	0.016%
78	28.003	4280	4283	4284	rBV2	1322	1310	0.15%	0.016%
79	28.302	4333	4334	4337	rBV2	1641	1633	0.19%	0.020%
80	28.767	4412	4413	4415	rBV	1301	1156	0.13%	0.014%
81	29.160	4479	4480	4482	rBV	1847	1368	0.16%	0.016%
82	29.184	4482	4484	4485	rBV2	2229	1242	0.14%	0.015%
83	29.219	4487	4490	4491	rBV2	2839	2592	0.30%	0.031%
84	29.489	4535	4536	4539	rVB2	1888	1156	0.13%	0.014%
85	29.513	4539	4540	4543	rBV2	1093	1173	0.13%	0.014%
86	30.065	4631	4634	4635	rBV4	1372	1262	0.14%	0.015%
87	30.177	4651	4653	4655	rBV3	1348	1314	0.15%	0.016%
88	30.329	4678	4679	4681	rBV2	1432	1150	0.13%	0.014%
89	30.888	4771	4774	4775	rBV3	1070	1104	0.13%	0.013%
90	30.923	4777	4780	4782	rBV2	1032	1187	0.14%	0.014%
91	31.181	4821	4824	4826	rBV4	1886	2357	0.27%	0.028%
92	31.516	4879	4881	4882	rBV2	1631	1428	0.16%	0.017%
93	31.552	4884	4887	4888	rBV3	1500	1758	0.20%	0.021%
94	31.669	4904	4907	4908	rBV3	1690	1770	0.20%	0.021%
95	31.822	4931	4933	4935	rBV3	1450	1402	0.16%	0.017%
96	31.851	4935	4938	4939	rVV3	1924	1426	0.16%	0.017%
97	31.945	4951	4954	4956	rVB3	1391	1344	0.15%	0.016%
98	32.368	5023	5026	5027	rBV3	1254	1540	0.18%	0.019%
99	32.509	5047	5050	5051	rBV2	1189	1242	0.14%	0.015%
100	32.639	5070	5072	5073	rBV2	1391	1080	0.12%	0.013%


Sum of corrected areas: 8322272

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
Data File : BG020172.D
Acq On : 15 Dec 2015 3:32
Operator : UM/SJ
Sample : PB87250BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK50

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

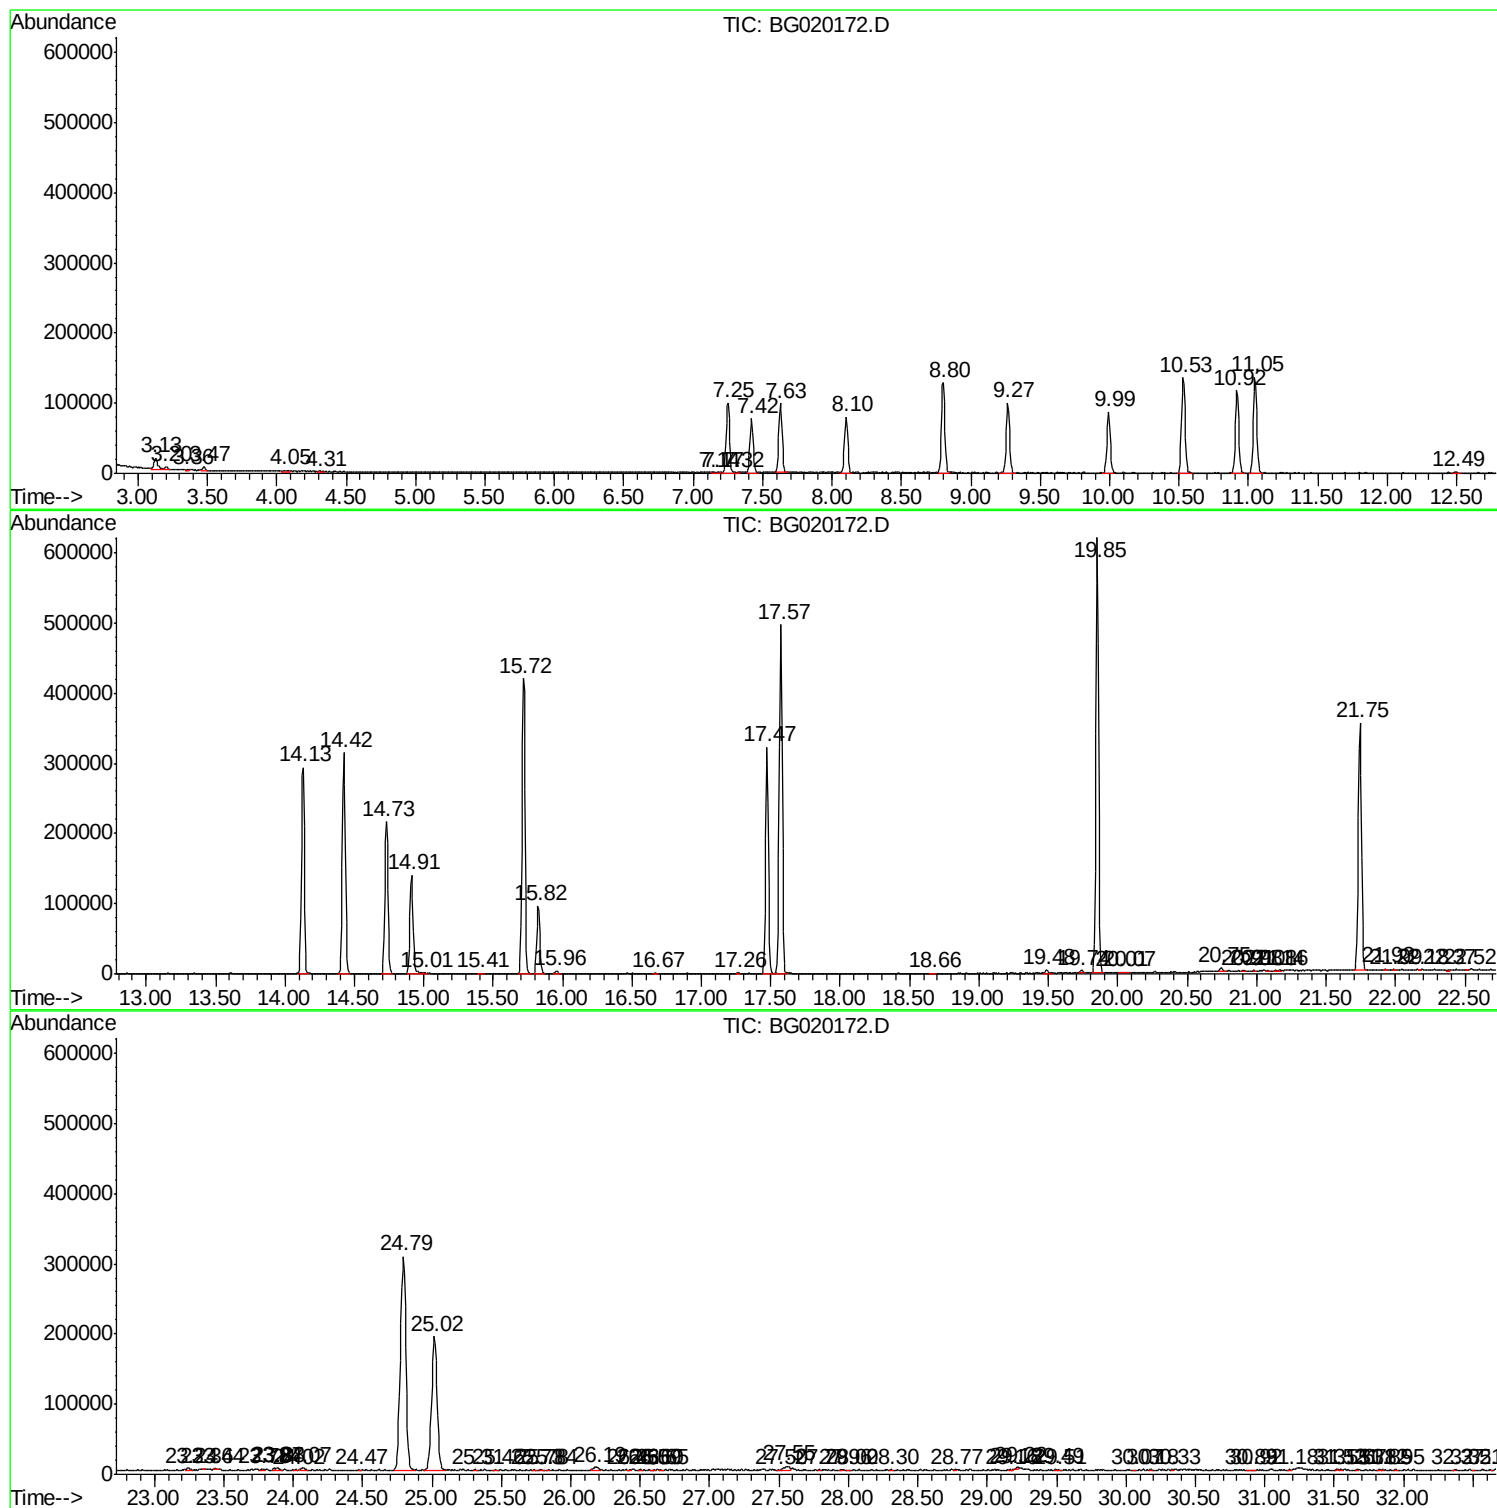

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
Data File : BG020172.D
Acq On : 15 Dec 2015 3:32
Operator : UM/SJ
Sample : PB87250BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK50

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
Data File : BG020172.D
Acq On : 15 Dec 2015 3:32
Operator : UM/SJ
Sample : PB87250BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK50

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc