
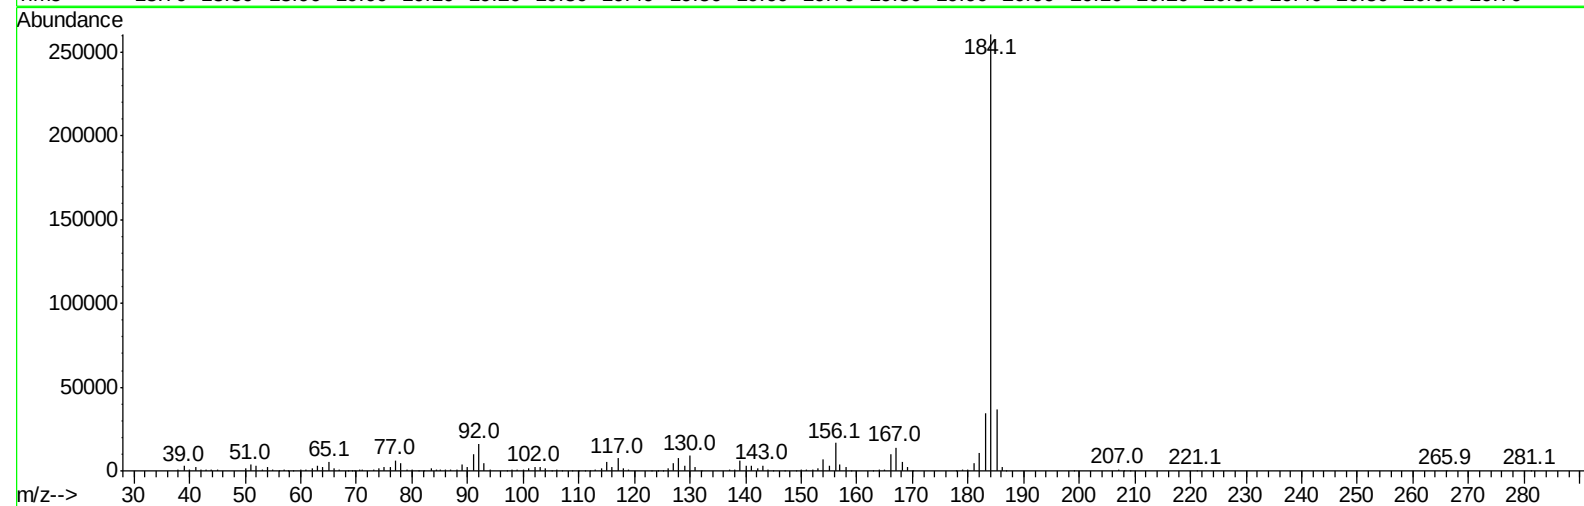


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG121517\
Data File : BG031592.D
Acq On : 15 Dec 2017 16:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 01:23:44 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

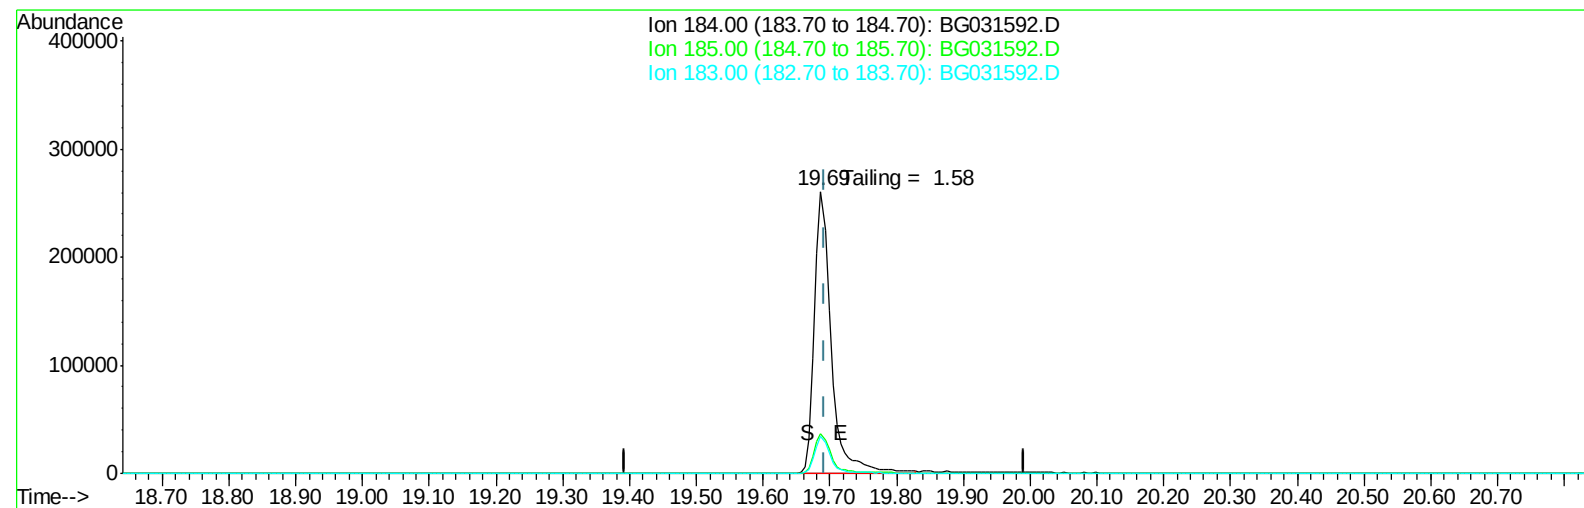

TIC: BG031592.D

(76) Benzidine



19.687min (-0.006) 309394.37ng

response 446413

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.22
183.00	13.30	13.30
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG121517\
Data File : BG031592.D
Acq On : 15 Dec 2017 16:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 01:23:44 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

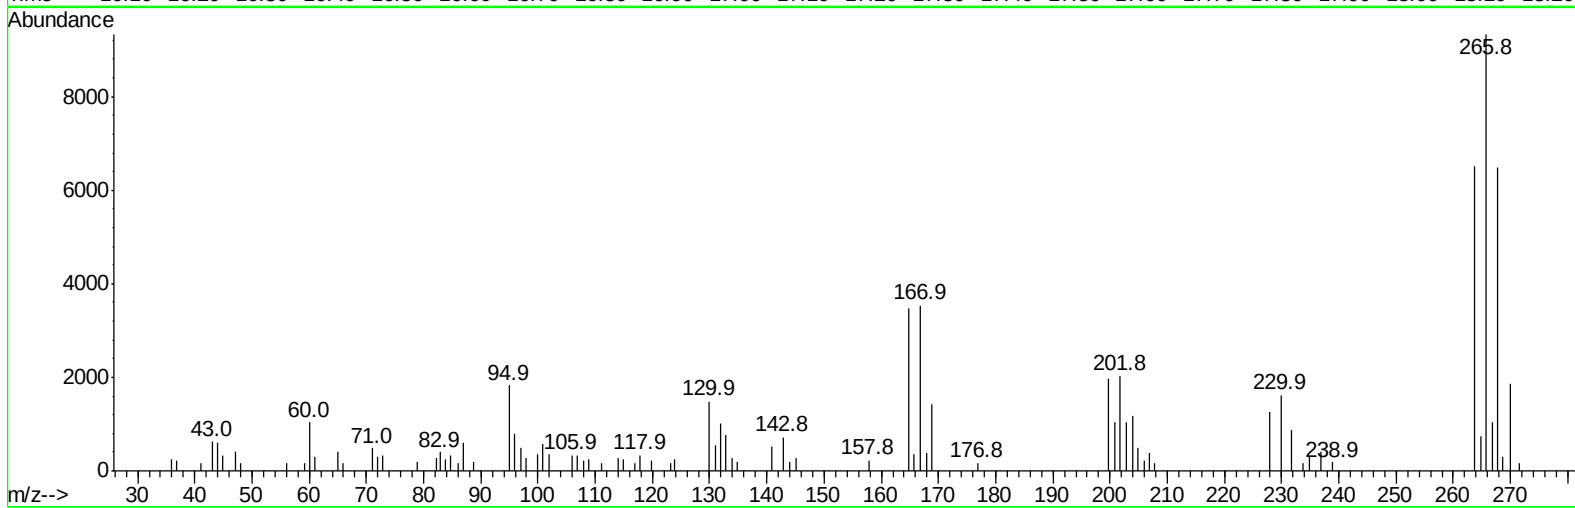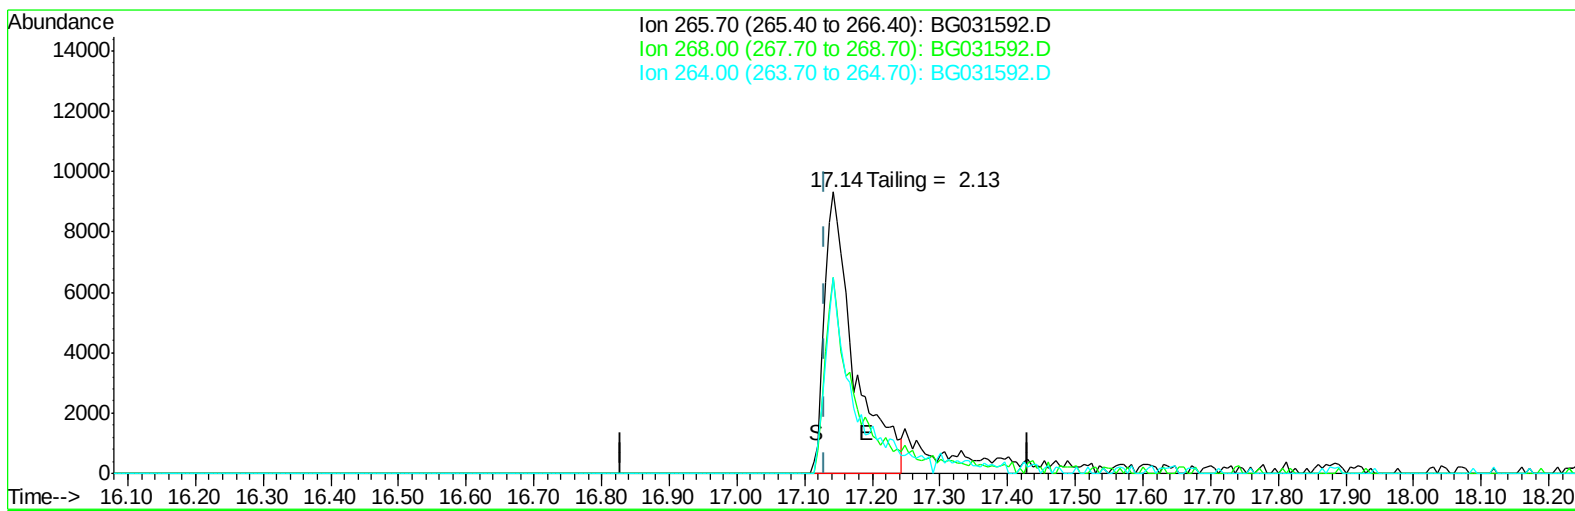

TIC: BG031592.D

(69) Pentachlorophenol (C)

17.143min (+0.013) 0.00ng

response 28471

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	72.82
264.00	62.00	69.77
0.00	0.00	0.00