


Data Path : Z:\HPCHEM1\BNA_G\Data\BG121517\
 Data File : BG031592.D
 Acq On : 15 Dec 2017 16:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG121117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 11 17:25:55 2017

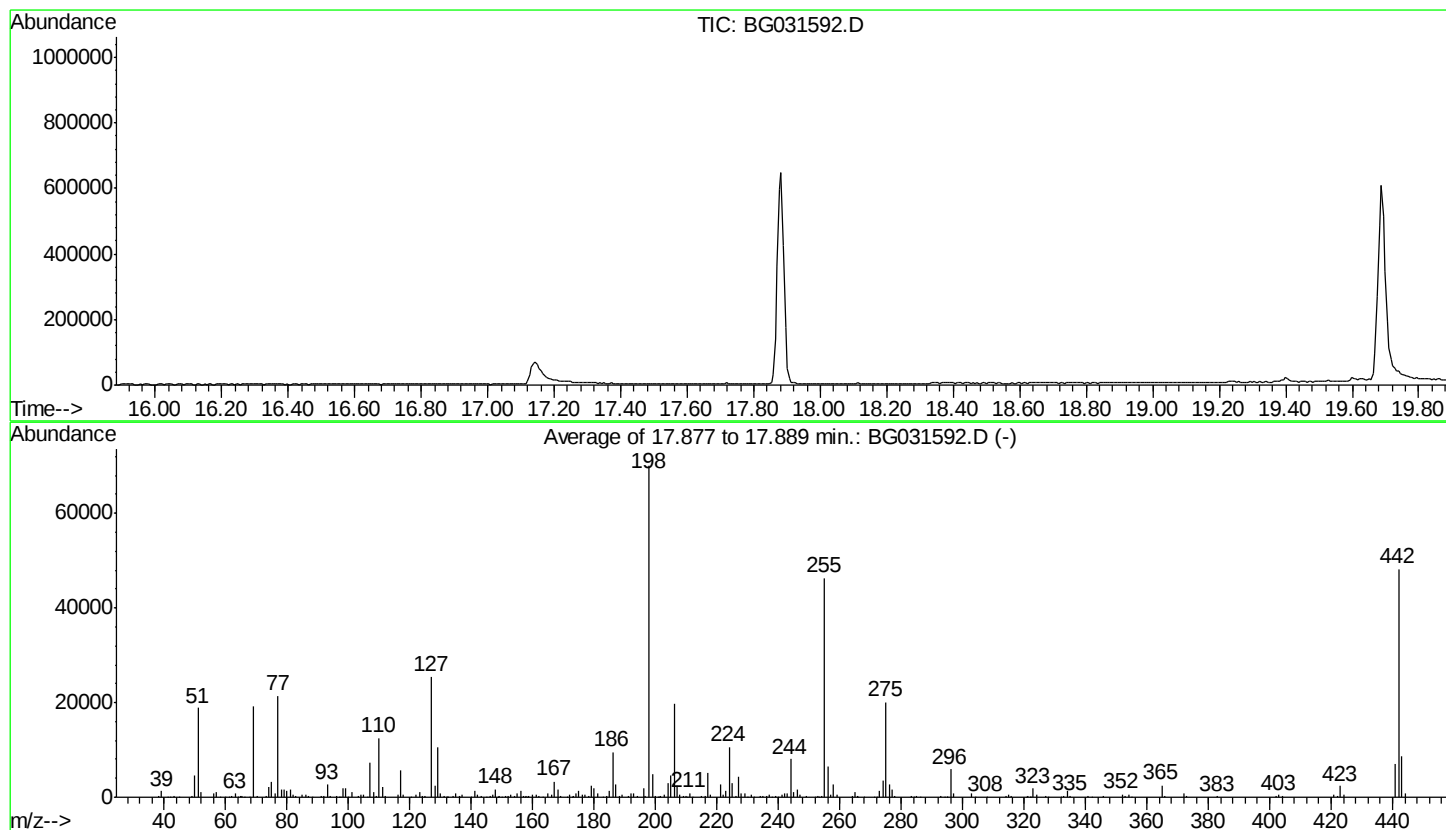

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	18854	PASS
68	69	0.00	2	0.7	139	PASS
69	198	0.00	100	27.3	19151	PASS
70	69	0.00	2	0.8	162	PASS
127	198	10	80	36.3	25456	PASS
197	198	0.00	2	0.5	360	PASS
198	198	100	100	100.0	70074	PASS
199	198	5	9	7.0	4902	PASS
275	198	10	60	28.8	20162	PASS
365	198	1	100	3.6	2523	PASS
441	442	0.01	24	14.8	7134	PASS
442	198	50	100	68.9	48250	PASS
443	442	15	24	18.1	8711	PASS