
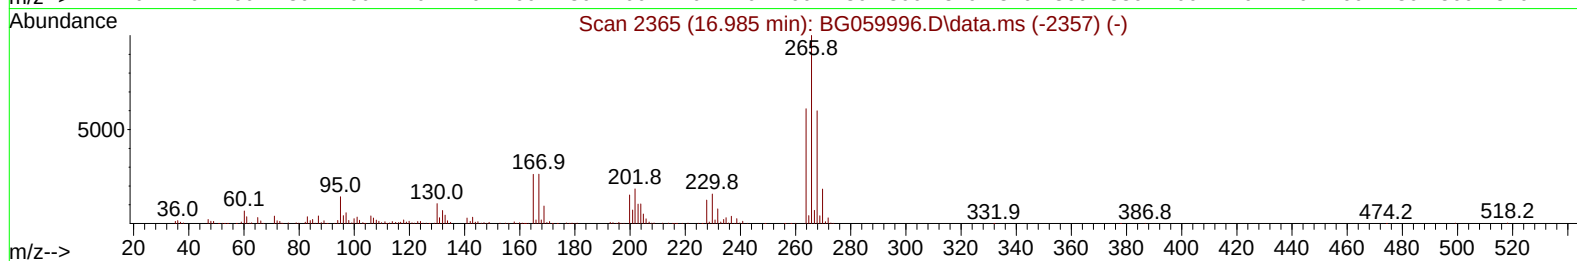
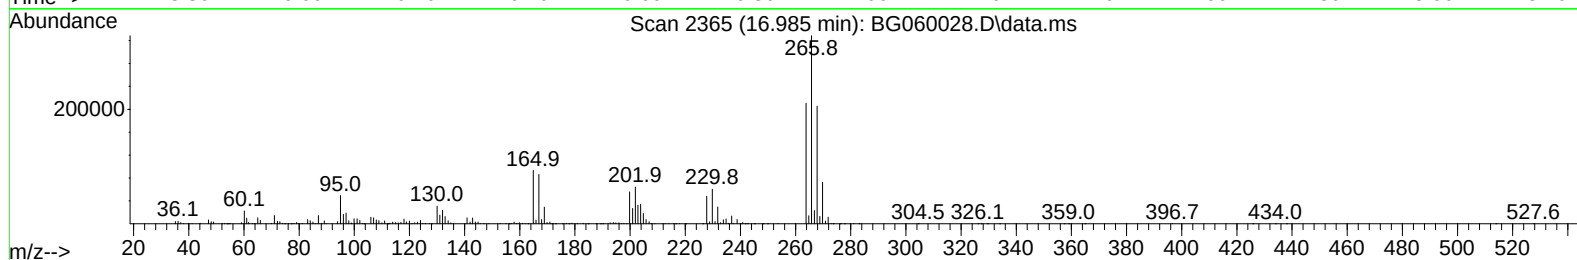


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121523\
Data File : BG060028.D
Acq On : 15 Dec 2023 9:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 11:18:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

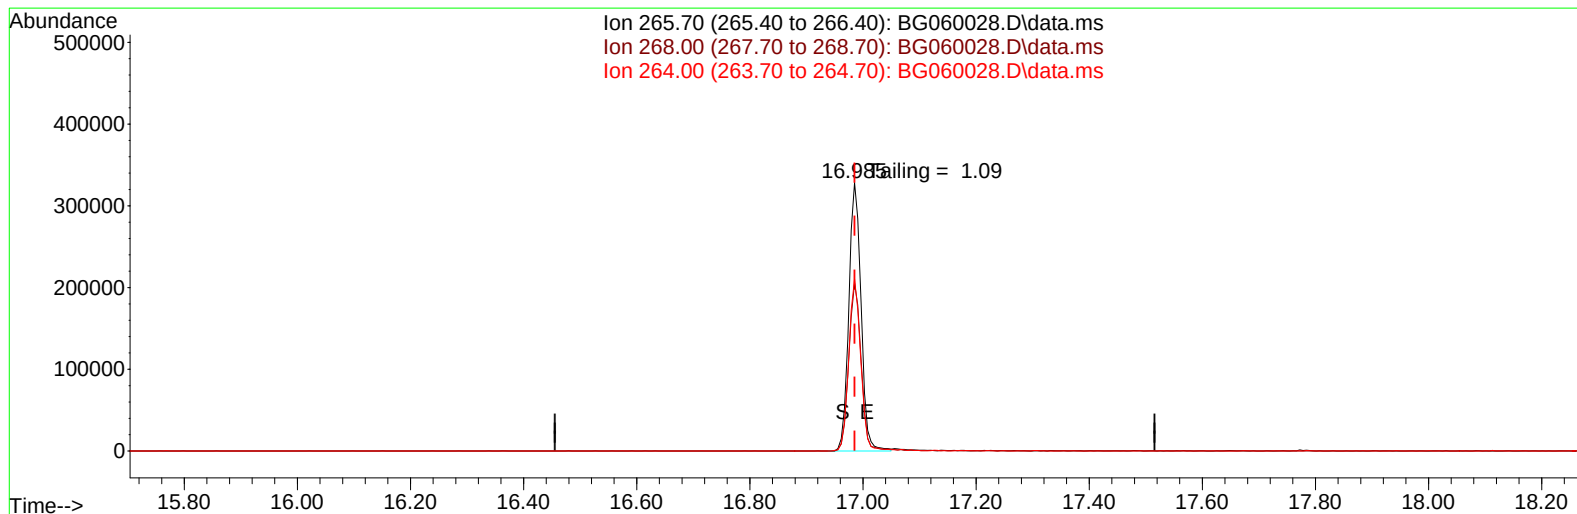

TIC: BG060028.D\data.ms

(70) Pentachlorophenol (C)




16.985min (-0.000) 54639.77 ng

response 493928

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	62.56
264.00	61.00	64.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121523\
Data File : BG060028.D
Acq On : 15 Dec 2023 9:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 11:18:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

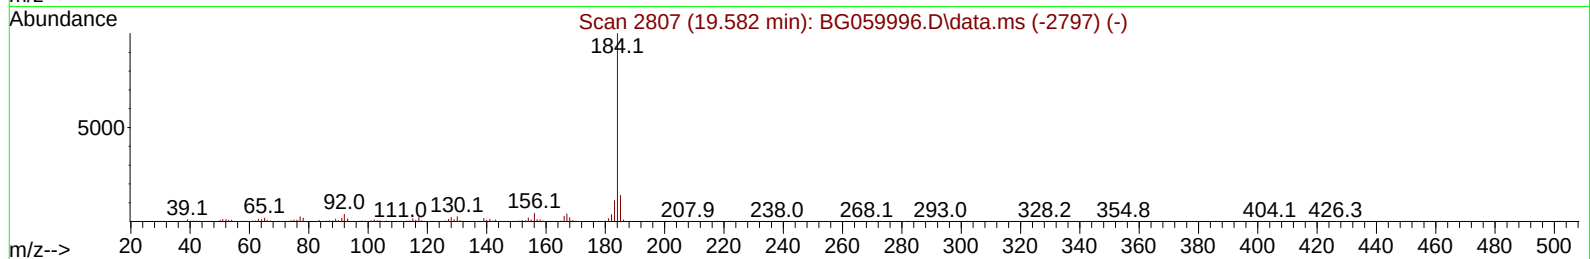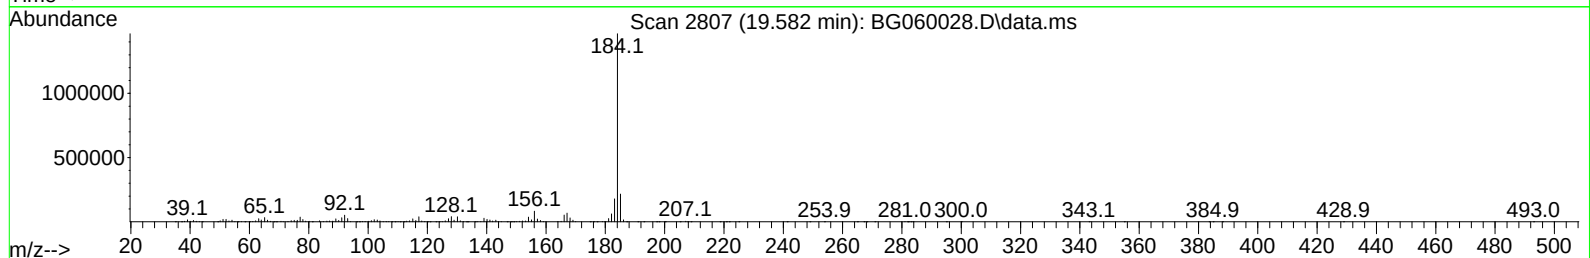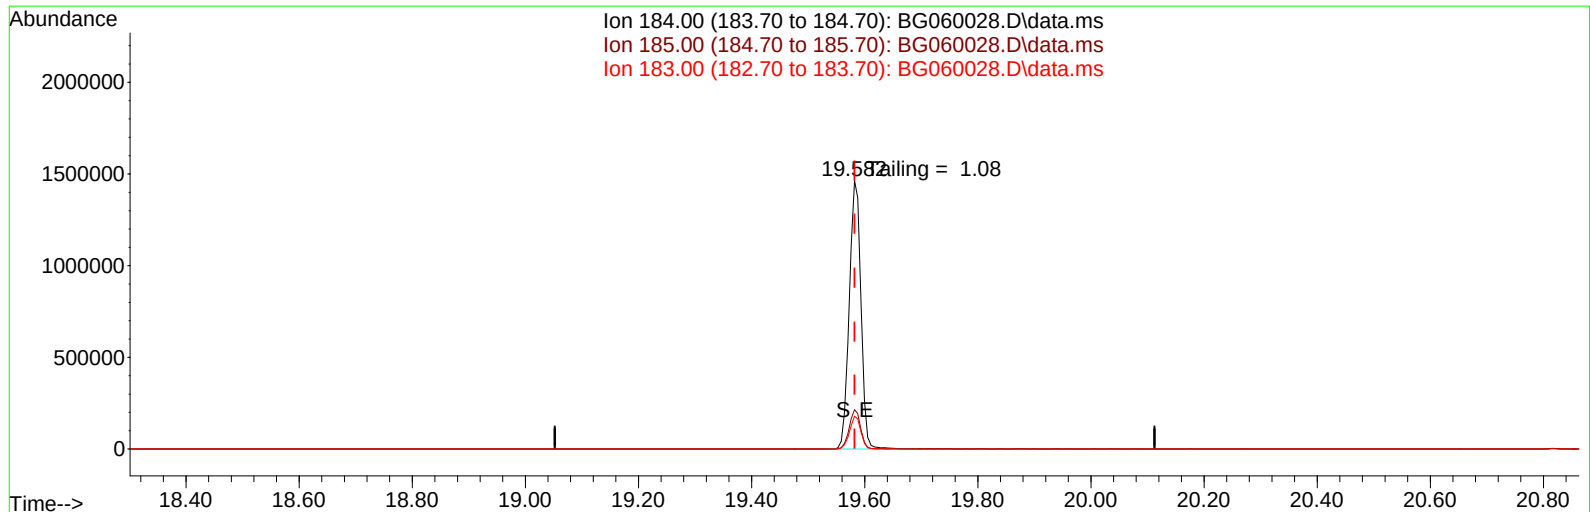

TIC: BG060028.D\data.ms

(77) Benzidine**19.582min (-0.000) 90165.94 ng****response 2102053**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.69
183.00	11.20	12.22
0.00	0.00	0.00