
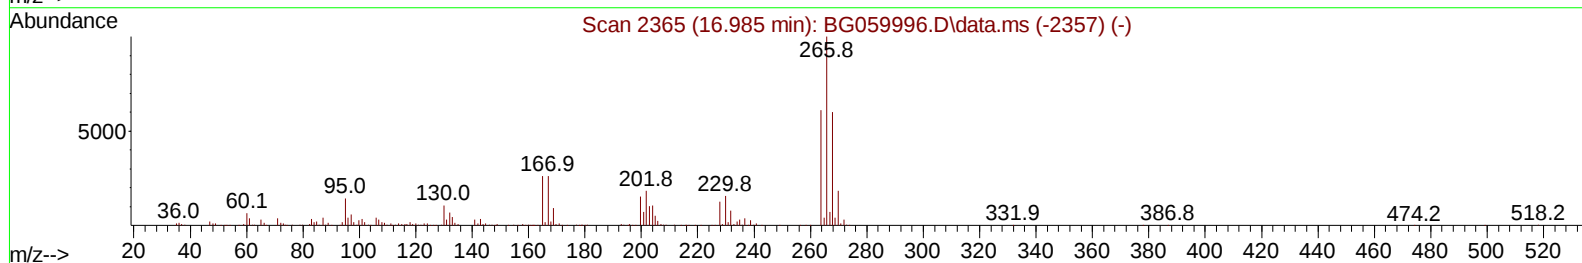
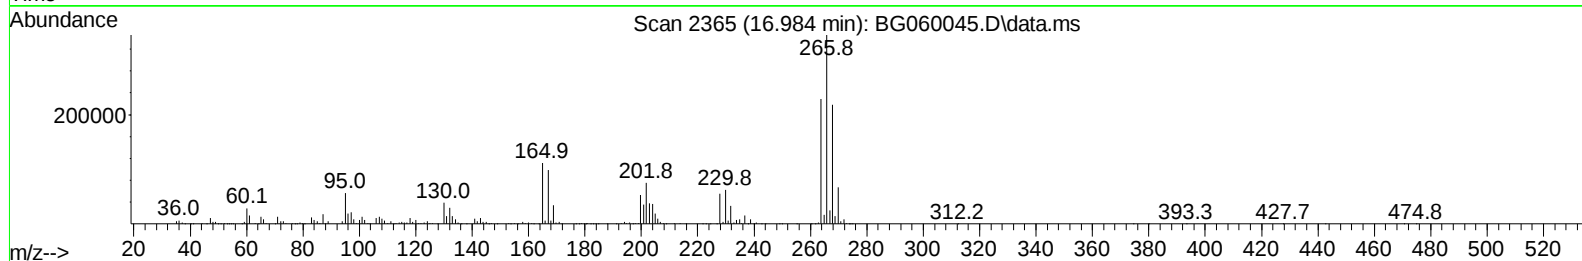


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121523\
Data File : BG060045.D
Acq On : 15 Dec 2023 21:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 01:04:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

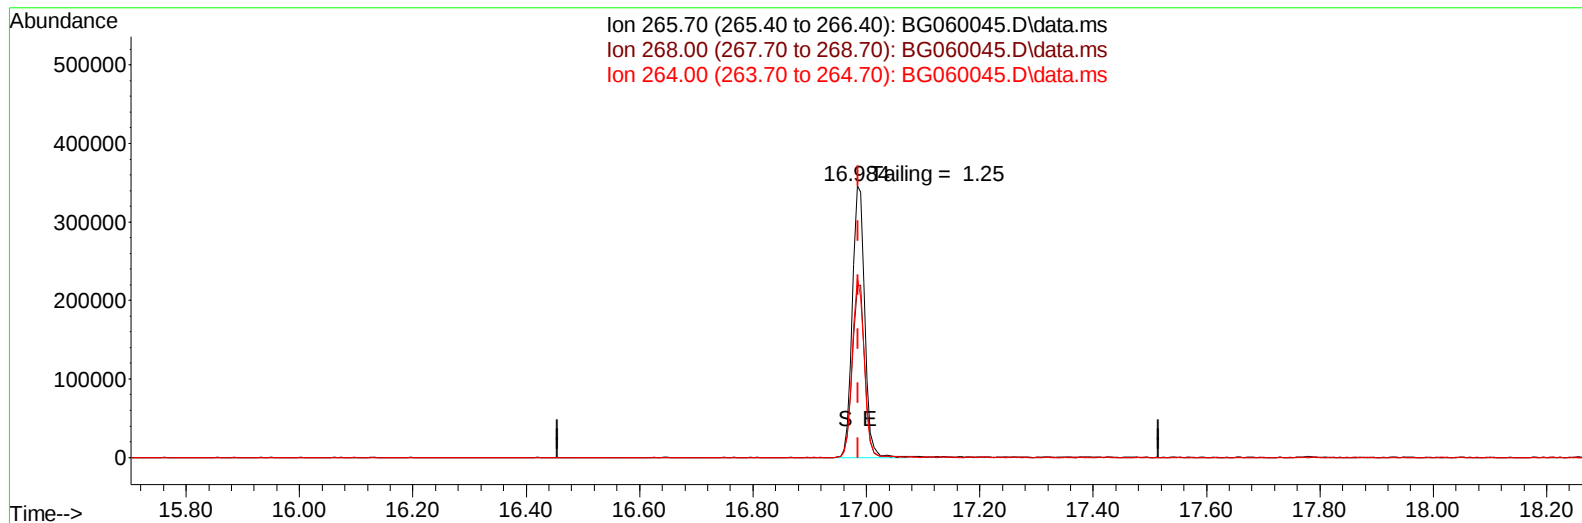

TIC: BG060045.D\data.ms

(70) Pentachlorophenol (C)




16.984min (-0.002) 27787.97 ng

response 524363

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	63.13
264.00	61.00	66.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121523\
Data File : BG060045.D
Acq On : 15 Dec 2023 21:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 01:04:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

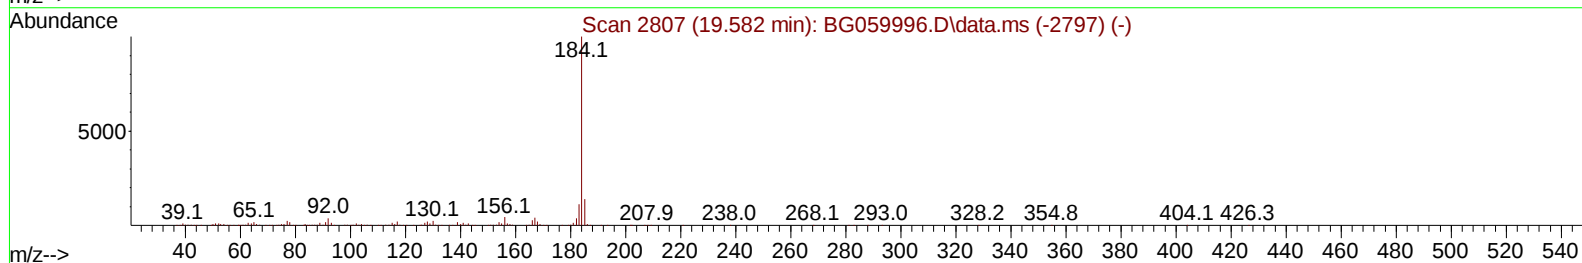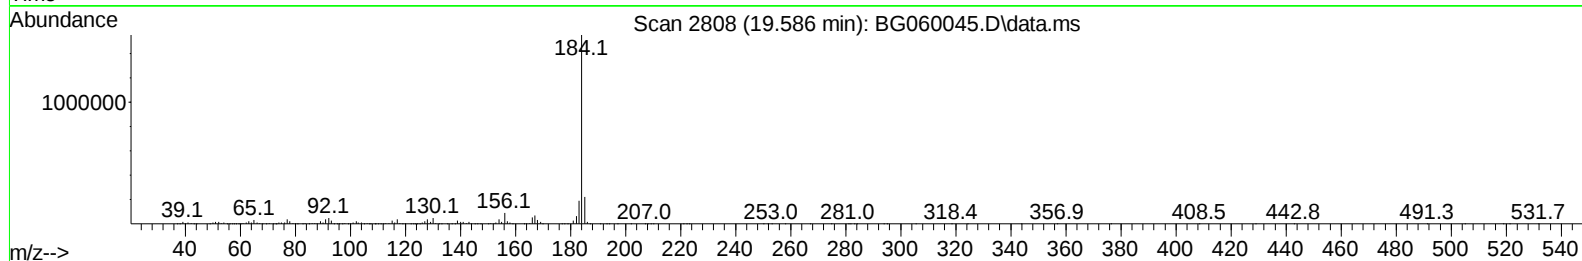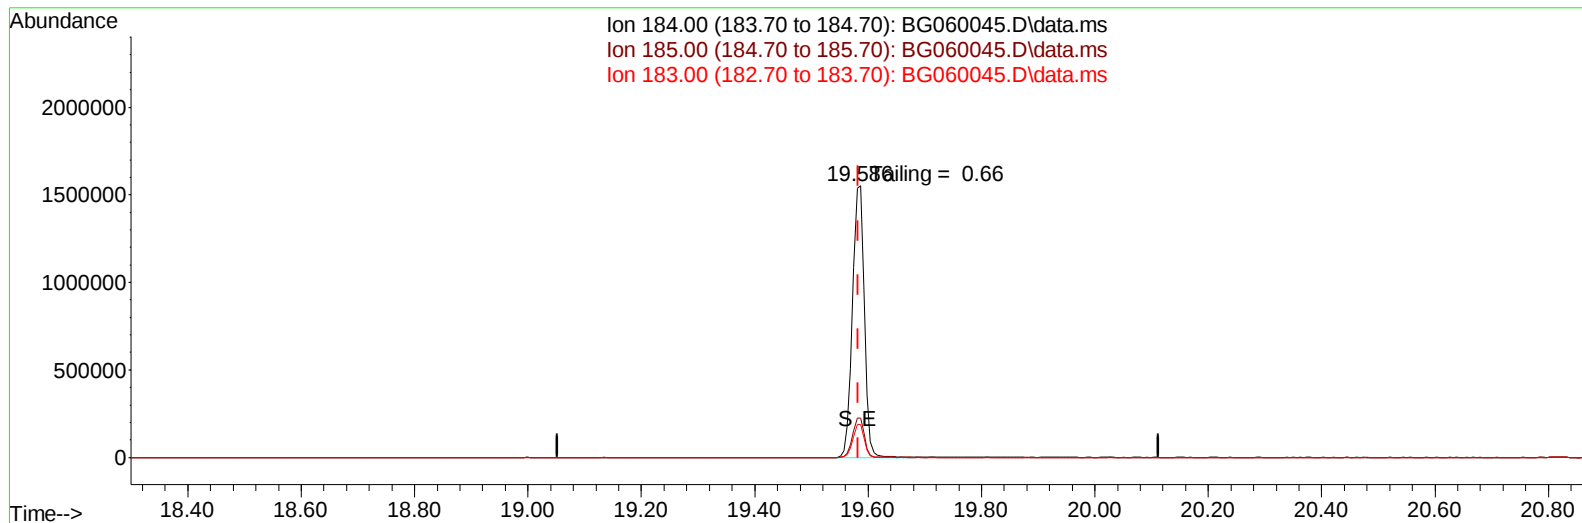

TIC: BG060045.D\data.ms

(77) Benzidine**19.586min (+ 0.004) 59657.78 ng****response 2264379**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.41
183.00	11.20	12.15
0.00	0.00	0.00