
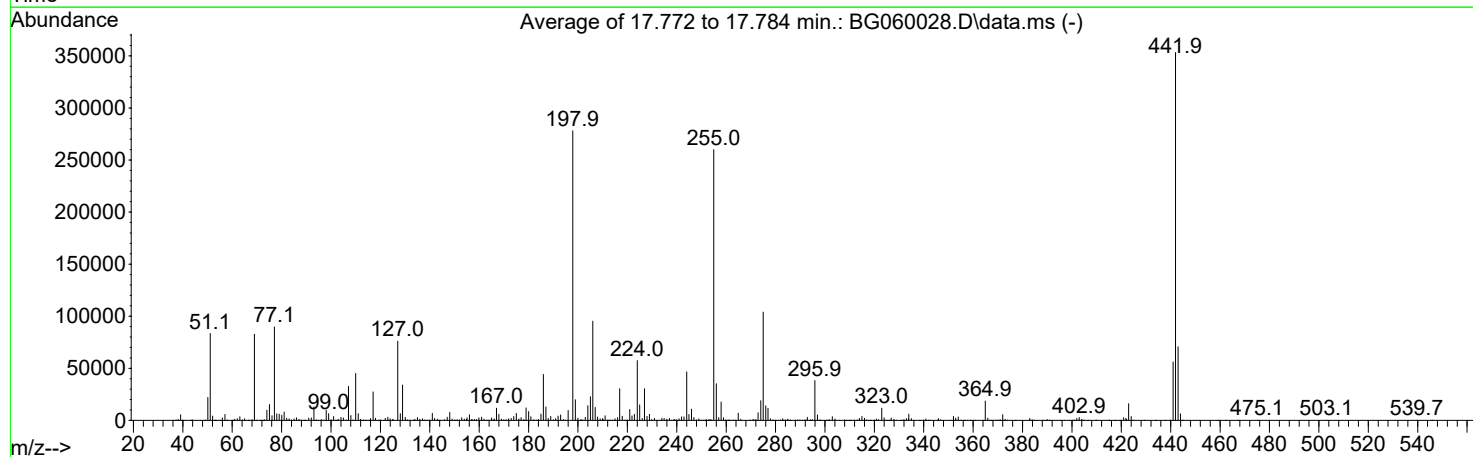


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121523\
 Data File : BG060028.D
 Acq On : 15 Dec 2023 9:45
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 14 01:47:12 2023

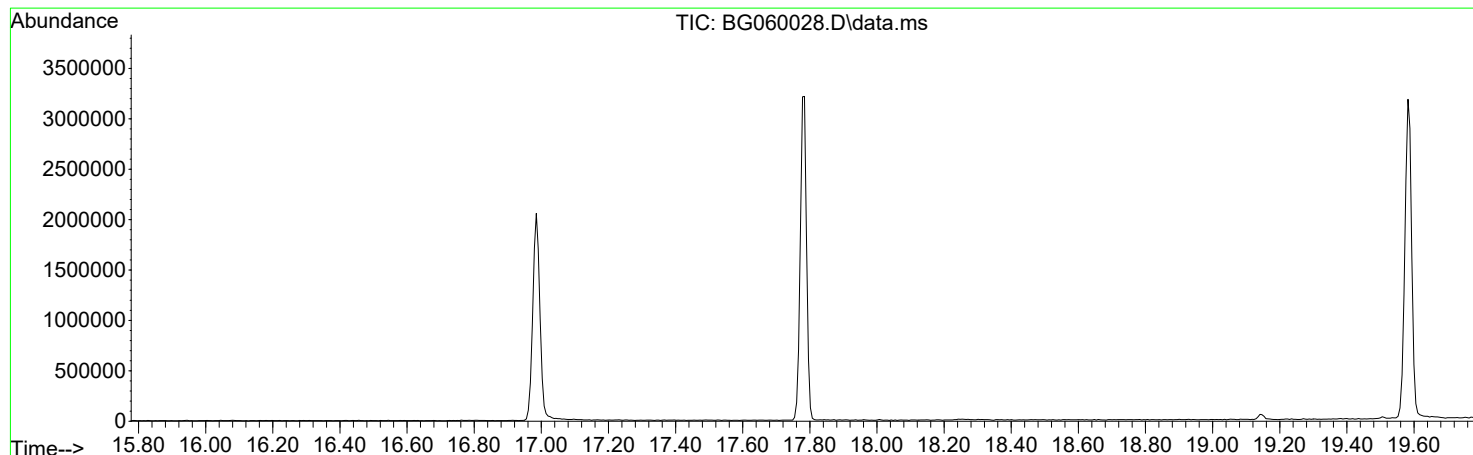

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	83501	PASS
68	69	0.00	2	0.7	603	PASS
69	198	0.00	100	29.7	82661	PASS
70	69	0.00	2	0.4	342	PASS
127	198	10	80	27.4	76104	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	278187	PASS
199	198	5	9	7.1	19889	PASS
275	198	10	60	37.4	104008	PASS
365	198	1	100	6.7	18685	PASS
441	198	0.01	100	20.1	56051	PASS
442	442	50	100	100.0	353259	PASS
443	442	15	24	20.0	70619	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/15/2023	BNA_G	<u>BG060028.D</u>
Compound Name	Response	Retention Time
DDT	1138525	20.822
DDD	20210	20.375
DDE	877	19.87
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21087	1159612	1.82

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121523\
Data File : BG060028.D
Acq On : 15 Dec 2023 9:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 15 11:18:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

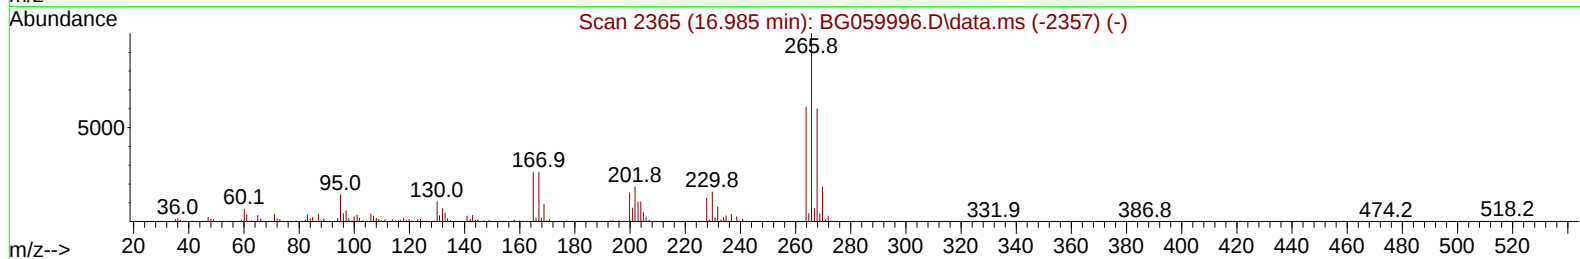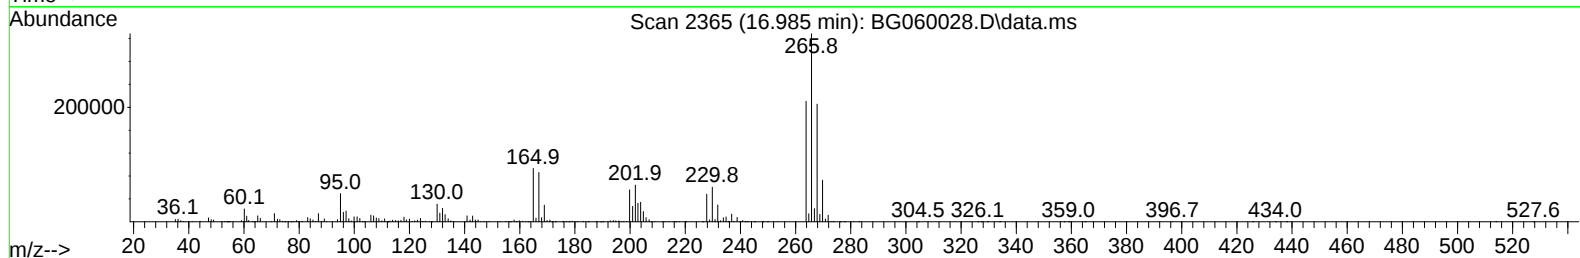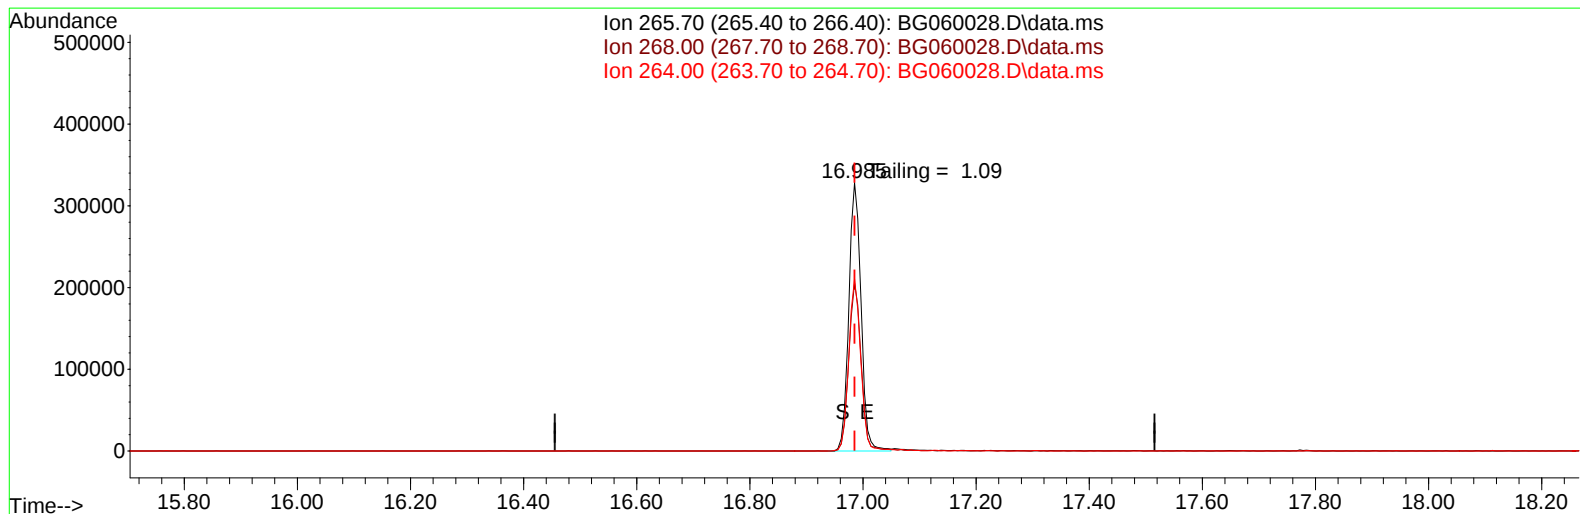

TIC: BG060028.D\data.ms

(70) Pentachlorophenol (C)

16.985min (-0.000) 54639.77 ng




response 493928

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	62.56
264.00	61.00	64.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121523\
Data File : BG060028.D
Acq On : 15 Dec 2023 9:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 15 11:18:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

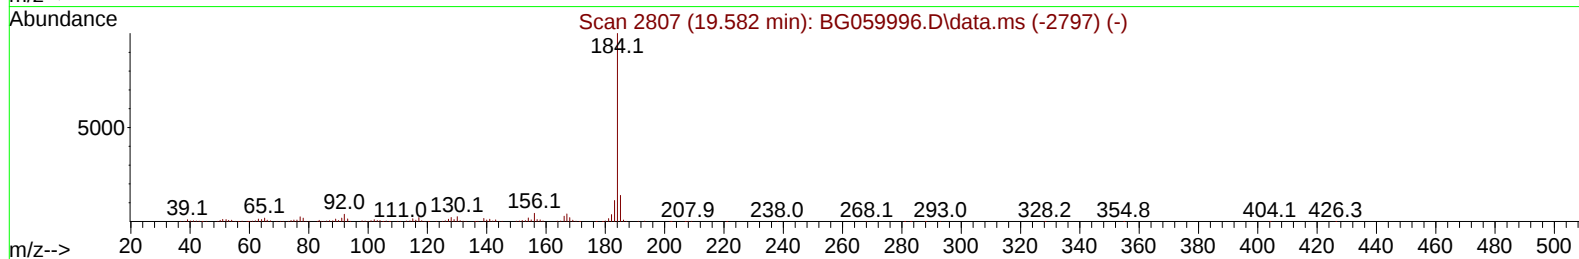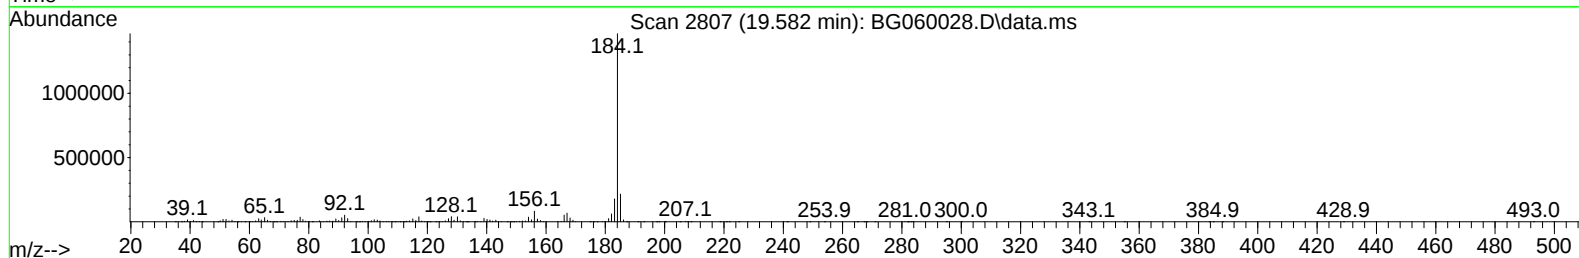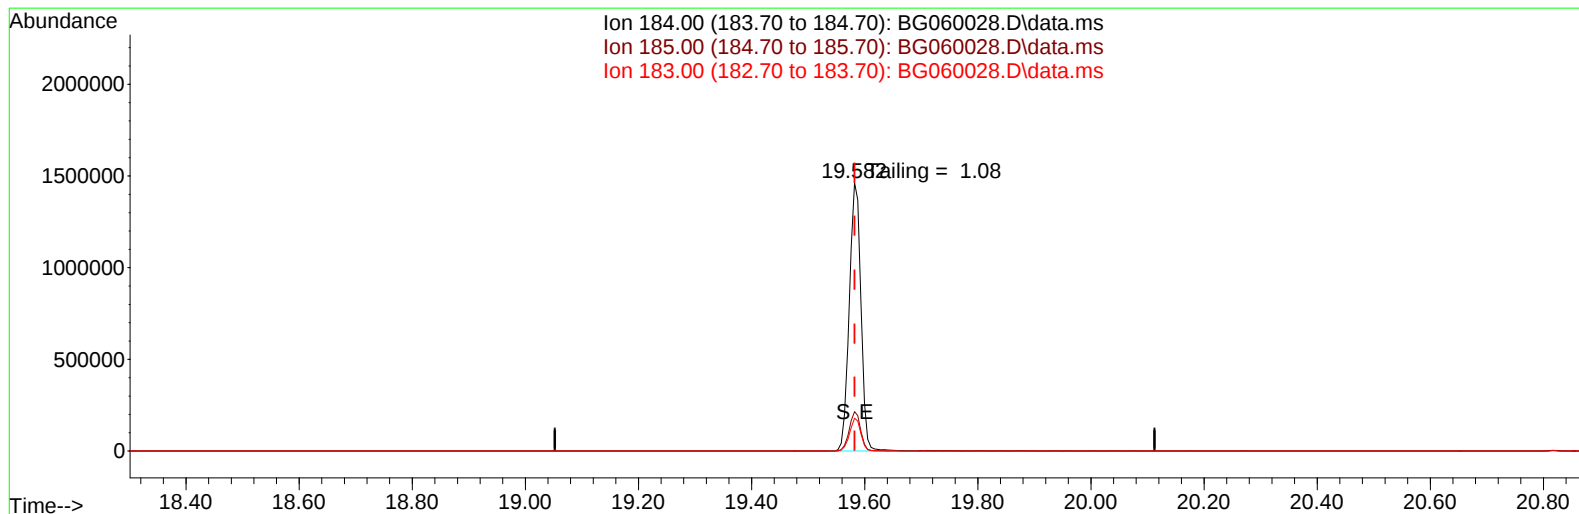

TIC: BG060028.D\data.ms

(77) Benzidine

19.582min (-0.000) 90165.94 ng

response 2102053

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.69
183.00	11.20	12.22
0.00	0.00	0.00