


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121523\
Data File : BG060045.D
Acq On : 15 Dec 2023 21:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 14 01:47:12 2023

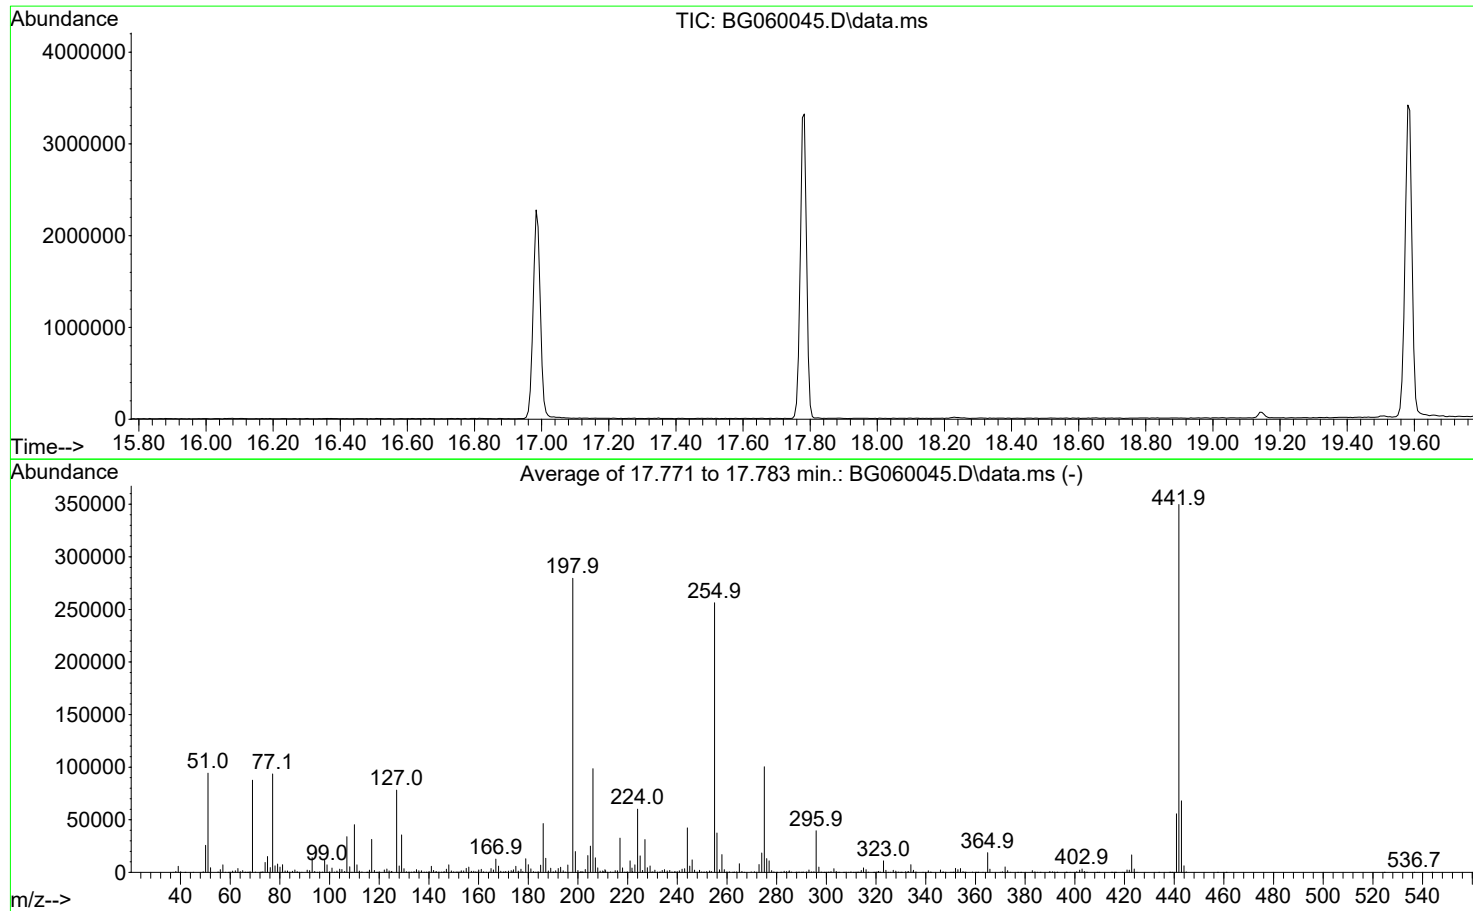

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	94394	PASS
68	69	0.00	2	0.7	599	PASS
69	198	0.00	100	31.3	87593	PASS
70	69	0.00	2	0.4	388	PASS
127	198	10	80	28.0	78157	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	279573	PASS
199	198	5	9	7.1	19794	PASS
275	198	10	60	35.9	100419	PASS
365	198	1	100	6.7	18647	PASS
441	198	0.01	100	19.9	55632	PASS
442	442	50	100	100.0	349739	PASS
443	442	15	24	19.4	67957	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/15/2023	BNA_G	BG060045.D
Compound Name	Response	Retention Time
DDT	1207437	20.82
DDD	26558	20.374
DDE	718	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27276	1234713	2.21

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121523\
Data File : BG060045.D
Acq On : 15 Dec 2023 21:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 18 01:04:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

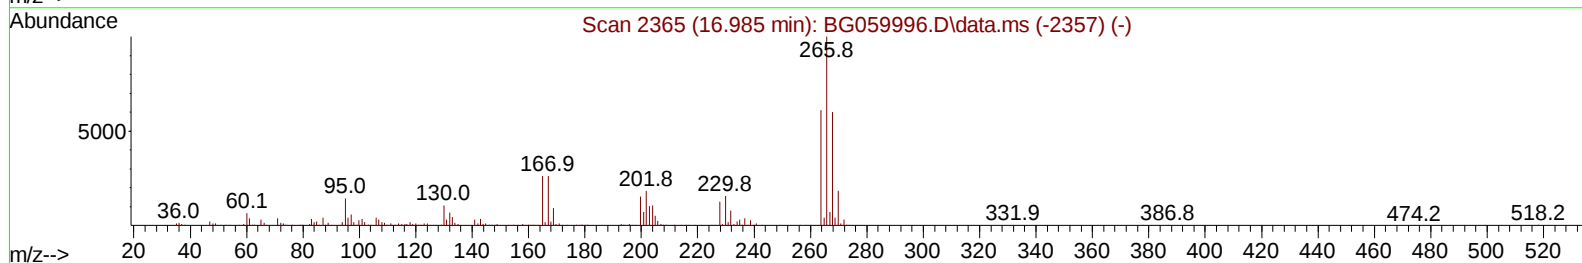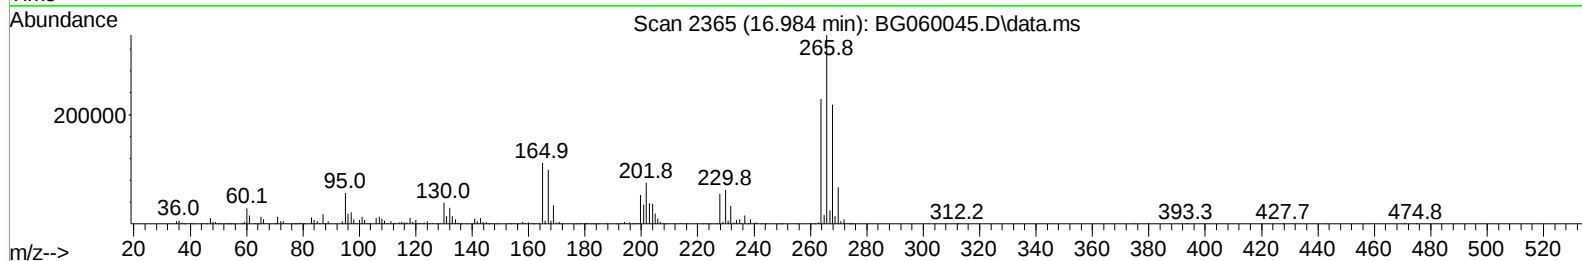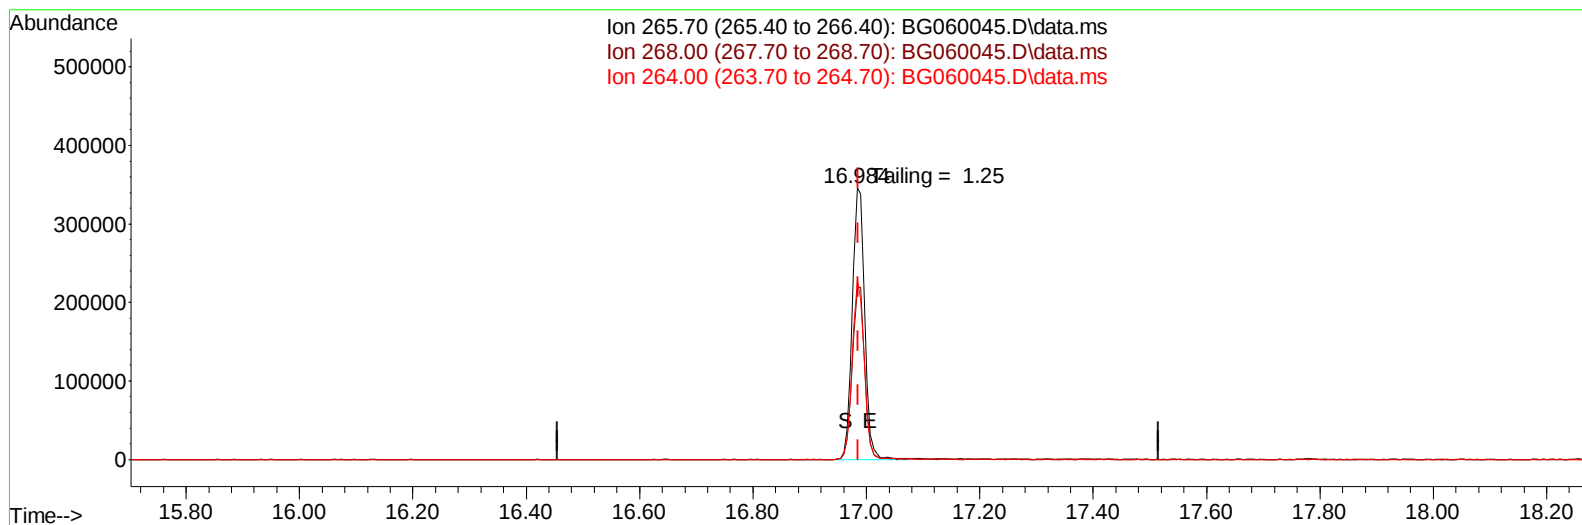

TIC: BG060045.D\data.ms

(70) Pentachlorophenol (C)

16.984min (-0.002) 27787.97 ng




response 524363

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	63.13
264.00	61.00	66.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121523\
 Data File : BG060045.D
 Acq On : 15 Dec 2023 21:55
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Dec 18 01:04:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 14 01:47:12 2023
 Response via : Initial Calibration

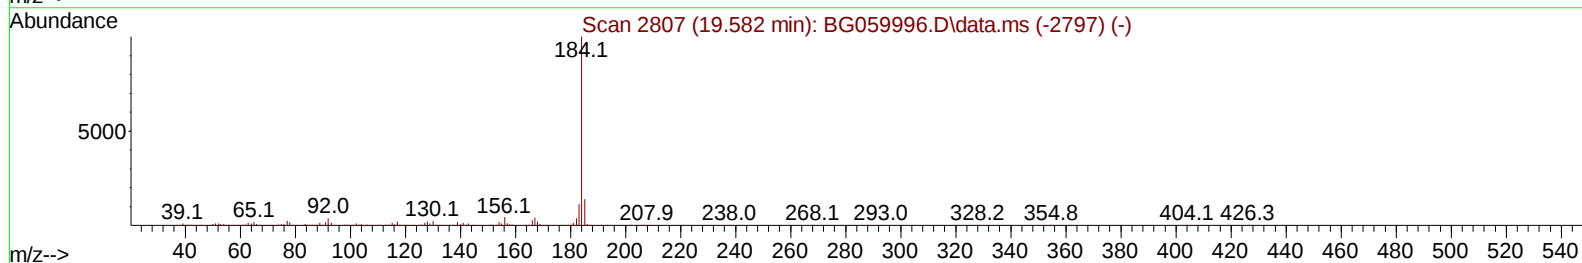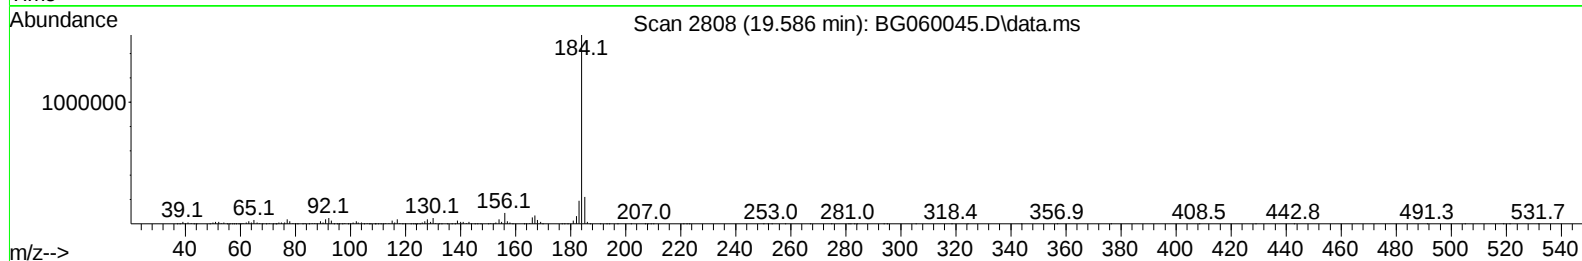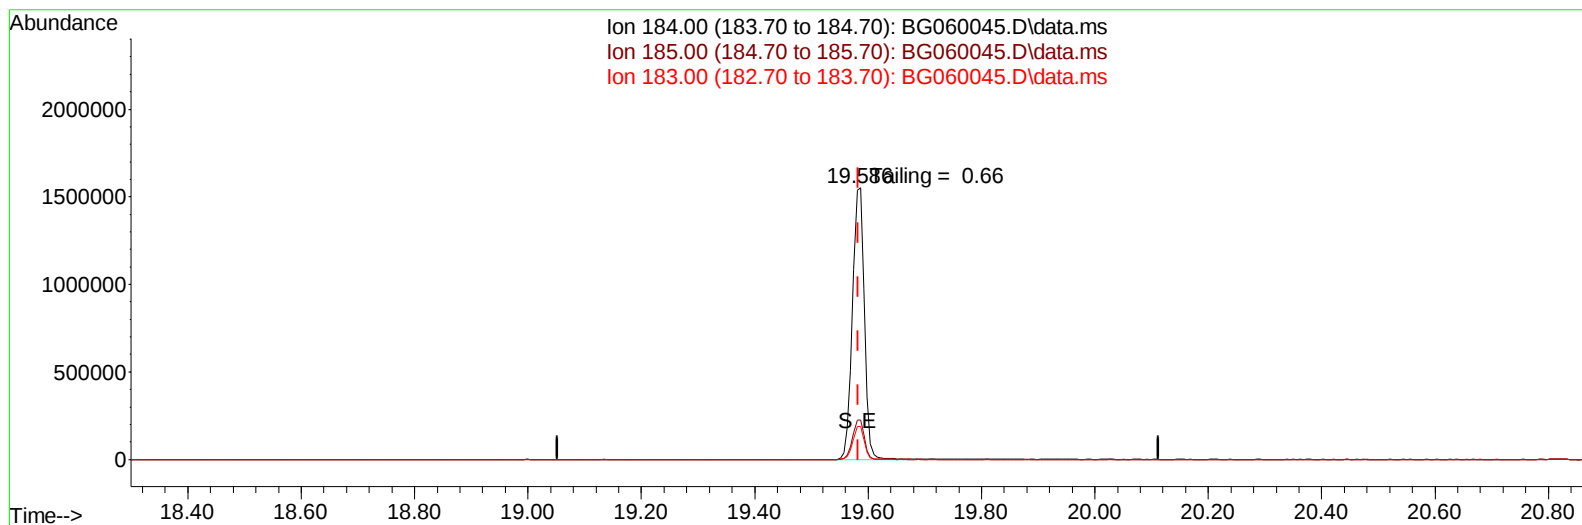

TIC: BG060045.D\data.ms

(77) Benzidine**19.586min (+ 0.004) 59657.78 ng****response 2264379**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.41
183.00	11.20	12.15
0.00	0.00	0.00