

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121615\
 Data File : BG020208.D
 Acq On : 16 Dec 2015 3:14
 Operator : UM/SJ
 Sample : PB87297BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK97

Quant Time: Dec 16 04:19:35 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 16 03:45:51 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	16616	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	78627	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	63324	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	171368	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	187980	20.00	ng/ul	0.00
86) Perylene-d12	25.01	264	174069	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.47	96	2119	7.04	ng/uL	0.00
5) Phenol-d5	7.25	99	51873	35.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.42	67	31463	35.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.62	132	38694	36.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	46399	37.03	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	21711	35.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	26108	38.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	48396	35.03	ng/ul	0.00
29) 4-Chloroaniline-d4	11.04	131	69228	44.61	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	205693	40.16	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	220693	37.03	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	35139	38.25	ng/ul	0.00
58) Fluorene-d10	15.72	176	179905	38.72	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	36913	36.34	ng/ul	0.00
71) Anthracene-d10	17.57	188	314926	39.88	ng/ul	0.00
79) Pyrene-d10	19.85	212	357261	40.78	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	370545	42.68	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.80	70	1198	1.15 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121615\
Data File : BG020208.D
Acq On : 16 Dec 2015 3:14
Operator : UM/SJ
Sample : PB87297BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK97

Quant Time: Dec 16 04:19:35 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 16 03:45:51 2015
Response via : Initial Calibration

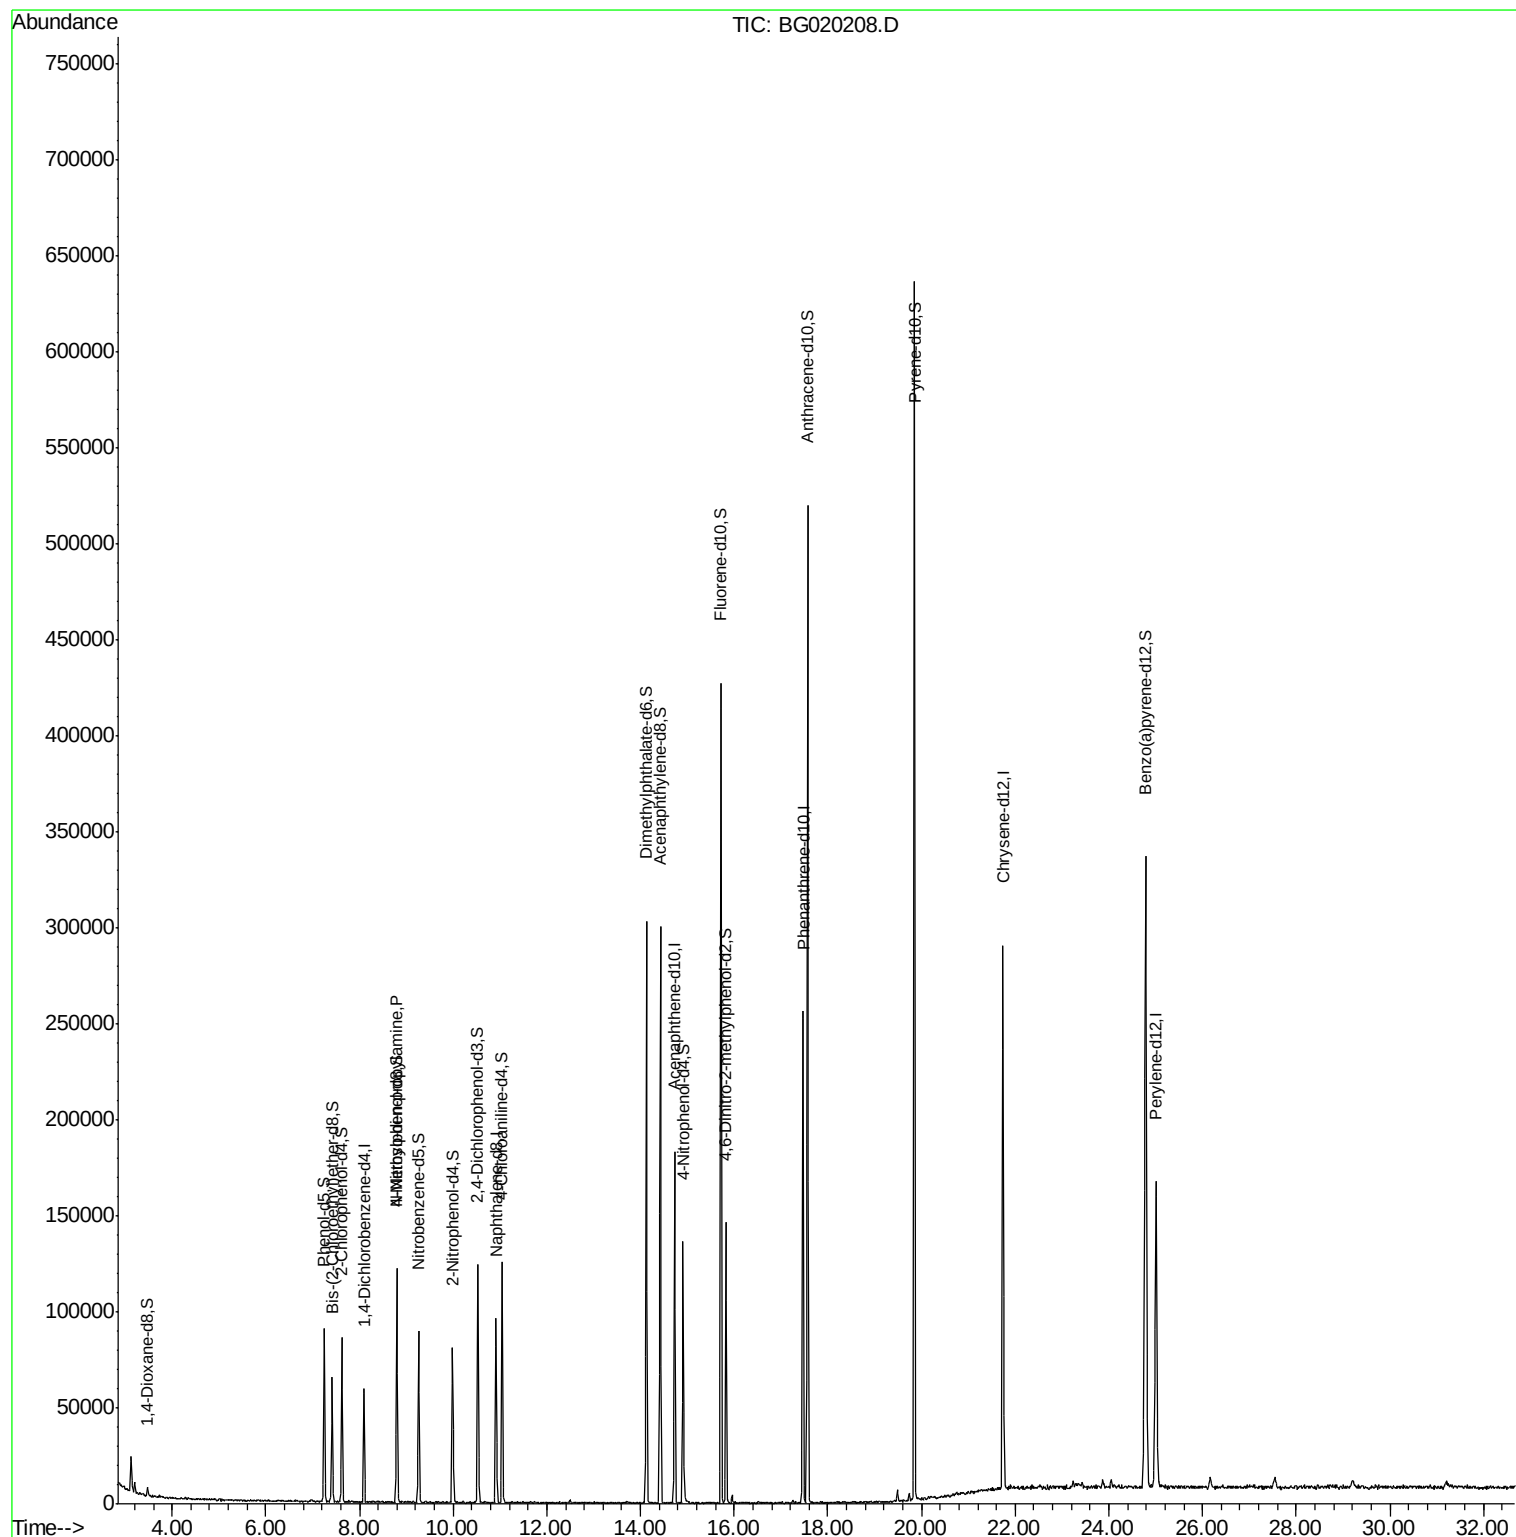

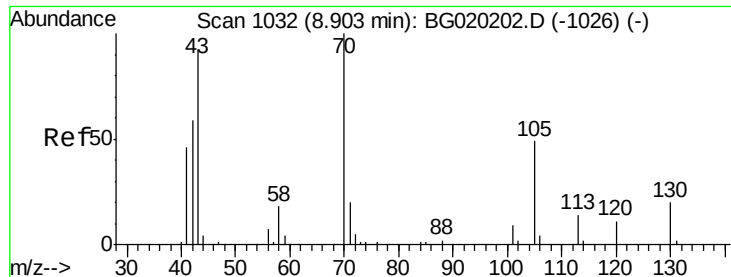

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.15 ng/ul
 RT: 8.80 min Scan# 1014
 Delta R.T. -0.10 min
 Lab File: BG020208.D
 Acq: 16 Dec 2015 3:14

Instrument :
 BNA_G
 ClientSampleId :
 SBLK97

Tgt Ion: 70 Resp: 1198
 Ion Ratio Lower Upper
 70 100
 42 300.1 44.3 66.5#
 101 0.0 7.6 11.4#
 130 0.0 17.0 25.4#

