

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121715\
 Data File : BG020225.D
 Acq On : 16 Dec 2015 16:09
 Operator : UM/SJ
 Sample : G4786-15DL2 100X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 G9C88DL2

Quant Time: Dec 17 00:43:58 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 17 00:37:15 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	15558	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	68570	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.72	164	55068	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	143381	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	163955	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	147358	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
44) Dimethylphthalate-d6	14.12	166	256	0.06	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	299	0.06	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.71	176	673	0.17	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	17.47	188	143381	21.70	ng/ul	-0.10
79) Pyrene-d10	19.84	212	579	0.08	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	403	0.05	ng/ul	0.00


Target Compounds					Qvalue
28) Naphthalene	10.96	128	27165	7.59 ng/ul	99
30) 4-Chloroaniline	10.96	127	3541	2.56 ng/ul#	29
34) 2-Methylnaphthalene	12.56	142	3486	1.27 ng/ul	98
35) 1-Methylnaphthalene	12.78	142	2686	1.02 ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121715\
Data File : BG020225.D
Acq On : 16 Dec 2015 16:09
Operator : UM/SJ
Sample : G4786-15DL2 100X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
G9C88DL2

Quant Time: Dec 17 00:43:58 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 17 00:37:15 2015
Response via : Initial Calibration

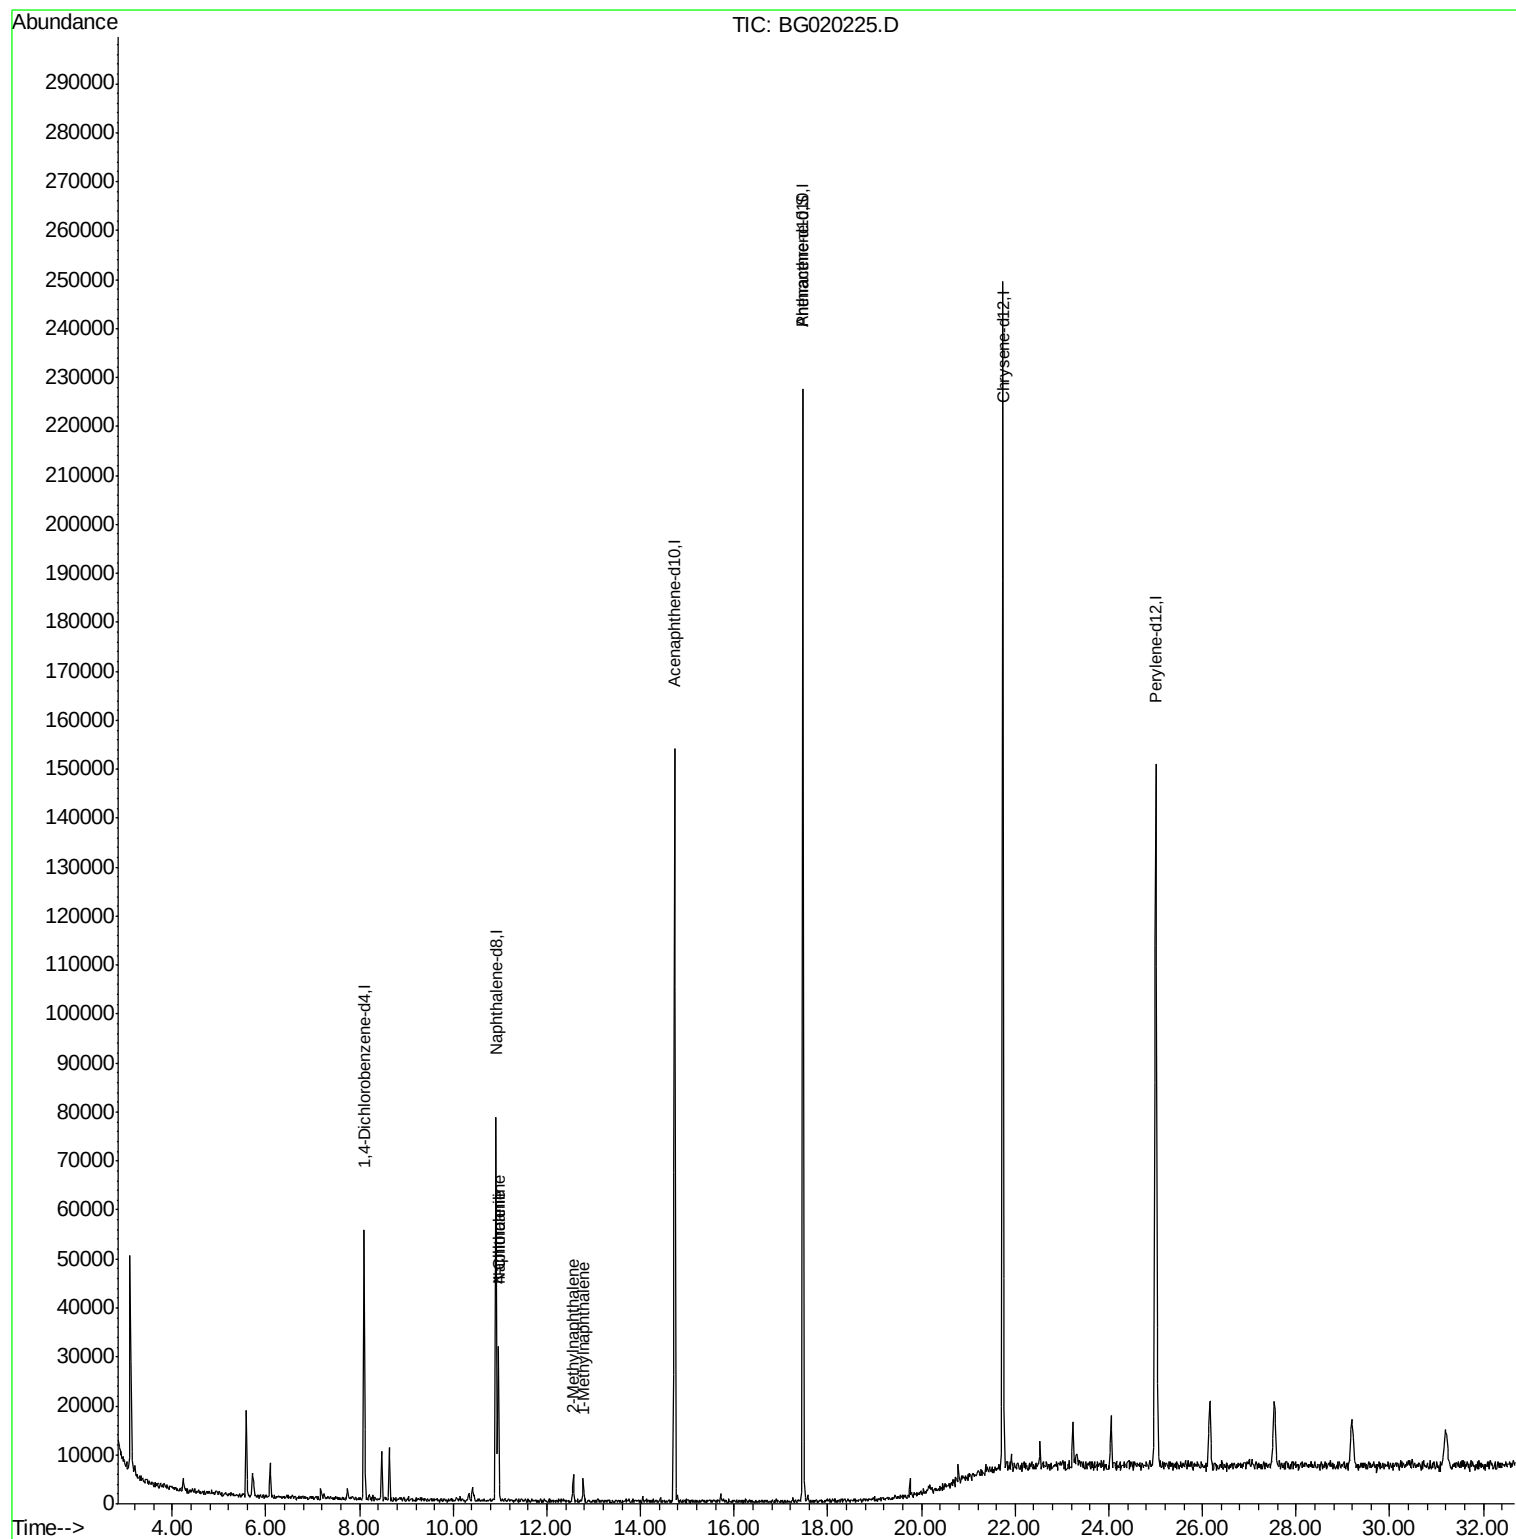

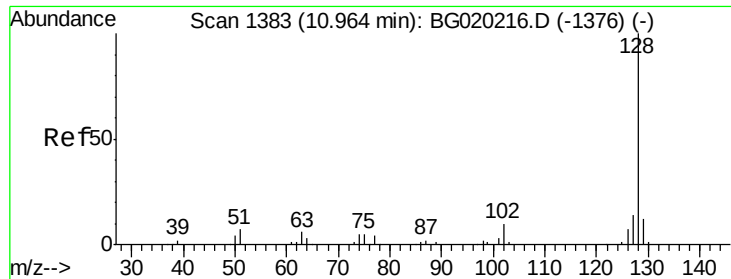

#28

Naphthalene

Concen: 7.59 ng/ul

RT: 10.96 min Scan# 1383

Delta R.T. -0.00 min

Lab File: BG020225.D

Acq: 16 Dec 2015 16:09

Instrument :

BNA_G

ClientSampleId :

G9C88DL2


Tgt Ion:128 Resp: 27165

Ion Ratio Lower Upper

128 100

129 10.9 8.6 12.8




127 13.4 10.1 15.1

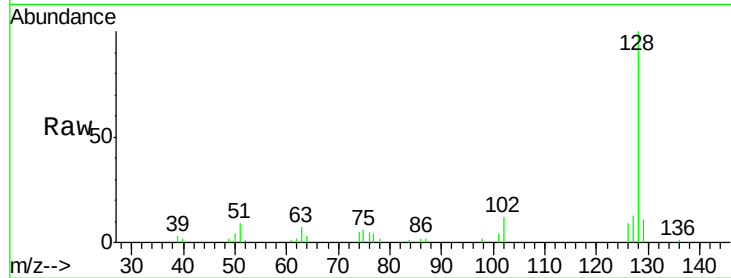

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

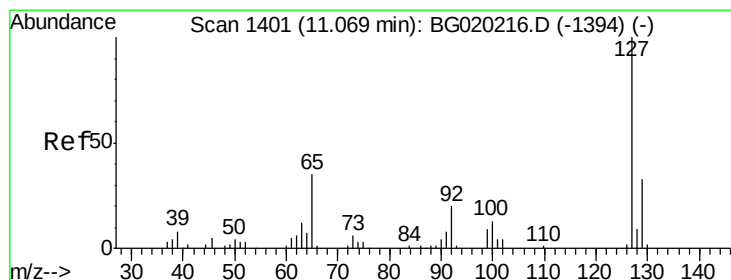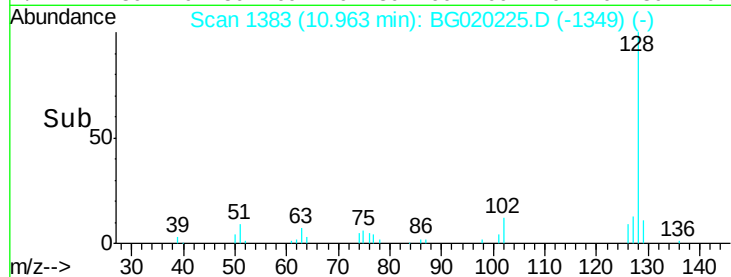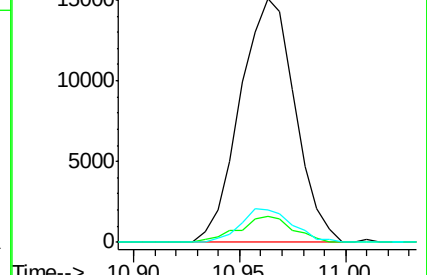

#30

4-Chloroaniline

Concen: 2.56 ng/ul

RT: 10.96 min Scan# 1382

Delta R.T. -0.11 min

Lab File: BG020225.D


Acq: 16 Dec 2015 16:09

Tgt Ion:127 Resp: 3541

Ion Ratio Lower Upper



127 100


129 71.5 25.7 38.5#

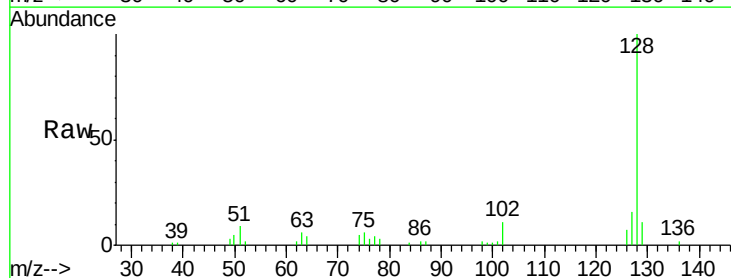

Abundance Ion 127.00 (126.70 to 127.70): E

Ion 129.00 (128.70 to 129.70): E



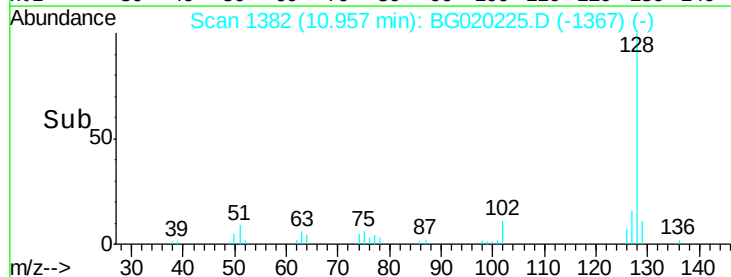
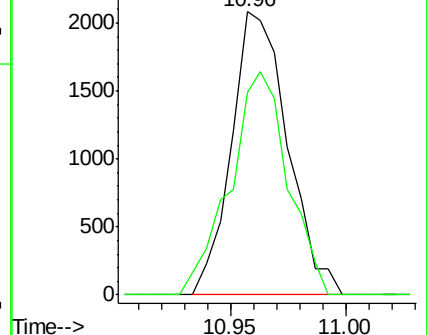


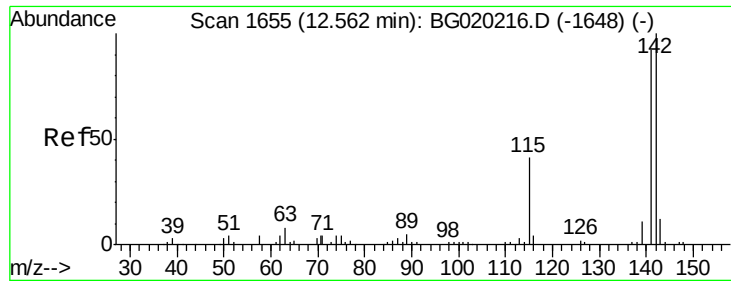

#34
2-Methylnaphthalene
Concen: 1.27 ng/ul
RT: 12.56 min Scan# 1655
Delta R.T. -0.00 min
Lab File: BG020225.D
Acq: 16 Dec 2015 16:09

Instrument :
BNA_G
ClientSampleId :
G9C88DL2

Tgt Ion:142 Resp: 3486
Ion Ratio Lower Upper
142 100
141 95.4 74.9 112.3

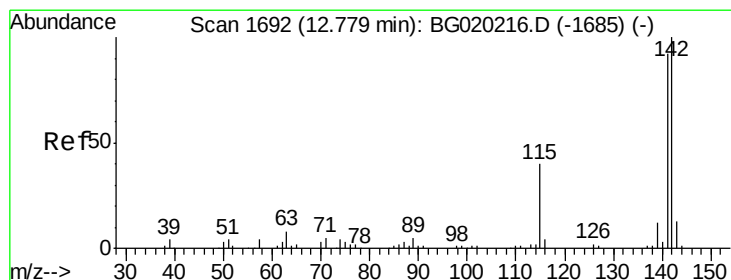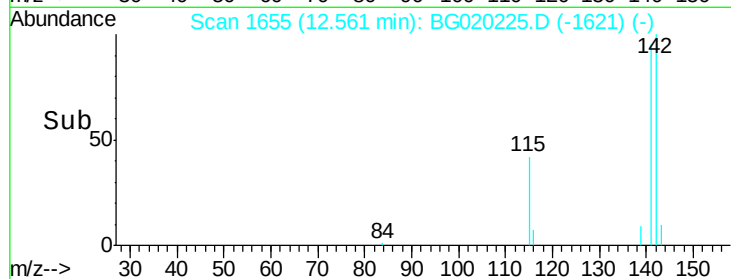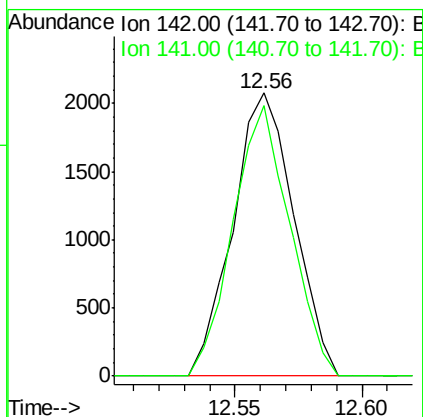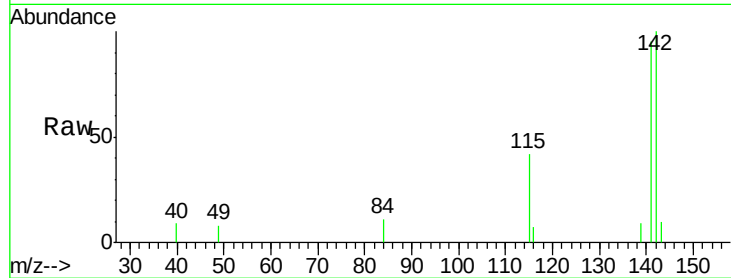

#35
1-Methylnaphthalene
Concen: 1.02 ng/ul
RT: 12.78 min Scan# 1692
Delta R.T. -0.00 min
Lab File: BG020225.D
Acq: 16 Dec 2015 16:09

Tgt Ion:142 Resp: 2686
Ion Ratio Lower Upper
142 100
141 98.6 73.0 109.6
116 0.0 3.0 4.6#

