

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121715\
 Data File : BG020234.D
 Acq On : 16 Dec 2015 23:31
 Operator : UM/SJ
 Sample : G4787-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 G9BN7

Quant Time: Dec 17 03:59:22 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 17 03:53:00 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	15307	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	79785	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	69234	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	184976	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	205965	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	196549	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	1157	4.17	ng/uL	0.00
5) Phenol-d5	7.25	99	27331	20.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.41	67	18585	23.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.62	132	22277	22.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	21312	18.46	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	12482	20.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	14209	20.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	25411	18.13	ng/ul	0.00
29) 4-Chloroaniline-d4	11.04	131	31409	19.95	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	107040	19.11	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	104775	16.08	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	13133	13.08	ng/ul	0.00
58) Fluorene-d10	15.71	176	84242	16.58	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	13959	12.73	ng/ul	0.00
71) Anthracene-d10	17.56	188	136499	16.01	ng/ul	0.00
79) Pyrene-d10	19.84	212	138677	14.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	128156	13.07	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.17	163	63362	11.08	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121715\
Data File : BG020234.D
Acq On : 16 Dec 2015 23:31
Operator : UM/SJ
Sample : G4787-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
G9BN7

Quant Time: Dec 17 03:59:22 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 17 03:53:00 2015
Response via : Initial Calibration

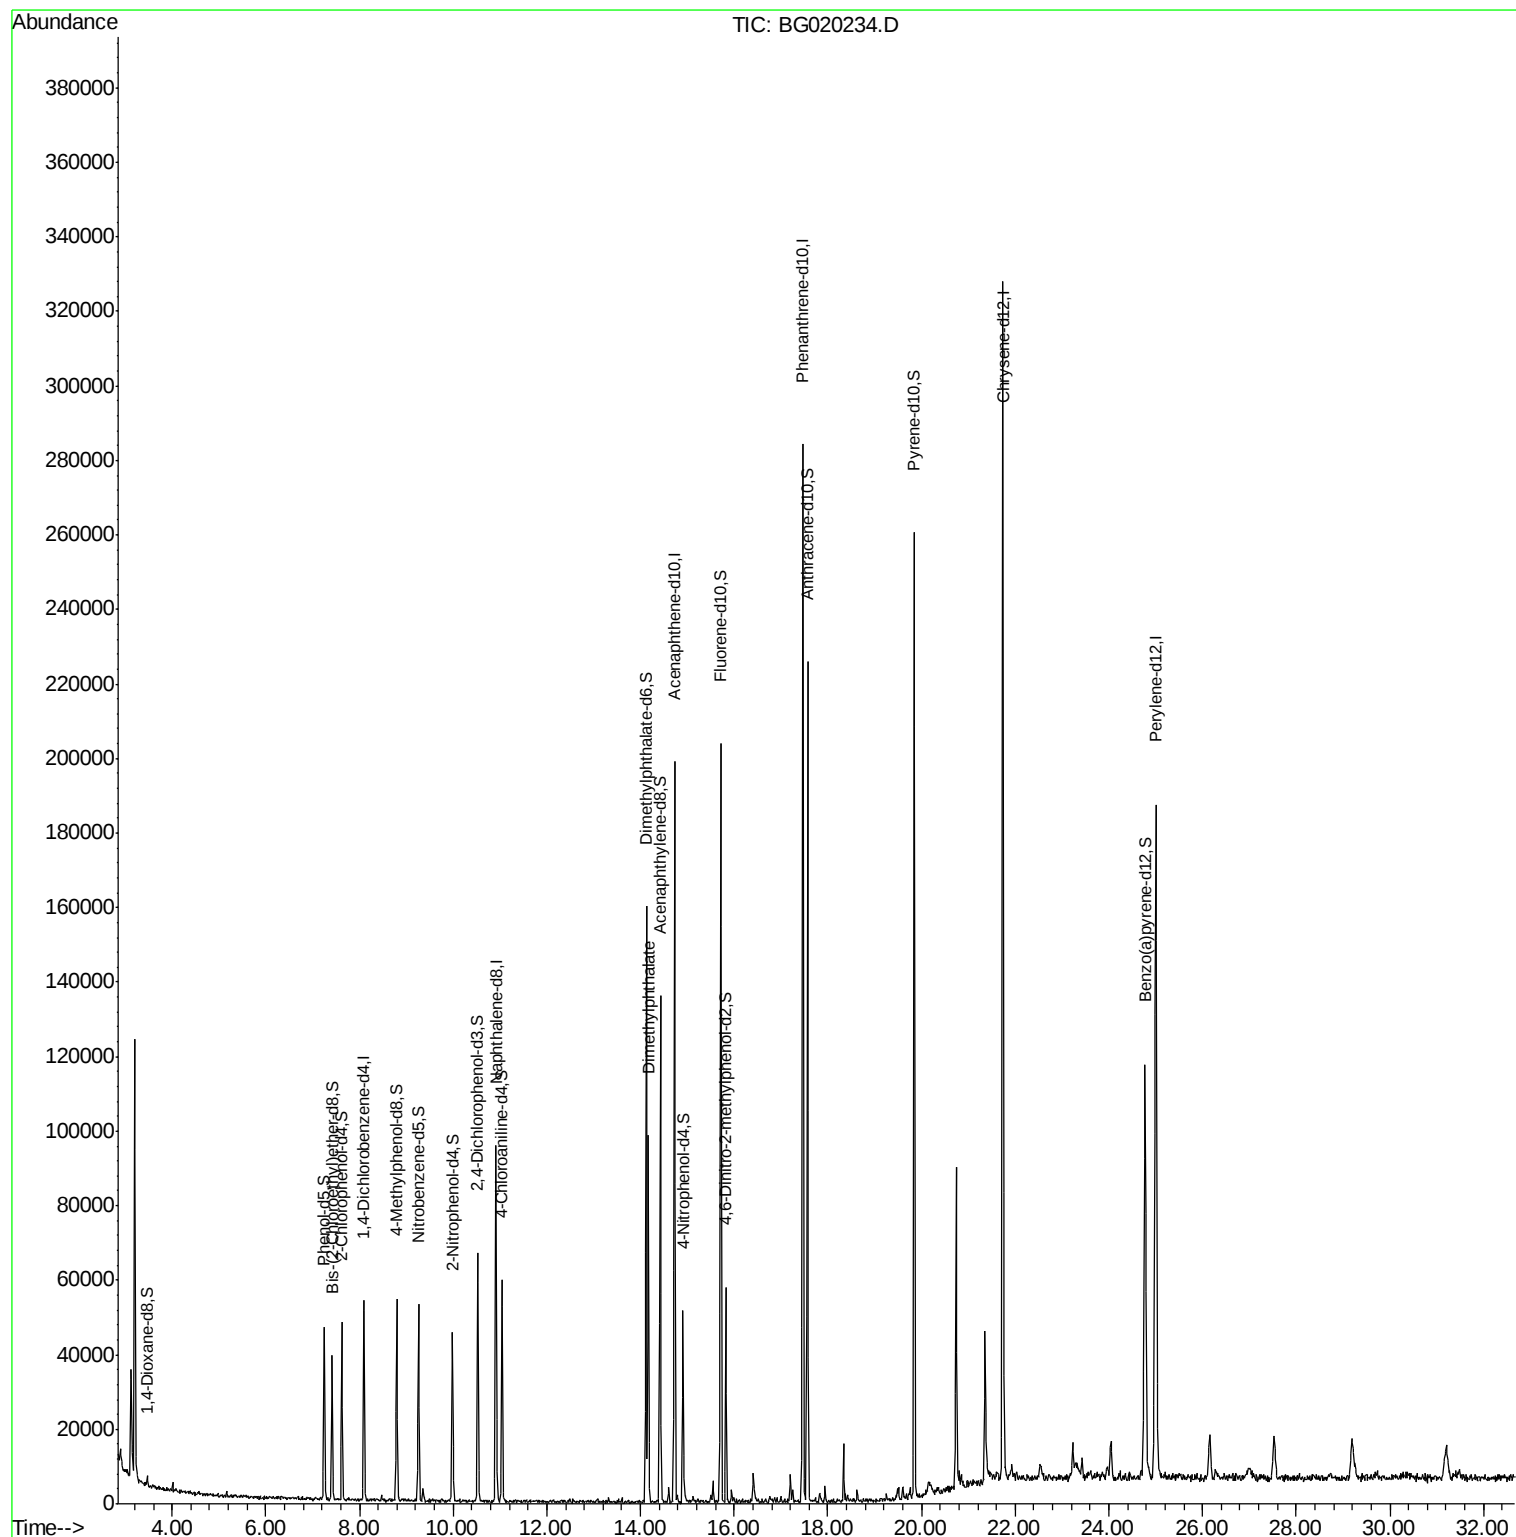

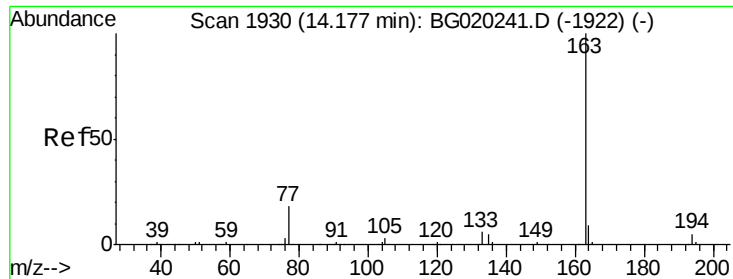

#45

Dimethylphthalate

Concen: 11.08 ng/ul

RT: 14.17 min Scan# 1928

Delta R.T. -0.01 min

Lab File: BG020234.D


Acq: 16 Dec 2015 23:31

Instrument :

BNA_G

ClientSampleId :

G9BN7

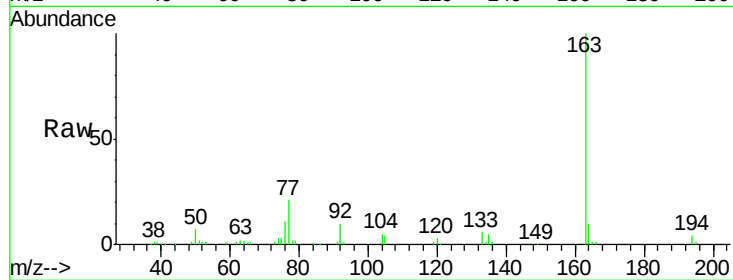

Tgt Ion:	163	Resp:	63362
Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.5	5.3
164	10.2	7.7	11.5

