


Data Path : Z:\HPCHEM1\BNA G\Data\BG121716\
 Data File : BG025268.D
 Acq On : 17 Dec 2016 10:36
 Operator : UM/SJ
 Sample : DFTPP21
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG113016.M
 Title : SVOA CALIBRATION
 Last Update : Sun Dec 18 00:18:21 2016

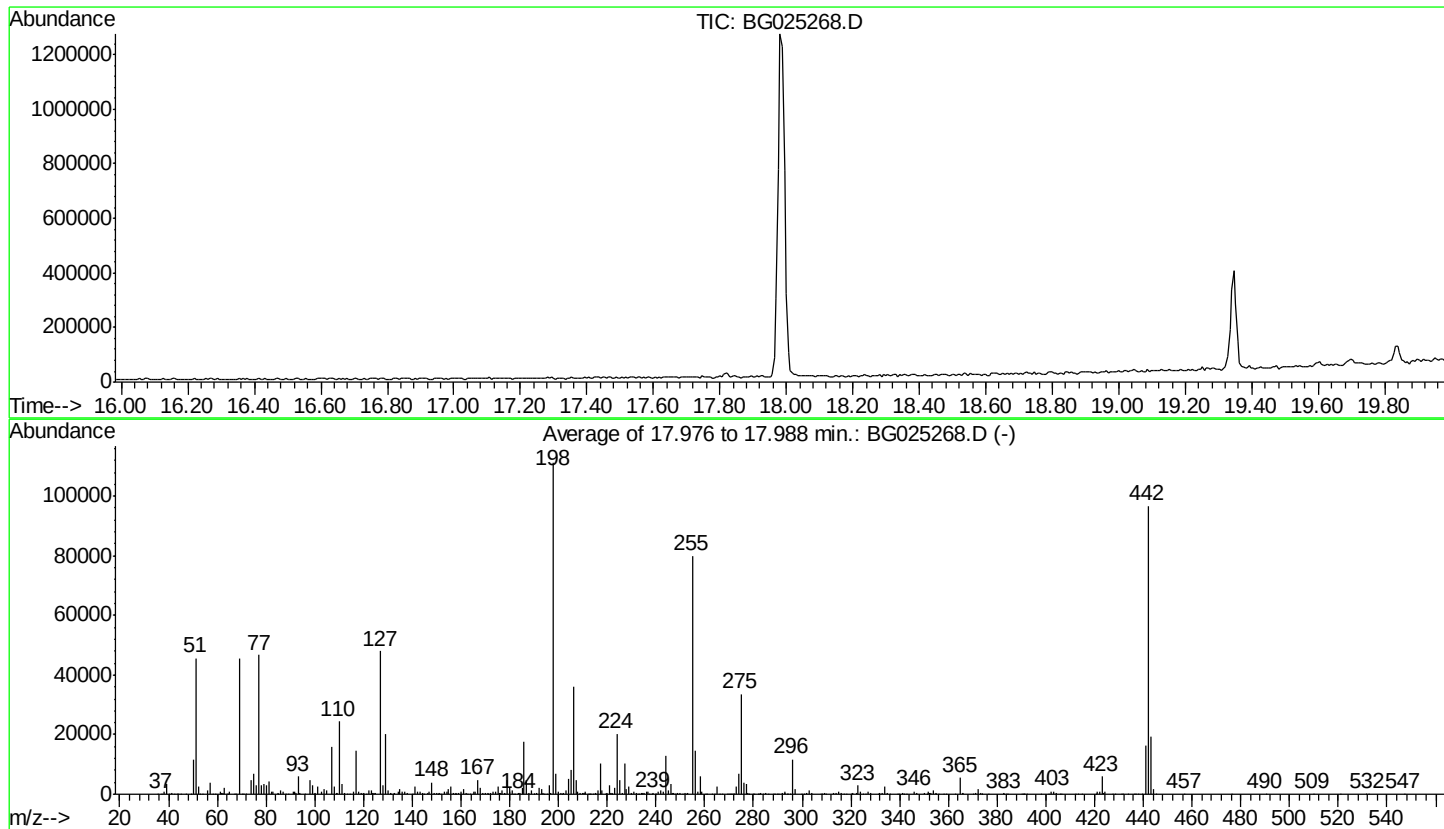

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	45640	PASS
68	69	0.00	2	0.4	186	PASS
69	198	0.00	100	40.8	45382	PASS
70	69	0.00	2	0.4	159	PASS
127	198	10	80	43.2	48034	PASS
197	198	0.00	2	0.5	554	PASS
198	198	100	100	100.0	111232	PASS
199	198	5	9	6.3	6953	PASS
275	198	10	60	30.1	33514	PASS
365	198	1	100	4.8	5389	PASS
441	442	0.01	100	17.0	16488	PASS
442	198	50	100	87.0	96752	PASS
443	442	15	24	20.2	19541	PASS