

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121716\
 Data File : BG025285.D
 Acq On : 17 Dec 2016 22:06
 Operator : UM/SJ
 Sample : H6040-10DL 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DA8W3DL

Manual Integrations
 APPROVED

umangi
 12/20/2016 10:54:35 AM

Quant Time: Dec 18 04:20:43 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG113016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Dec 18 03:57:56 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.23	152	73793	20.00	ng/ul	0.00
18) Naphthalene-d8	11.06	136	296918	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.85	164	226578	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.60	188	494734	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	639831	20.00	ng/ul	0.00
83) Perylene-d12	25.32	264	639103	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
5) Phenol-d5	7.40	99	19048	2.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.54	67	12537	3.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.77	132	12739	2.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.95	113	16437	3.09	ng/ul	0.00
19) Nitrobenzene-d5	9.43	128	7050	3.35	ng/ul	0.00
22) 2-Nitrophenol-d4	10.14	143	8737	3.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.69	165	15343	3.04	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
43) Dimethylphthalate-d6	14.25	166	56421	3.62	ng/ul	0.00
46) Acenaphthylene-d8	14.55	160	63483	3.72	ng/ul	0.00
51) 4-Nitrophenol-d4	15.10	143	10363	3.87	ng/ul	0.01
57) Fluorene-d10	15.84	176	70975	4.84	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul	
70) Anthracene-d10	17.70	188	83966	4.02	ng/ul	0.00
76) Pyrene-d10	19.97	212	97633	3.70	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.08	264	91864	3.55	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
6) Phenol	7.43	94	8503	1.30	ng/ul#	74
11) 2-Methylphenol	8.68	108	31938	6.64	ng/ul	93
16) 4-Methylphenol	9.02	108	88517	16.54	ng/ul	89
24) 2,4-Dimethylphenol	10.22	107	189860m	31.22	ng/ul	
28) Naphthalene	11.11	128	115341	8.36	ng/ul#	92
34) 2-Methylnaphthalene	12.70	142	125912	11.56	ng/ul	91
40) 1,1'-Biphenyl	13.68	154	28141	2.05	ng/ul#	95
53) Dibenzofuran	15.25	168	30169	1.68	ng/ul	88
58) Fluorene	15.90	166	45910	3.14	ng/ul#	95
69) Phenanthrene	17.64	178	48404	2.05	ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG121716\
Data File : BG025285.D
Acq On : 17 Dec 2016 22:06
Operator : UM/SJ
Sample : H6040-10DL 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
DA8W3DL

Quant Time: Dec 18 04:20:43 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG113016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Dec 18 03:57:56 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
12/20/2016 10:54:35 AM

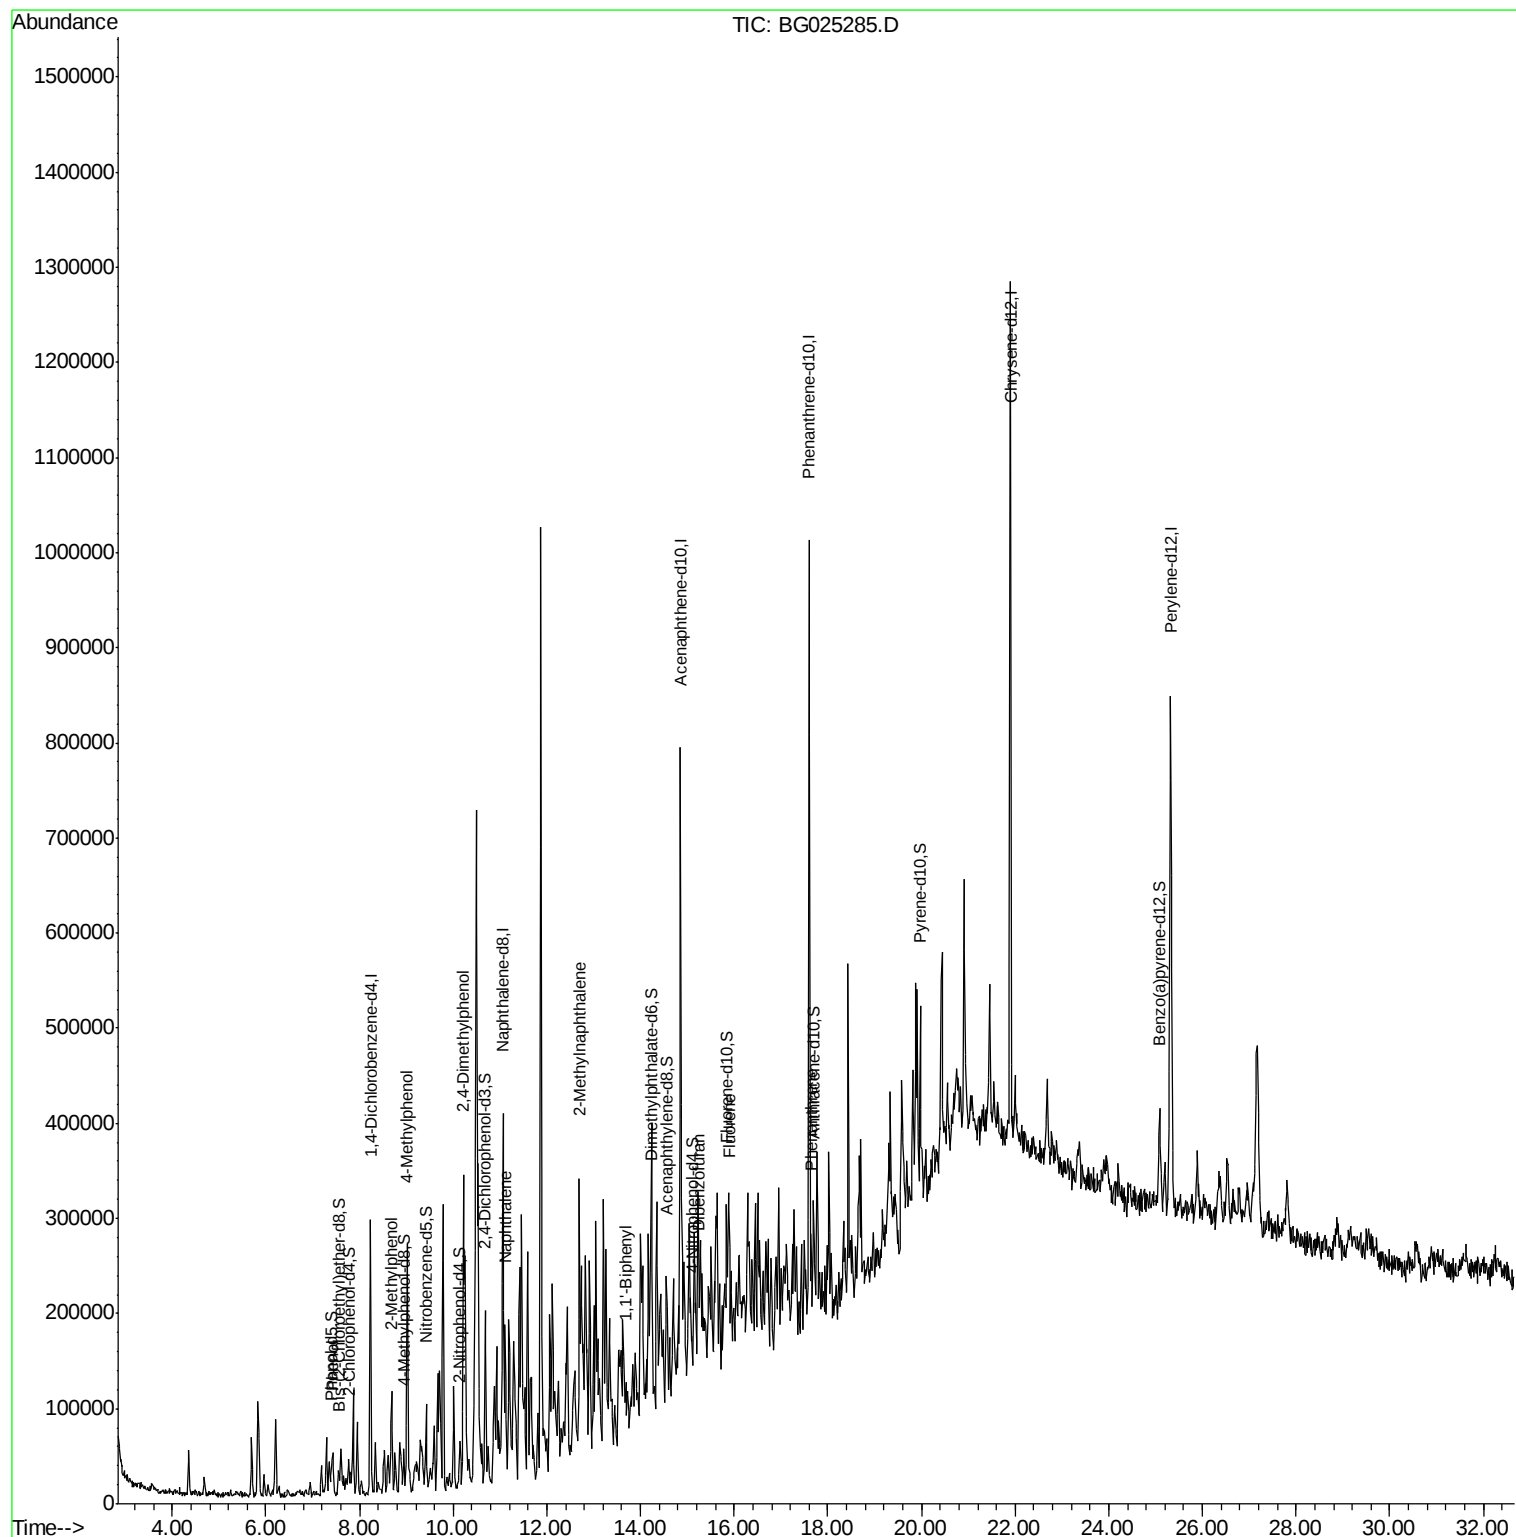

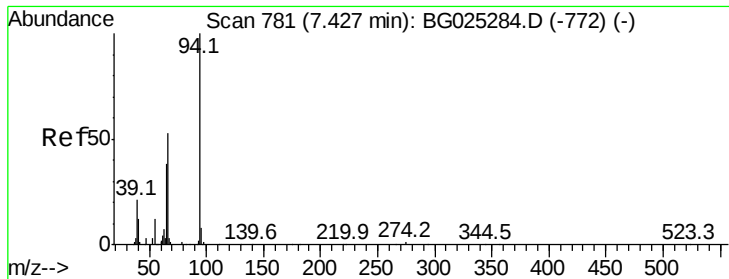

#6

Phenol

Concen: 1.30 ng/ul

RT: 7.43 min Scan# 781

Delta R.T. 0.00 min

Lab File: BG025285.D

Acq: 17 Dec 2016 22:06

Instrument :

BNA_G





ClientSampleId :

DA8W3DL

Tot Ion:	94	Resp:	8503
Ion Ratio	Lower	Upper	
94	100		
65	43.1	26.8	40.2#
66	32.3	44.4	66.6#

Manual Integrations
APPROVED

umangi
12/20/2016 10:54:35 AM

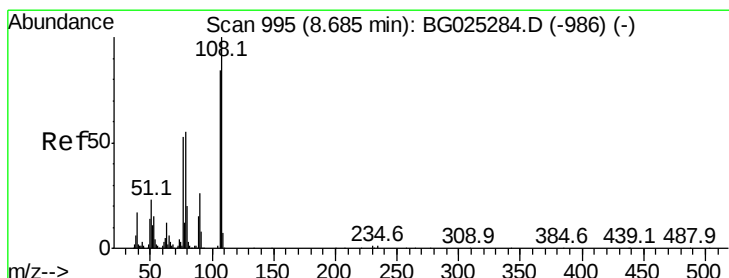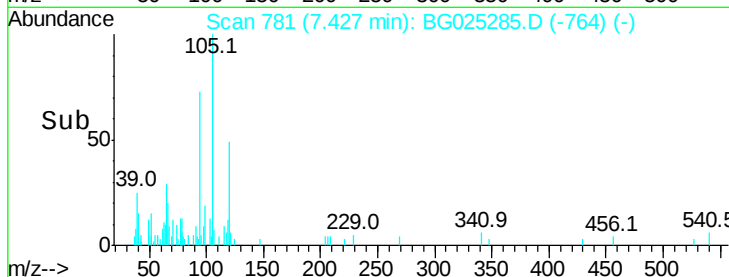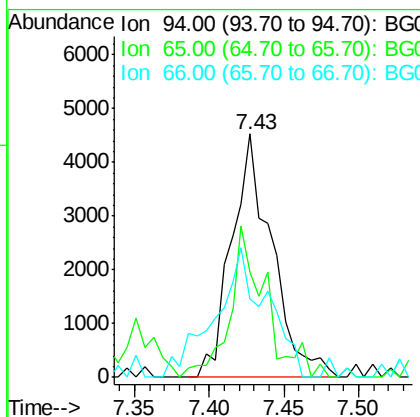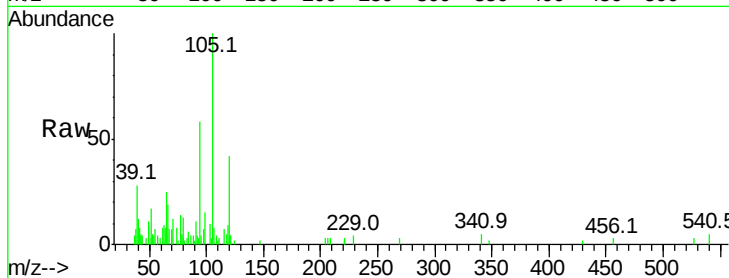

#11

2-Methylphenol

Concen: 6.64 ng/ul




RT: 8.68 min Scan# 995


Delta R.T. 0.00 min

Lab File: BG025285.D

Acq: 17 Dec 2016 22:06

Tgt Ion:	108	Resp:	31938
Ion Ratio	Lower	Upper	
108	100		
107	88.7	76.7	115.1

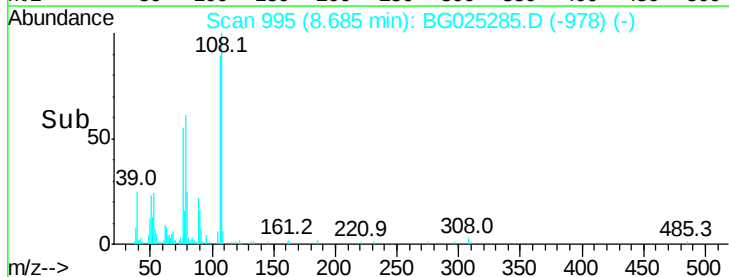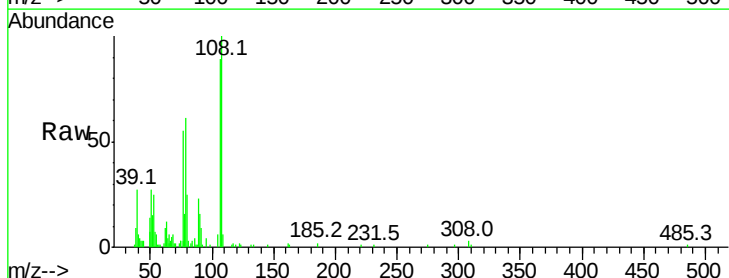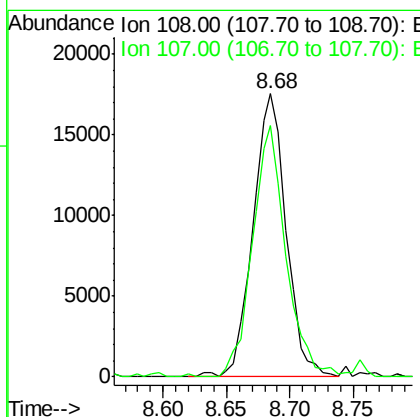

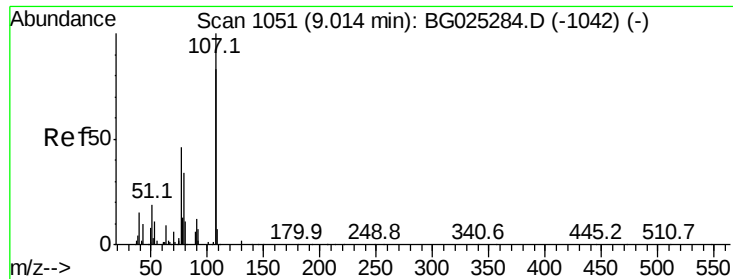





#16
4-Methylphenol
Concen: 16.54 ng/ul
RT: 9.02 min Scan# 1052
Delta R.T. 0.01 min
Lab File: BG025285.D
Acq: 17 Dec 2016 22:06

Instrument :
BNA_G
ClientSampled :
DA8W3DL

Tot Ion	Ratio	Lower	Upper
108	100		
107	102.2	91.7	137.5




Manual Integrations
APPROVED


umangi
12/20/2016 10:54:35 AM

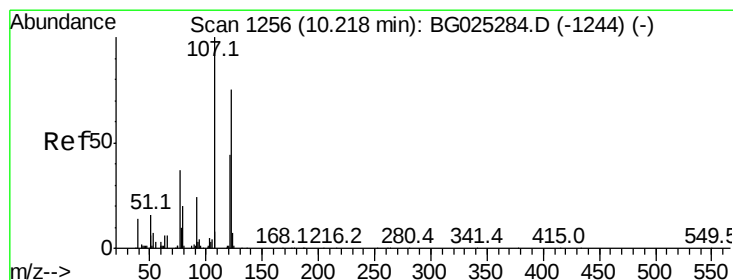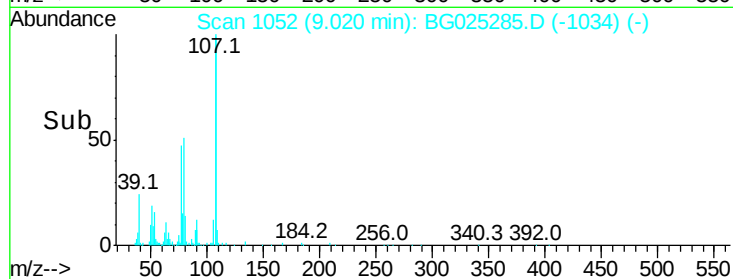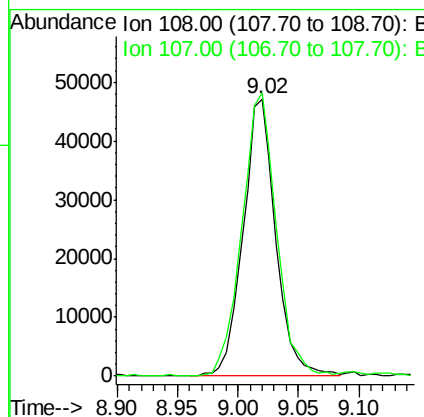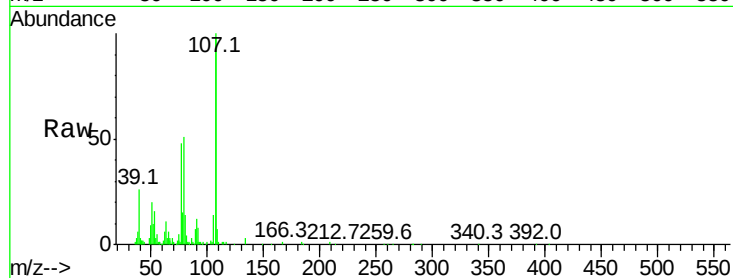

#24
2,4-Dimethylphenol
Concen: 31.22 ng/ul m
RT: 10.22 min Scan# 1256
Delta R.T. 0.00 min
Lab File: BG025285.D
Acq: 17 Dec 2016 22:06

Tgt Ion	Ratio	Lower	Upper
107	100		
121	43.4	32.3	48.5
122	73.1	61.2	91.8

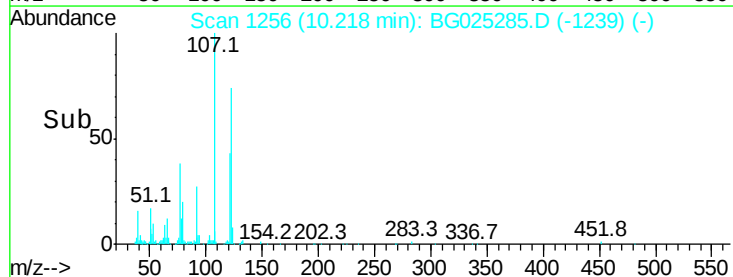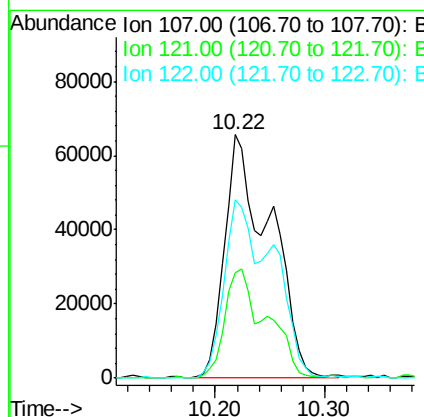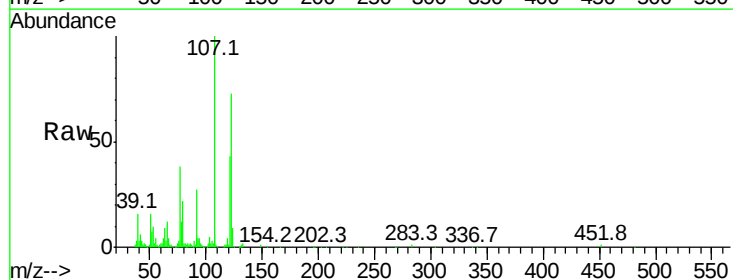

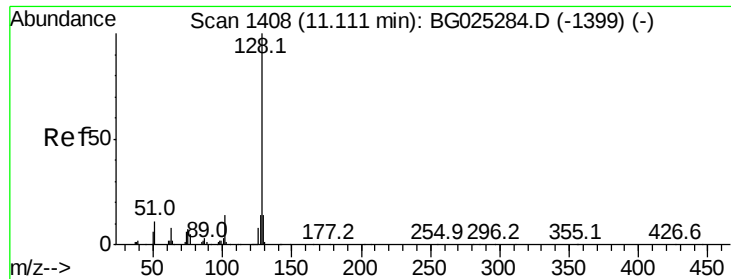





#28
Naphthalene
Concen: 8.36 ng/ul
RT: 11.11 min Scan# 1408
Delta R.T. 0.00 min
Lab File: BG025285.D
Acq: 17 Dec 2016 22:06

Instrument :
BNA_G
ClientSampleId :
DA8W3DL

Tot Ion	Ratio	Lower	Upper
128	100		
129	10.5	9.4	14.2
127	17.4	10.3	15.5#




Manual Integrations
APPROVED


umangi
12/20/2016 10:54:35 AM

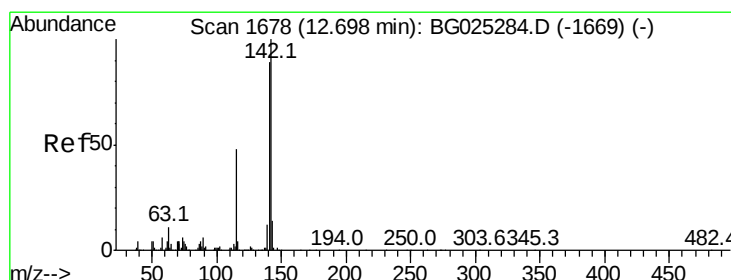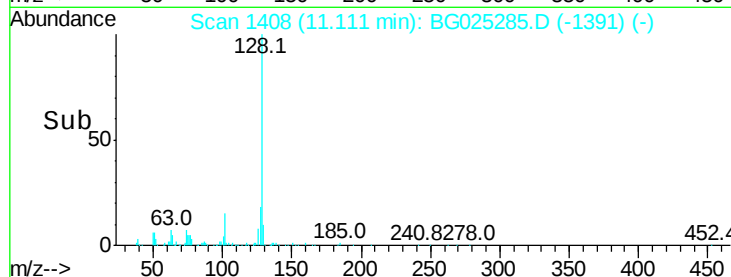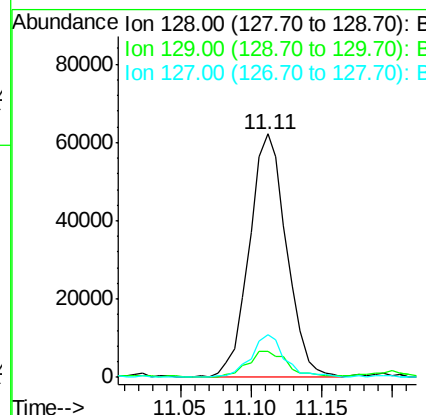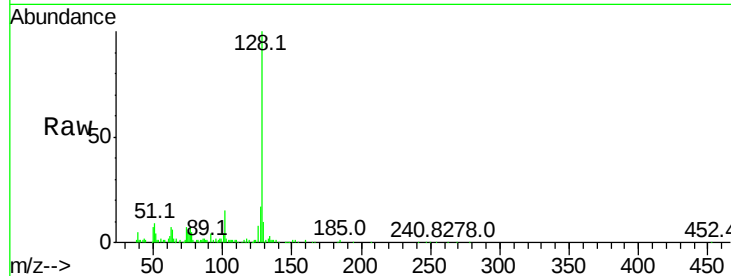

#34
2-Methylnaphthalene
Concen: 11.56 ng/ul
RT: 12.70 min Scan# 1678
Delta R.T. 0.00 min
Lab File: BG025285.D
Acq: 17 Dec 2016 22:06

Tgt Ion	Ratio	Lower	Upper
142	100		
141	93.5	68.6	102.8

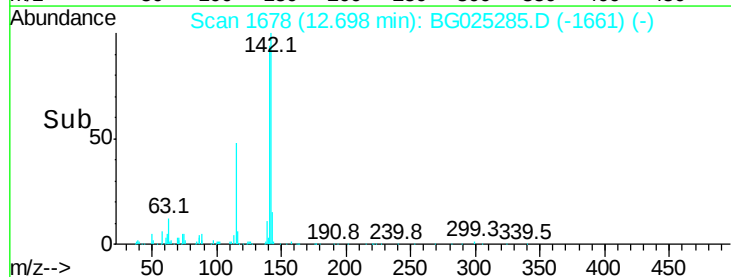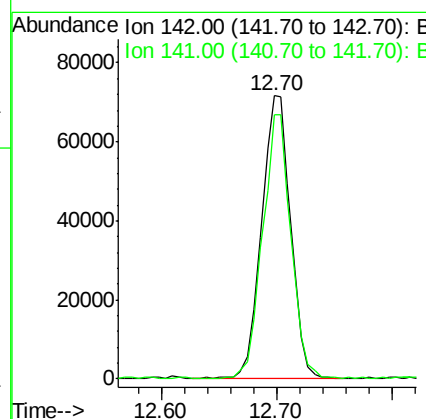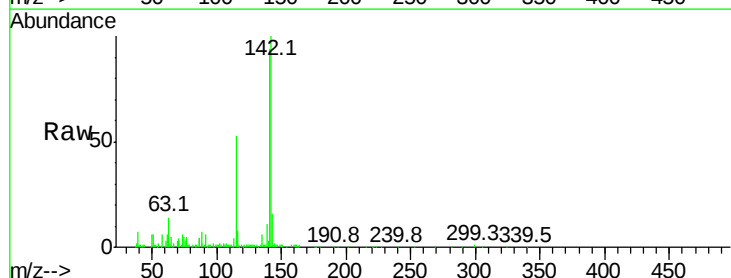

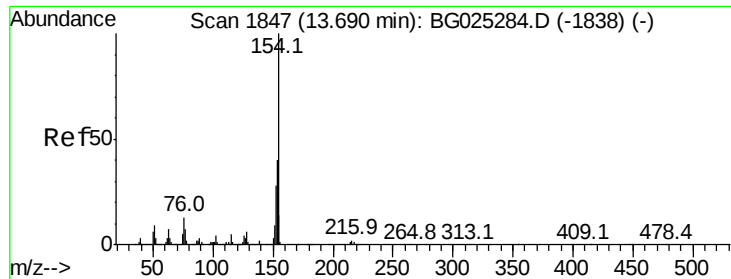

#40

1,1'-Biphenyl

Concen: 2.05 ng/ul

RT: 13.68 min Scan# 1846

Delta R.T. -0.01 min

Lab File: BG025285.D

Acq: 17 Dec 2016 22:06

Instrument :

BNA_G





ClientSampleId :

DA8W3DL

Tot Ion:	154	Resp:	28141
Ion Ratio	Lower	Upper	
154	100		
153	37.7	32.2	48.2
76	15.7	9.6	14.4

Manual Integrations
APPROVED

umangi
12/20/2016 10:54:35 AM

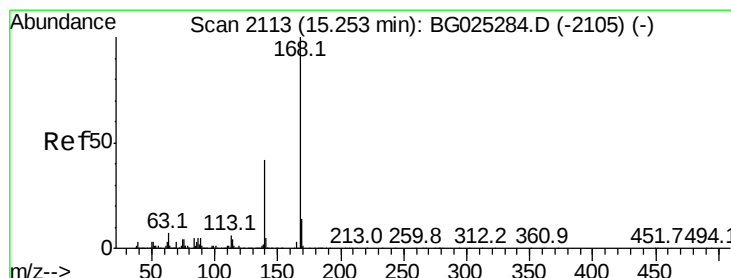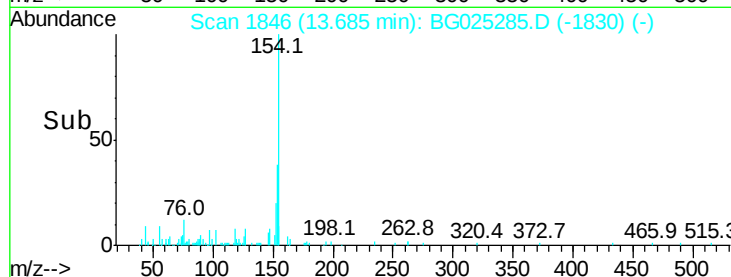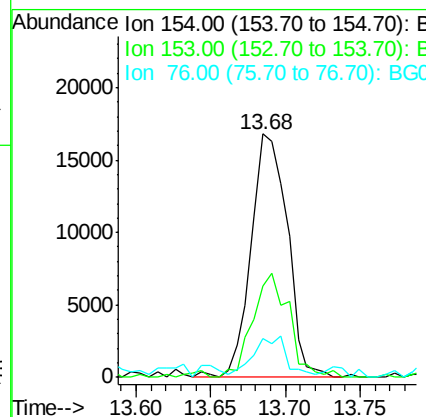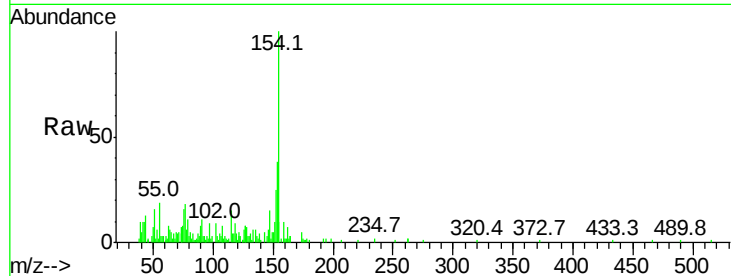

#53

Dibenzofuran

Concen: 1.68 ng/ul




RT: 15.25 min Scan# 2113


Delta R.T. 0.00 min

Lab File: BG025285.D

Acq: 17 Dec 2016 22:06

Tgt Ion:	168	Resp:	30169
Ion Ratio	Lower	Upper	
168	100		
139	49.7	33.8	50.8

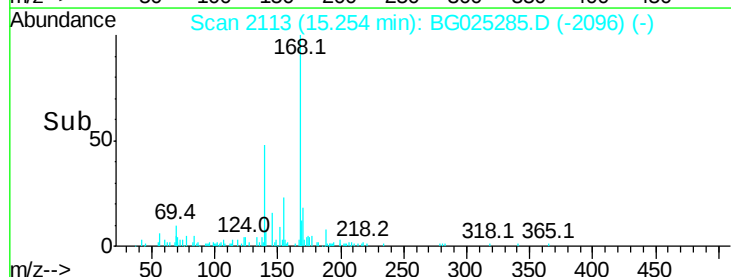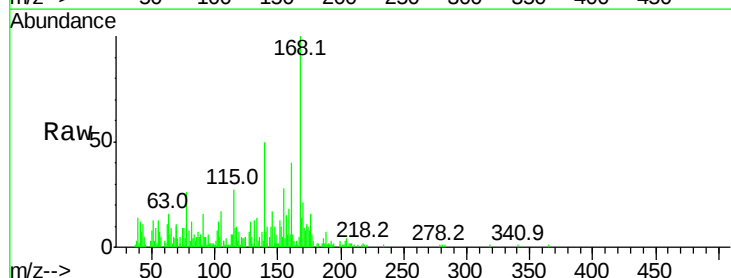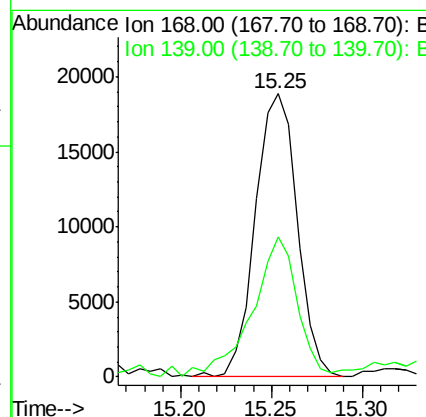

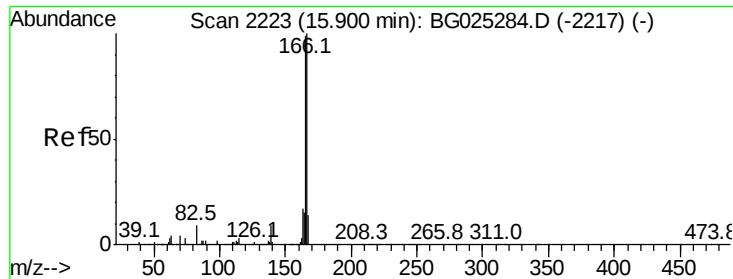

#58

Fluorene

Concen: 3.14 ng/ul

RT: 15.90 min Scan# 2223

Delta R.T. 0.00 min

Lab File: BG025285.D

Acq: 17 Dec 2016 22:06

Instrument :

BNA_G





ClientSampleId :

DA8W3DL

Tot Ion	Ratio	Lower	Upper
166	100		
165	104.1	79.7	119.5
167	17.5	11.4	17.2#

Manual Integrations
APPROVED

umangi
12/20/2016 10:54:35 AM

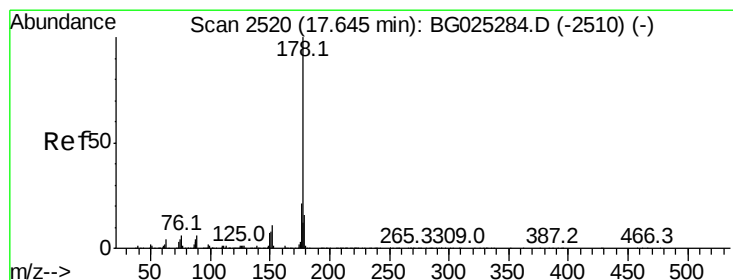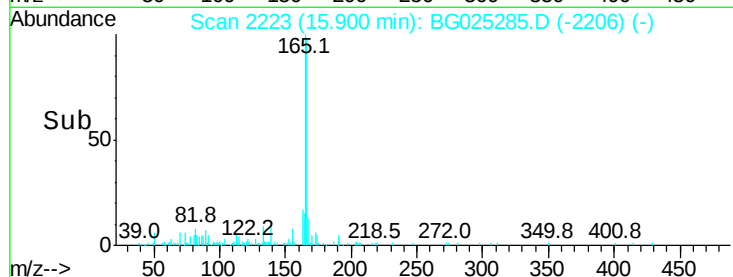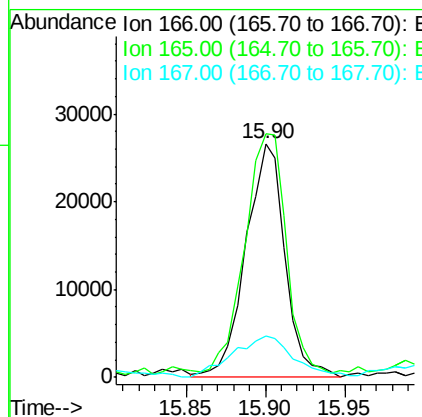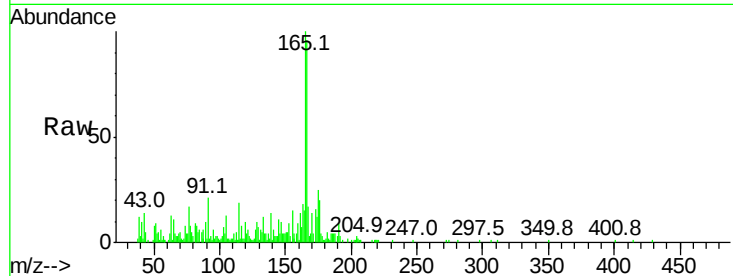

#69

Phenanthrene

Concen: 2.05 ng/ul

RT: 17.64 min Scan# 2520

Delta R.T. 0.00 min

Lab File: BG025285.D

Acq: 17 Dec 2016 22:06

Tgt Ion	Ratio	Lower	Upper
178	100		
179	20.0	12.4	18.6#
176	22.1	16.5	24.7

