

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121724\
 Data File : BG063694.D
 Acq On : 17 Dec 2024 12:22
 Operator : RC/JU
 Sample : PB165586BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK586

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063694.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	36	rVB4	44480	73692	1.45%	0.152%
2	3.675	95	100	114	rBV	540891	928851	18.26%	1.917%
3	4.580	253	254	257	rBV	8504	7278	0.14%	0.015%
4	4.880	302	305	306	rBV3	10369	8269	0.16%	0.017%
5	4.944	314	316	321	rBV5	7143	8647	0.17%	0.018%
6	5.567	419	422	423	rBV3	7022	8321	0.16%	0.017%
7	5.691	442	443	446	rVB2	11426	7644	0.15%	0.016%
8	6.014	496	498	501	rBV3	6596	9782	0.19%	0.020%
9	6.049	503	504	508	rVB3	10018	10019	0.20%	0.021%
10	6.219	531	533	536	rBV3	9849	12466	0.25%	0.026%
11	6.560	589	591	595	rBV3	10586	12853	0.25%	0.027%
12	6.613	597	600	601	rBV3	8568	8248	0.16%	0.017%
13	6.736	619	621	624	rBV4	6335	7518	0.15%	0.016%
14	6.995	659	665	674	rBV	675687	1157800	22.76%	2.390%
15	7.136	683	689	700	rVB	511990	844111	16.60%	1.742%
16	7.271	711	712	716	rBV3	7637	10380	0.20%	0.021%
17	7.347	717	725	735	rVV	654442	1120531	22.03%	2.313%
18	7.436	738	740	743	rVB2	7176	8083	0.16%	0.017%
19	7.718	784	788	789	rBV2	6928	8835	0.17%	0.018%
20	7.806	797	803	811	rBV	651186	1055724	20.76%	2.179%
21	8.029	837	841	844	rVB4	5806	7857	0.15%	0.016%
22	8.235	875	876	879	rBV3	7094	8363	0.16%	0.017%
23	8.393	902	903	908	rVB4	8299	9722	0.19%	0.020%
24	8.522	919	925	935	rVB	769365	1343559	26.42%	2.773%
25	8.805	972	973	977	rBV3	7703	8897	0.17%	0.018%
26	8.963	993	1000	1007	rBV	581466	1024518	20.14%	2.115%
27	9.680	1116	1122	1131	rBV	498377	852585	16.76%	1.760%
28	9.897	1157	1159	1162	rBV3	8420	10499	0.21%	0.022%
29	9.980	1171	1173	1178	rBV3	6638	9818	0.19%	0.020%
30	10.044	1180	1184	1186	rBV2	7976	7676	0.15%	0.016%
31	10.150	1200	1202	1206	rVB3	6670	8578	0.17%	0.018%
32	10.232	1209	1216	1228	rVV	714161	1320405	25.96%	2.726%
33	10.356	1235	1237	1243	rVB4	8589	13119	0.26%	0.027%
34	10.597	1269	1278	1287	rBV	771611	1413654	27.79%	2.918%
35	10.732	1293	1301	1319	rVB	618746	1205640	23.70%	2.489%
36	11.084	1360	1361	1364	rBV	7138	7180	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121724\
 Data File : BG063694.D
 Acq On : 17 Dec 2024 12:22
 Operator : RC/JU
 Sample : PB165586BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK586

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Title : SVOA CALIBRATION

37	11.343	1403	1405	1409	rVB2	10419	11816	0.23%	0.024%
38	11.719	1467	1469	1472	rVB	7801	7929	0.16%	0.016%
39	11.772	1474	1478	1480	rBV5	9199	10056	0.20%	0.021%
40	11.854	1490	1492	1494	rVB3	10102	7481	0.15%	0.015%

41	12.195	1544	1550	1553	rBV4	14916	25525	0.50%	0.053%
42	12.224	1553	1555	1558	rVB3	6752	6795	0.13%	0.014%
43	12.606	1617	1620	1625	rBV3	6554	10329	0.20%	0.021%
44	12.911	1669	1672	1675	rVB5	5769	7178	0.14%	0.015%
45	12.947	1675	1678	1679	rBV3	8393	7084	0.14%	0.015%

46	13.123	1705	1708	1711	rBV2	9897	10321	0.20%	0.021%
47	13.170	1714	1716	1718	rVB2	8456	7389	0.15%	0.015%
48	13.193	1718	1720	1722	rBV3	6897	7202	0.14%	0.015%
49	13.311	1735	1740	1741	rBV2	9598	7350	0.14%	0.015%
50	13.346	1741	1746	1747	rBV5	7271	10877	0.21%	0.022%

51	13.611	1790	1791	1795	rBV3	7726	6876	0.14%	0.014%
52	13.852	1826	1832	1843	rVB	1390038	1993871	39.20%	4.116%
53	14.139	1872	1881	1892	rBV2	1439887	2310634	45.43%	4.770%
54	14.257	1900	1901	1904	rBV3	9709	6653	0.13%	0.014%
55	14.380	1918	1922	1923	rBV3	10130	11037	0.22%	0.023%

56	14.445	1925	1933	1941	rVV	1333798	2047481	40.26%	4.226%
57	14.680	1966	1973	1986	rBV	473220	996113	19.58%	2.056%
58	14.980	2021	2024	2027	rBV4	6503	7539	0.15%	0.016%
59	15.103	2042	2045	2046	rVB3	9624	6745	0.13%	0.014%
60	15.121	2046	2048	2052	rVB3	9125	7767	0.15%	0.016%

61	15.197	2059	2061	2063	rBV3	6544	6850	0.13%	0.014%
62	15.262	2071	2072	2074	rBV	10046	8521	0.17%	0.018%
63	15.332	2082	2084	2088	rVB4	8225	10535	0.21%	0.022%
64	15.444	2096	2103	2114	rVB	1983978	3061234	60.19%	6.319%
65	15.573	2120	2125	2138	rBV	446656	759035	14.92%	1.567%

66	15.920	2181	2184	2185	rBV2	7564	6933	0.14%	0.014%
67	16.067	2206	2209	2211	rBV3	8806	12113	0.24%	0.025%
68	16.695	2312	2316	2317	rBV4	4896	7044	0.14%	0.015%
69	16.872	2343	2346	2350	rBV5	11481	17410	0.34%	0.036%
70	16.977	2362	2364	2365	rBV2	13243	8475	0.17%	0.017%

71	17.054	2374	2377	2380	rBV4	8930	11218	0.22%	0.023%
72	17.142	2388	2392	2394	rBV4	9288	11605	0.23%	0.024%
73	17.195	2395	2401	2409	rVV2	2013541	3008843	59.16%	6.211%
74	17.295	2412	2418	2430	rVB2	2649234	3883326	76.35%	8.016%
75	17.706	2486	2488	2491	rVB4	8402	8502	0.17%	0.018%

76	17.870	2512	2516	2519	rBV4	13972	17833	0.35%	0.037%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121724\
Data File : BG063694.D
Acq On : 17 Dec 2024 12:22
Operator : RC/JU
Sample : PB165586BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK586

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Title : SVOA CALIBRATION

77	19.157	2731	2735	2738	rBV4	40147	51608	1.01%	0.107%
78	19.228	2744	2747	2752	rBV2	40295	54956	1.08%	0.113%
79	19.592	2804	2809	2822	rBV	3427966	5086126	100.00%	10.499%
80	21.443	3118	3124	3131	rBV	2402394	3796183	74.64%	7.836%
81	24.251	3594	3602	3616	rVB	1799346	4669951	91.82%	9.640%
82	24.463	3629	3638	3647	rVB2	1437554	3853074	75.76%	7.954%




Sum of corrected areas: 48444545

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121724\
Data File : BG063694.D
Acq On : 17 Dec 2024 12:22
Operator : RC/JU
Sample : PB165586BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK586

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

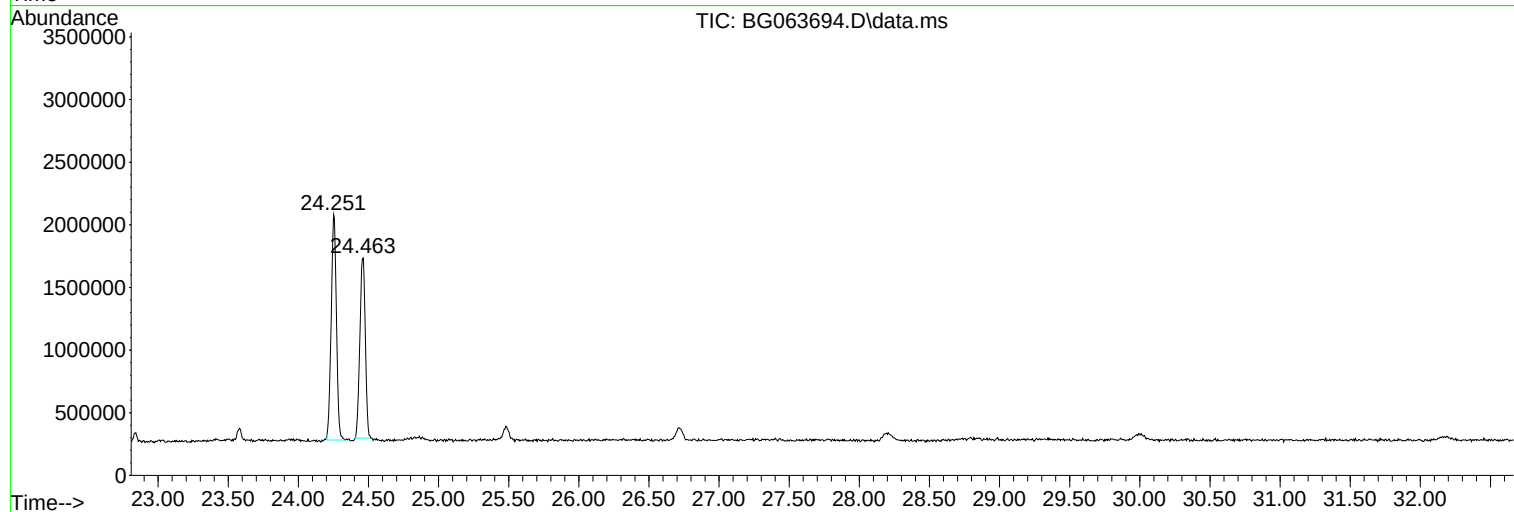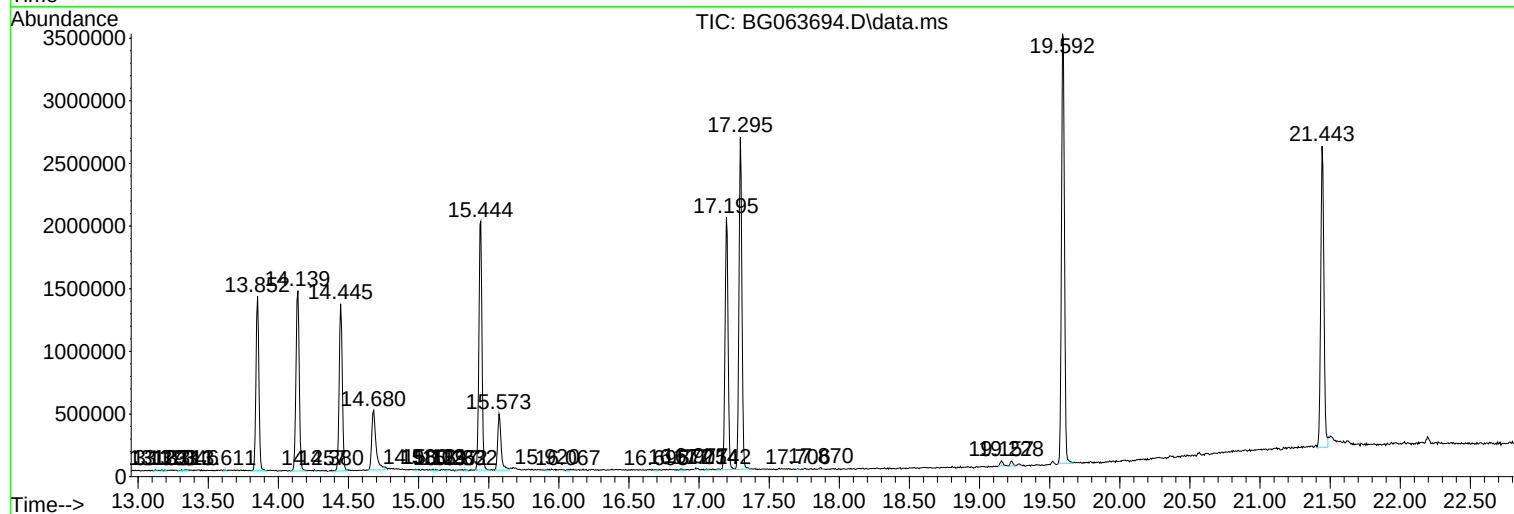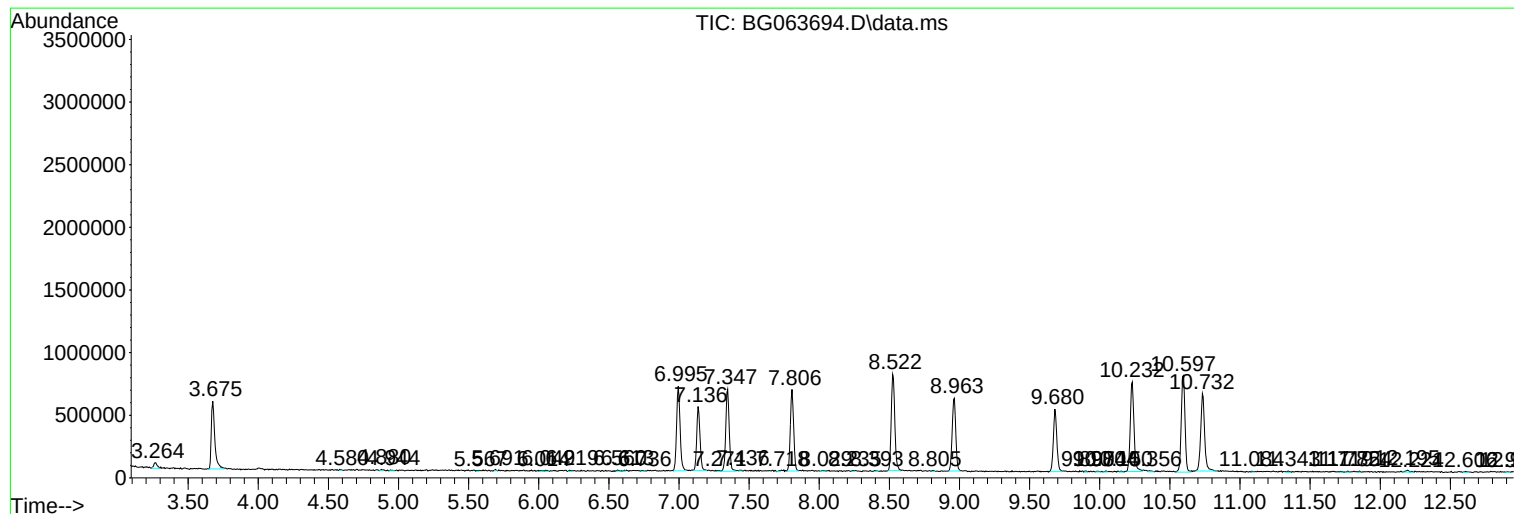

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121724\
Data File : BG063694.D
Acq On : 17 Dec 2024 12:22
Operator : RC/JU
Sample : PB165586BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK586

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121724\
Data File : BG063694.D
Acq On : 17 Dec 2024 12:22
Operator : RC/JU
Sample : PB165586BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK586

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------