

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121815\
 Data File : BG020254.D
 Acq On : 17 Dec 2015 20:31
 Operator : UM/SJ
 Sample : G4767-06DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9N28DL

Quant Time: Dec 18 02:43:25 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 18 02:40:02 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	16101	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	70488	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	50694	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	132674	20.00	ng/ul	0.00
78) Chrysene-d12	21.75	240	171083	20.00	ng/ul	0.00
86) Perylene-d12	25.02	264	162463	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.47	96	288	0.99	ng/uL	0.00
5) Phenol-d5	7.25	99	9576	6.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.42	67	6454	7.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.62	132	7634	7.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	8508	7.01	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	4017	7.31	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.98	143	4744	7.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	8640	6.98	ng/ul	0.00
29) 4-Chloroaniline-d4	11.04	131	11377	8.18	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	33513	8.17	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	37219	7.80	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	4238	5.76	ng/ul	0.00
58) Fluorene-d10	15.71	176	28927	7.78	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	2964	3.77	ng/ul	0.00
71) Anthracene-d10	17.57	188	49854	8.15	ng/ul	0.00
79) Pyrene-d10	19.85	212	58545	7.34	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	64444	7.95	ng/ul	-0.01

Target Compounds


					Qvalue
28) Naphthalene	10.96	128	95395	25.92 ng/ul	98
30) 4-Chloroaniline	10.97	127	12532	8.82 ng/ul#	8
34) 2-Methylnaphthalene	12.56	142	25595	9.10 ng/ul	93
35) 1-Methylnaphthalene	12.78	142	12054	4.46 ng/ul#	97
41) 1,1'-Biphenyl	13.56	154	9909	2.59 ng/ul#	94
45) Dimethylphthalate	14.17	163	13117	3.13 ng/ul#	97
50) Acenaphthene	14.79	153	45533	13.35 ng/ul	97
54) Dibenzofuran	15.13	168	46776	9.22 ng/ul	99
59) Fluorene	15.77	166	47467	11.65 ng/ul	100
70) Phenanthrene	17.52	178	234898	32.37 ng/ul	99
72) Anthracene	17.60	178	32094	4.36 ng/ul	95
75) Carbazole	17.87	167	19119	3.09 ng/ul	97
77) Fluoranthene	19.52	202	131834	15.54 ng/ul	100
80) Pyrene	19.88	202	89693	8.66 ng/ul	98
83) Benzo(a)anthracene	21.72	228	21747	2.18 ng/ul	96
85) Chrysene	21.79	228	18019	1.92 ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121815\
Data File : BG020254.D
Acq On : 17 Dec 2015 20:31
Operator : UM/SJ
Sample : G4767-06DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9N28DL

Quant Time: Dec 18 02:43:25 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 18 02:40:02 2015
Response via : Initial Calibration




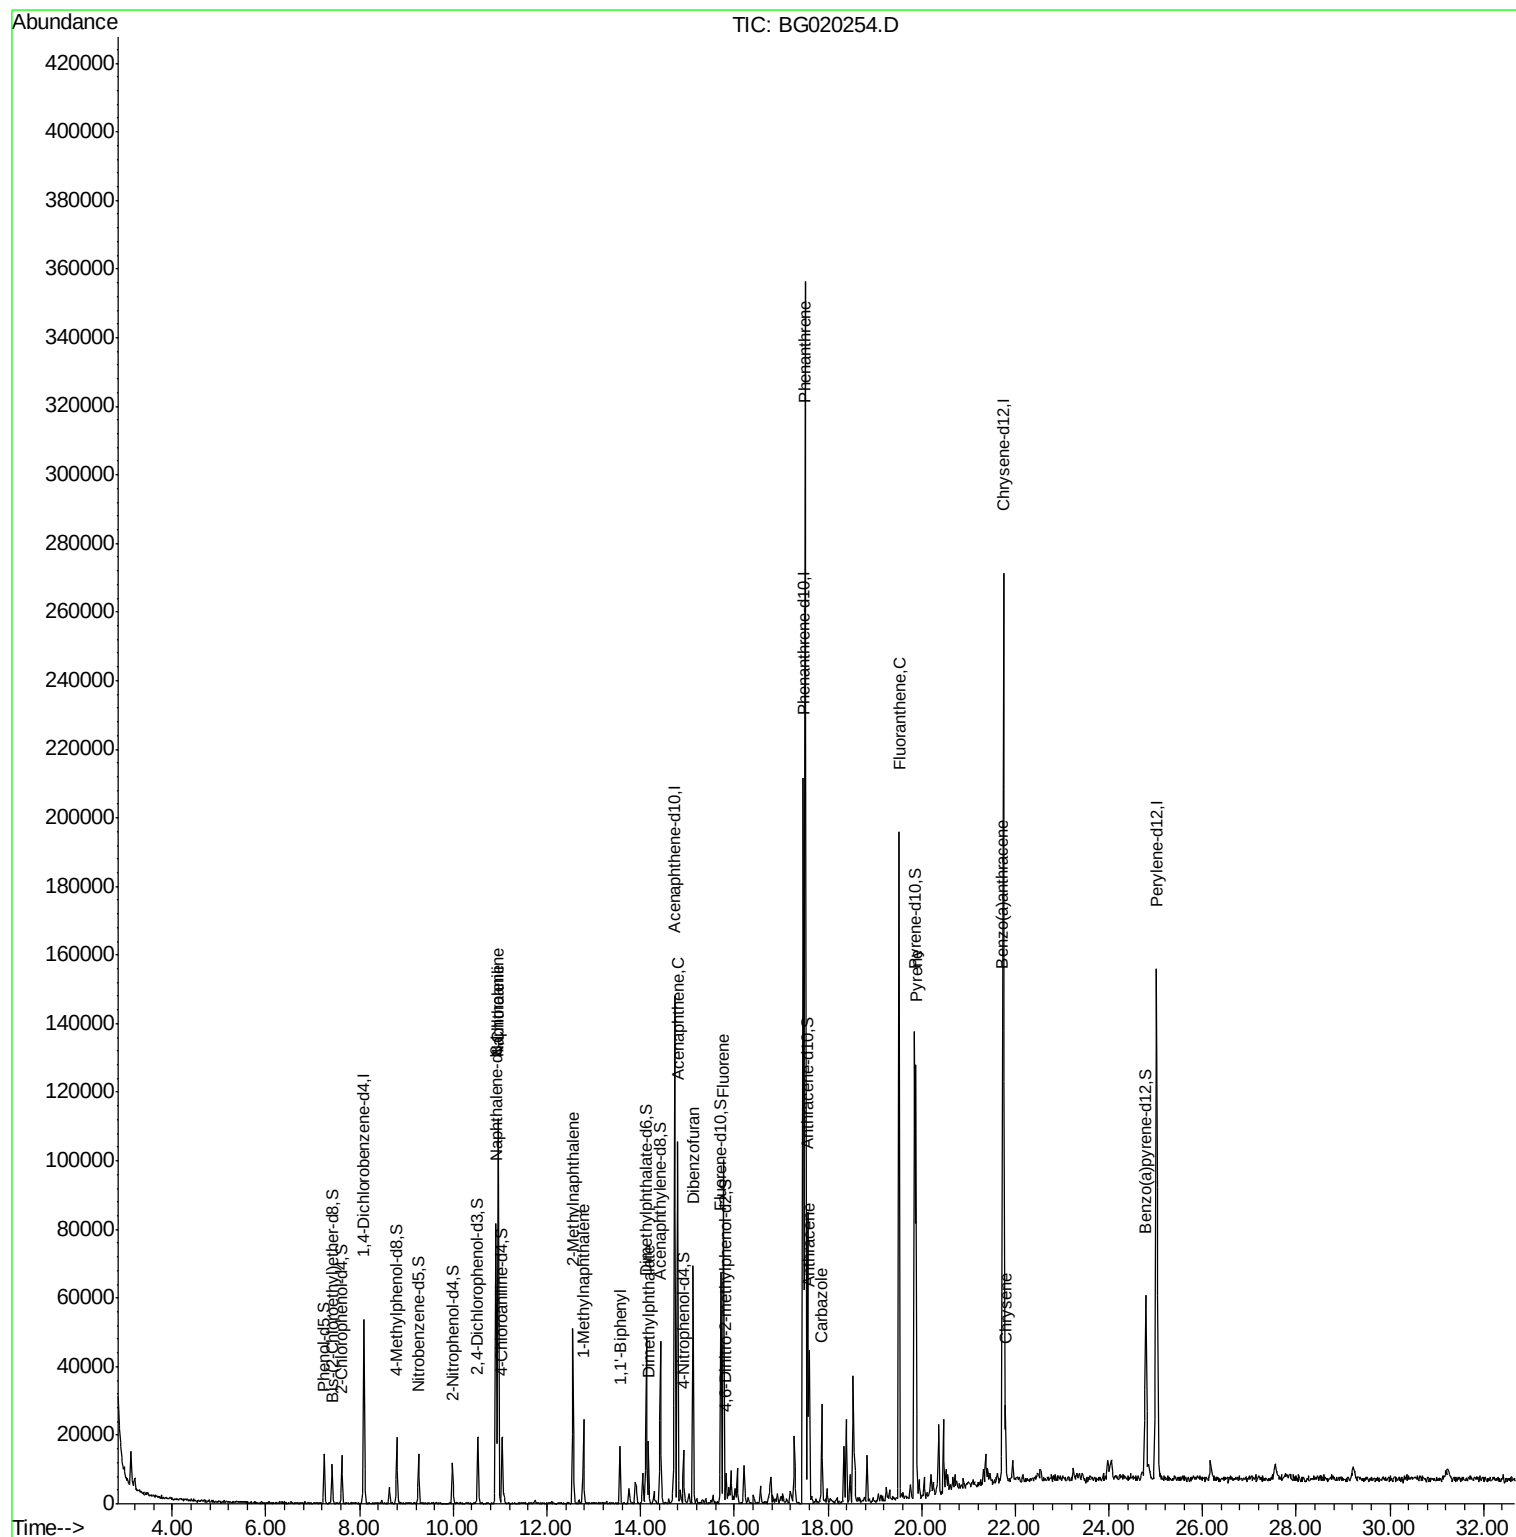


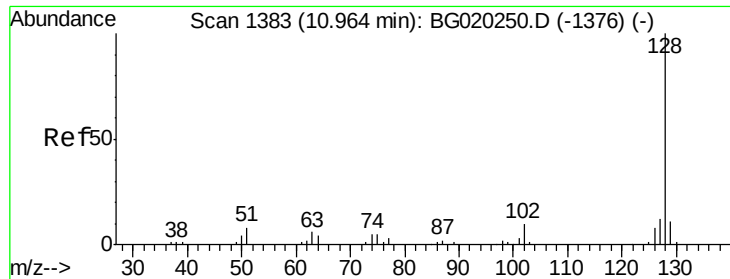

#28
Naphthalene
Concen: 25.92 ng/ul
RT: 10.96 min Scan# 1382
Delta R.T. -0.00 min
Lab File: BG020254.D
Acq: 17 Dec 2015 20:31




Instrument :
BNA_G
ClientSampleId :
D9N28DL


Tgt Ion:128 Resp: 95395
Ion Ratio Lower Upper
128 100
129 11.3 8.6 12.8
127 11.6 10.1 15.1

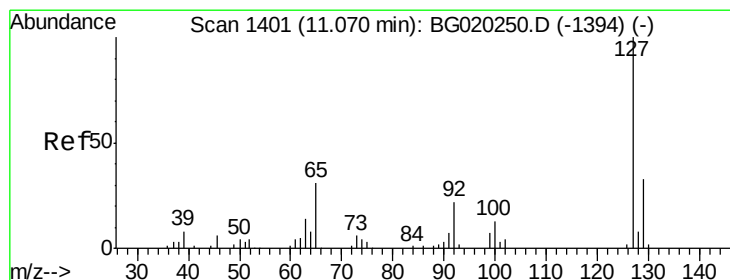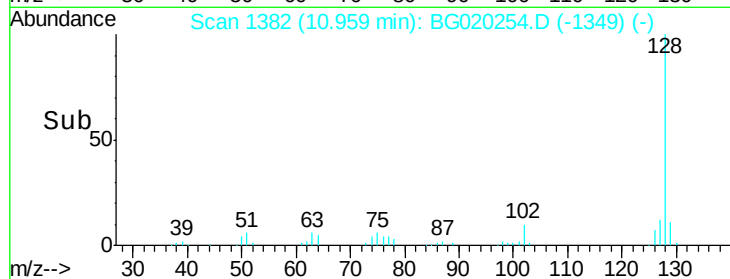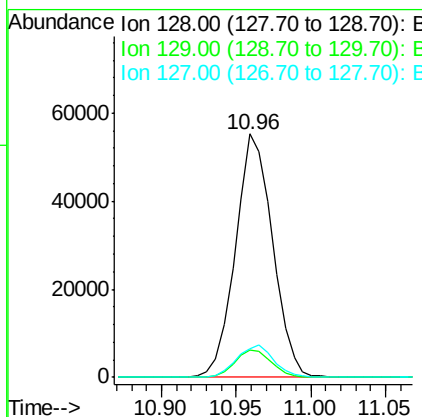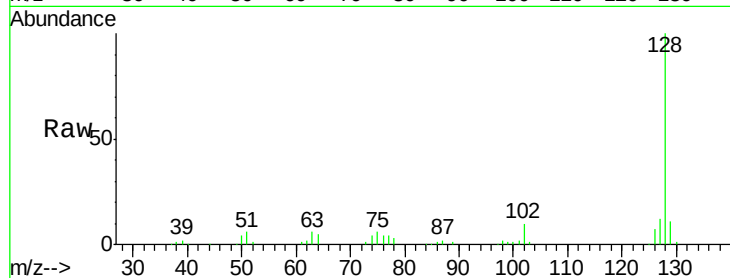

#30
4-Chloroaniline
Concen: 8.82 ng/ul
RT: 10.97 min Scan# 1383
Delta R.T. -0.10 min
Lab File: BG020254.D
Acq: 17 Dec 2015 20:31

Tgt Ion:127 Resp: 12532
Ion Ratio Lower Upper
127 100
129 83.6 25.7 38.5#

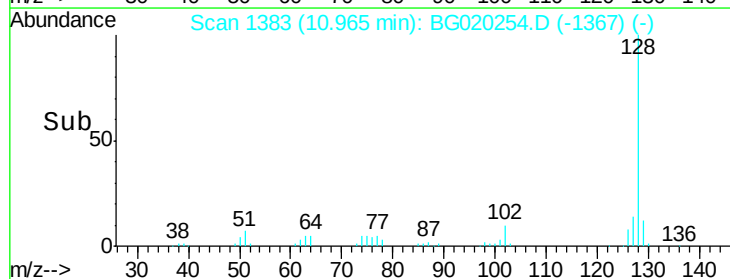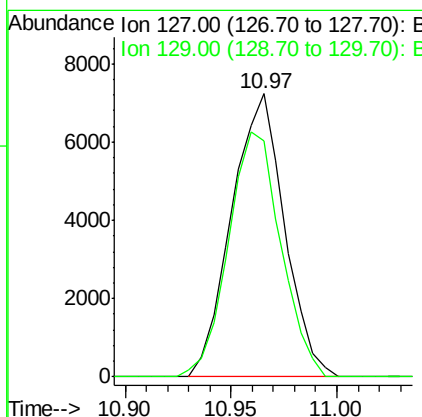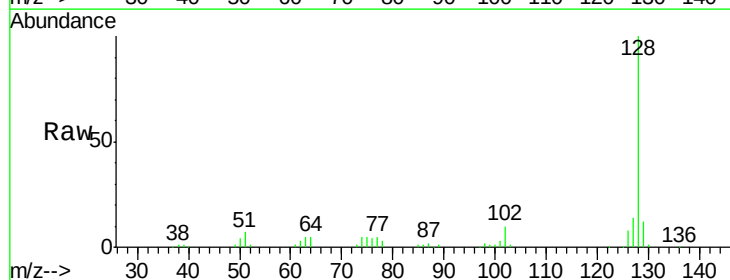


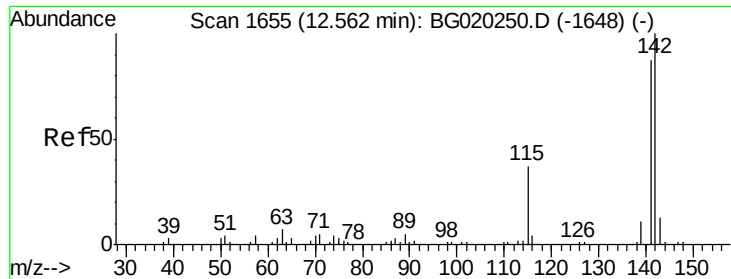




#34
 2-Methylnaphthalene
 Concen: 9.10 ng/ul
 RT: 12.56 min Scan# 1654
 Delta R.T. -0.00 min
 Lab File: BG020254.D
 Acq: 17 Dec 2015 20:31

Instrument :
 BNA_G
 ClientSampleId :
 D9N28DL

Tgt Ion:142 Resp: 25595
 Ion Ratio Lower Upper
 142 100
 141 86.6 74.9 112.3

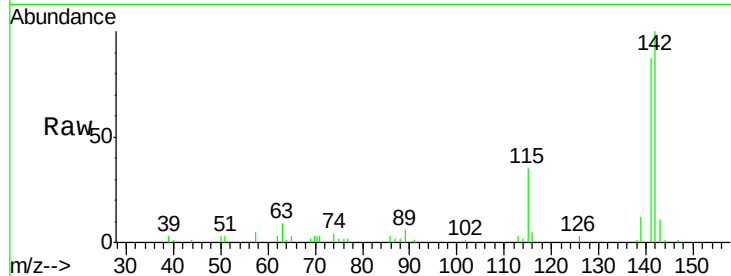


Abundance Ion 142.00 (141.70 to 142.70): E
 Ion 141.00 (140.70 to 141.70): E

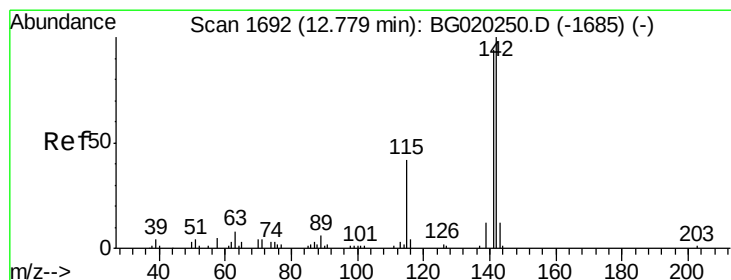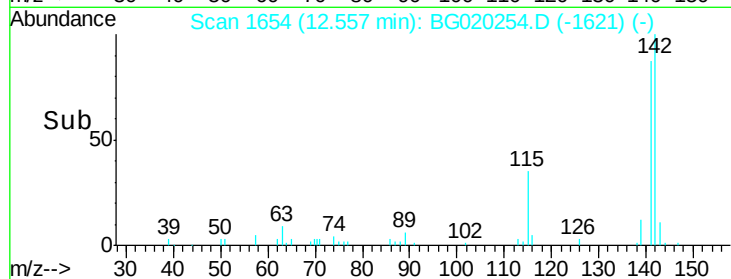
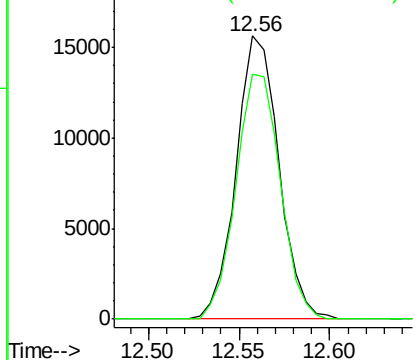



#35
 1-Methylnaphthalene
 Concen: 4.46 ng/ul
 RT: 12.78 min Scan# 1692
 Delta R.T. 0.00 min
 Lab File: BG020254.D
 Acq: 17 Dec 2015 20:31

Tgt Ion:142 Resp: 12054
 Ion Ratio Lower Upper
 142 100
 141 94.3 73.0 109.6
 116 5.2 3.0 4.6#

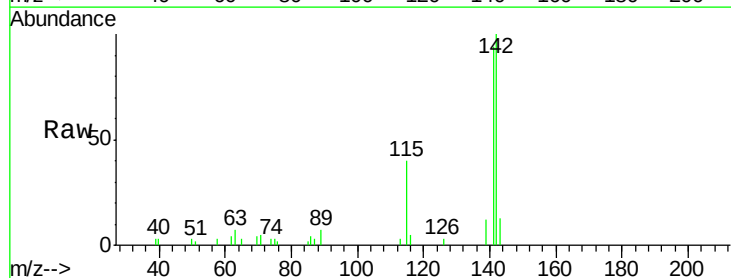

Abundance Ion 142.00 (141.70 to 142.70): E
 Ion 141.00 (140.70 to 141.70): E
 Ion 116.00 (115.70 to 116.70): E

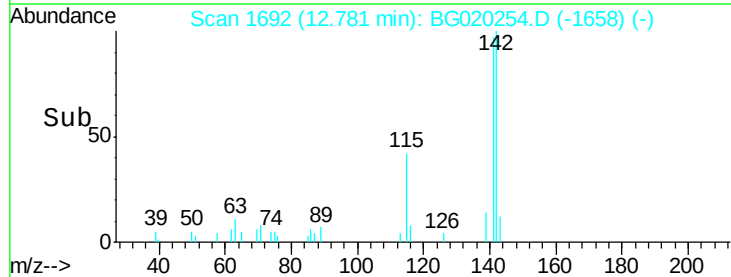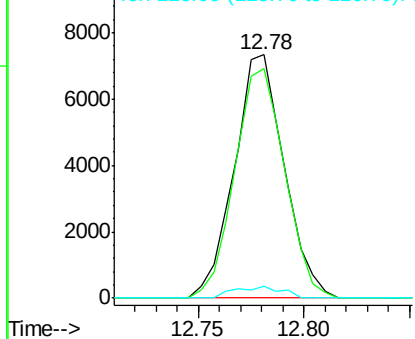


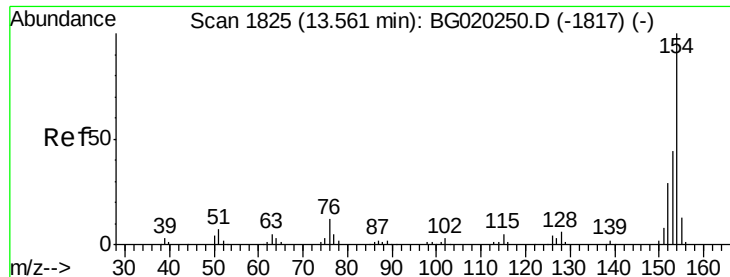




#41
 1,1'-Biphenyl
 Concen: 2.59 ng/ul
 RT: 13.56 min Scan# 1825
 Delta R.T. 0.00 min
 Lab File: BG020254.D
 Acq: 17 Dec 2015 20:31

Instrument :
 BNA_G
 ClientSampleId :
 D9N28DL

Tgt Ion:154 Resp: 9909
 Ion Ratio Lower Upper
 154 100
 153 41.7 35.5 53.3
 76 8.2 10.4 15.6#

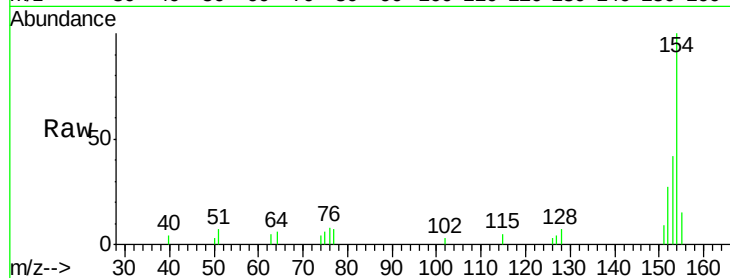


Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 76.00 (75.70 to 76.70): BGC

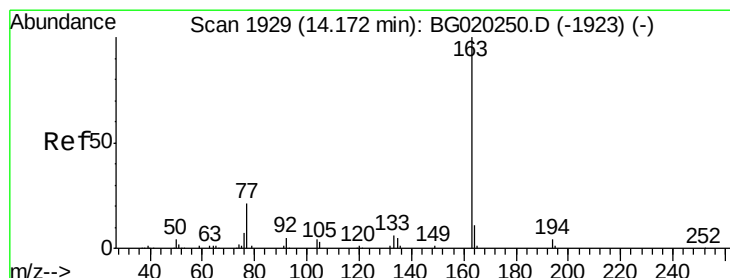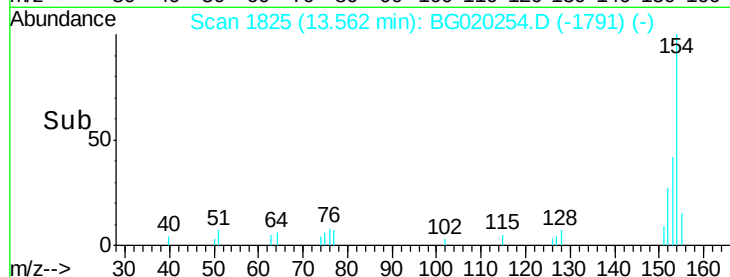
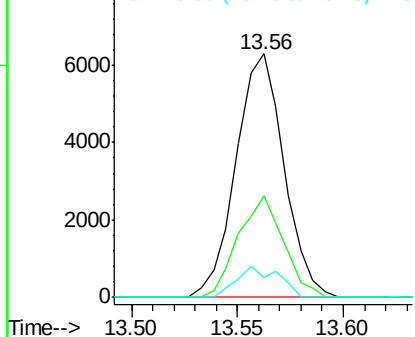



#45
 Dimethylphthalate
 Concen: 3.13 ng/ul
 RT: 14.17 min Scan# 1929
 Delta R.T. 0.00 min
 Lab File: BG020254.D
 Acq: 17 Dec 2015 20:31

Tgt Ion:163 Resp: 13117
 Ion Ratio Lower Upper
 163 100
 194 5.6 3.5 5.3#
 164 8.6 7.7 11.5

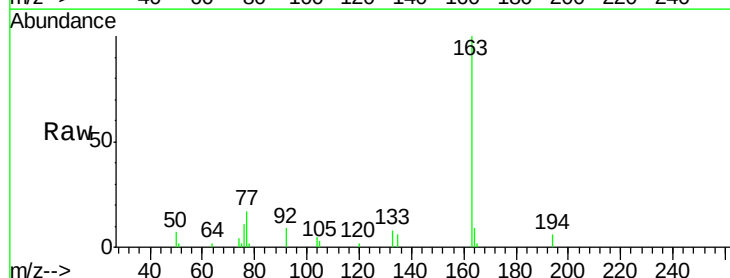

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

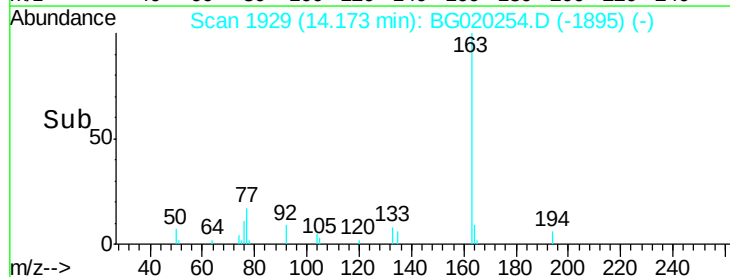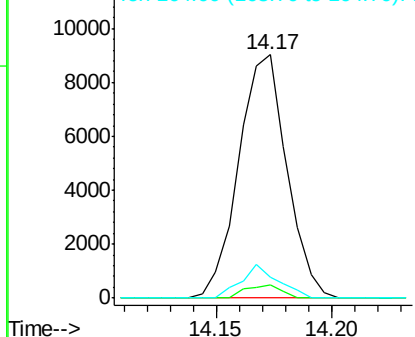

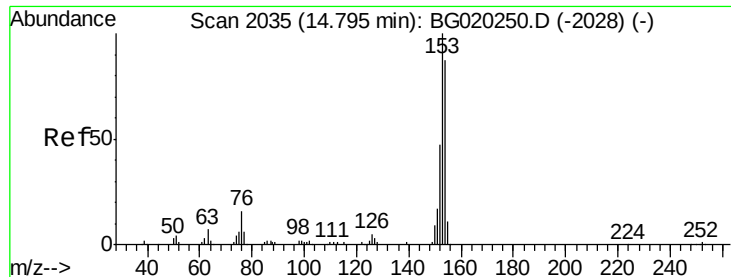

#50

Acenaphthene

Concen: 13.35 ng/ul

RT: 14.79 min Scan# 2034

Delta R.T. -0.00 min

Lab File: BG020254.D

Acq: 17 Dec 2015 20:31

Instrument :

BNA_G

ClientSampleId :

D9N28DL


Tgt Ion:153 Resp: 45533

Ion Ratio Lower Upper

153 100

152 48.6 37.6 56.4




154 87.9 67.9 101.9

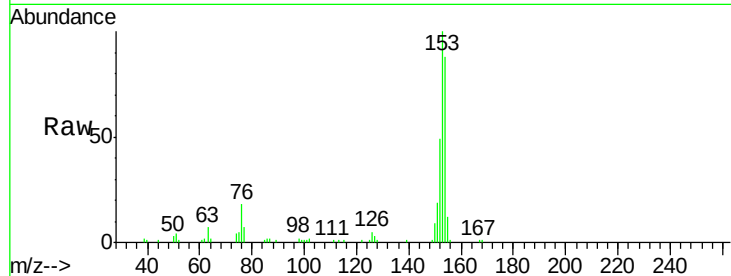

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

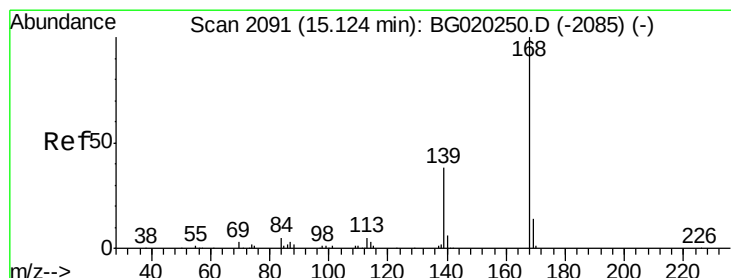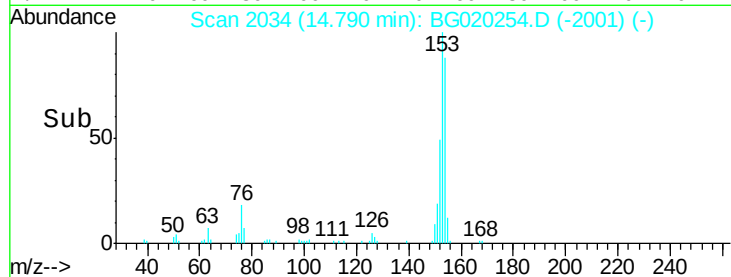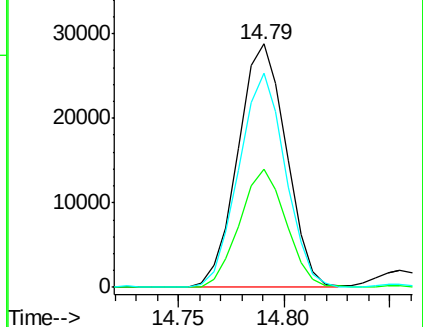

#54

Dibenzofuran

Concen: 9.22 ng/ul

RT: 15.13 min Scan# 2091

Delta R.T. 0.00 min

Lab File: BG020254.D


Acq: 17 Dec 2015 20:31

Tgt Ion:168 Resp: 46776

Ion Ratio Lower Upper



168 100


139 37.5 30.5 45.7

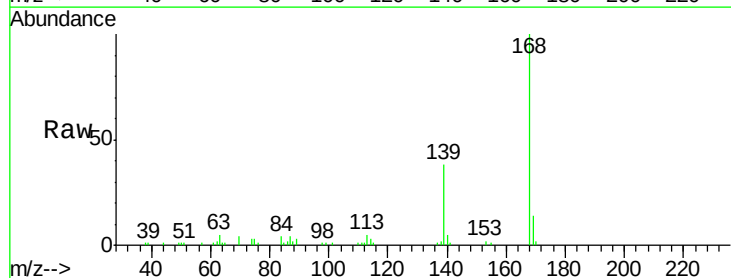

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E



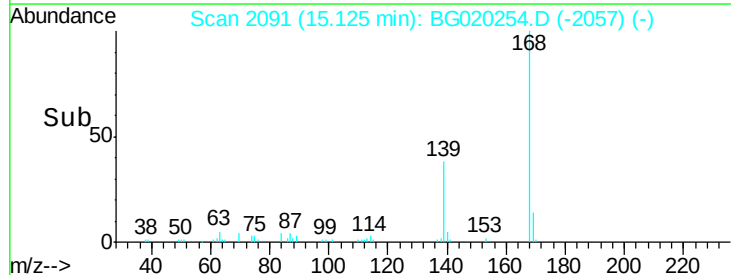
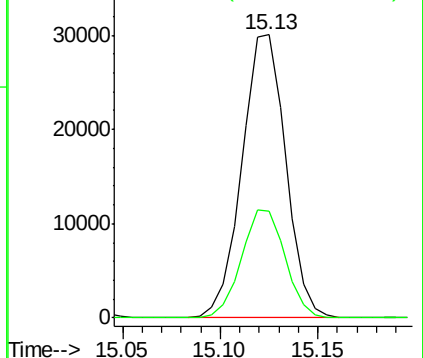


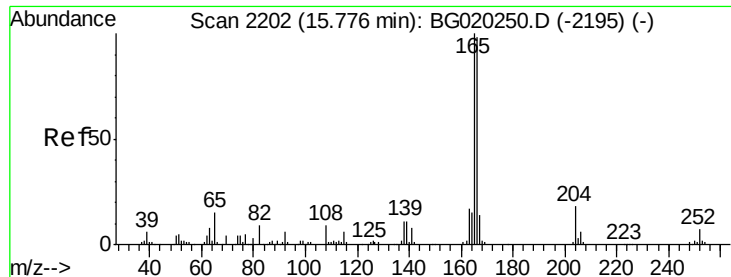

#59
 Fluorene
 Concen: 11.65 ng/ul
 RT: 15.77 min Scan# 2201
 Delta R.T. -0.00 min
 Lab File: BG020254.D
 Acq: 17 Dec 2015 20:31




Instrument :
 BNA_G
 ClientSampleId :
 D9N28DL


Tgt Ion:166 Resp: 47467
 Ion Ratio Lower Upper
 166 100
 165 101.2 81.4 122.0
 167 13.9 11.2 16.8

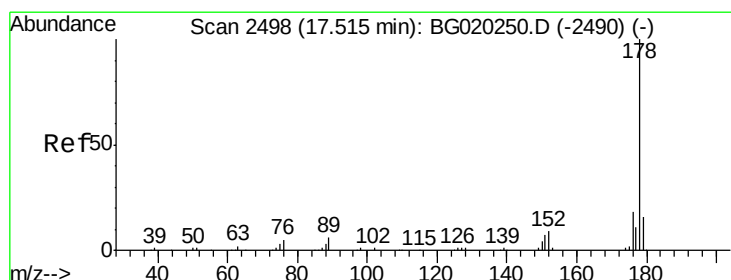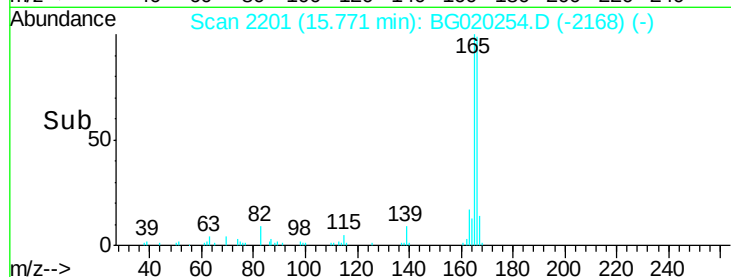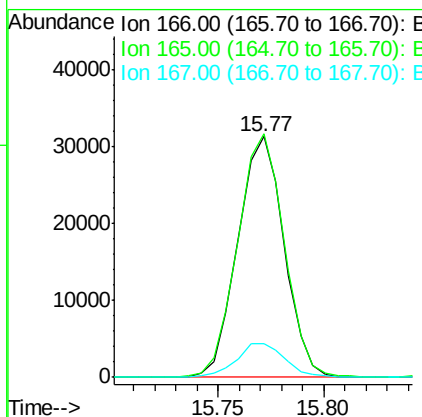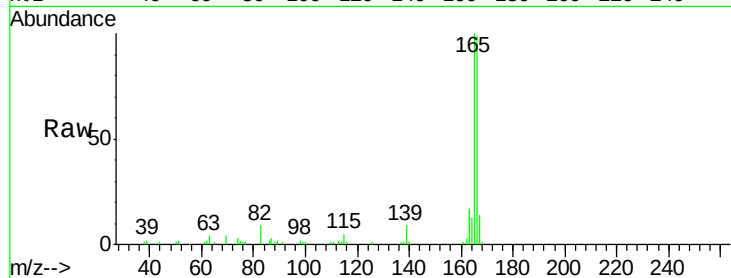

#70
 Phenanthrene
 Concen: 32.37 ng/ul
 RT: 17.52 min Scan# 2498
 Delta R.T. 0.00 min
 Lab File: BG020254.D
 Acq: 17 Dec 2015 20:31

Tgt Ion:178 Resp: 234898
 Ion Ratio Lower Upper
 178 100
 179 15.7 12.9 19.3
 176 18.9 15.3 22.9

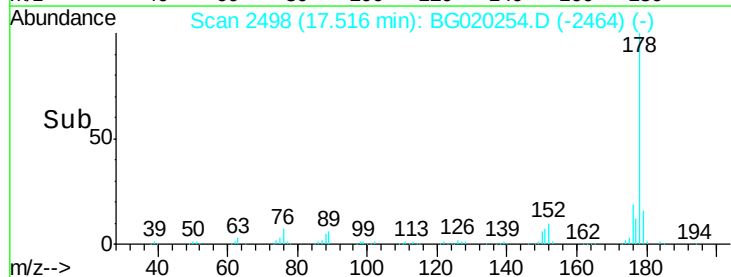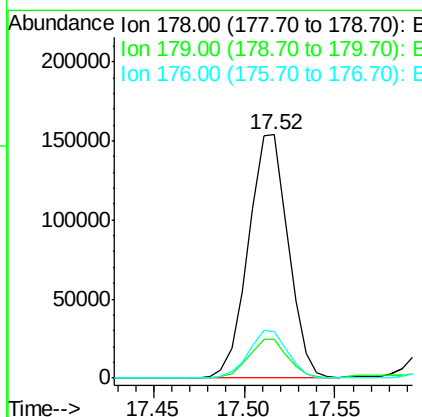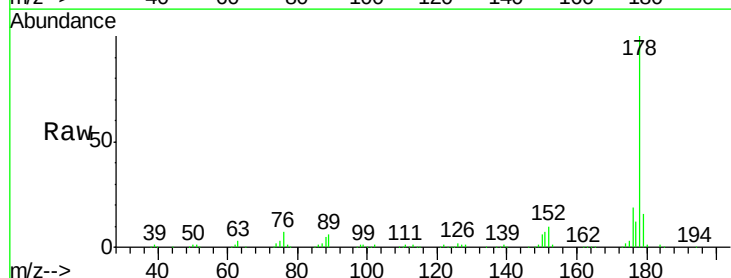

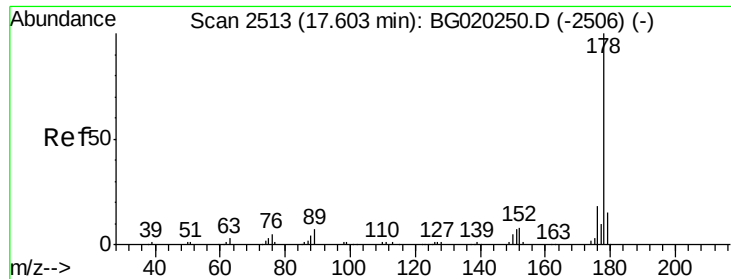

#72

Anthracene

Concen: 4.36 ng/ul

RT: 17.60 min Scan# 2513

Delta R.T. 0.00 min

Lab File: BG020254.D

Acq: 17 Dec 2015 20:31

Instrument :

BNA_G

ClientSampleId :

D9N28DL


Tgt Ion:178 Resp: 32094

Ion Ratio Lower Upper

178 100

179 17.9 12.3 18.5




176 16.1 14.3 21.5

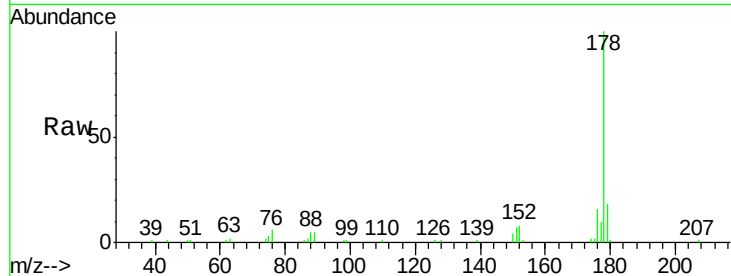

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

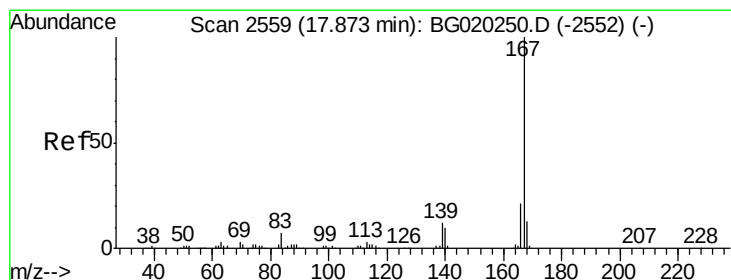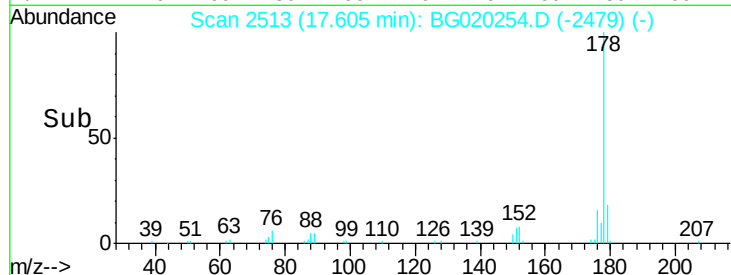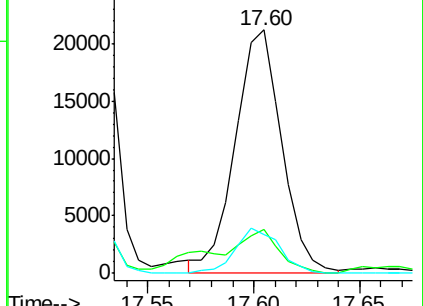

#75

Carbazole

Concen: 3.09 ng/ul

RT: 17.87 min Scan# 2558

Delta R.T. -0.00 min

Lab File: BG020254.D

Acq: 17 Dec 2015 20:31


Tgt Ion:167 Resp: 19119

Ion Ratio Lower Upper

167 100

166 23.1 17.0 25.6



139 13.4 10.1 15.1

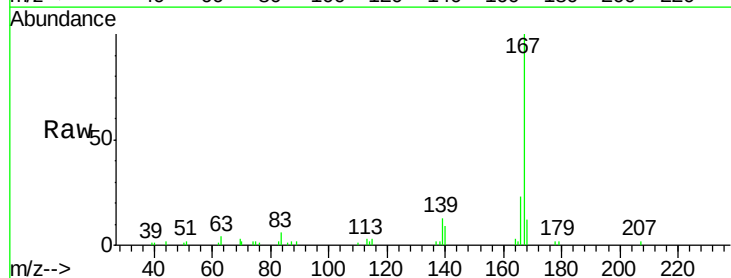


Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E



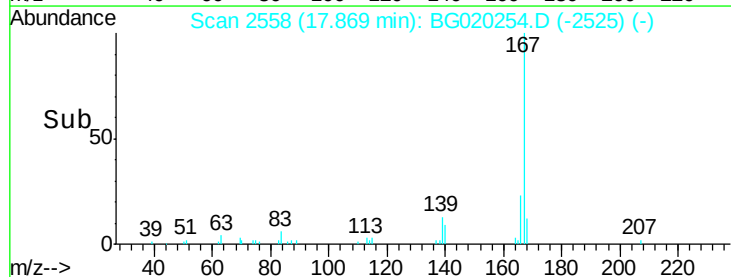
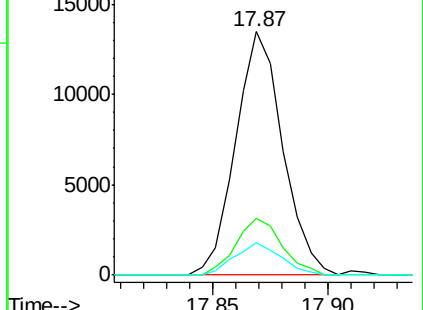


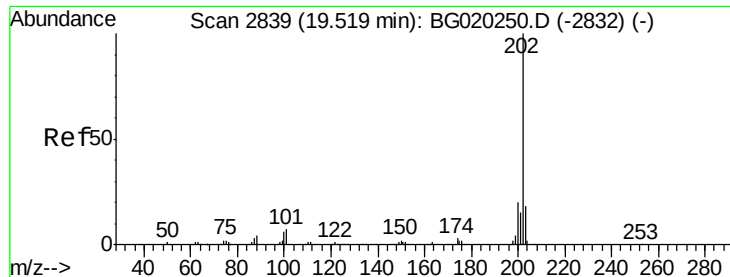

#77
Fluoranthene
 Concen: 15.54 ng/ul
 RT: 19.52 min Scan# 2839
 Delta R.T. 0.00 min
 Lab File: BG020254.D
 Acq: 17 Dec 2015 20:31




Instrument :
 BNA_G
 ClientSampleId :
 D9N28DL


Tgt Ion	Ratio	Lower	Upper
202	100		
101	7.6	6.2	9.4
100	6.5	5.1	7.7

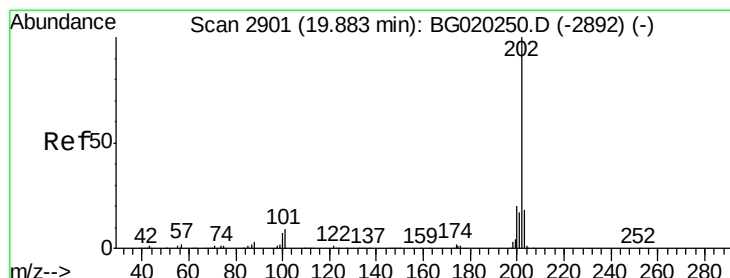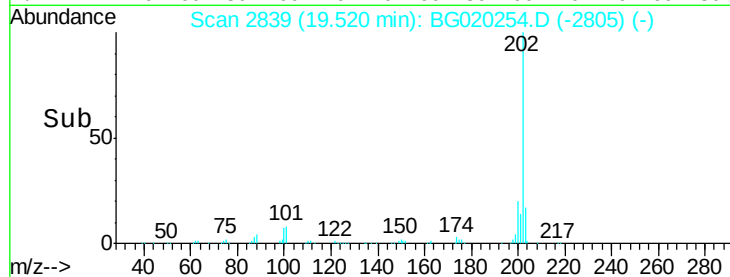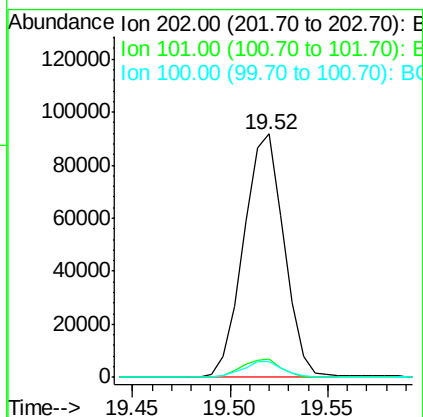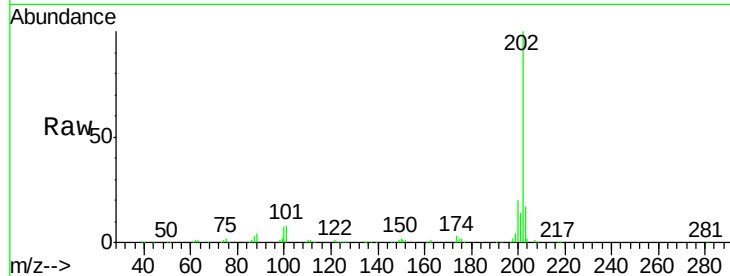

#80
Pyrene
 Concen: 8.66 ng/ul
 RT: 19.88 min Scan# 2900
 Delta R.T. -0.00 min
 Lab File: BG020254.D
 Acq: 17 Dec 2015 20:31

Tgt Ion	Ratio	Lower	Upper
202	100		
101	9.9	7.0	10.4
100	7.8	6.4	9.6

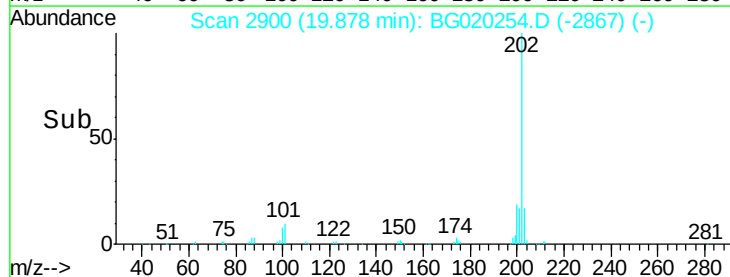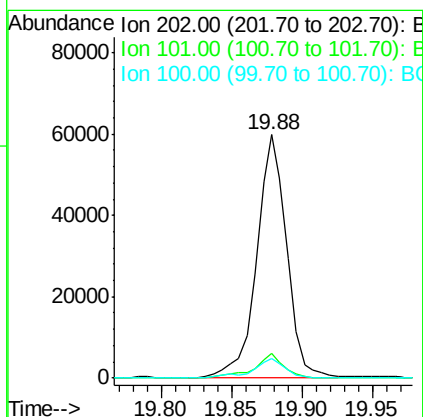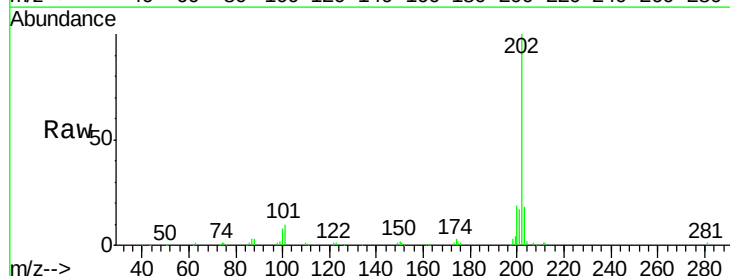

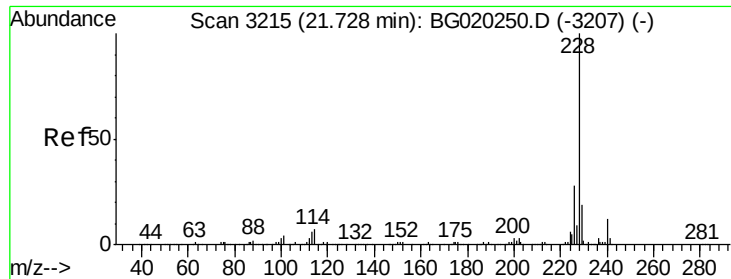

#83

Benzo(a)anthracene

Concen: 2.18 ng/ul

RT: 21.72 min Scan# 3214

Delta R.T. -0.00 min

Lab File: BG020254.D

Acq: 17 Dec 2015 20:31





Instrument :

BNA_G

ClientSampleId :

D9N28DL

Tgt Ion:	228	Resp:	21747
Ion	Ratio	Lower	Upper
228	100		
229	18.5	15.8	23.8
226	24.4	21.8	32.6

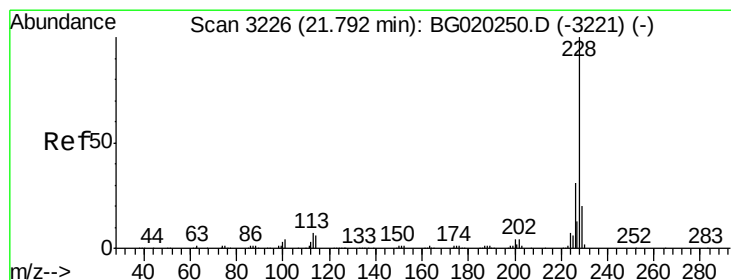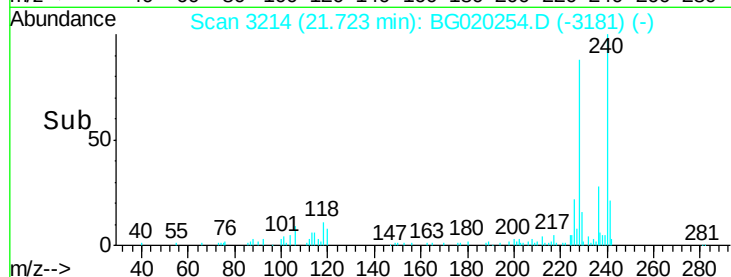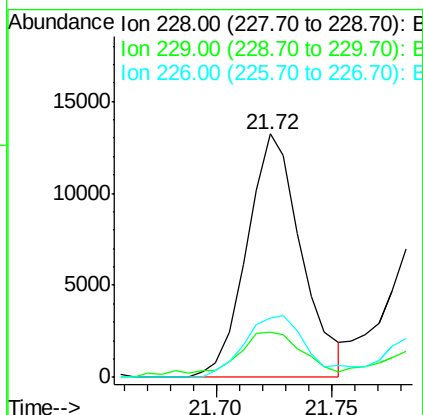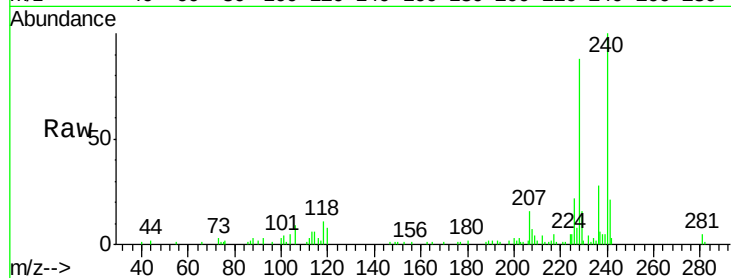

#85

Chrysene

Concen: 1.92 ng/ul

RT: 21.79 min Scan# 3226

Delta R.T. 0.00 min

Lab File: BG020254.D

Acq: 17 Dec 2015 20:31

Tgt Ion:	228	Resp:	18019
Ion	Ratio	Lower	Upper
228	100		
226	32.0	23.9	35.9
229	18.3	15.6	23.4

