

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121817\  
 Data File : BG031632.D  
 Acq On : 18 Dec 2017 13:25  
 Operator : SJ/JU  
 Sample : I6909-02  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :

Quant Time: Dec 19 07:00:12 2017  
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Dec 11 17:25:55 2017  
 Response via : Initial Calibration

| Internal Standards          | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|-----------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 8.10  | 152  | 73830    | 20.00 | ng    | 0.00     |
| 21) Naphthalene-d8          | 10.91 | 136  | 326016   | 20.00 | ng    | 0.00     |
| 38) Acenaphthene-d10        | 14.72 | 164  | 222894   | 20.00 | ng    | -0.01    |
| 63) Phenanthrene-d10        | 17.47 | 188  | 582547   | 20.00 | ng    | -0.01    |
| 75) Chrysene-d12            | 21.74 | 240  | 621321   | 20.00 | ng    | -0.01    |
| 86) Perylene-d12            | 25.01 | 264  | 527979   | 20.00 | ng    | -0.02    |
| System Monitoring Compounds |       |      |          |       |       |          |
| 5) 2-Fluorophenol           | 5.66  | 112  | 172502   | 41.41 | ng    | -0.01    |
| 7) Phenol-d6                | 7.27  | 99   | 133524   | 23.09 | ng    | 0.00     |
| 23) Nitrobenzene-d5         | 9.27  | 82   | 461385   | 87.23 | ng    | 0.00     |
| 41) 2,4,6-Tribromophenol    | 16.21 | 330  | 259459   | 99.36 | ng    | -0.01    |
| 44) 2-Fluorobiphenyl        | 13.35 | 172  | 1414410  | 93.15 | ng    | 0.00     |
| 78) Terphenyl-d14           | 20.06 | 244  | 2310600  | 84.61 | ng    | -0.01    |

Target Compounds Qvalue


-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121817\  
Data File : BG031632.D  
Acq On : 18 Dec 2017 13:25  
Operator : SJ/JU  
Sample : I6909-02  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :

Quant Time: Dec 19 07:00:12 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 11 17:25:55 2017  
Response via : Initial Calibration

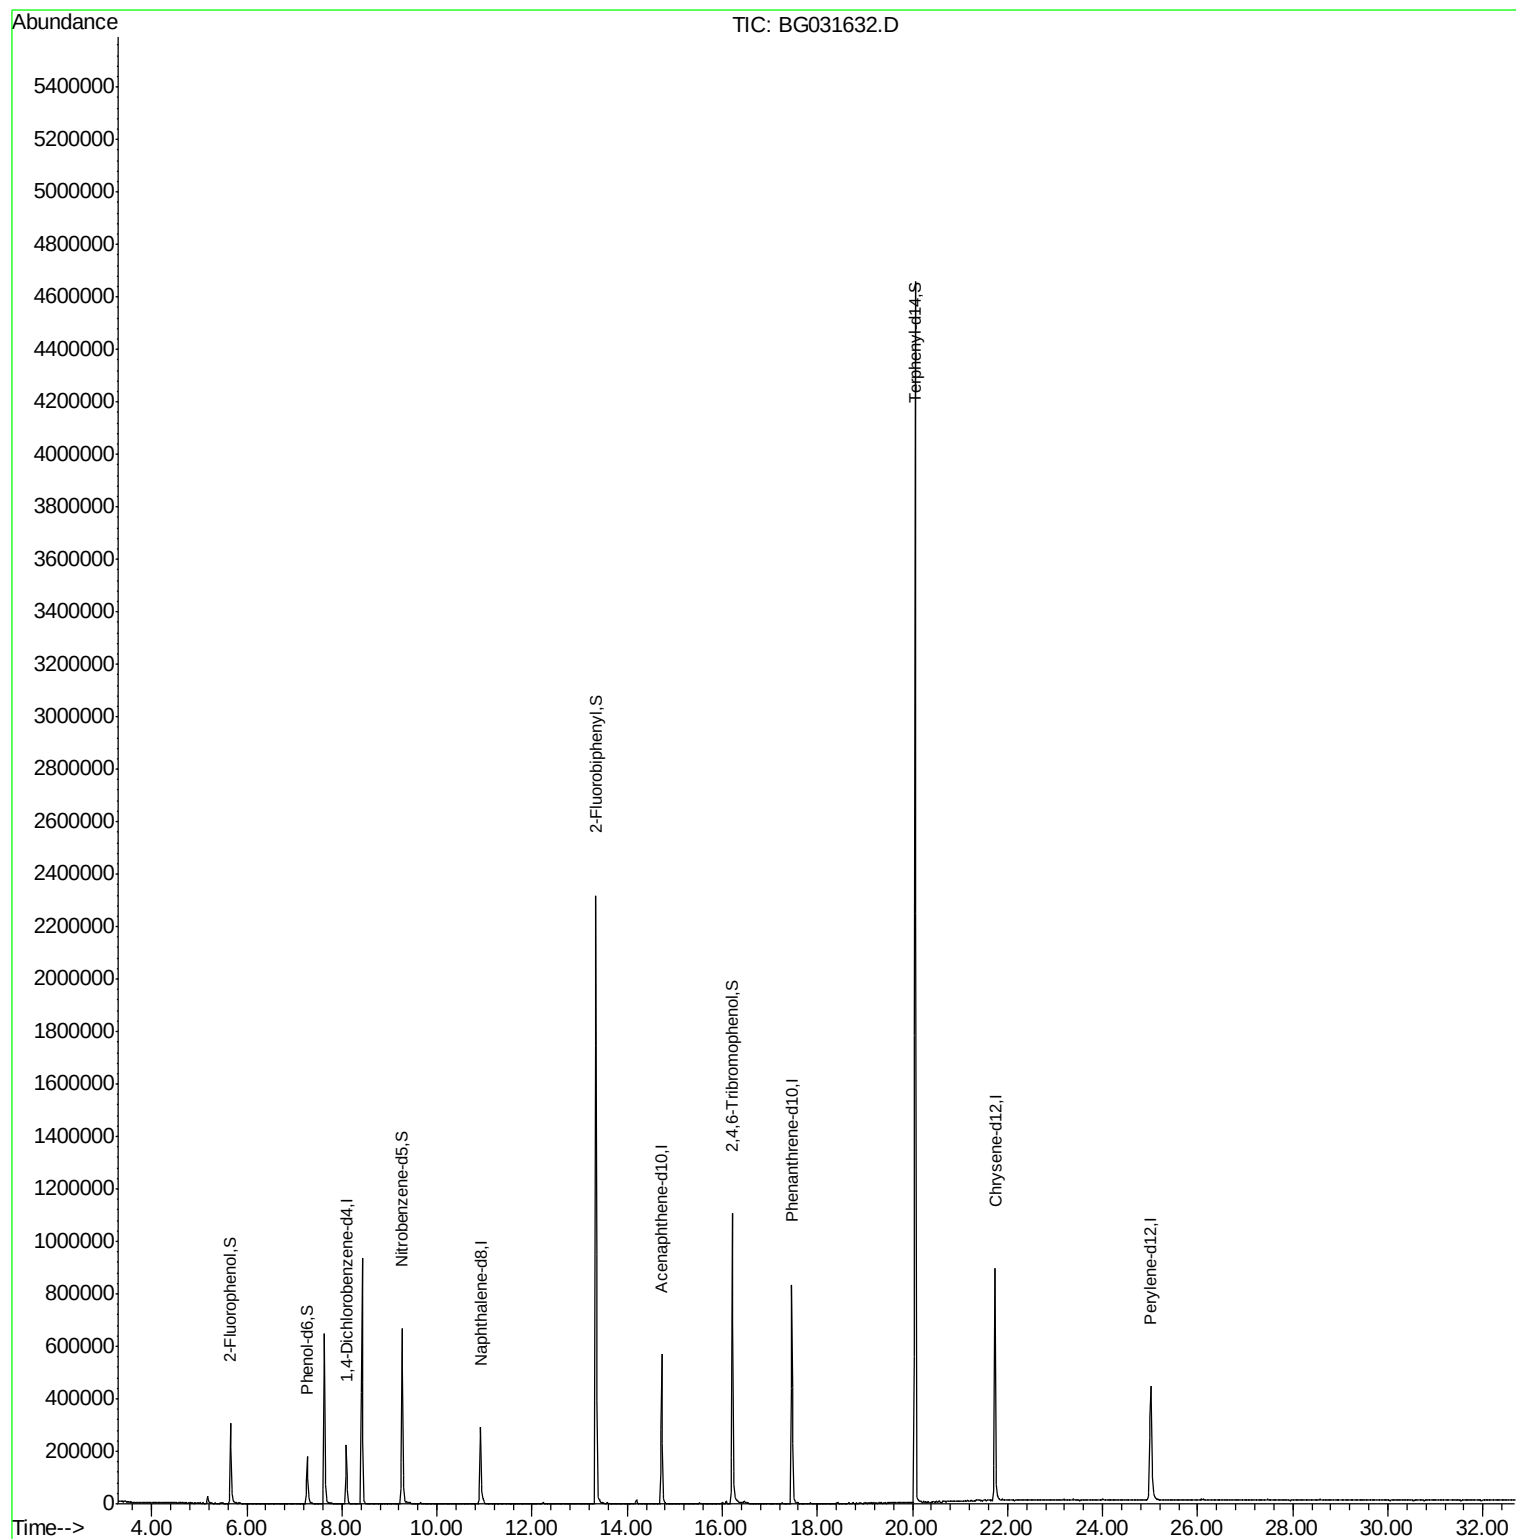

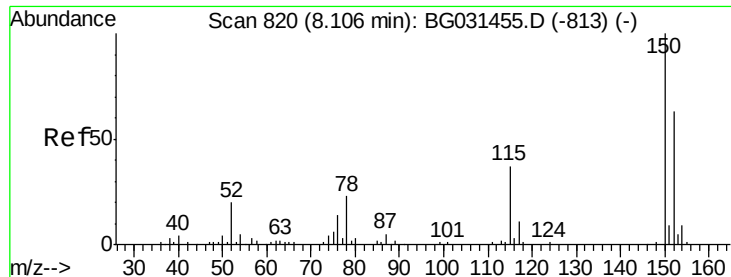


#1




1,4-Dichlorobenzene-d4  
Concen: 20.000 ng  
RT: 8.10 min Scan# 819  
Delta R.T. -0.01 min  
Lab File: BG031632.D  
Acq: 18 Dec 2017 13:25

Instrument :  
BNA\_G  
ClientSampleId :

Tot Ion:152 Resp: 73830  
Ion Ratio Lower Upper  
152 100  
150 149.9 126.6 189.8  
115 52.5 53.0 79.4#

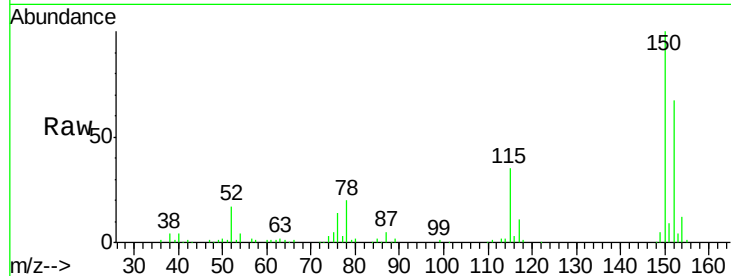


Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 150.00 (149.70 to 150.70): E  
Ion 115.00 (114.70 to 115.70): E

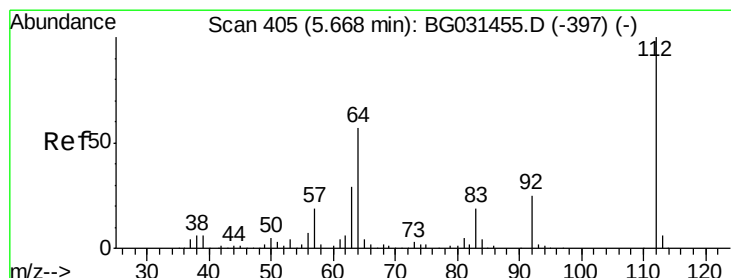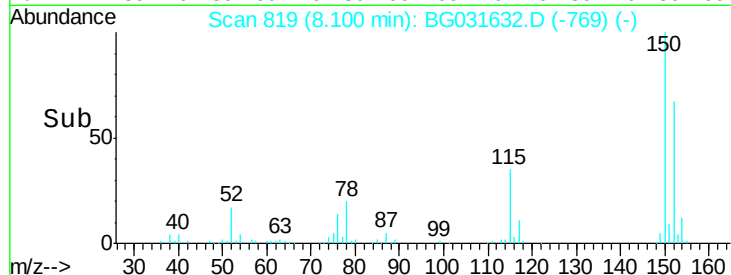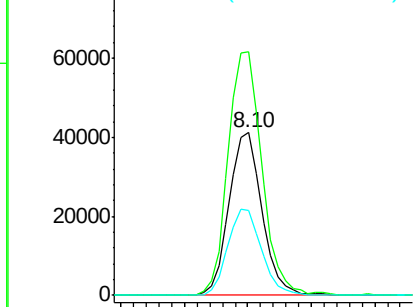



#5


2-Fluorophenol  
Concen: 41.414 ng  
RT: 5.66 min Scan# 403  
Delta R.T. -0.01 min  
Lab File: BG031632.D  
Acq: 18 Dec 2017 13:25

Tgt Ion:112 Resp: 172502  
Ion Ratio Lower Upper  
112 100  
64 57.4 56.3 84.5  
63 29.4 30.1 45.1#

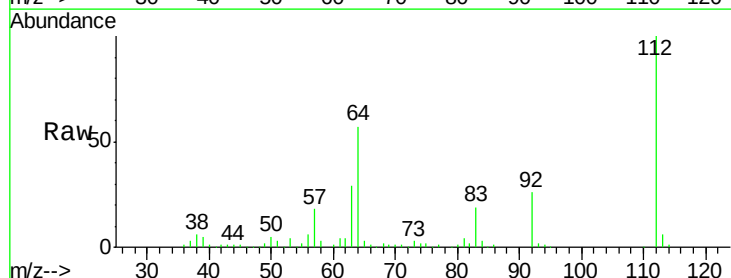

Abundance Ion 112.00 (111.70 to 112.70): E  
Ion 64.00 (63.70 to 64.70): BGC  
Ion 63.00 (62.70 to 63.70): BGC

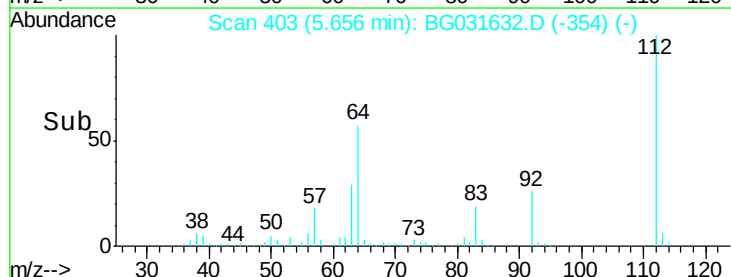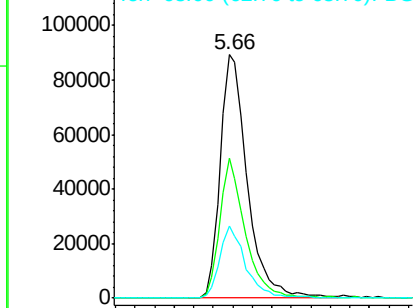

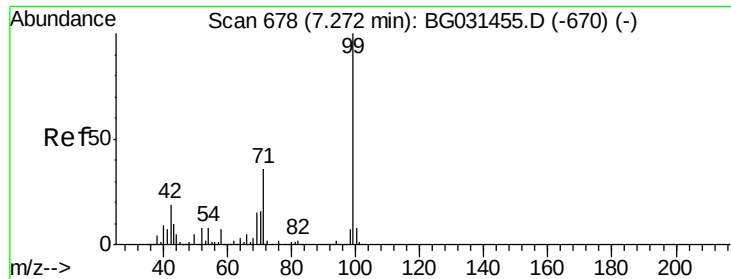

#7

Phenol-d6

Concen: 23.092 ng

RT: 7.27 min Scan# 677

Delta R.T. -0.01 min

Lab File: BG031632.D

Acq: 18 Dec 2017 13:25

Instrument :

BNA\_G

ClientSampleId :


Tot Ion: 99 Resp: 133524

Ion Ratio Lower Upper




99 100

42 17.4 14.1 21.1

71 34.1 26.1 39.1

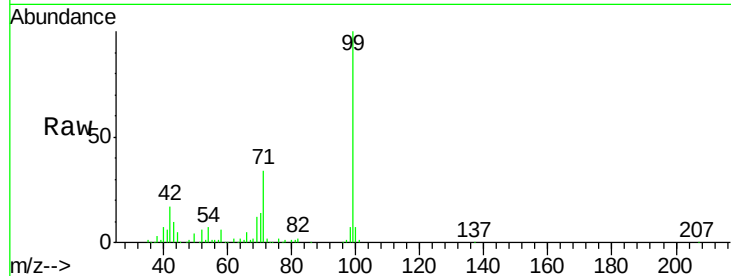

Abundance Ion 99.00 (98.70 to 99.70): BGC  
Ion 42.00 (41.70 to 42.70): BGC  
Ion 71.00 (70.70 to 71.70): BGC

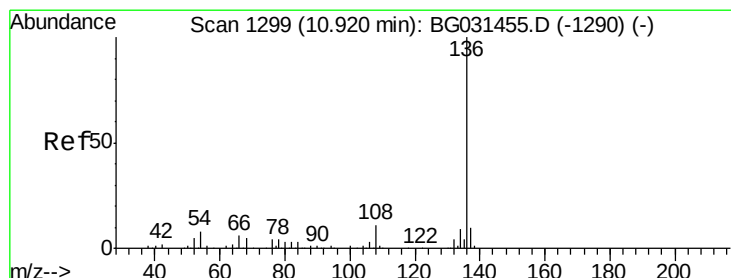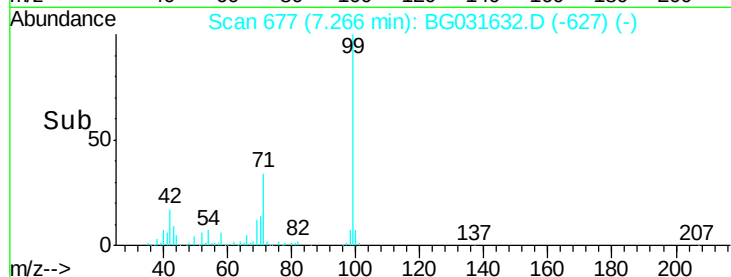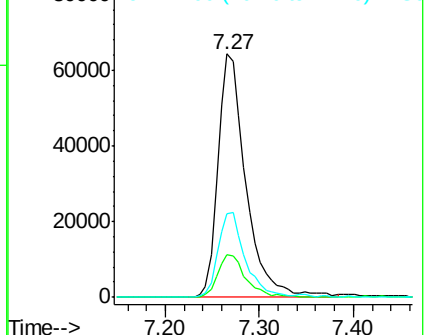

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.91 min Scan# 1298

Delta R.T. -0.01 min

Lab File: BG031632.D

Acq: 18 Dec 2017 13:25

Tgt Ion: 136 Resp: 326016


Ion Ratio Lower Upper

136 100



137 10.5 9.2 13.8


54 6.8 10.3 15.5#

68 4.8 4.5 6.7

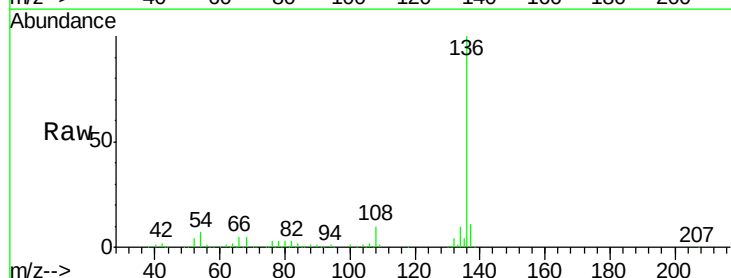

Abundance Ion 136.00 (135.70 to 136.70): BGC  
Ion 137.00 (136.70 to 137.70): BGC  
Ion 54.00 (53.70 to 54.70): BGC  
Ion 68.00 (67.70 to 68.70): BGC



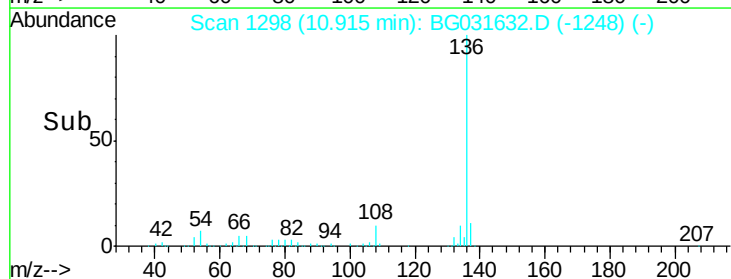
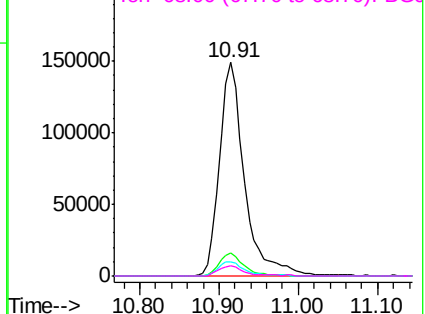


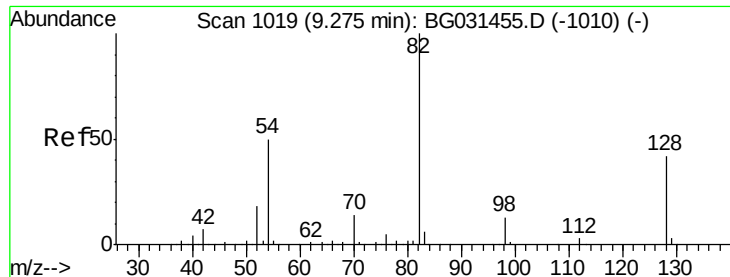

#23  
 Nitrobenzene-d5  
 Concen: 87.230 ng  
 RT: 9.27 min Scan# 1018  
 Delta R.T. -0.01 min  
 Lab File: BG031632.D  
 Acq: 18 Dec 2017 13:25




Instrument :  
 BNA\_G  
 ClientSampleId :


Tot Ion: 82 Resp: 461385  
 Ion Ratio Lower Upper  
 82 100  
 128 46.2 29.7 44.5#  
 54 48.4 43.1 64.7

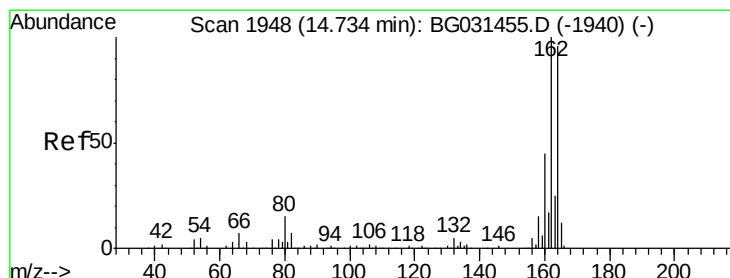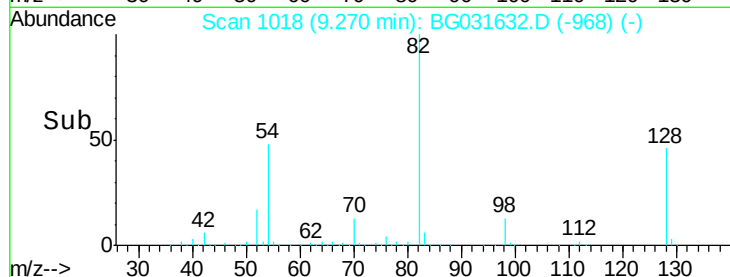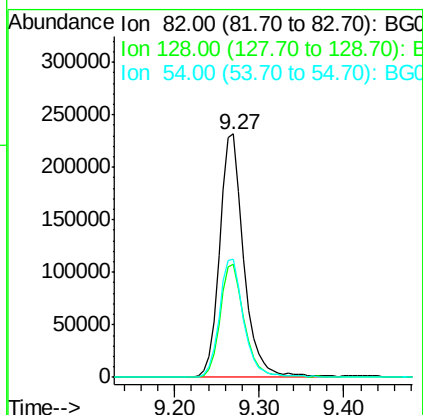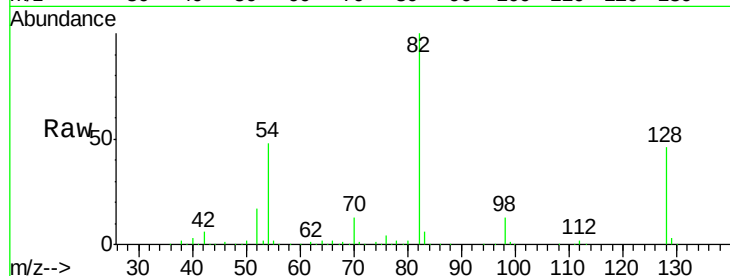

#38  
 Acenaphthene-d10  
 Concen: 20.000 ng  
 RT: 14.72 min Scan# 1946  
 Delta R.T. -0.01 min  
 Lab File: BG031632.D  
 Acq: 18 Dec 2017 13:25

Tgt Ion:164 Resp: 222894  
 Ion Ratio Lower Upper  
 164 100  
 162 101.8 78.8 118.2  
 160 43.8 35.4 53.0


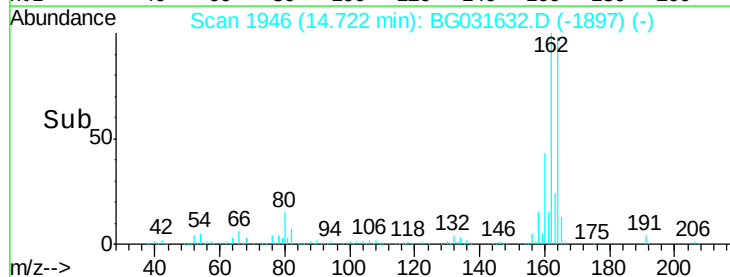
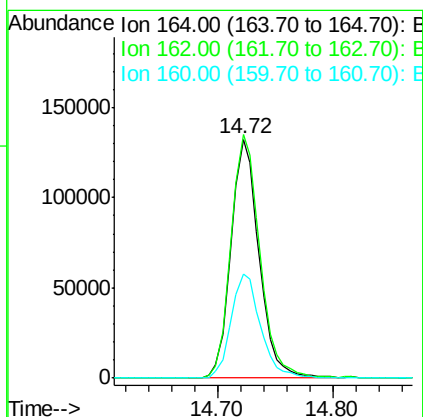
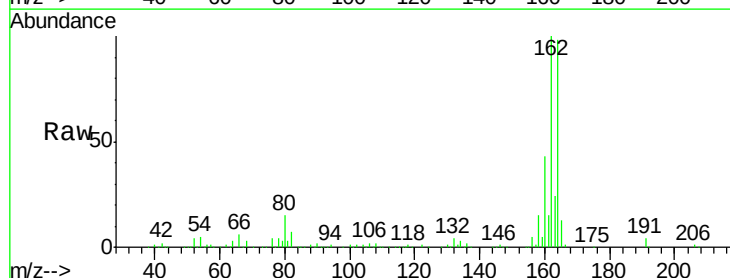


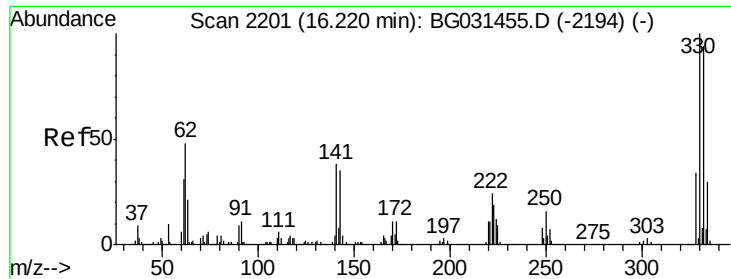

#41  
 2,4,6-Tribromophenol  
 Concen: 99.360 ng  
 RT: 16.21 min Scan# 2199  
 Delta R.T. -0.01 min  
 Lab File: BG031632.D  
 Acq: 18 Dec 2017 13:25




Instrument :  
 BNA\_G  
 ClientSampleId :


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 330     | 100   |       |       |
| 332     | 95.5  | 77.0  | 115.6 |
| 141     | 33.5  | 25.2  | 37.8  |

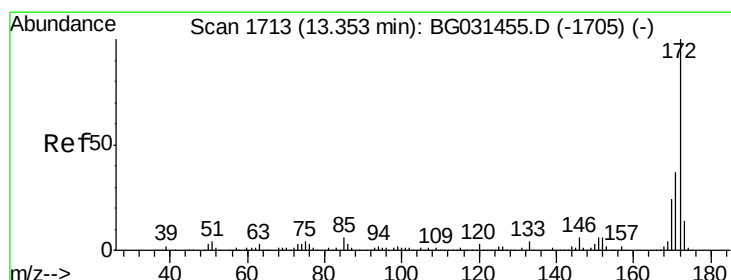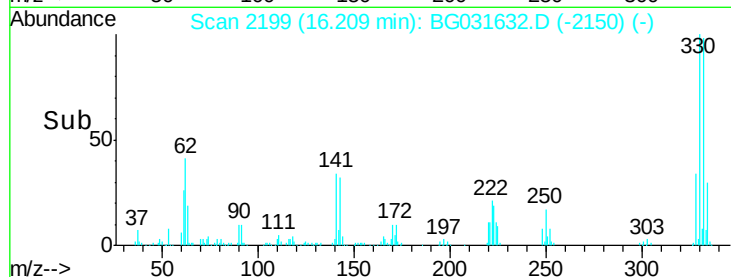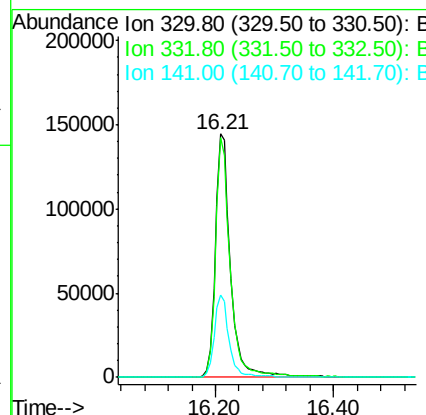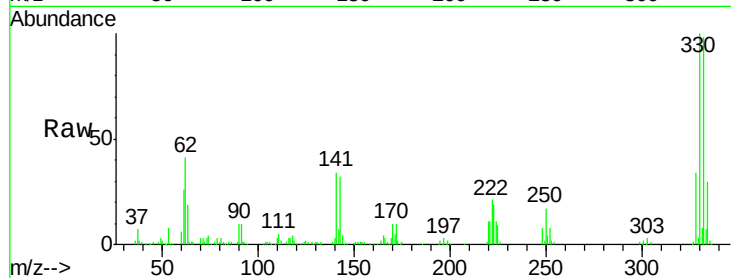

#44  
 2-Fluorobiphenyl  
 Concen: 93.146 ng  
 RT: 13.35 min Scan# 1712  
 Delta R.T. -0.01 min  
 Lab File: BG031632.D  
 Acq: 18 Dec 2017 13:25

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 172     | 100   |       |       |
| 171     | 38.5  | 30.0  | 45.0  |
| 170     | 24.2  | 19.5  | 29.3  |

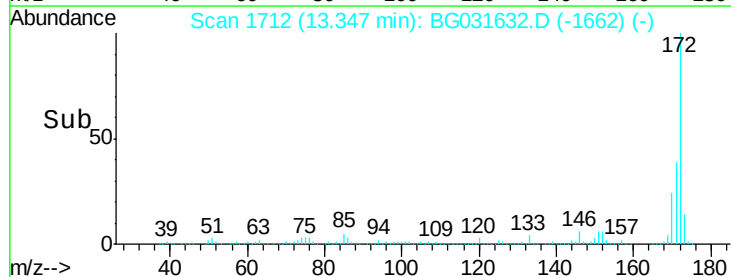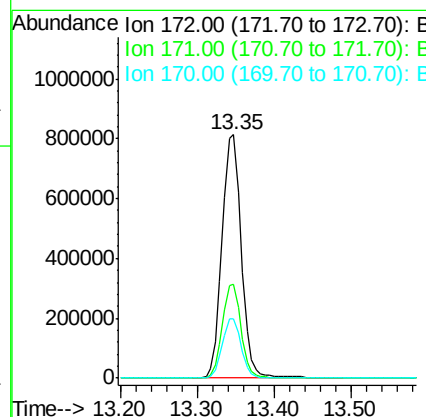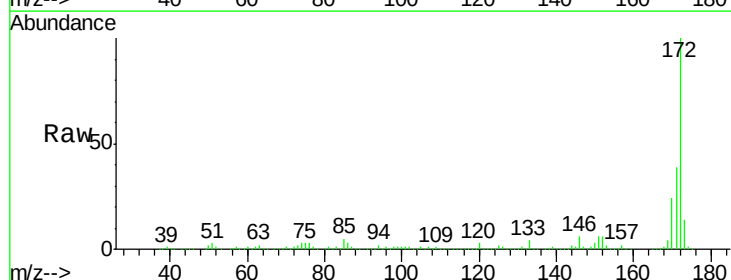

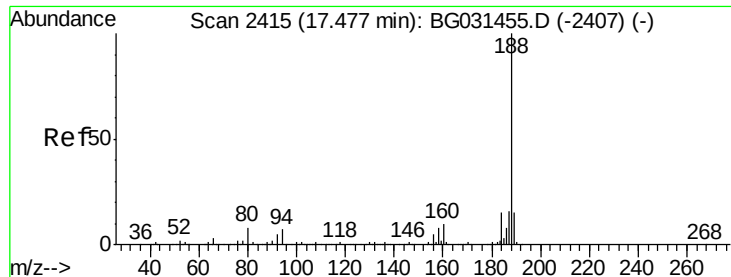

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.47 min Scan# 2413

Delta R.T. -0.01 min

Lab File: BG031632.D

Acq: 18 Dec 2017 13:25

Instrument :

BNA\_G

ClientSampleId :


Tot Ion:188 Resp: 582547

Ion Ratio Lower Upper

188 100

94 6.2 6.9 10.3#




80 7.1 7.7 11.5#

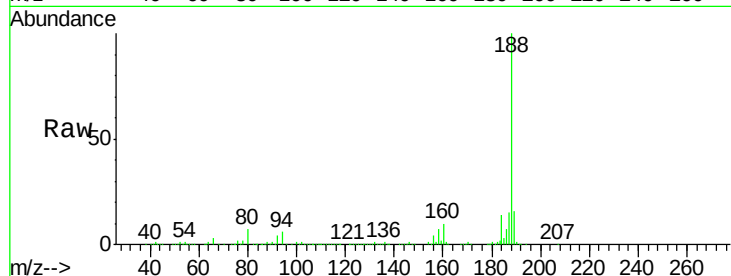

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

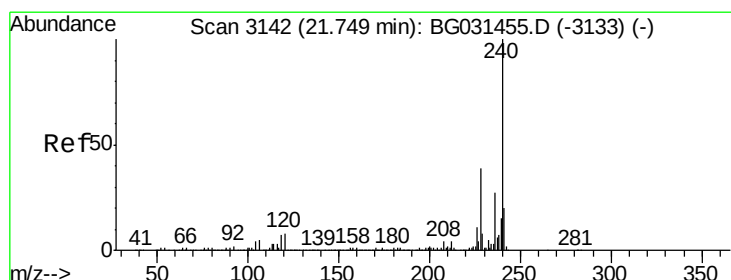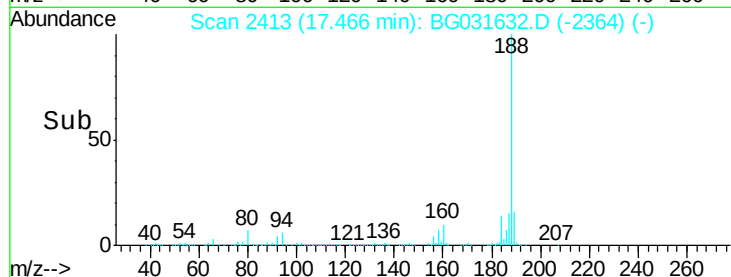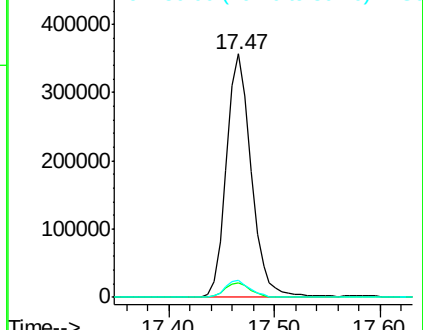

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.74 min Scan# 3140

Delta R.T. -0.01 min

Lab File: BG031632.D

Acq: 18 Dec 2017 13:25


Tgt Ion:240 Resp: 621321

Ion Ratio Lower Upper

240 100

120 7.3 6.8 10.2



236 27.3 20.9 31.3

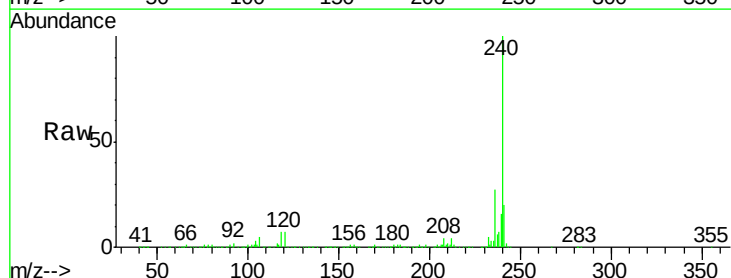


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

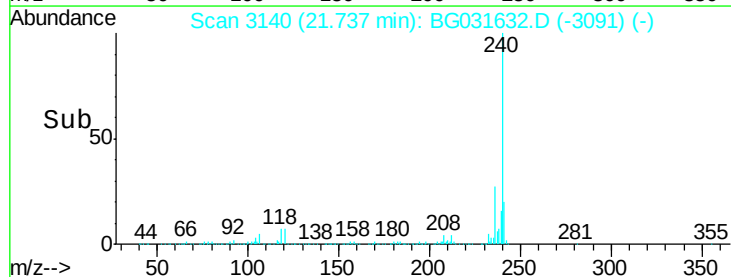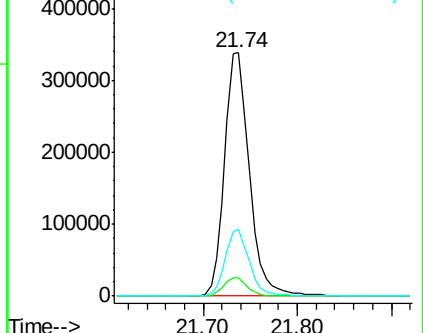

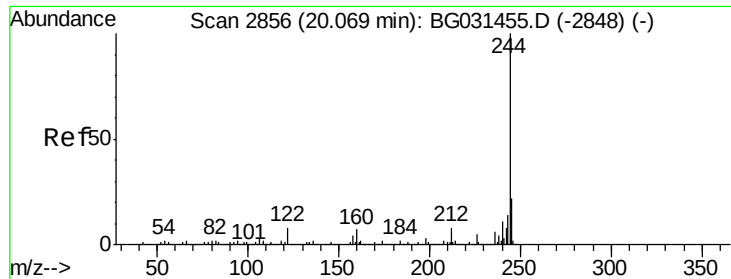

#78

Terphenyl-d14

Concen: 84.610 ng

RT: 20.06 min Scan# 2854

Delta R.T. -0.01 min

Lab File: BG031632.D

Acq: 18 Dec 2017 13:25

Instrument :

BNA\_G

ClientSampleId :


Tot Ion:244 Resp: 2310600

Ion Ratio Lower Upper

244 100

212 8.9 5.8 8.8#




122 8.7 7.0 10.4

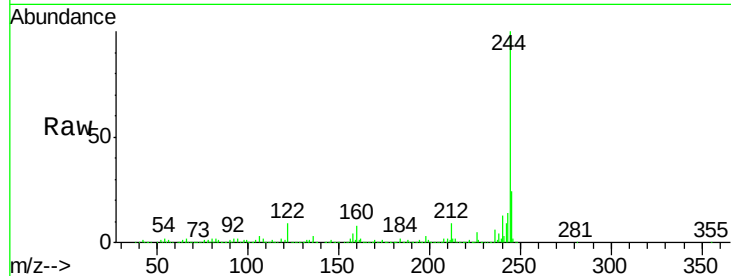

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

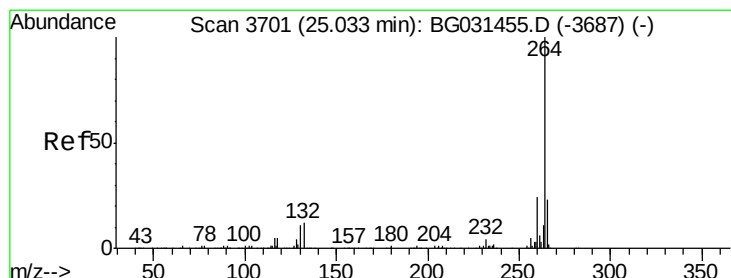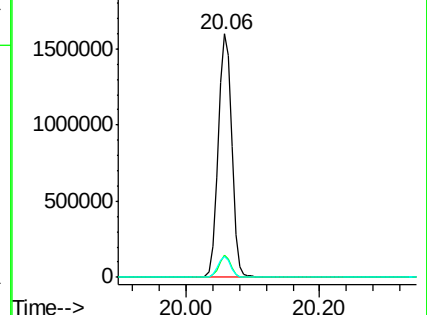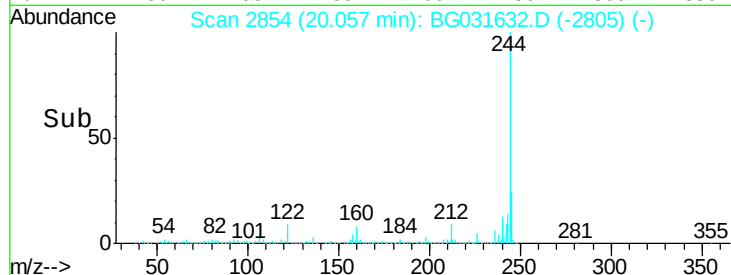

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.01 min Scan# 3697

Delta R.T. -0.02 min

Lab File: BG031632.D

Acq: 18 Dec 2017 13:25


Tgt Ion:264 Resp: 527979

Ion Ratio Lower Upper

264 100

260 24.3 17.4 26.0

265 21.6 17.7 26.5

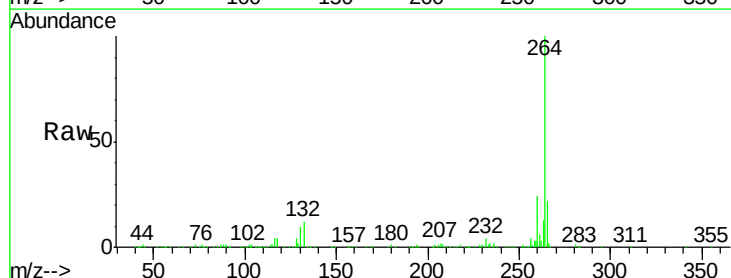

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

