
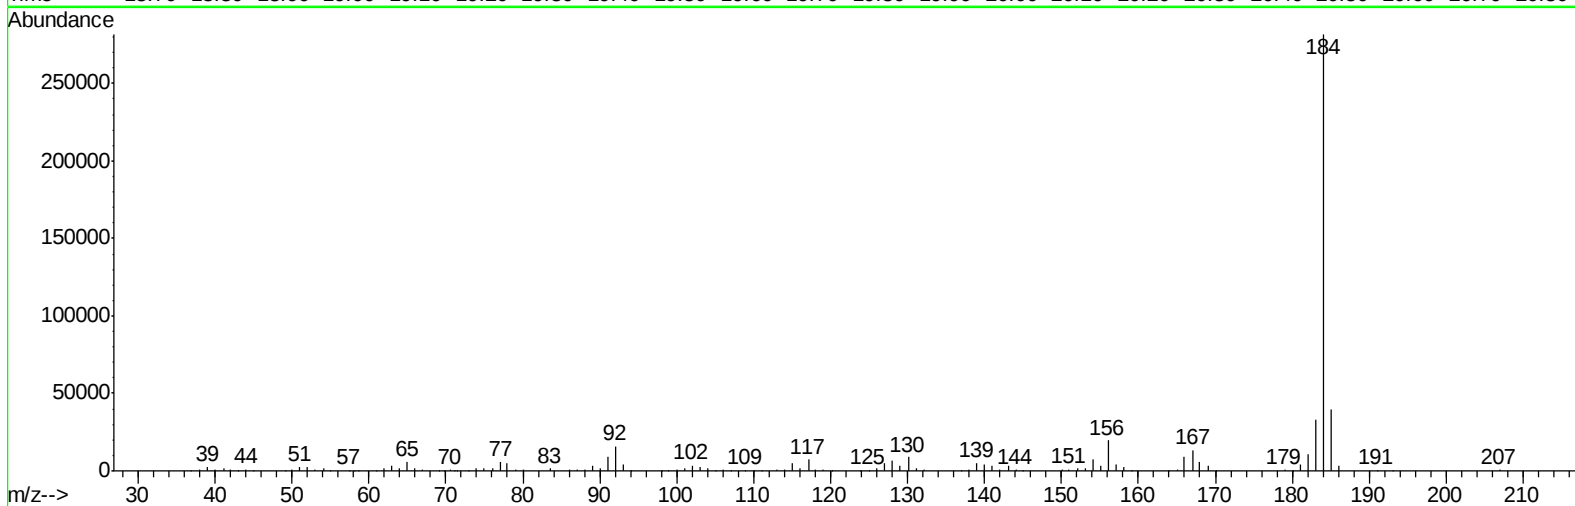


Data Path : Z:\HPCHEM1\BNA G\DATA\BG121817\
Data File : BG031626.D
Acq On : 18 Dec 2017 9:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 08:33:31 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

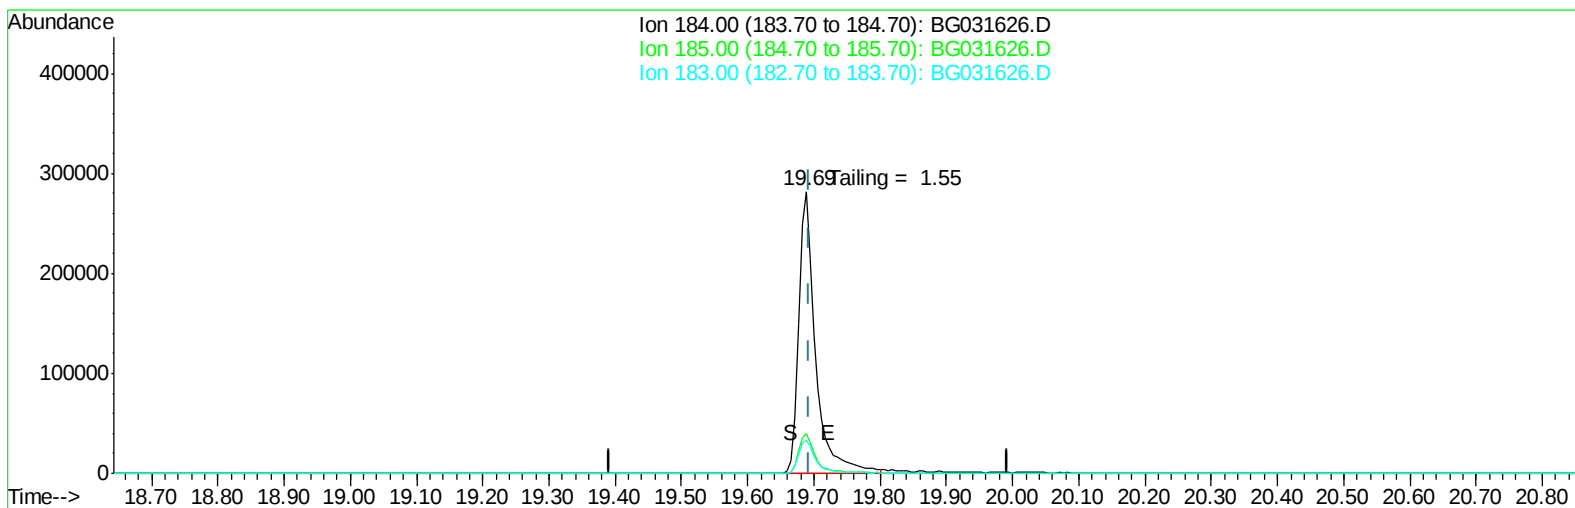

TIC: BG031626.D

(76) Benzidine



19.689min (-0.004) 0.00ng

response 509526

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.98
183.00	13.30	11.82
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121817\
Data File : BG031626.D
Acq On : 18 Dec 2017 9:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 08:33:31 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

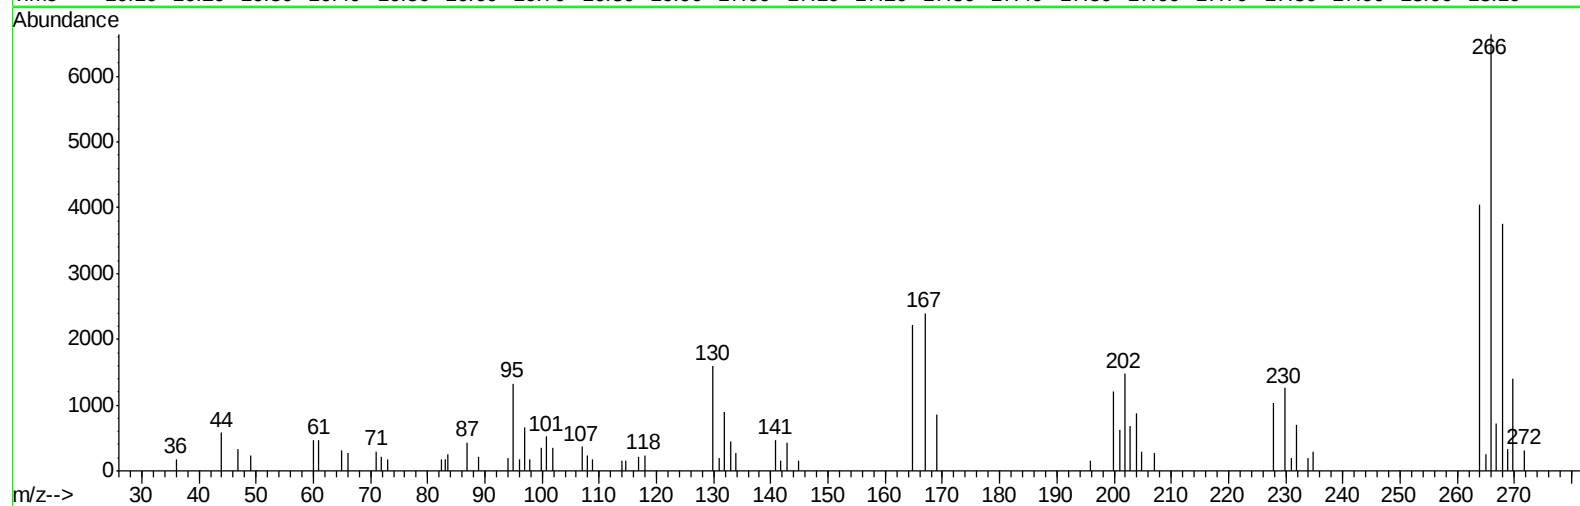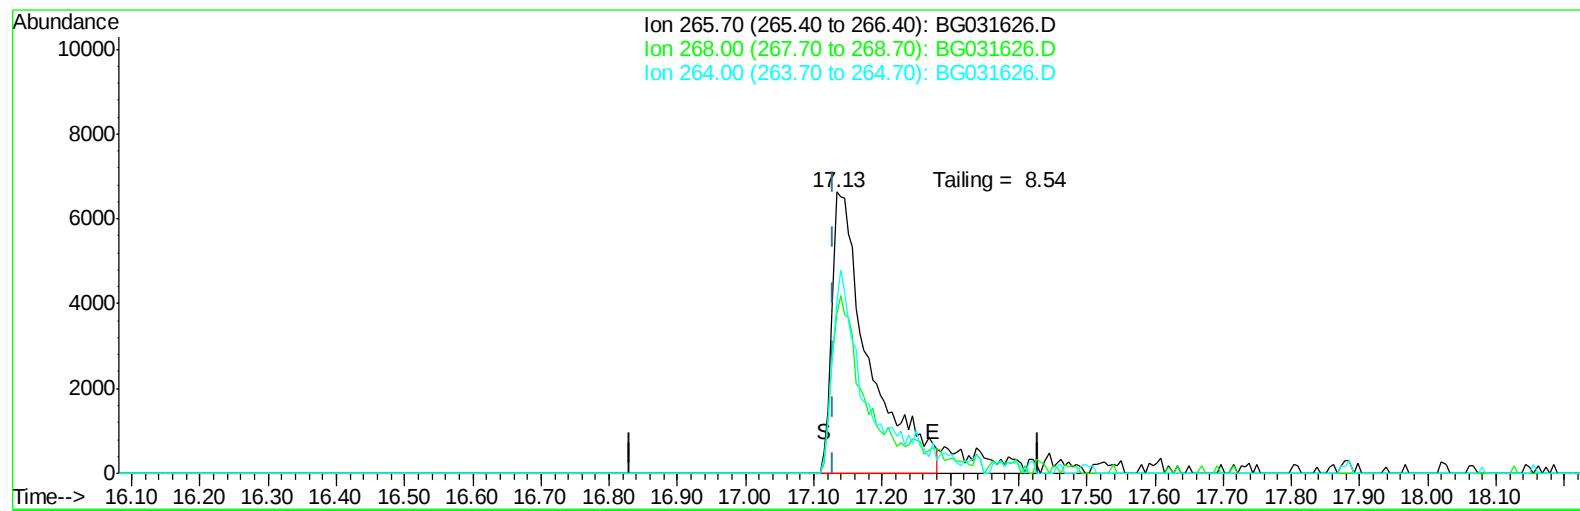

TIC: BG031626.D

(69) Pentachlorophenol (C)

17.133min (+0.003) 0.00ng

response 21931

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	56.75
264.00	62.00	61.12
0.00	0.00	0.00