
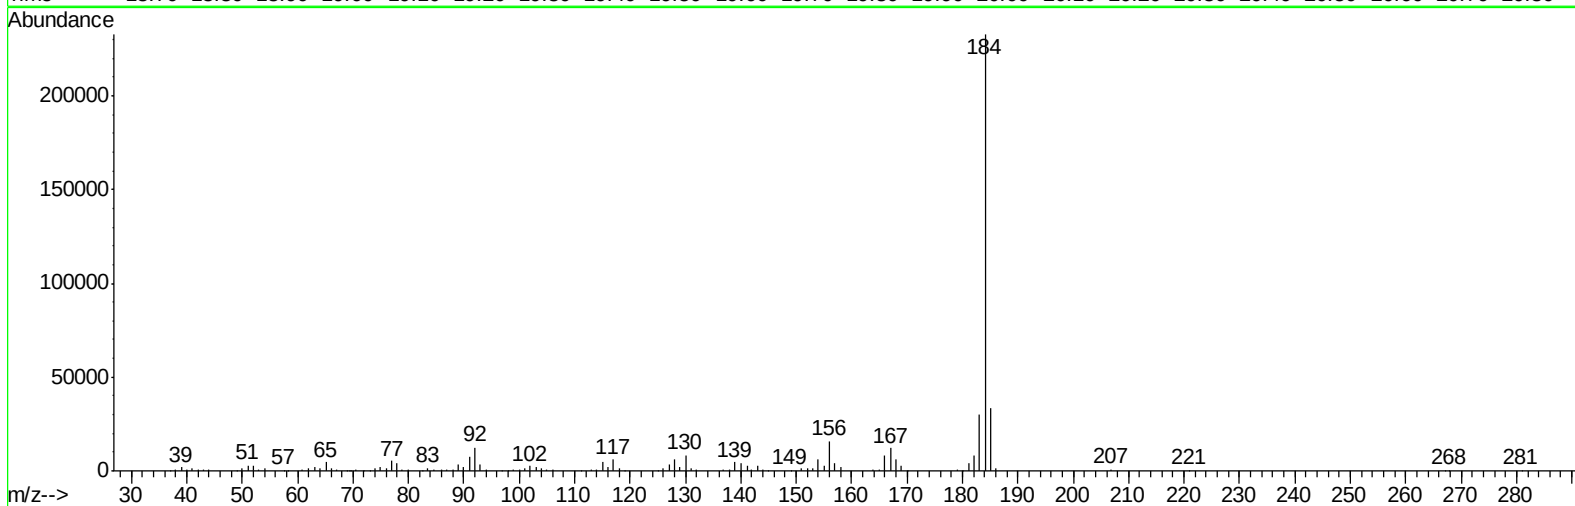


Data Path : Z:\HPCHEM1\BNA G\DATA\BG121817\
Data File : BG031636.D
Acq On : 18 Dec 2017 16:27
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 08:34:53 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

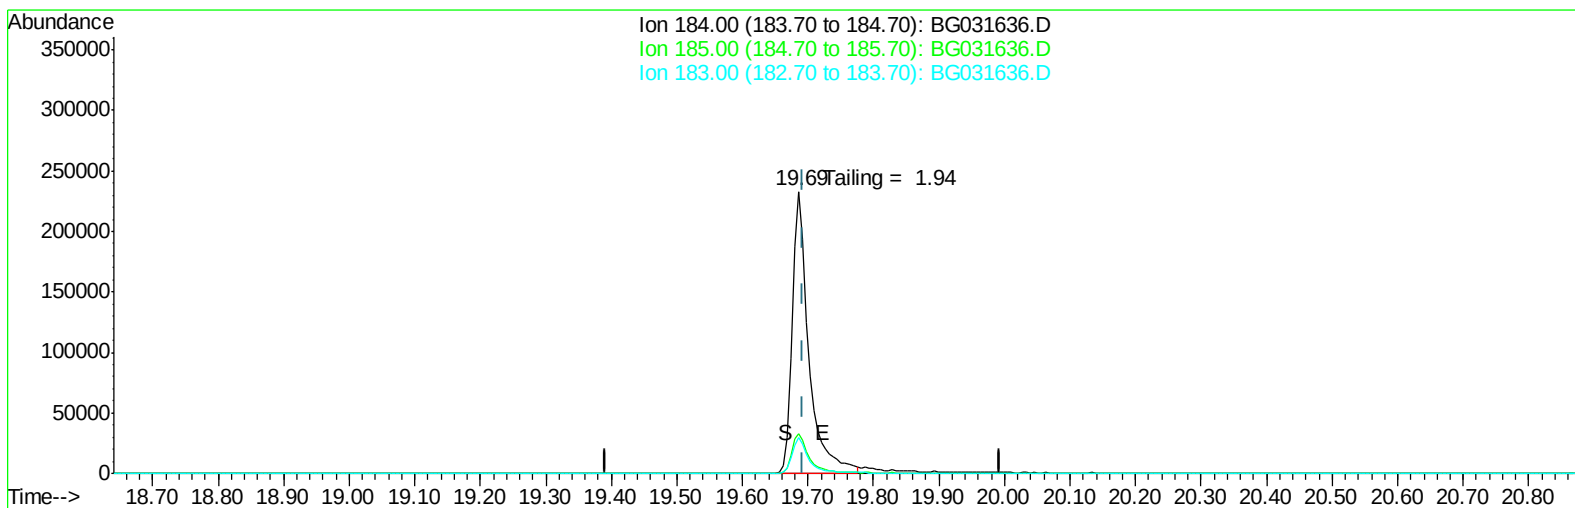

TIC: BG031636.D

(76) Benzidine



19.687min (-0.006) 338766.62ng

response 425723

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.31
183.00	13.30	12.86
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121817\
Data File : BG031636.D
Acq On : 18 Dec 2017 16:27
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 08:34:53 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

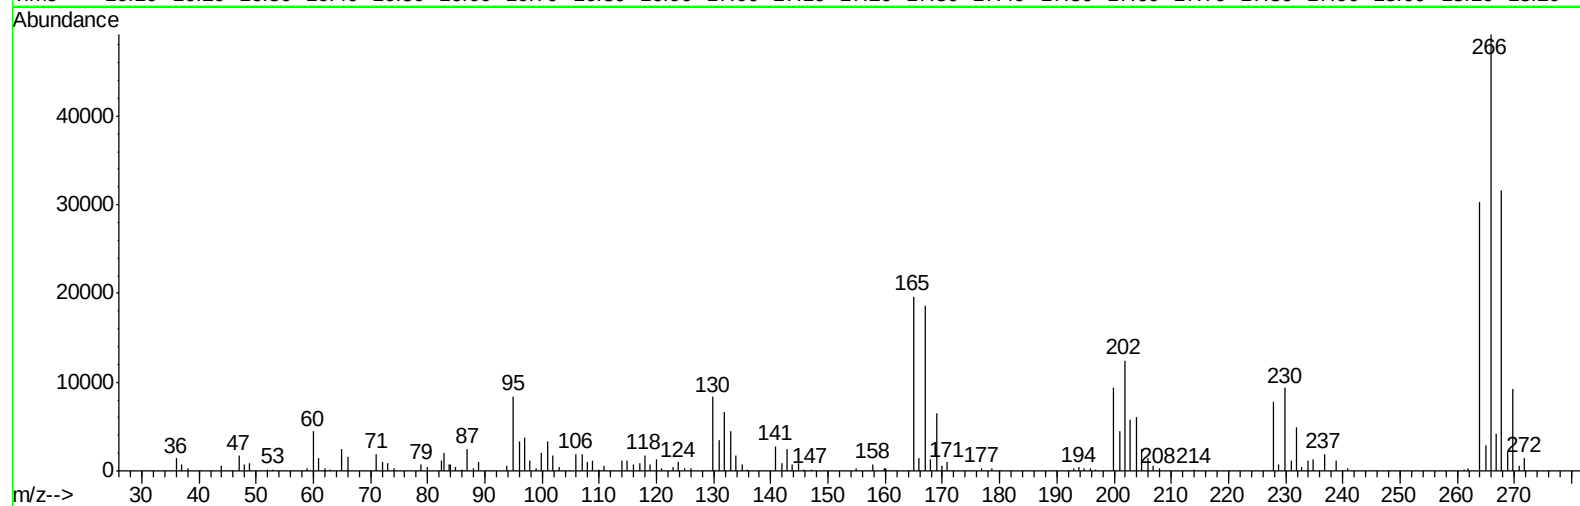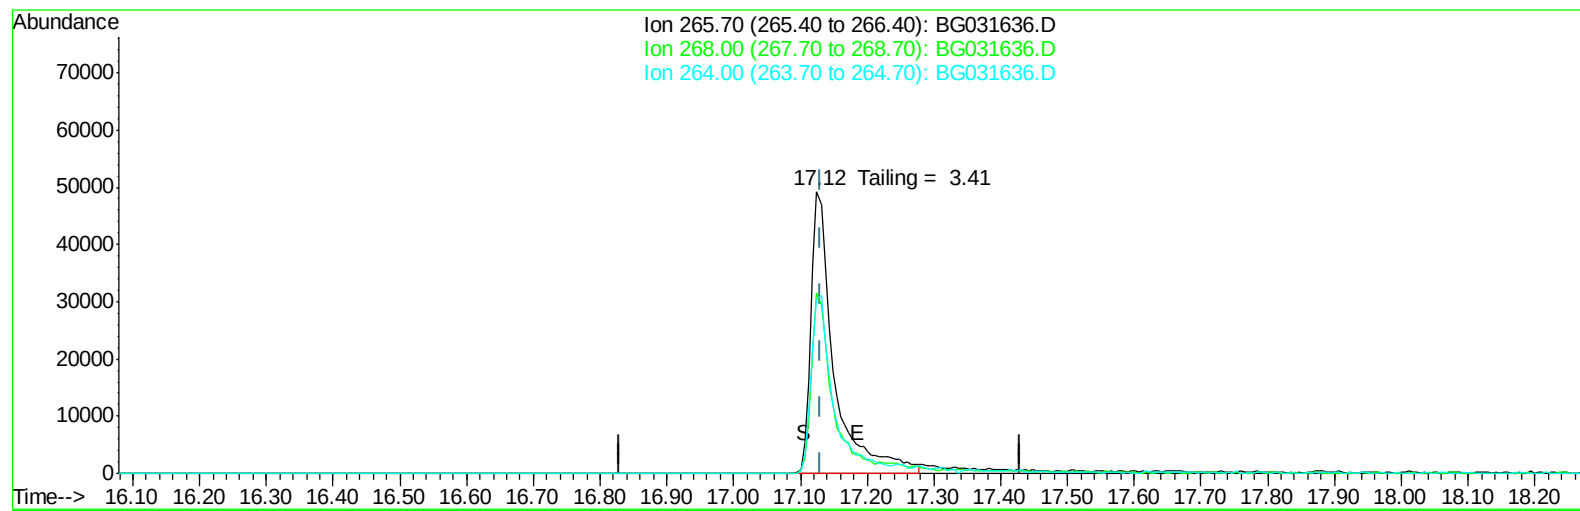

TIC: BG031636.D

(69) Pentachlorophenol (C)

17.125min (-0.005) 0.00ng

response 115453

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.27
264.00	62.00	61.74
0.00	0.00	0.00