


Data Path : Z:\HPCHEM1\BNA_G\Data\BG121817\
 Data File : BG031626.D
 Acq On : 18 Dec 2017 9:39
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG121117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 11 17:25:55 2017

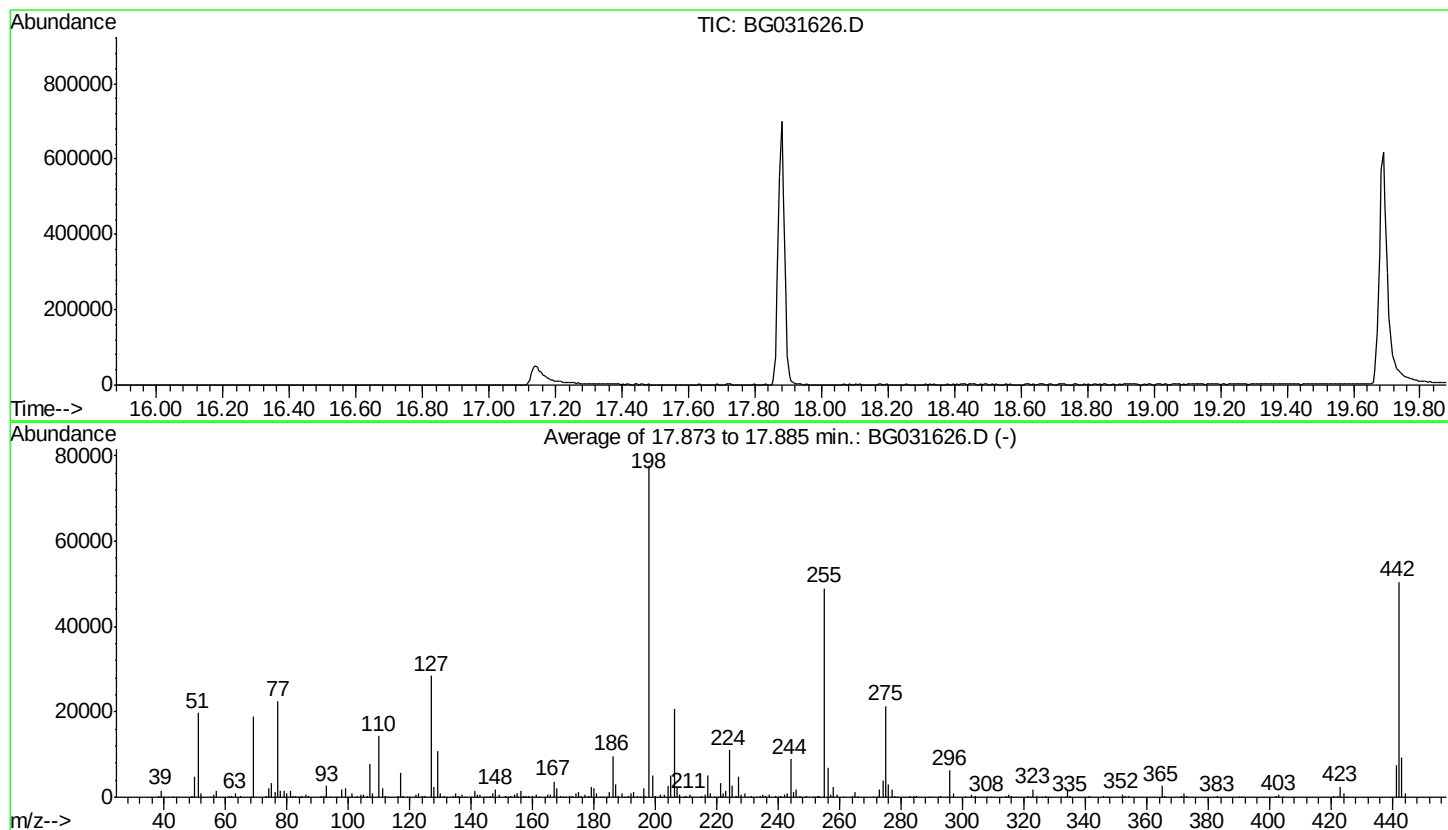

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	19675	PASS
68	69	0.00	2	0.8	156	PASS
69	198	0.00	100	24.5	18994	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.6	28424	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	77664	PASS
199	198	5	9	6.7	5188	PASS
275	198	10	60	27.6	21408	PASS
365	198	1	100	3.3	2577	PASS
441	442	0.01	24	15.2	7650	PASS
442	198	50	100	65.0	50453	PASS
443	442	15	24	18.3	9226	PASS