
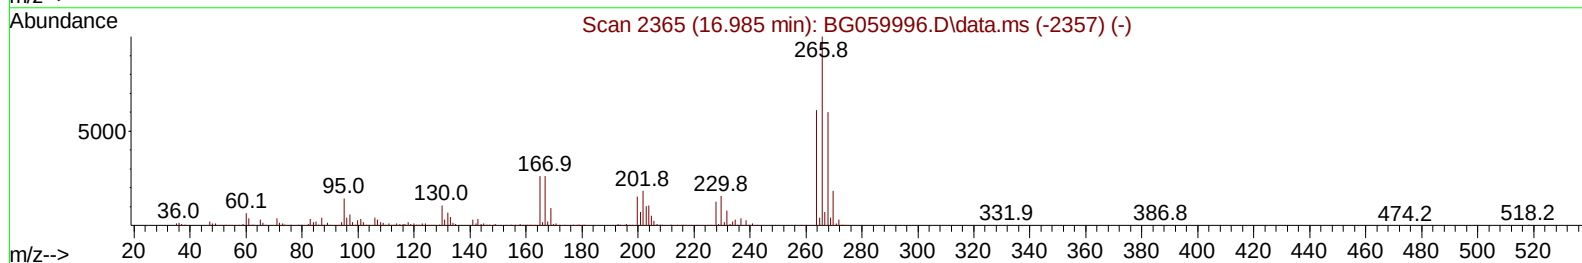
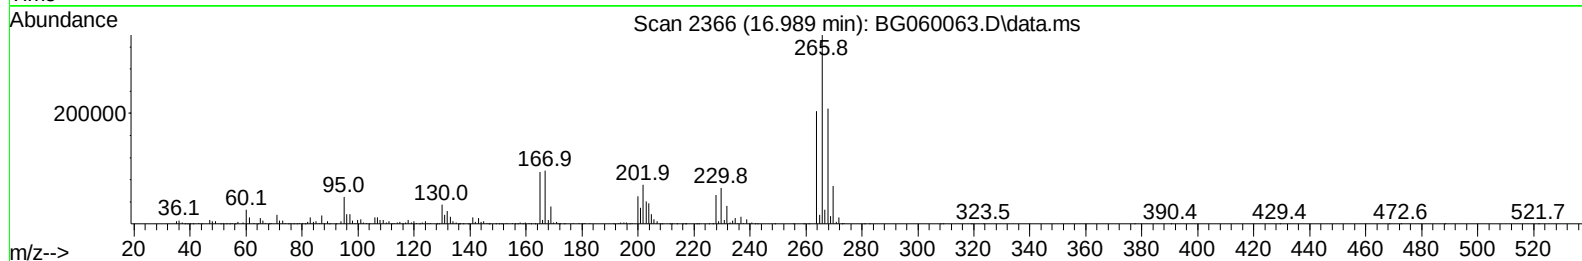


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121823\
Data File : BG060063.D
Acq On : 18 Dec 2023 12:42
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 04:34:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

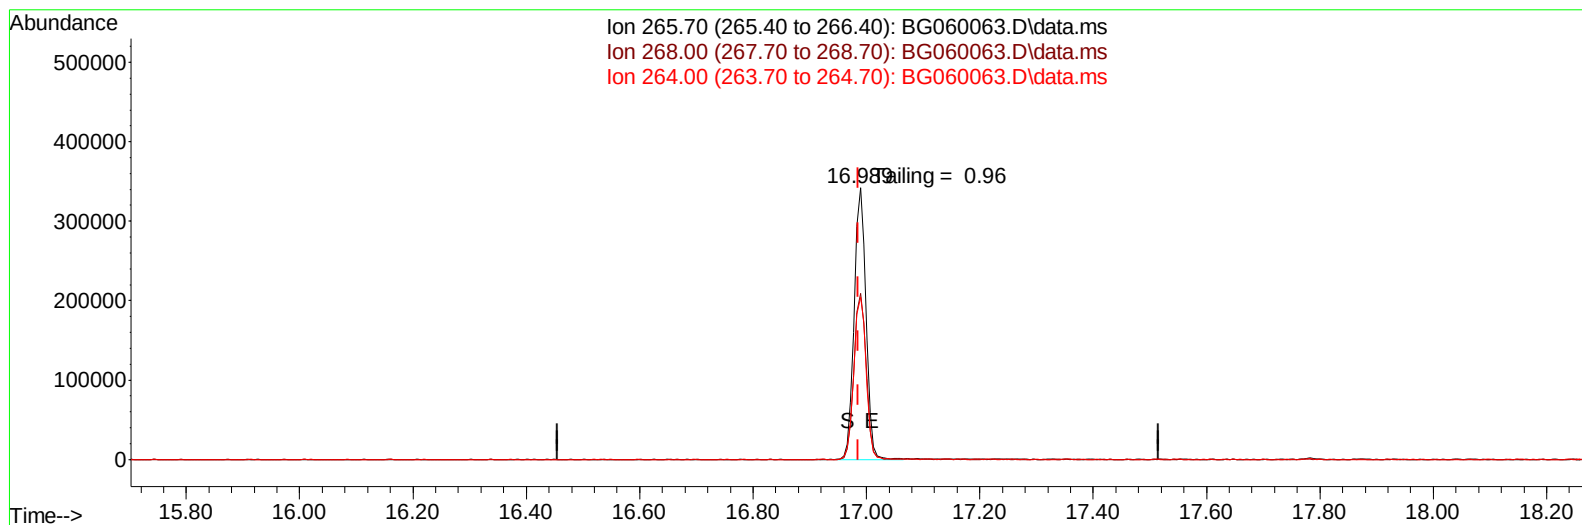

TIC: BG060063.D\data.ms

(70) Pentachlorophenol (C)




16.989min (+ 0.004) 502138.03 ng

response 493623

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	61.15
264.00	61.00	59.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121823\
Data File : BG060063.D
Acq On : 18 Dec 2023 12:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 04:34:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

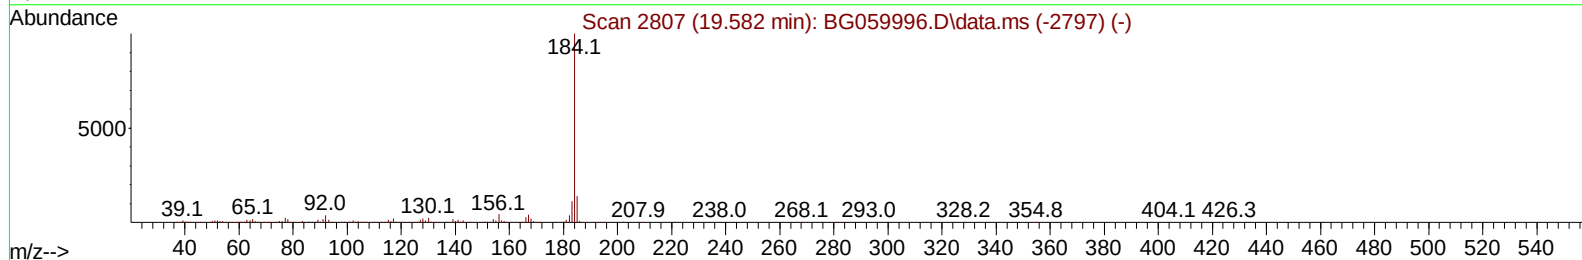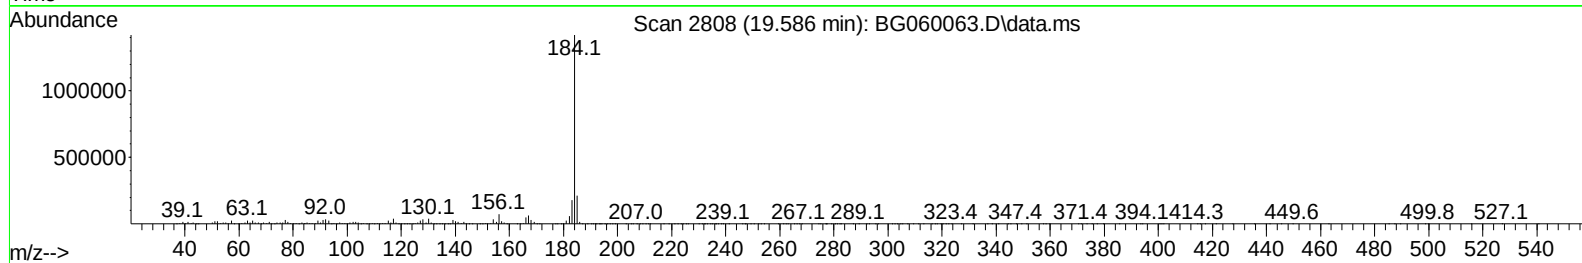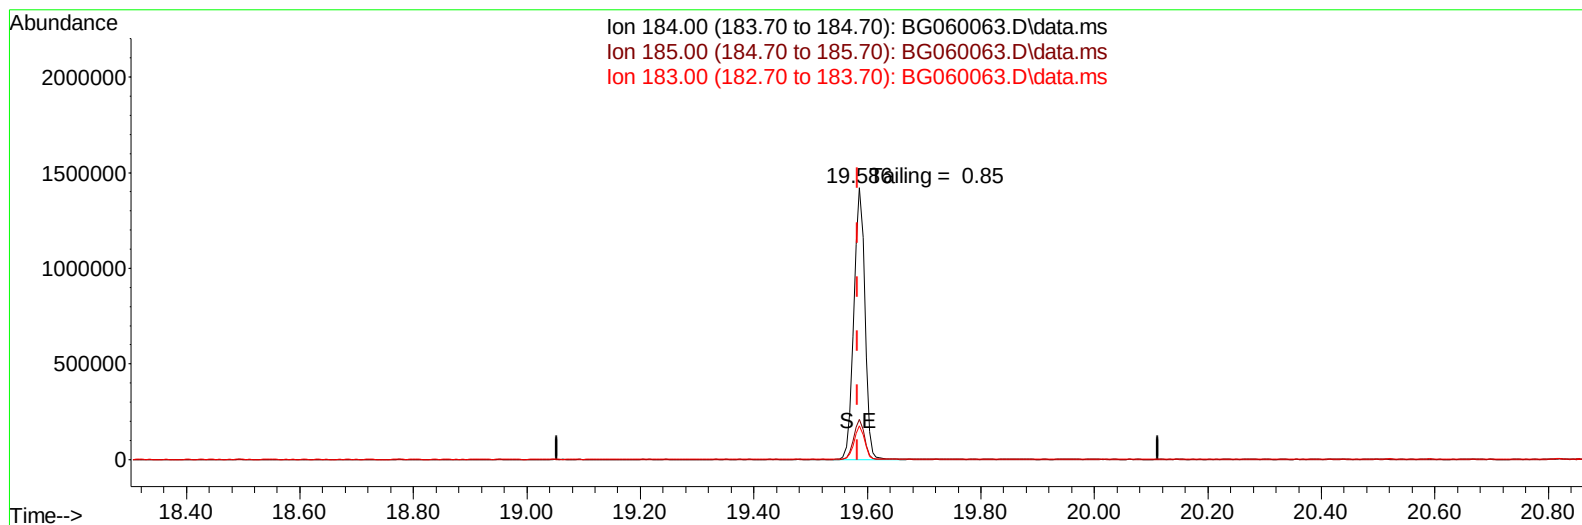

TIC: BG060063.D\data.ms

(77) Benzidine**19.586min (+ 0.004) 71181.74 ng****response 1915478**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.87
183.00	11.20	12.46
0.00	0.00	0.00