


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121823\
Data File : BG060063.D
Acq On : 18 Dec 2023 12:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Dec 19 04:37:23 2023

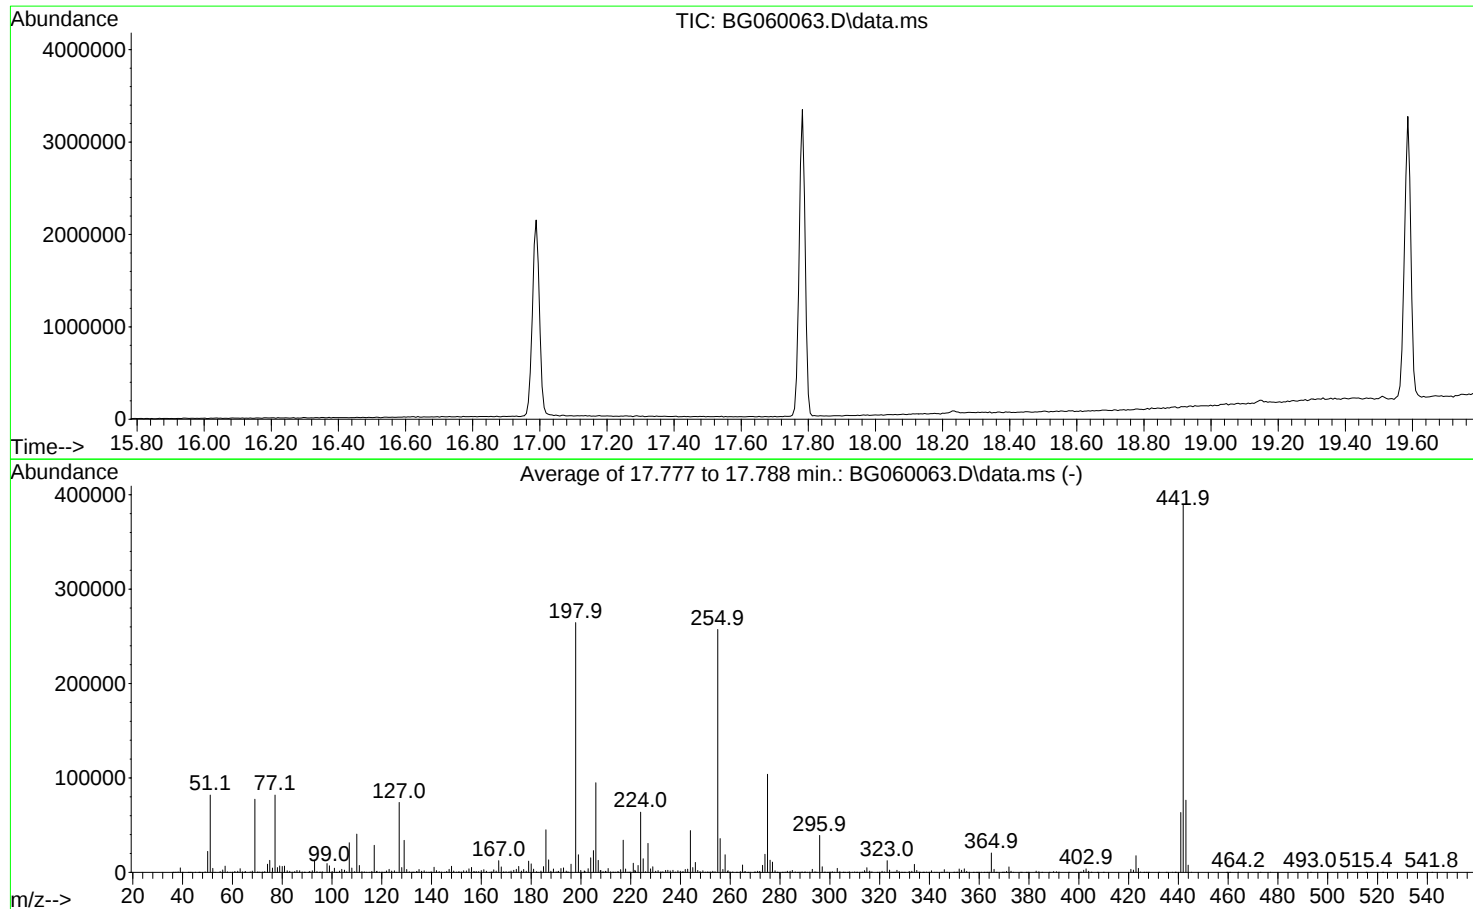




AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	81893	PASS
68	69	0.00	2	1.8	1428	PASS
69	198	0.00	100	29.3	77438	PASS
70	69	0.00	2	0.5	390	PASS
127	198	10	80	28.0	74016	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	264555	PASS
199	198	5	9	7.0	18642	PASS
275	198	10	60	39.2	103816	PASS
365	198	1	100	7.8	20536	PASS
441	198	0.01	100	24.0	63477	PASS
442	442	50	100	100.0	389632	PASS
443	442	15	24	19.6	76421	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121823\
 Data File : BG060063.D
 Acq On : 18 Dec 2023 12:42
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Dec 19 04:34:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 14 01:47:12 2023
 Response via : Initial Calibration

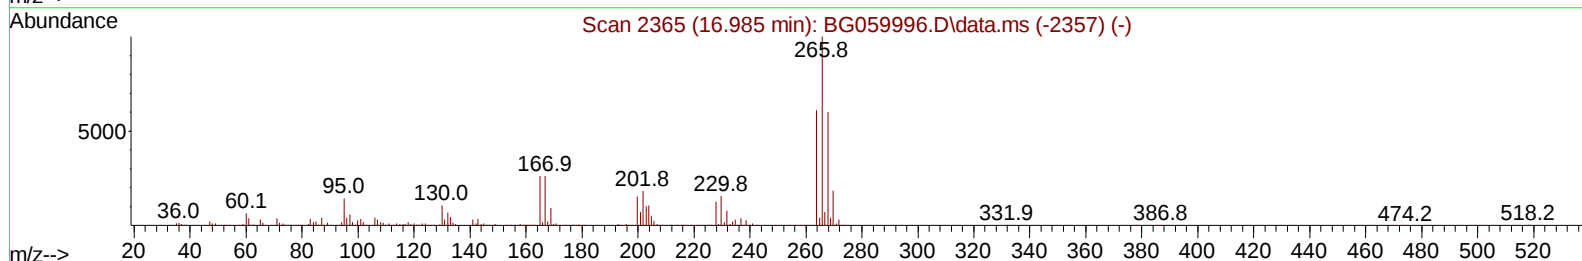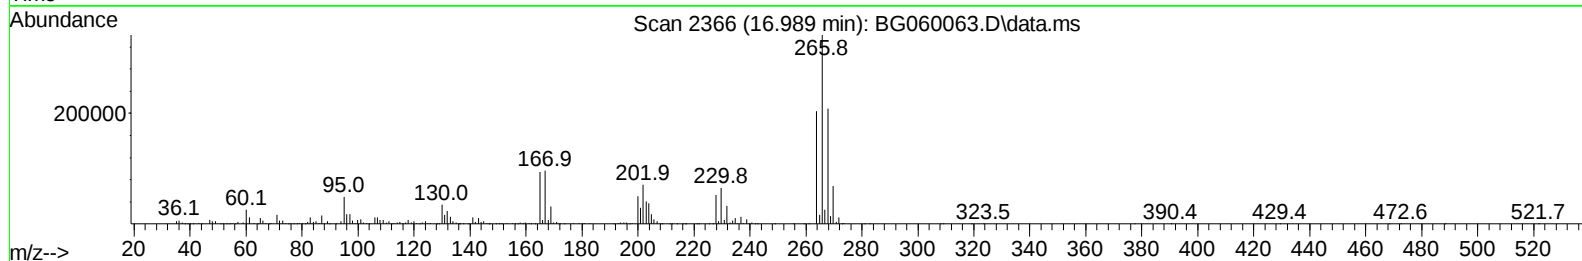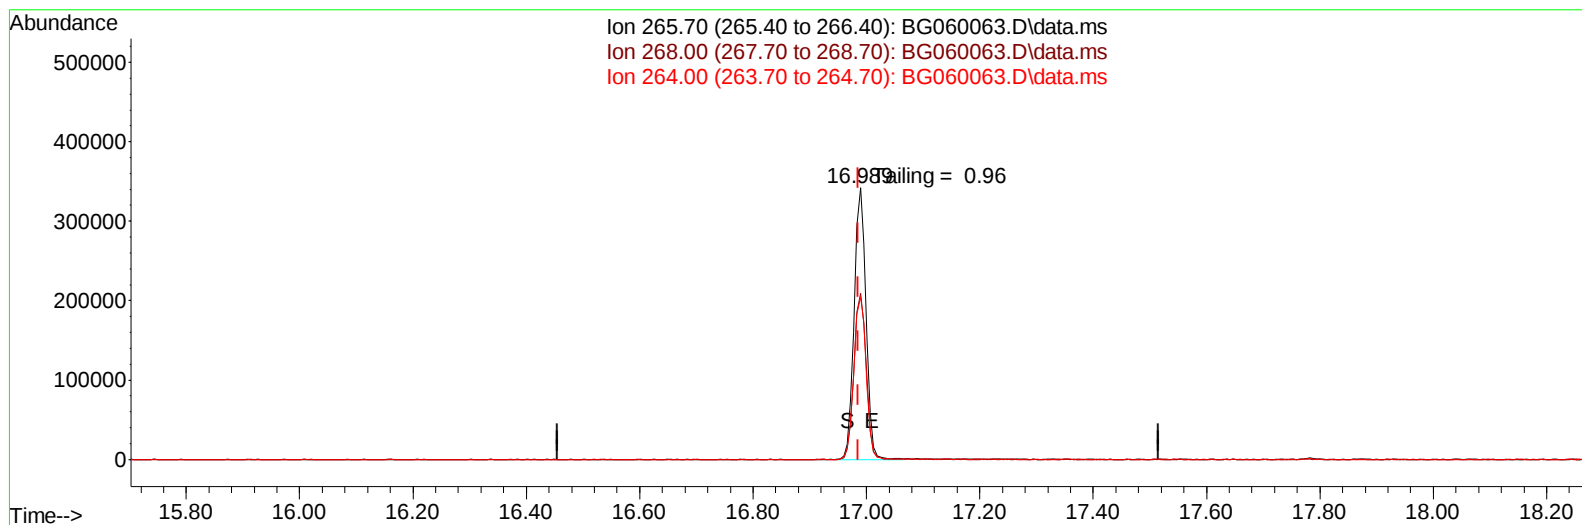

TIC: BG060063.D\data.ms

(70) Pentachlorophenol (C)

16.989min (+ 0.004) 502138.03 ng




response 493623

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	61.15
264.00	61.00	59.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121823\
Data File : BG060063.D
Acq On : 18 Dec 2023 12:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 19 04:34:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

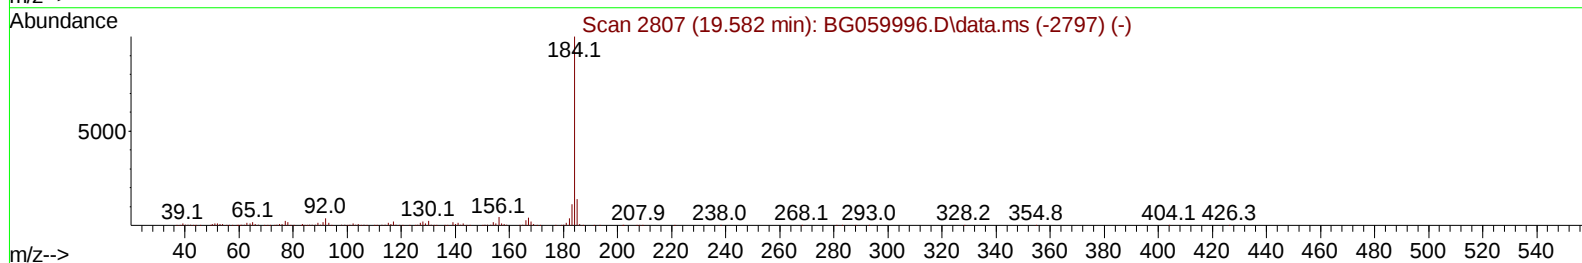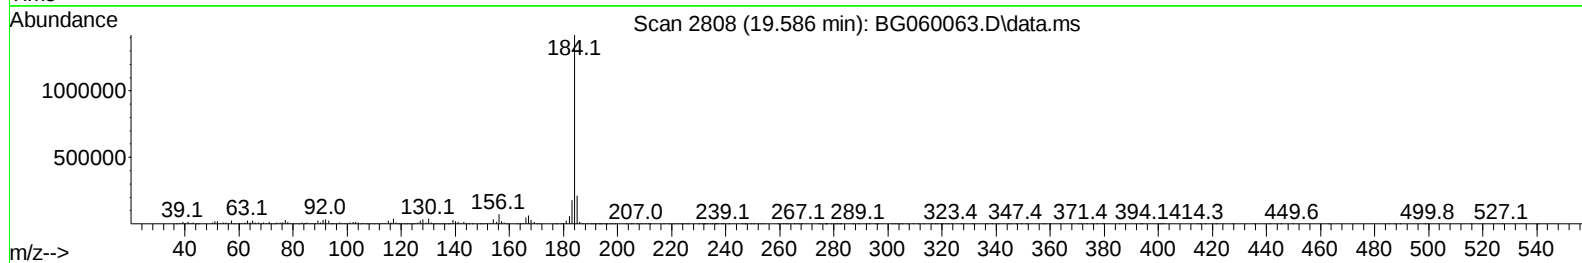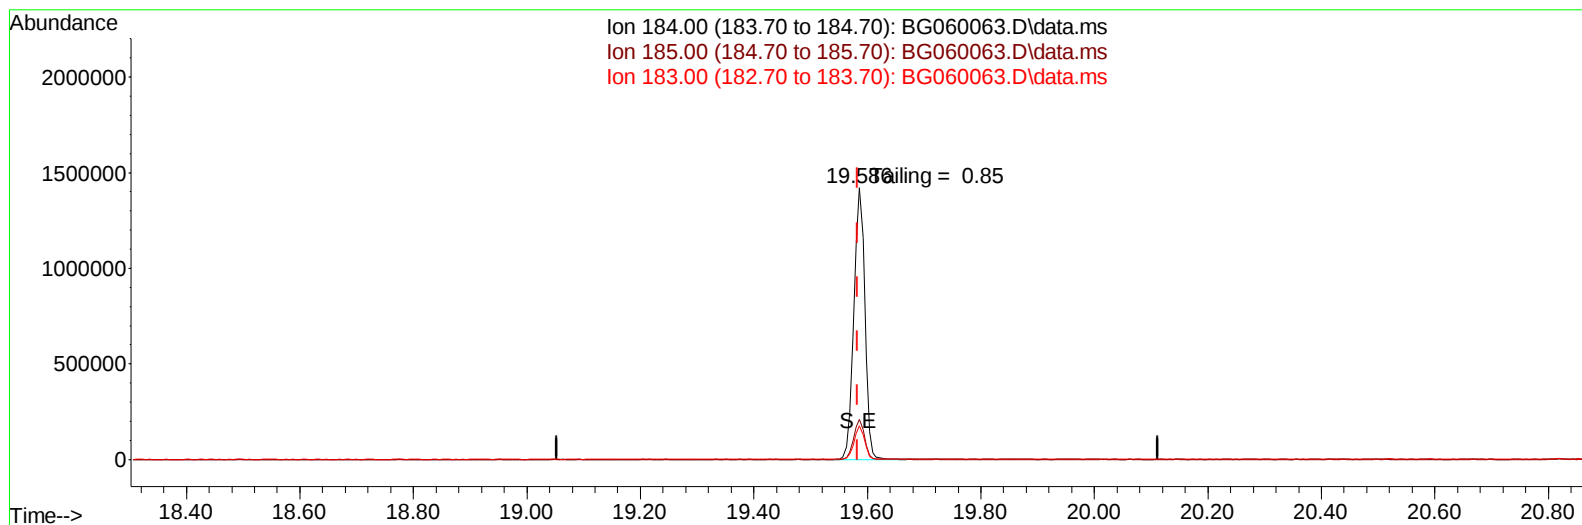

TIC: BG060063.D\data.ms

(77) Benzidine

19.586min (+ 0.004) 71181.74 ng

response 1915478

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.87
183.00	11.20	12.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/18/2023	BNA_G	<u>BG060063.D</u>
Compound Name	Response	Retention Time
DDT	980461	20.82
DDD	31092	20.373
DDE	0	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31092	1011553	3.07

Instrument :
BNA_G
ClientSampleId :
DFTPP