

Data Path : Z:\HPCHEM1\BNA_G\Data\BG121915\
 Data File : BG020268.D
 Acq On : 18 Dec 2015 10:24
 Operator : UM/SJ
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD02004

Quant Time: Dec 18 23:40:06 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 18 02:40:02 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	17033	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	74447	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.72	164	54477	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	144475	20.00	ng/ul	0.00
78) Chrysene-d12	21.75	240	182631	20.00	ng/ul	0.00
86) Perylene-d12	25.02	264	168755	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.47	96	2345	7.60	ng/uL	0.00
5) Phenol-d5	7.24	99	29520	19.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.42	67	18512	20.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.62	132	23745	21.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	25933	20.19	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	12373	21.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	14362	22.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	28483	21.78	ng/ul	0.00
29) 4-Chloroaniline-d4	11.04	131	34011	23.15	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	94868	21.53	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	109655	21.39	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	16172	20.46	ng/ul	0.00
58) Fluorene-d10	15.72	176	86693	21.69	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	15950	18.62	ng/ul	0.00
71) Anthracene-d10	17.57	188	140729	21.14	ng/ul	0.00
79) Pyrene-d10	19.85	212	166220	19.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	183483	21.80	ng/ul	0.00

Target Compounds

					Qvalue
2) 1,4-Dioxane	3.50	88	3113	6.83 ng/uL	94
4) Benzaldehyde	7.23	77	20749	21.34 ng/ul	98
6) Phenol	7.27	94	32455	20.18 ng/ul	95
8) Bis(2-Chloroethyl)ether	7.50	93	23360	21.17 ng/ul	98
10) 2-Chlorophenol	7.66	128	24178	21.13 ng/ul	95
11) 2-Methylphenol	8.53	108	24900	20.29 ng/ul	97
12) 2,2'-oxybis(1-Chloropropan	8.63	45	31335	19.71 ng/ul#	96
14) Acetophenone	8.92	105	42259	21.01 ng/ul	98
15) N-Nitroso-di-n-propylamine	8.90	70	22023	20.68 ng/ul	94
16) 4-Methylphenol	8.85	108	27596	20.32 ng/ul	98
17) Hexachloroethane	9.18	117	9924	20.64 ng/ul	95
20) Nitrobenzene	9.30	77	31755	20.65 ng/ul	99
21) Isophorone	9.82	82	60516	20.61 ng/ul	99
23) 2-Nitrophenol	10.01	139	15228	21.99 ng/ul	96
24) 2,4-Dimethylphenol	10.07	107	33431	21.26 ng/ul	95
25) Bis(2-Chloroethoxy)methane	10.31	93	33905	21.32 ng/ul#	96
27) 2,4-Dichlorophenol	10.55	162	28850	21.47 ng/ul	95
28) Naphthalene	10.96	128	85562	22.01 ng/ul	99
30) 4-Chloroaniline	11.06	127	34153	22.77 ng/ul	99
31) Hexachlorobutadiene	11.24	225	22388	22.35 ng/ul	95
32) Caprolactam	11.82	113	9720	20.50 ng/ul	95
33) 4-Chloro-3-methylphenol	12.18	107	31990	20.04 ng/ul	89
34) 2-Methylnaphthalene	12.56	142	64881	21.85 ng/ul	95

Data Path : Z:\HPCHEM1\BNA_G\Data\BG121915\
 Data File : BG020268.D
 Acq On : 18 Dec 2015 10:24
 Operator : UM/SJ
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleID :
 SSTD02004

Quant Time: Dec 18 23:40:06 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 18 02:40:02 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	12.78	142	61499	21.54	ng/ul	94
37) 1,2,4,5-Tetrachlorobenzene	12.93	216	44670	21.85	ng/ul	97
38) Hexachlorocyclopentadiene	12.90	237	18269	14.46	ng/ul	97
39) 2,4,6-Trichlorophenol	13.16	196	27777	21.18	ng/ul	97
40) 2,4,5-Trichlorophenol	13.23	196	31205	21.41	ng/ul	99
41) 1,1'-Biphenyl	13.56	154	88886	21.63	ng/ul	95
42) 2-Chloronaphthalene	13.61	162	70868	21.54	ng/ul	98
43) 2-Nitroaniline	13.81	65	22345	19.97	ng/ul	88
45) Dimethylphthalate	14.17	163	95675	21.26	ng/ul	98
46) 2,6-Dinitrotoluene	14.30	165	19977	21.46	ng/ul	96
48) Acenaphthylene	14.45	152	117532	21.58	ng/ul	98
49) 3-Nitroaniline	14.62	138	20246	22.40	ng/ul	85
50) Acenaphthene	14.79	153	78995	21.56	ng/ul	98
51) 2,4-Dinitrophenol	14.83	184	8719	16.46	ng/ul	91
53) 4-Nitrophenol	14.93	109	15298	20.12	ng/ul	94
54) Dibenzofuran	15.12	168	117626	21.58	ng/ul	99
55) 2,4-Dinitrotoluene	15.08	165	29609	21.67	ng/ul	93
56) 2,3,4,6-Tetrachlorophenol	15.35	232	29862	21.31	ng/ul	98
57) Diethylphthalate	15.53	149	100349	21.49	ng/ul	98
59) Fluorene	15.77	166	95360	21.78	ng/ul	97
60) 4-Chlorophenyl-phenylether	15.76	204	54094	21.91	ng/ul	95
61) 4-Nitroaniline	15.79	138	21823	22.34	ng/ul	99
64) 4,6-Dinitro-2-methylphenol	15.85	198	17256	18.77	ng/ul	93
65) N-Nitrosodiphenylamine	15.98	169	85366	21.25	ng/ul	98
66) 4-Bromophenyl-phenylether	16.66	248	37160	21.92	ng/ul	96
67) Hexachlorobenzene	16.77	284	40115	22.03	ng/ul#	88
68) Atrazine	16.92	200	37038	21.62	ng/ul	96
69) Pentachlorophenol	17.12	266	17540	15.97	ng/ul	94
70) Phenanthrene	17.52	178	168803	21.36	ng/ul	99
72) Anthracene	17.60	178	171842	21.44	ng/ul	99
73) 1,2,3,4-Tetrachlorobenzene	13.53	216	47773	21.11	ng/uL	95
74) Pentachlorobenzene	15.04	250	46241	22.03	ng/uL	96
75) Carbazole	17.87	167	148582	22.06	ng/ul	99
76) Di-n-butylphthalate	18.42	149	173798	22.21	ng/ul	100
77) Fluoranthene	19.52	202	215818	23.37	ng/ul	99
80) Pyrene	19.88	202	220212	19.92	ng/ul	98
81) Butylbenzylphthalate	20.76	149	79252	20.63	ng/ul	90
82) 3,3'-Dichlorobenzidine	21.64	252	75780	22.71	ng/ul	95
83) Benzo(a)anthracene	21.73	228	227770	21.37	ng/ul	99
84) Bis(2-ethylhexyl)phthalate	21.62	149	112779	20.54	ng/ul	99
85) Chrysene	21.79	228	213654	21.29	ng/ul	99
87) Di-n-octyl phthalate	22.84	149	190598	20.56	ng/ul	100
88) Benzo(b)fluoranthene	23.98	252	211980	20.87	ng/ul	97
89) Benzo(k)fluoranthene	24.04	252	208808	21.42	ng/ul	97
91) Benzo(a)pyrene	24.87	252	211732	21.99	ng/ul	100
92) Indeno(1,2,3-cd)pyrene	28.75	276	231688	20.21	ng/ul	96
93) Dibenzo(a,h)anthracene	28.81	278	194699	20.46	ng/ul	96
94) Benzo(g,h,i)perylene	29.92	276	172816	18.39	ng/ul	97


Data Path : Z:\HPCHEM1\BNA_G\Data\BG121915\
Data File : BG020268.D
Acq On : 18 Dec 2015 10:24
Operator : UM/SJ
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD02004

Quant Time: Dec 18 23:40:06 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 18 02:40:02 2015
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						

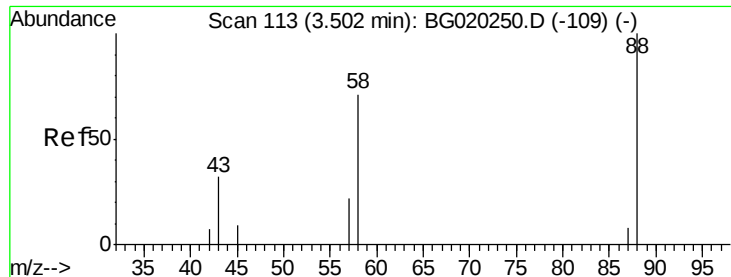

#2

1,4-Dioxane

Concen: 6.83 ng/uL

RT: 3.50 min Scan# 113

Delta R.T. 0.00 min

Lab File: BG020268.D

Acq: 18 Dec 2015 10:24

Instrument :

BNA_G

ClientSampleId :

SSTD02004


Tgt Ion: 88 Resp: 3113

Ion Ratio Lower Upper




88 100

43 41.2 27.8 41.8

58 71.2 59.9 89.9



Abundance Ion 88.00 (87.70 to 88.70): BGC
Ion 43.00 (42.70 to 43.70): BGC
Ion 58.00 (57.70 to 58.70): BGC

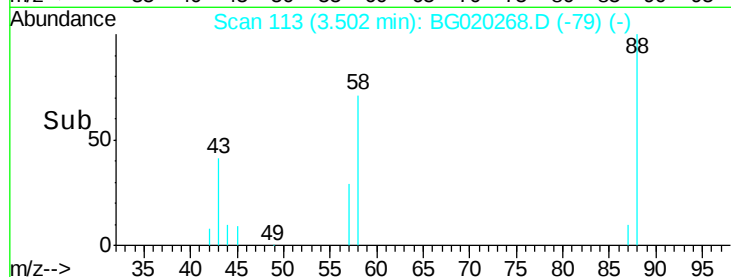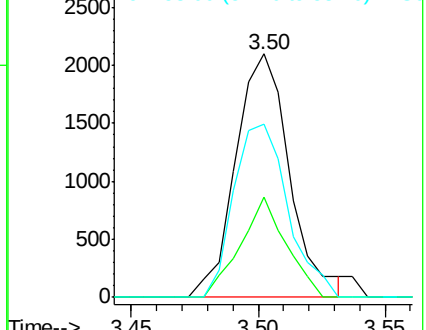

#4

Benzaldehyde

Concen: 21.34 ng/uL

RT: 7.23 min Scan# 747

Delta R.T. 0.00 min

Lab File: BG020268.D

Acq: 18 Dec 2015 10:24


Tgt Ion: 77 Resp: 20749

Ion Ratio Lower Upper



77 100


105 95.9 77.8 116.6

106 87.3 72.6 109.0



Abundance Ion 77.00 (76.70 to 77.70): BGC
Ion 105.00 (104.70 to 105.70): BGC
Ion 106.00 (105.70 to 106.70): BGC

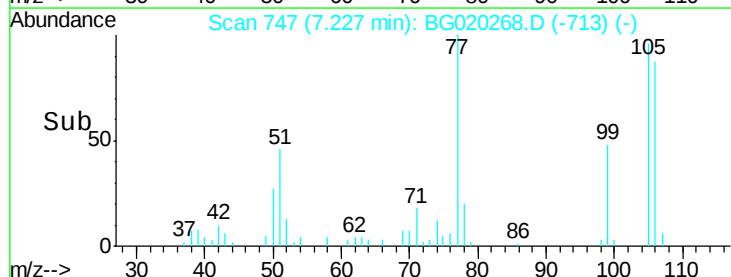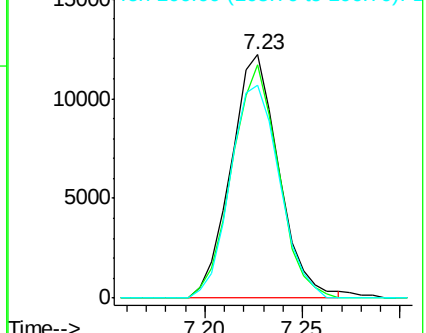

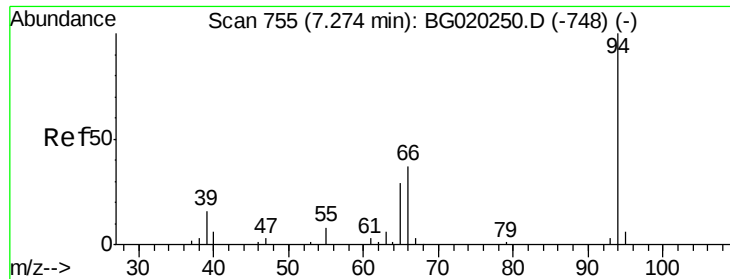

#6

Phenol

Concen: 20.18 ng/ul

RT: 7.27 min Scan# 754

Delta R.T. -0.01 min

Lab File: BG020268.D

Acq: 18 Dec 2015 10:24

Instrument :

BNA_G

ClientSampleId :

SSTD02004


Tgt Ion: 94 Resp: 32455

Ion Ratio Lower Upper




94 100

65 29.8 26.3 39.5

66 38.7 33.3 49.9

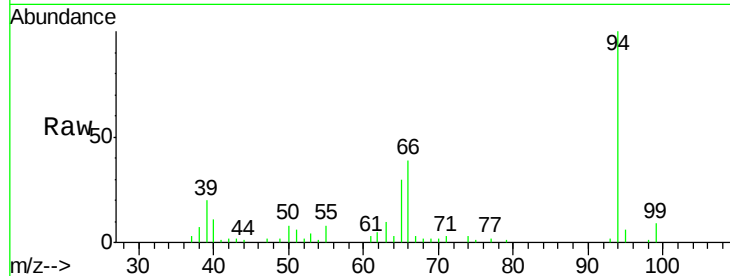

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

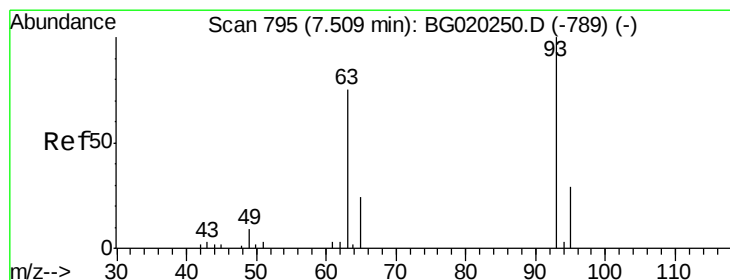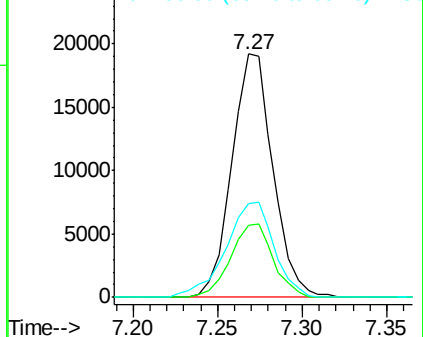

#8

Bis(2-Chloroethyl)ether

Concen: 21.17 ng/ul

RT: 7.50 min Scan# 794

Delta R.T. -0.01 min

Lab File: BG020268.D

Acq: 18 Dec 2015 10:24


Tgt Ion: 93 Resp: 23360

Ion Ratio Lower Upper



93 100


63 77.1 63.6 95.4

95 30.4 23.7 35.5

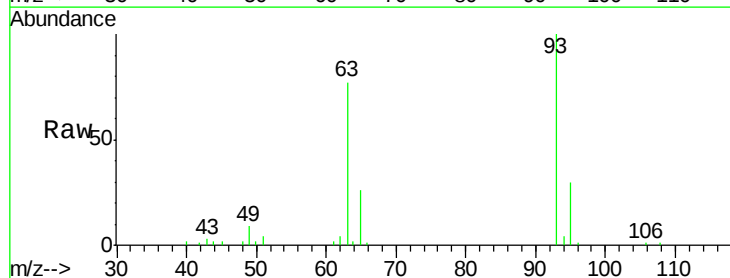

Abundance Ion 93.00 (92.70 to 93.70): BGC
Ion 63.00 (62.70 to 63.70): BGC
Ion 95.00 (94.70 to 95.70): BGC

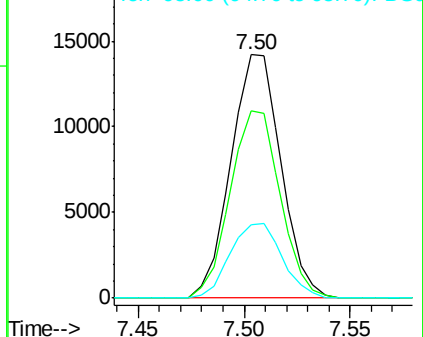







#10
2-Chlorophenol
Concen: 21.13 ng/ul
RT: 7.66 min Scan# 820
Delta R.T. 0.00 min
Lab File: BG020268.D
Acq: 18 Dec 2015 10:24

Instrument :
BNA_G
ClientSampleId :
SSTD02004

Tgt Ion:128 Resp: 24178
Ion Ratio Lower Upper
128 100
64 46.5 39.4 59.0
130 34.4 24.6 36.8

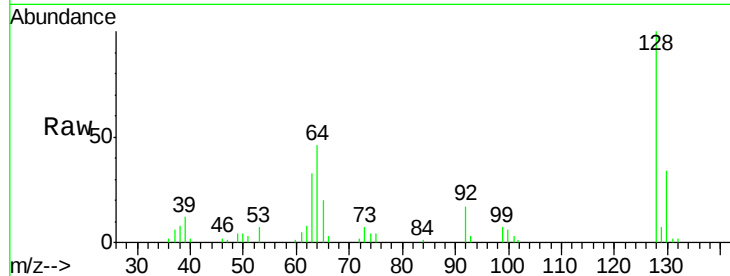


Abundance Ion 128.00 (127.70 to 128.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 130.00 (129.70 to 130.70): E

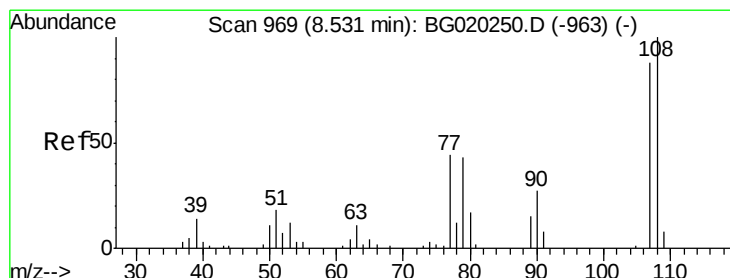
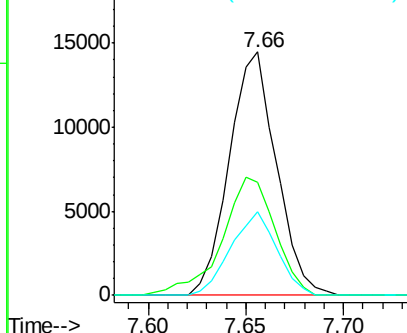



#11
2-Methylphenol
Concen: 20.29 ng/ul
RT: 8.53 min Scan# 969
Delta R.T. 0.00 min
Lab File: BG020268.D
Acq: 18 Dec 2015 10:24

Tgt Ion:108 Resp: 24900
Ion Ratio Lower Upper
108 100
107 87.3 67.5 101.3

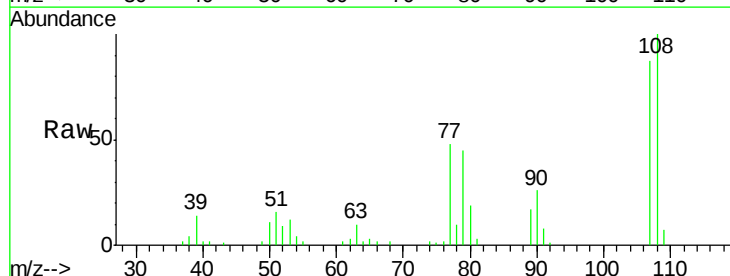

Abundance Ion 108.00 (107.70 to 108.70): E
Ion 107.00 (106.70 to 107.70): E




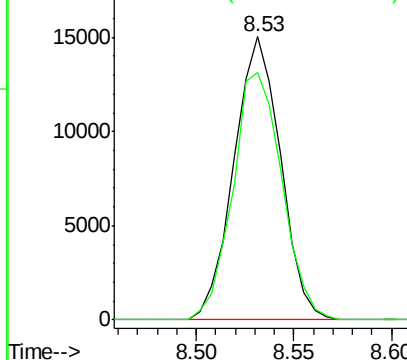


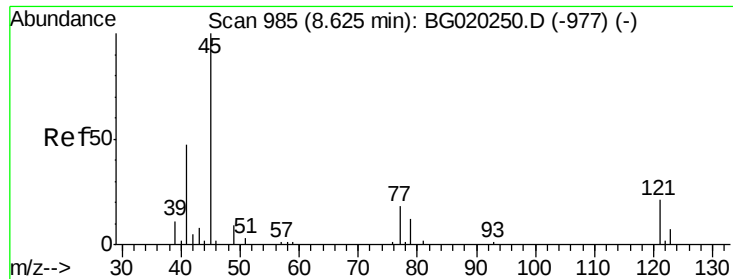

#12
2,2'-oxybis(1-chloropropane)
Concen: 19.71 ng/ul
RT: 8.63 min Scan# 985
Delta R.T. 0.00 min
Lab File: BG020268.D
Acq: 18 Dec 2015 10:24




Instrument :
BNA_G
ClientSampleId :
SSTD02004


Tgt Ion: 45 Resp: 31335
Ion Ratio Lower Upper
45 100
77 16.0 12.1 18.1
79 13.9 9.0 13.4#

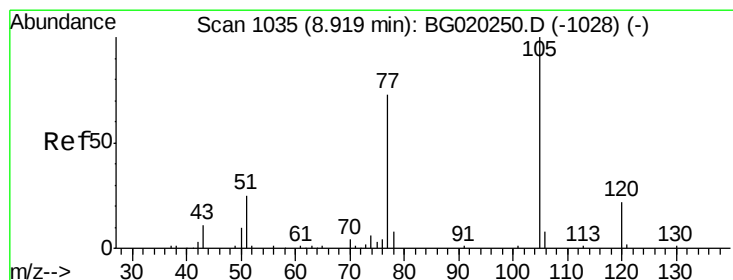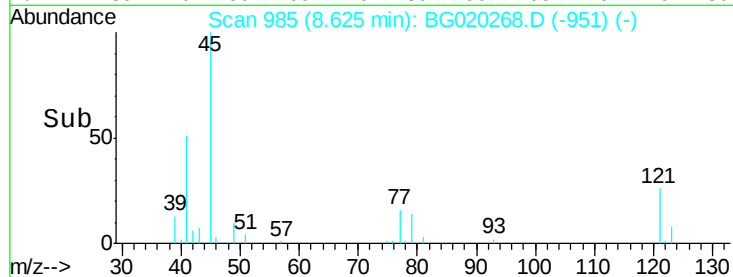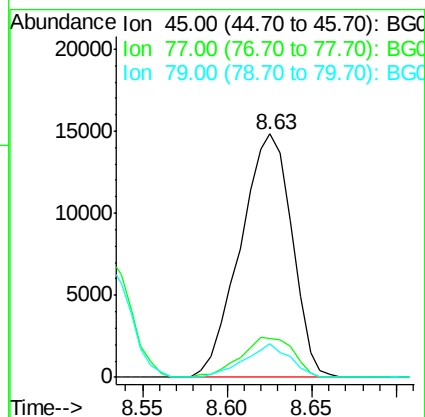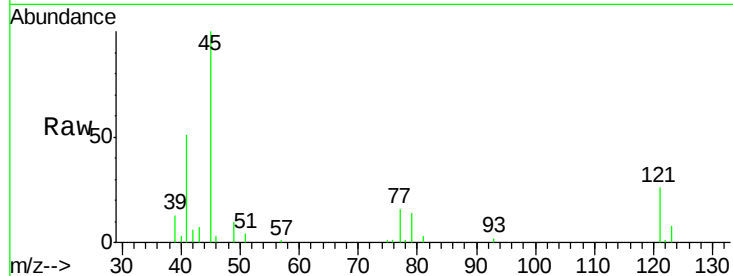

#14
Acetophenone
Concen: 21.01 ng/ul
RT: 8.92 min Scan# 1035
Delta R.T. 0.00 min
Lab File: BG020268.D
Acq: 18 Dec 2015 10:24

Tgt Ion: 105 Resp: 42259
Ion Ratio Lower Upper
105 100
77 80.3 65.2 97.8
51 26.0 22.6 33.8


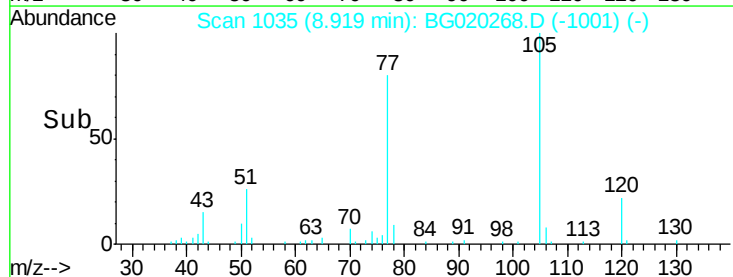
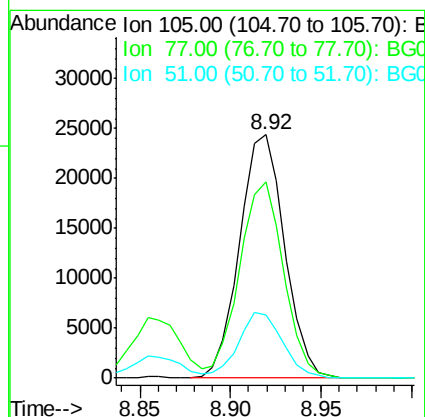
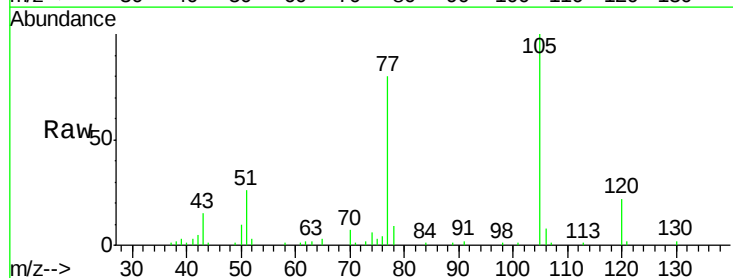


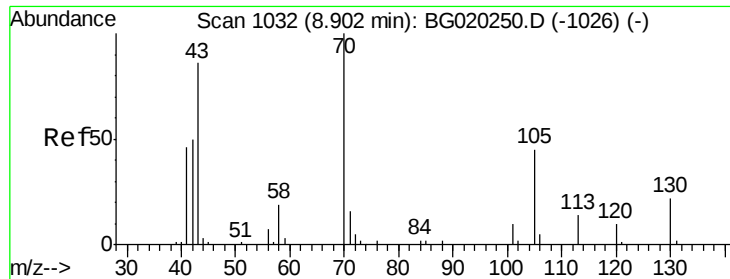

#15
N-Nitroso-di-n-propylamine
Concen: 20.68 ng/ul
RT: 8.90 min Scan# 1031
Delta R.T. -0.01 min
Lab File: BG020268.D
Acq: 18 Dec 2015 10:24




Instrument :
BNA_G
ClientSampleId :
SSTD02004


Tgt Ion: 70 Resp: 22023
Ion Ratio Lower Upper
70 100
42 49.5 44.3 66.5
101 9.8 7.6 11.4
130 20.6 17.0 25.4

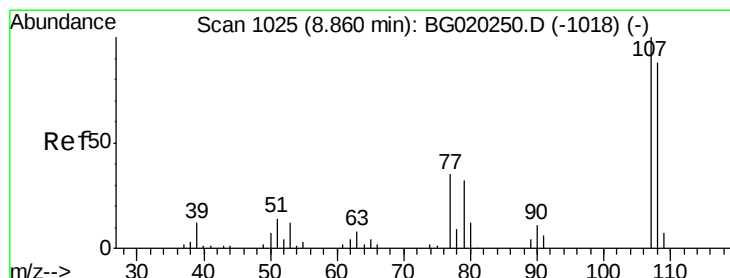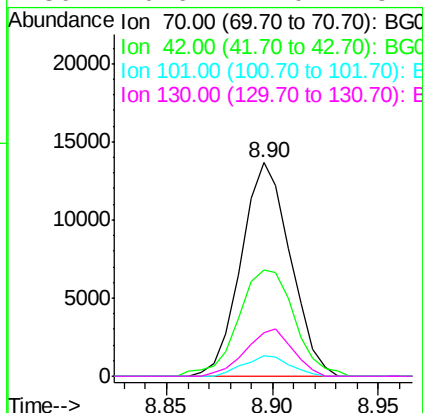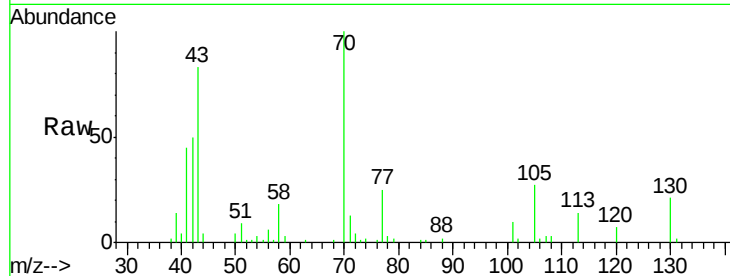

#16
4-Methylphenol
Concen: 20.32 ng/ul
RT: 8.85 min Scan# 1024
Delta R.T. -0.01 min
Lab File: BG020268.D
Acq: 18 Dec 2015 10:24

Tgt Ion: 108 Resp: 27596
Ion Ratio Lower Upper
108 100
107 113.1 88.9 133.3

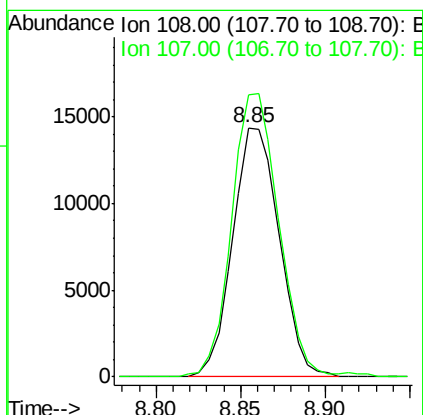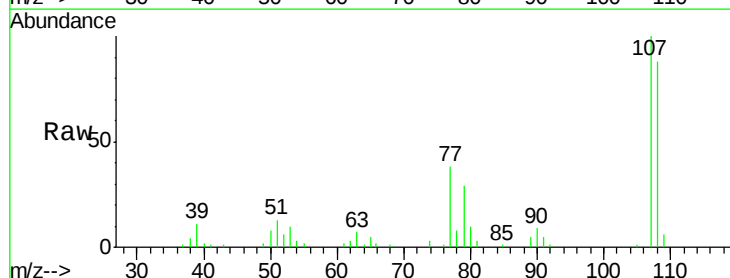

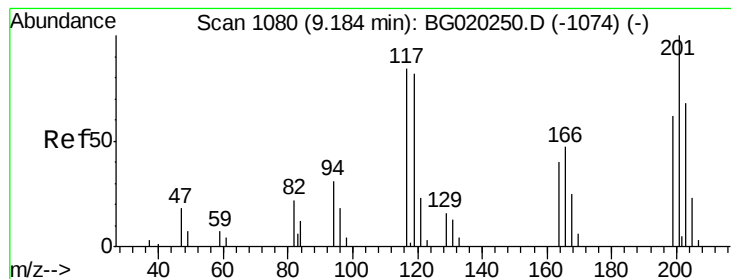

#17

Hexachloroethane

Concen: 20.64 ng/ul

RT: 9.18 min Scan# 1080

Delta R.T. 0.00 min

Lab File: BG020268.D

Acq: 18 Dec 2015 10:24

Instrument :

BNA_G

ClientSampleId :

SSTD02004


Tgt Ion: 117 Resp: 9924

Ion Ratio Lower Upper

117 100

201 137.1 102.7 154.1

199 83.1 65.8 98.8






Abundance

Ion 117.00 (116.70 to 117.70): E

Ion 201.00 (200.70 to 201.70): E

Ion 199.00 (198.70 to 199.70): E

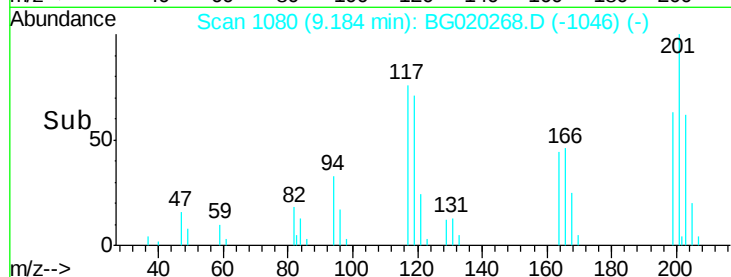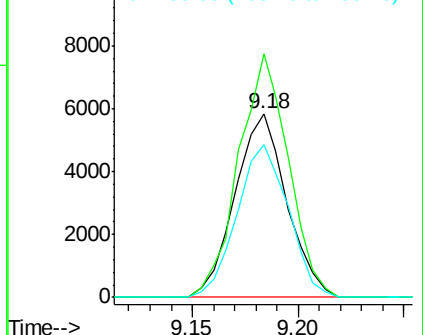

#20

Nitrobenzene

Concen: 20.65 ng/ul

RT: 9.30 min Scan# 1100

Delta R.T. -0.01 min

Lab File: BG020268.D

Acq: 18 Dec 2015 10:24


Tgt Ion: 77 Resp: 31755

Ion Ratio Lower Upper

77 100

123 41.9 33.4 50.0

65 12.8 11.7 17.5






Abundance

Ion 77.00 (76.70 to 77.70): BGC

Ion 123.00 (122.70 to 123.70): E

Ion 65.00 (64.70 to 65.70): BGC

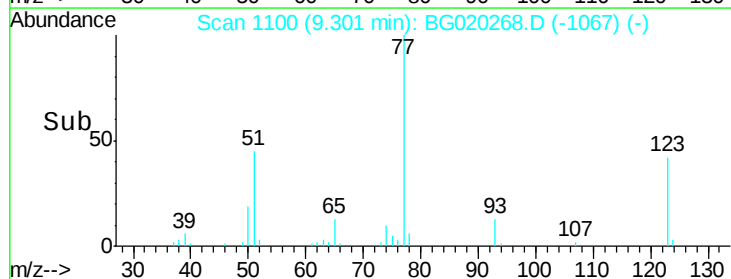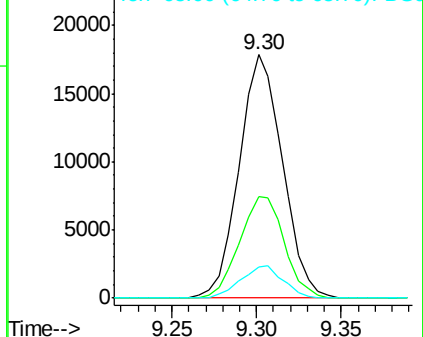

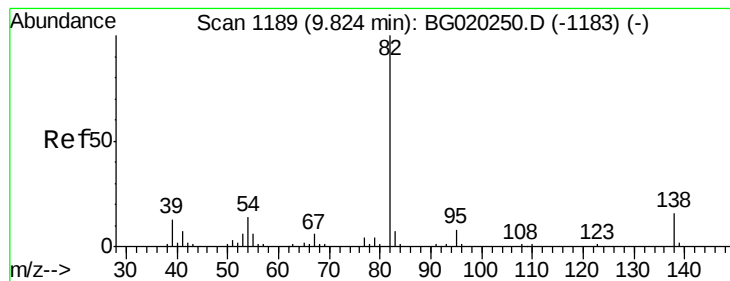

#21

Isophorone

Concen: 20.61 ng/ul

RT: 9.82 min Scan# 1189

Delta R.T. 0.00 min

Lab File: BG020268.D

Acq: 18 Dec 2015 10:24

Instrument :

BNA_G

ClientSampleId :

SSTD02004





Tgt Ion: 82 Resp: 60516

Ion Ratio Lower Upper

82 100

95 8.3 6.2 9.2

138 17.4 13.4 20.2

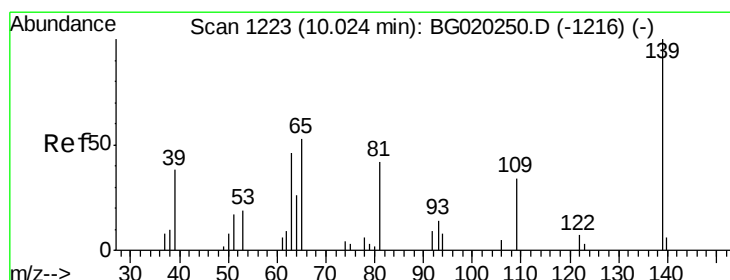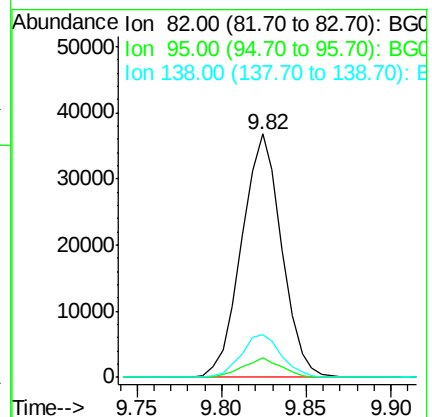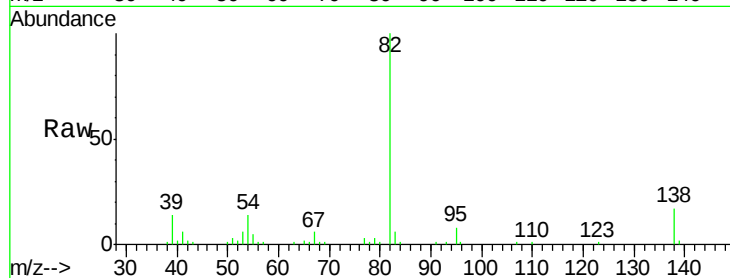

#23

2-Nitrophenol

Concen: 21.99 ng/ul

RT: 10.01 min Scan# 1221

Delta R.T. -0.01 min

Lab File: BG020268.D

Acq: 18 Dec 2015 10:24




Tgt Ion: 139 Resp: 15228


Ion Ratio Lower Upper

139 100

65 54.3 45.1 67.7

109 33.6 29.6 44.4



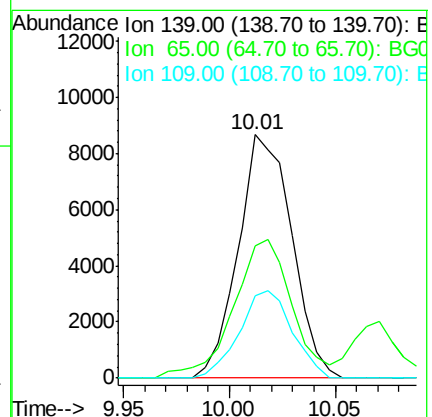
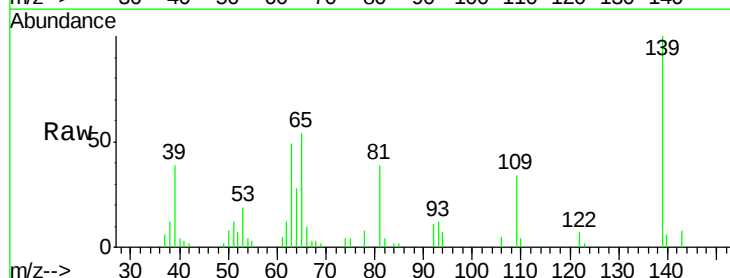


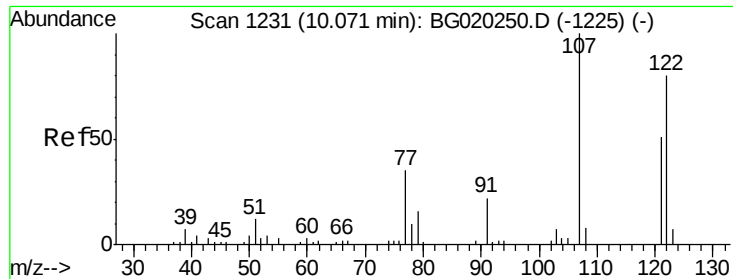

#24
 2,4-Dimethylphenol
 Concen: 21.26 ng/ul
 RT: 10.07 min Scan# 1231
 Delta R.T. 0.00 min
 Lab File: BG020268.D
 Acq: 18 Dec 2015 10:24




Instrument :
 BNA_G
 ClientSampleId :
 SSTD02004


Tgt Ion:	107	Resp:	33431
Ion	Ratio	Lower	Upper
107	100		
121	46.2	39.0	58.4
122	82.3	62.1	93.1

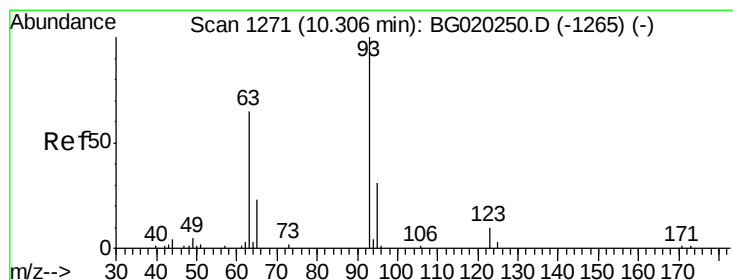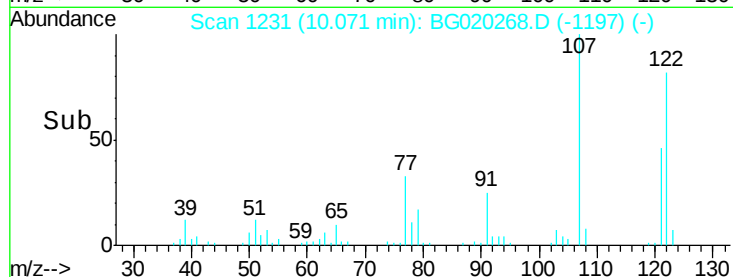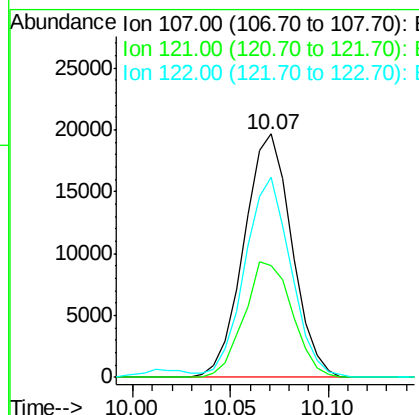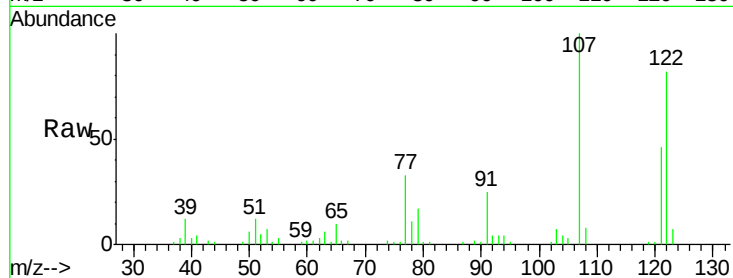

#25
 Bis(2-Chloroethoxy)methane
 Concen: 21.32 ng/ul
 RT: 10.31 min Scan# 1271
 Delta R.T. 0.00 min
 Lab File: BG020268.D
 Acq: 18 Dec 2015 10:24

Tgt Ion:	93	Resp:	33905
Ion	Ratio	Lower	Upper
93	100		
95	32.5	27.4	41.2
123	9.2	9.4	14.0#


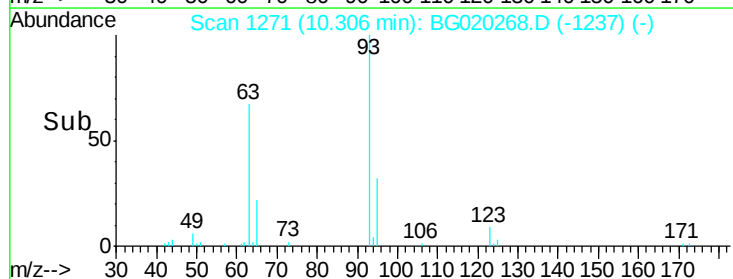
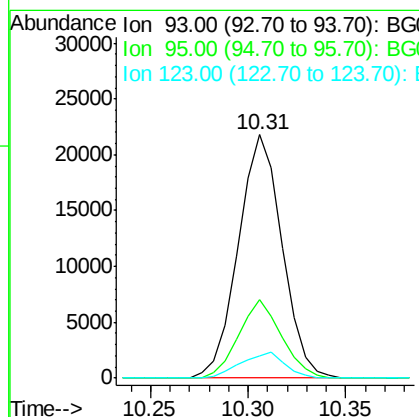
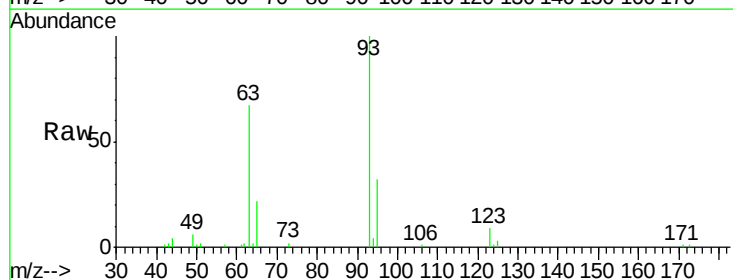


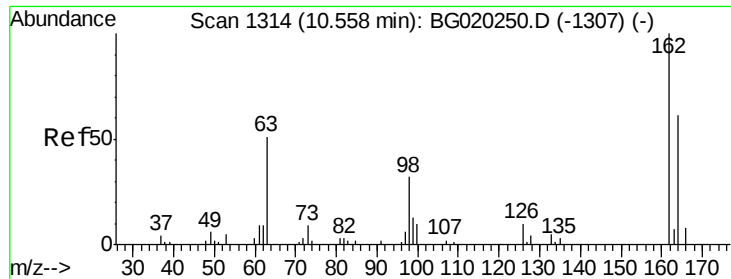

#27
 2,4-Dichlorophenol
 Concen: 21.47 ng/ul
 RT: 10.55 min Scan# 1313
 Delta R.T. -0.01 min
 Lab File: BG020268.D
 Acq: 18 Dec 2015 10:24




Instrument :
 BNA_G
 ClientSampleId :
 SST02004


Tgt Ion:162 Resp: 28850
 Ion Ratio Lower Upper
 162 100
 164 64.8 48.2 72.2
 98 35.8 27.2 40.8

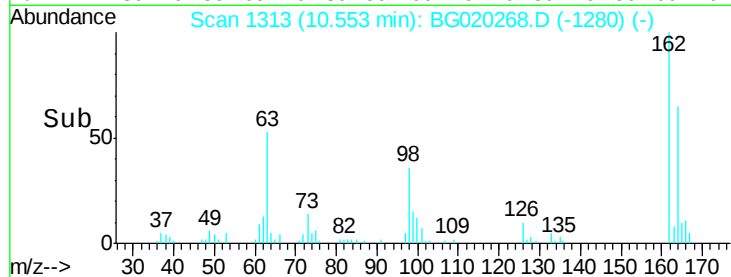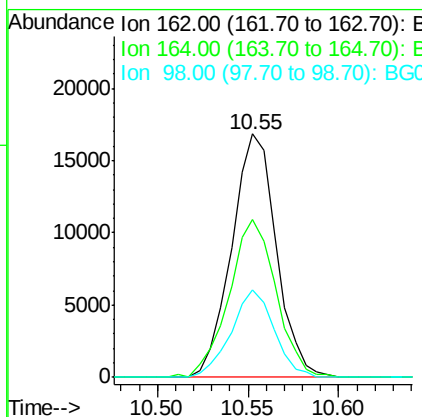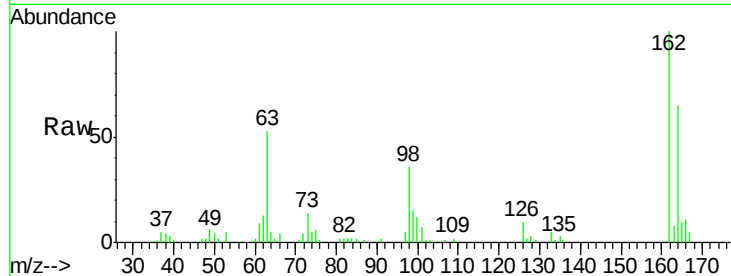

#28
 Naphthalene
 Concen: 22.01 ng/ul
 RT: 10.96 min Scan# 1383
 Delta R.T. 0.00 min
 Lab File: BG020268.D
 Acq: 18 Dec 2015 10:24

Tgt Ion:128 Resp: 85562
 Ion Ratio Lower Upper
 128 100
 129 10.3 8.6 12.8
 127 13.3 10.1 15.1

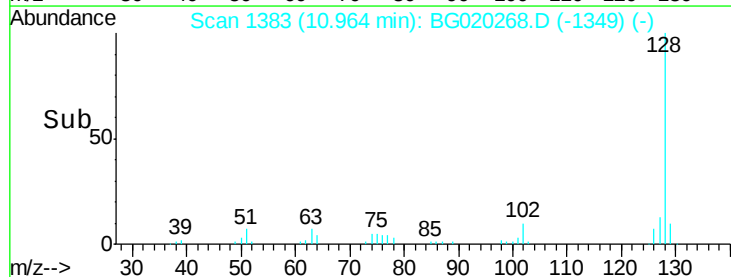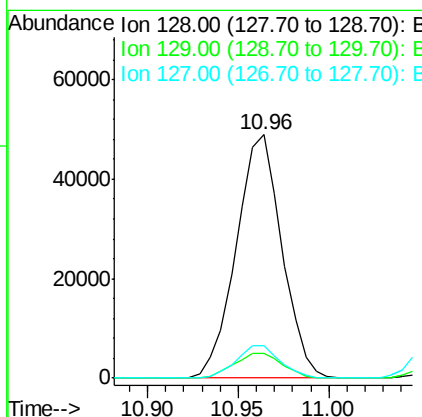


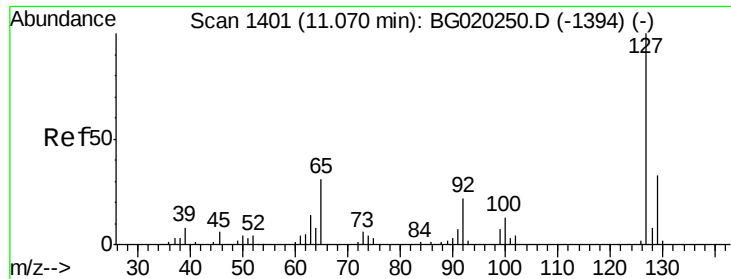




#30
4-Chloroaniline
Concen: 22.77 ng/ul
RT: 11.06 min Scan# 1400
Delta R.T. -0.01 min
Lab File: BG020268.D
Acq: 18 Dec 2015 10:24

Instrument :
BNA_G
ClientSampleId :
SSTD02004

Tgt Ion:127 Resp: 34153
Ion Ratio Lower Upper
127 100
129 32.7 25.7 38.5




Abundance Ion 127.00 (126.70 to 127.70): E
Ion 129.00 (128.70 to 129.70): E

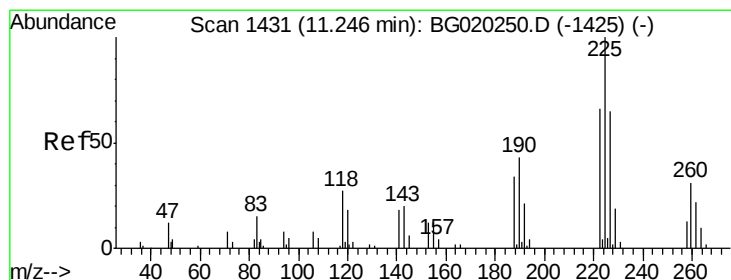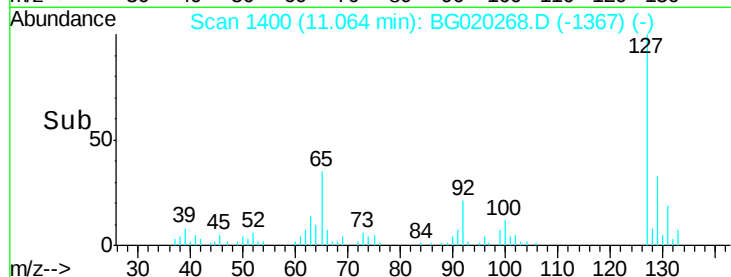
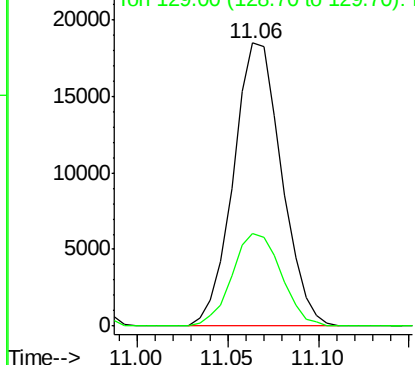



#31
Hexachlorobutadiene
Concen: 22.35 ng/ul
RT: 11.24 min Scan# 1430
Delta R.T. -0.01 min
Lab File: BG020268.D
Acq: 18 Dec 2015 10:24

Tgt Ion:225 Resp: 22388
Ion Ratio Lower Upper
225 100
223 65.1 47.0 70.6
227 63.9 49.7 74.5



Abundance Ion 225.00 (224.70 to 225.70): E
Ion 223.00 (222.70 to 223.70): E
Ion 227.00 (226.70 to 227.70): E



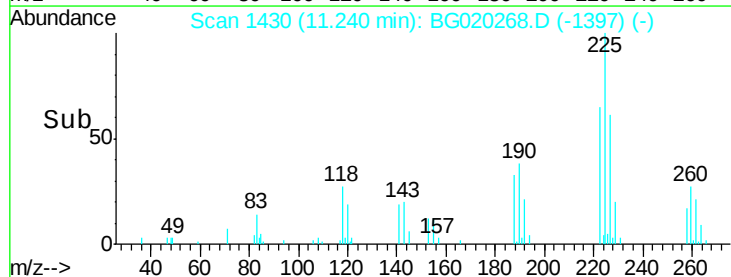
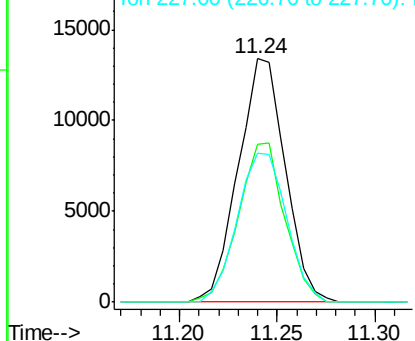


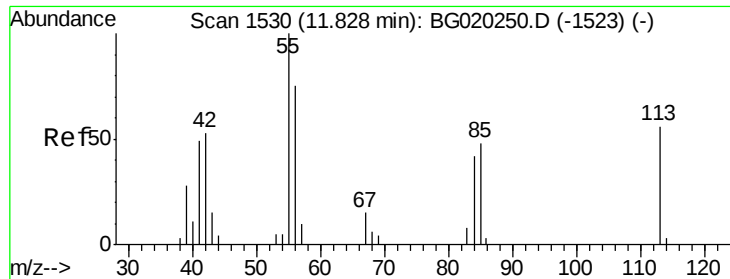

#32
 Caprolactam
 Concen: 20.50 ng/ul
 RT: 11.82 min Scan# 1529
 Delta R.T. -0.01 min
 Lab File: BG020268.D
 Acq: 18 Dec 2015 10:24




Instrument :
 BNA_G
 ClientSampleId :
 SSTD02004


Tgt Ion:113 Resp: 9720
 Ion Ratio Lower Upper
 113 100
 55 173.2 132.1 198.1
 56 124.8 103.3 154.9

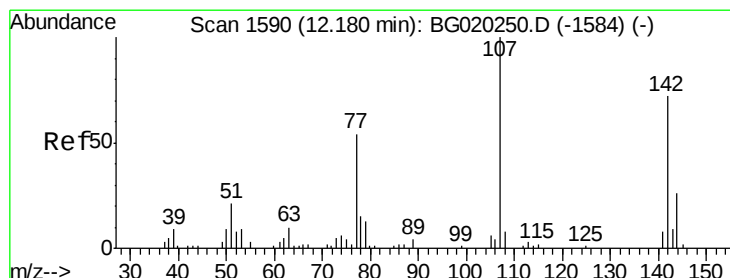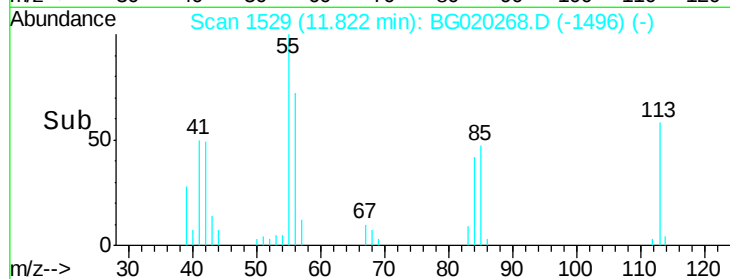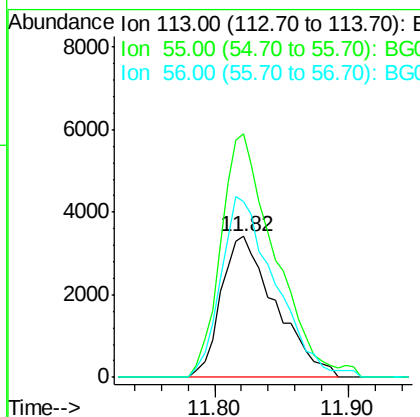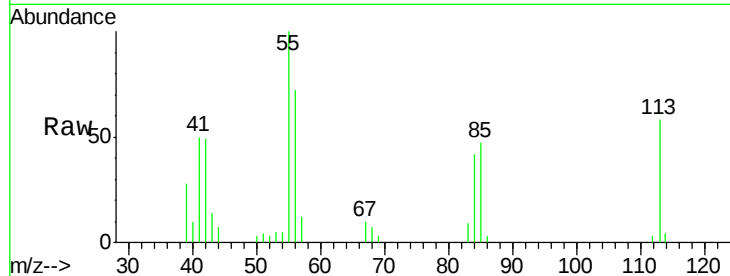

#33
 4-Chloro-3-methylphenol
 Concen: 20.04 ng/ul
 RT: 12.18 min Scan# 1590
 Delta R.T. 0.00 min
 Lab File: BG020268.D
 Acq: 18 Dec 2015 10:24

Tgt Ion:107 Resp: 31990
 Ion Ratio Lower Upper
 107 100
 144 25.8 18.7 28.1
 142 76.8 52.8 79.2



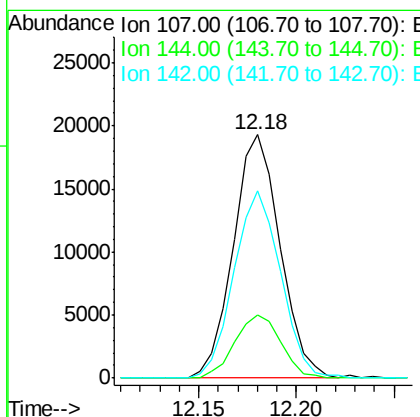
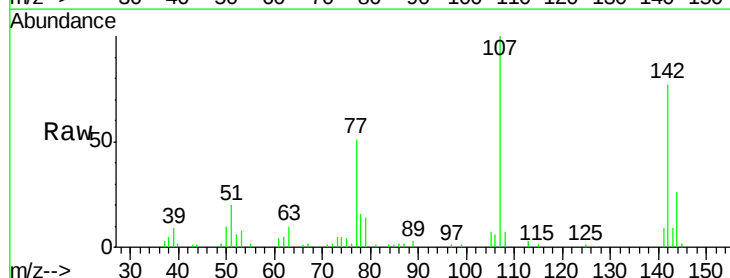


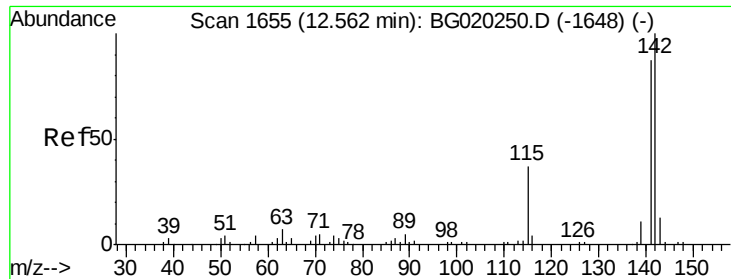

#34
 2-Methylnaphthalene
 Concen: 21.85 ng/ul
 RT: 12.56 min Scan# 1655
 Delta R.T. 0.00 min
 Lab File: BG020268.D
 Acq: 18 Dec 2015 10:24

Instrument :
 BNA_G
 ClientSampleId :
 SSTD02004

Tgt Ion:142 Resp: 64881
 Ion Ratio Lower Upper
 142 100
 141 88.7 74.9 112.3

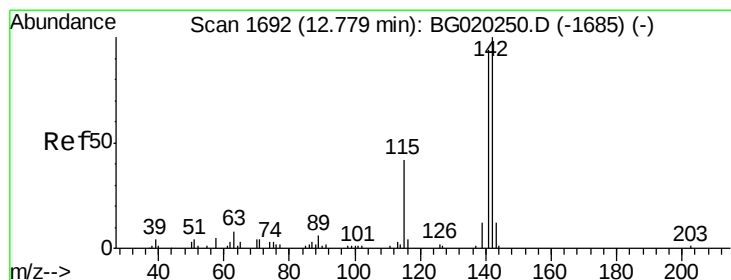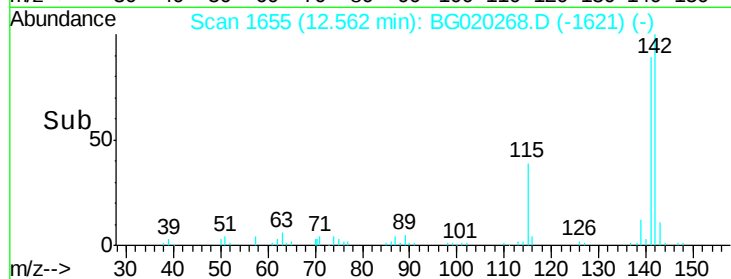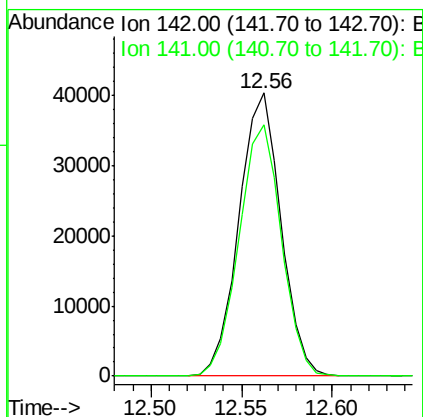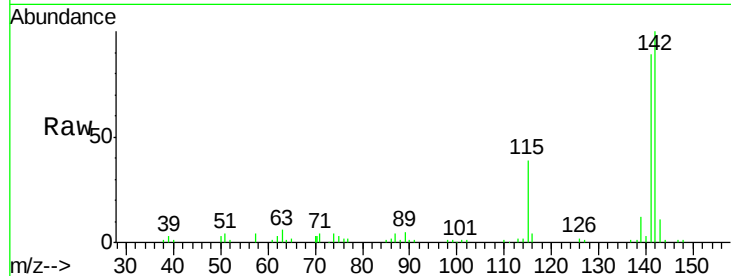

#35
 1-Methylnaphthalene
 Concen: 21.54 ng/ul
 RT: 12.78 min Scan# 1692
 Delta R.T. 0.00 min
 Lab File: BG020268.D
 Acq: 18 Dec 2015 10:24

Tgt Ion:142 Resp: 61499
 Ion Ratio Lower Upper
 142 100
 141 97.2 73.0 109.6
 116 4.1 3.0 4.6

