

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121915\
 Data File : BG020271.D
 Acq On : 18 Dec 2015 12:22
 Operator : UM/SJ
 Sample : PB87275BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK75

Quant Time: Dec 18 23:48:19 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 18 23:45:43 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	14718	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	63689	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.72	164	47265	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.57	188	220974	20.00	ng/ul	0.10
78) Chrysene-d12	21.74	240	159869	20.00	ng/ul	0.00
86) Perylene-d12	25.02	264	133553	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.47	96	1901	7.13	ng/uL	0.00
5) Phenol-d5	7.24	99	42864	33.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.41	67	26657	34.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.62	132	33395	35.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.79	113	37391	33.69	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	18451	37.16	ng/ul	0.00
22) 2-Nitrophenol-d4	9.98	143	21937	39.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	39275	35.10	ng/ul	0.00
29) 4-Chloroaniline-d4	11.04	131	46108	36.68	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	150393	39.34	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	170063	38.23	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	23069	33.64	ng/ul	0.00
58) Fluorene-d10	15.72	176	132598	38.24	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.90	200	137	0.10	ng/ul	0.08
71) Anthracene-d10	17.57	188	220757	21.68	ng/ul	0.00
79) Pyrene-d10	19.85	212	261429	35.09	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	288766	43.35	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.79	70	965	1.05 ng/ul#	1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121915\
Data File : BG020271.D
Acq On : 18 Dec 2015 12:22
Operator : UM/SJ
Sample : PB87275BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK75

Quant Time: Dec 18 23:48:19 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 18 23:45:43 2015
Response via : Initial Calibration

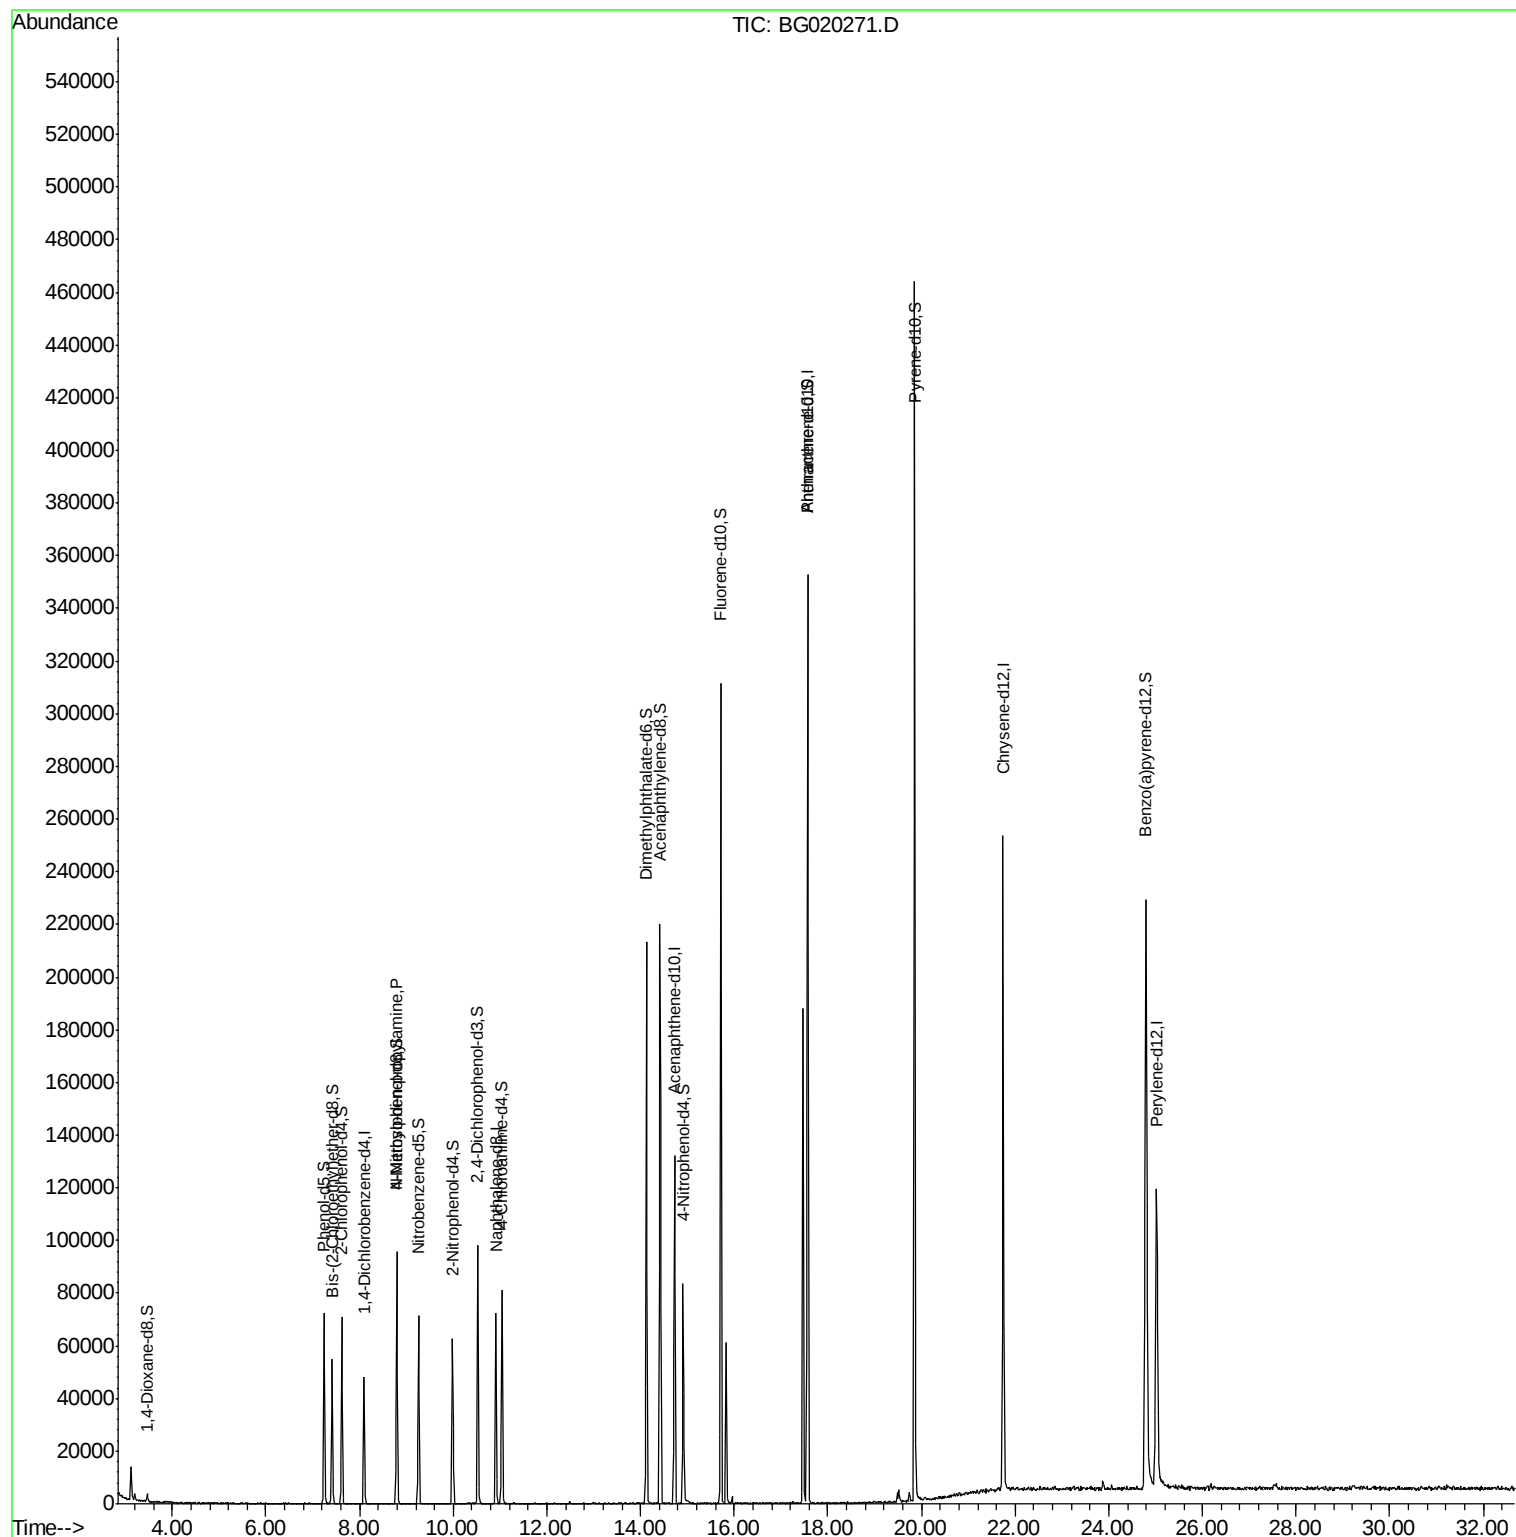

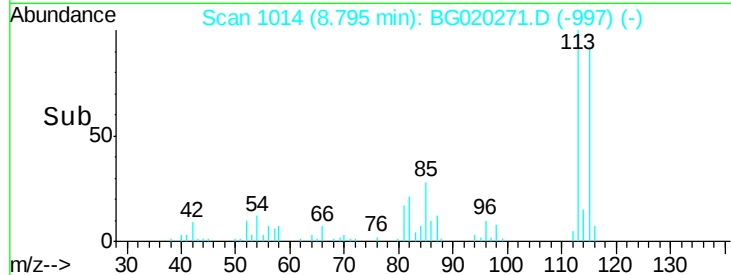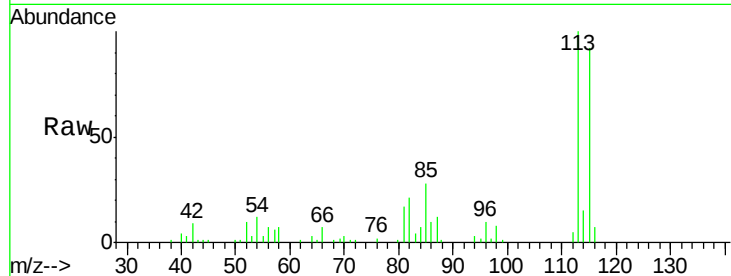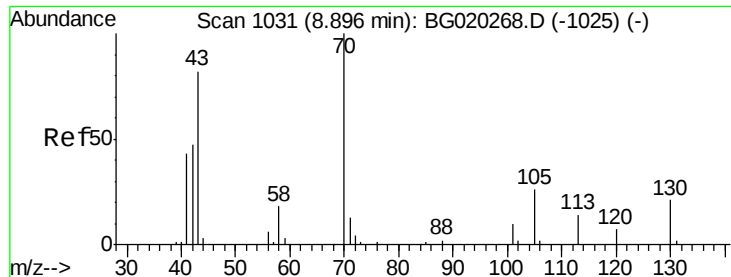

#15
N-Nitroso-di-n-propylamine
Concen: 1.05 ng/ul
RT: 8.79 min Scan# 1014
Delta R.T. -0.10 min
Lab File: BG020271.D
Acq: 18 Dec 2015 12:22

Instrument :
BNA_G
ClientSampleId :
SBLK75

Tgt Ion:	70	Resp:	965
Ion	Ratio	Lower	Upper
70	100		
42	333.8	44.3	66.5#
101	0.0	7.6	11.4#
130	0.0	17.0	25.4#

