

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121915\
 Data File : BG020278.D
 Acq On : 18 Dec 2015 16:57
 Operator : UM/SJ
 Sample : G4767-18DL2 30X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9N40DL2

Quant Time: Dec 19 00:48:11 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 19 00:45:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	15646	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	68373	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.72	164	50876	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	129920	20.00	ng/ul	0.00
78) Chrysene-d12	21.75	240	172591	20.00	ng/ul	0.00
86) Perylene-d12	25.02	264	157624	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.24	99	1077	0.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.42	67	643	0.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	886	0.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	902	0.76	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	351	0.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	517	0.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	991	0.82	ng/ul	0.00
29) 4-Chloroaniline-d4	11.05	131	1442	1.07	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	4377	1.06	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	5038	1.05	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	68	0.09	ng/ul	0.00
58) Fluorene-d10	15.72	176	4226	1.13	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	17.57	188	7153	1.19	ng/ul	0.00
79) Pyrene-d10	19.85	212	8047	1.00	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	7744	0.98	ng/ul	0.00

Target Compounds


						Qvalue
28) Naphthalene	10.96	128	130921	36.67	ng/ul	99
30) 4-Chloroaniline	10.96	127	17541	12.73	ng/ul#	15
34) 2-Methylnaphthalene	12.56	142	43432	15.92	ng/ul	98
35) 1-Methylnaphthalene	12.78	142	21995	8.39	ng/ul	98
41) 1,1'-Biphenyl	13.56	154	19584	5.10	ng/ul	96
48) Acenaphthylene	14.45	152	6645	1.31	ng/ul#	96
50) Acenaphthene	14.79	153	88433	25.84	ng/ul	99
54) Dibenzofuran	15.12	168	94846	18.63	ng/ul	99
59) Fluorene	15.77	166	90810	22.21	ng/ul	99
61) 4-Nitroaniline	15.76	138	1096	1.20	ng/ul#	10
70) Phenanthrene	17.52	178	448063	63.05	ng/ul	100
72) Anthracene	17.60	178	50562	7.01	ng/ul	98
75) Carbazole	17.87	167	34665	5.72	ng/ul	96
77) Fluoranthene	19.52	202	252739	30.43	ng/ul	97
80) Pyrene	19.88	202	172298	16.49	ng/ul	98
83) Benzo(a)anthracene	21.72	228	37780	3.75	ng/ul	98
85) Chrysene	21.72	228	37780	3.98	ng/ul	95
88) Benzo(b)fluoranthene	23.98	252	15192	1.60	ng/ul#	91
89) Benzo(k)fluoranthene	23.98	252	15192	1.67	ng/ul#	93
91) Benzo(a)pyrene	24.87	252	9296	1.03	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121915\
Data File : BG020278.D
Acq On : 18 Dec 2015 16:57
Operator : UM/SJ
Sample : G4767-18DL2 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9N40DL2

Quant Time: Dec 19 00:48:11 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 19 00:45:12 2015
Response via : Initial Calibration

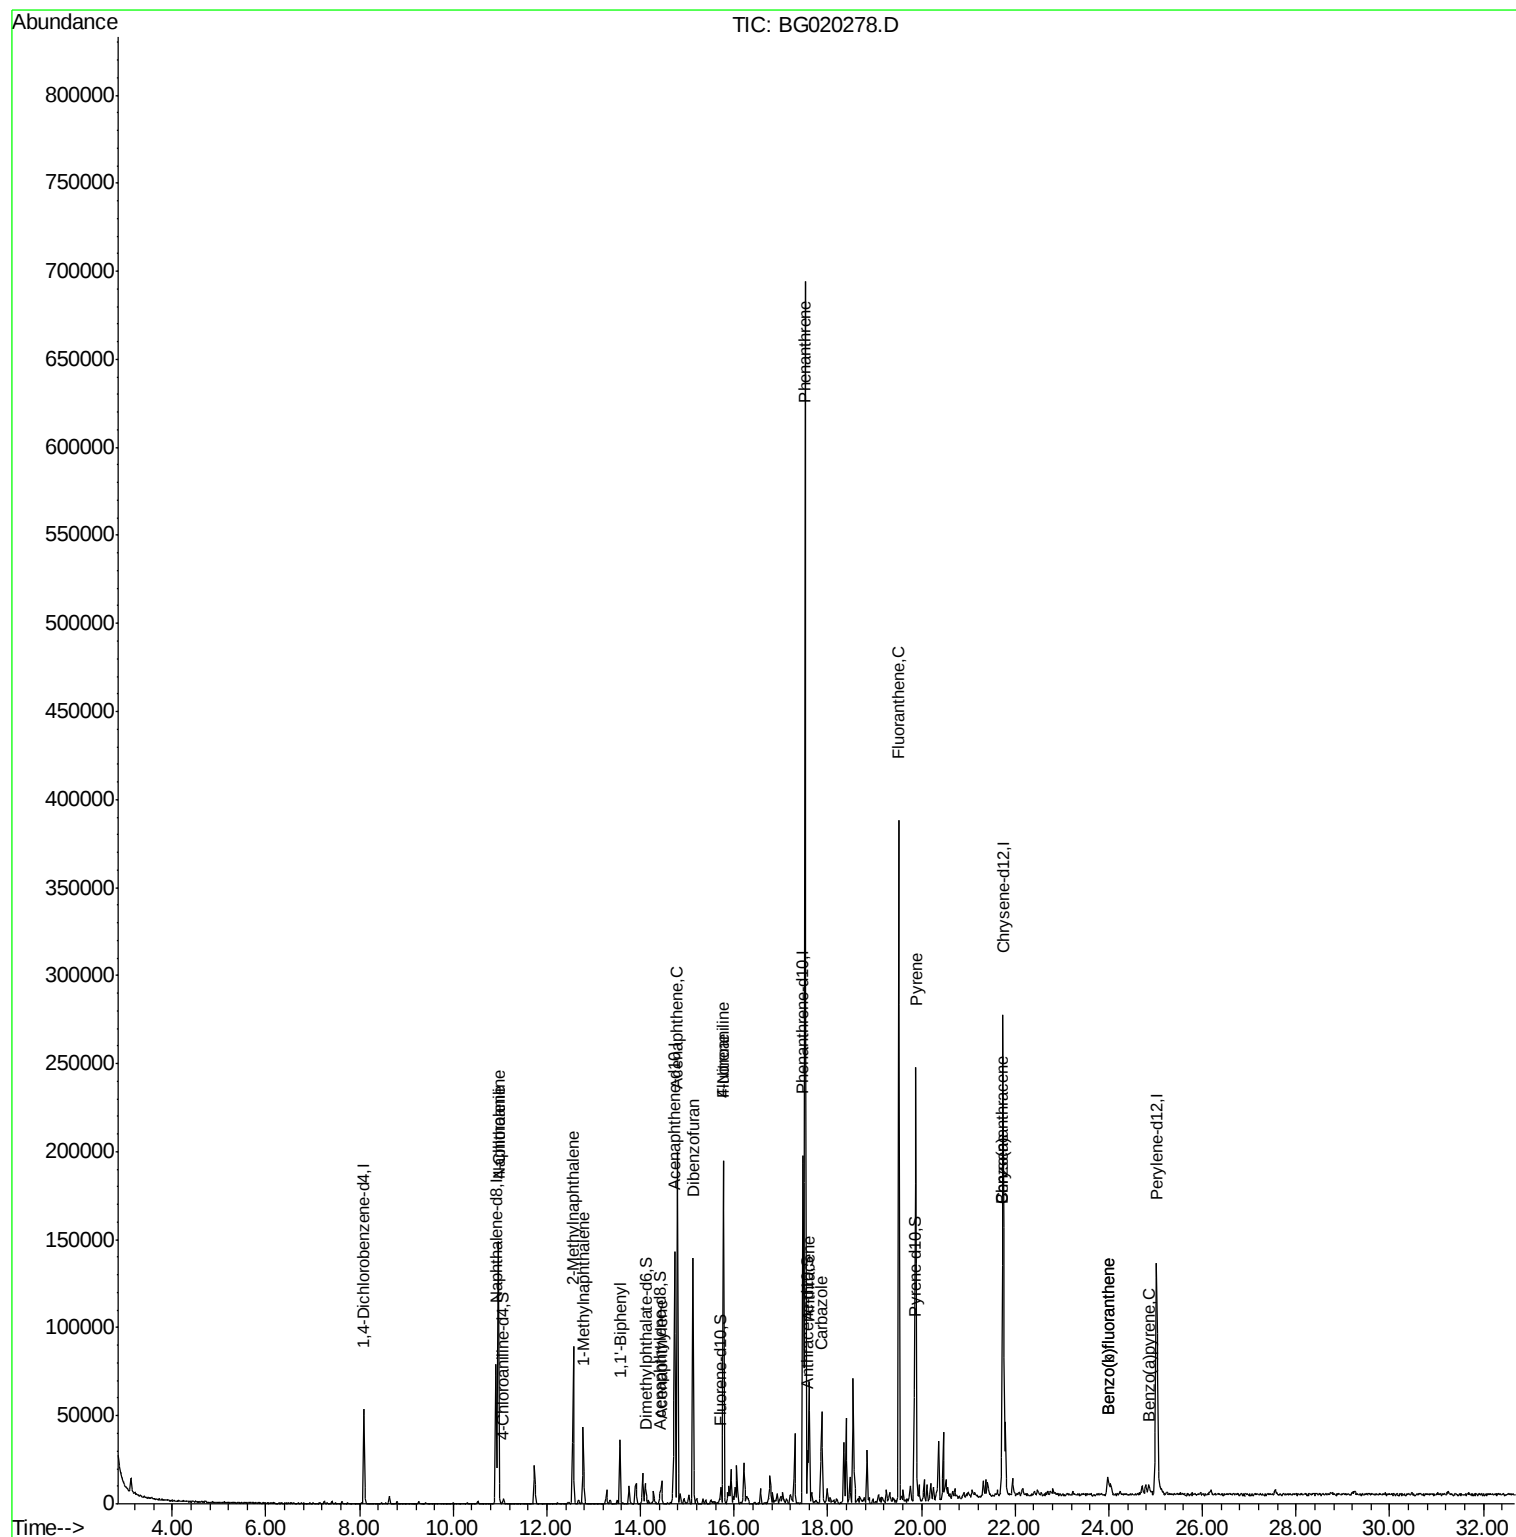


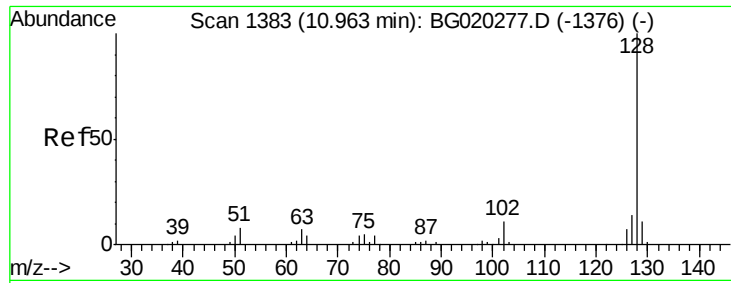




#28
Naphthalene
Concen: 36.67 ng/ul
RT: 10.96 min Scan# 1383
Delta R.T. 0.00 min
Lab File: BG020278.D
Acq: 18 Dec 2015 16:57

Instrument :
BNA_G
ClientSampleId :
D9N40DL2

Tgt Ion:128 Resp: 130921
Ion Ratio Lower Upper
128 100
129 10.7 8.6 12.8
127 13.3 10.1 15.1

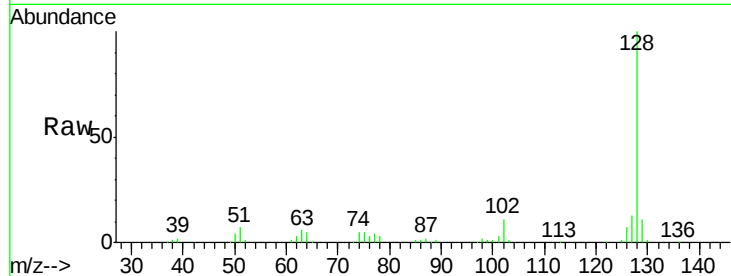


Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

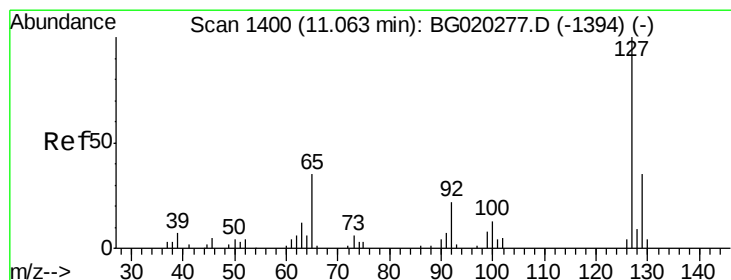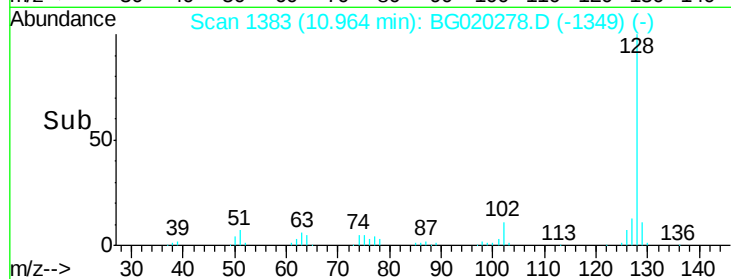
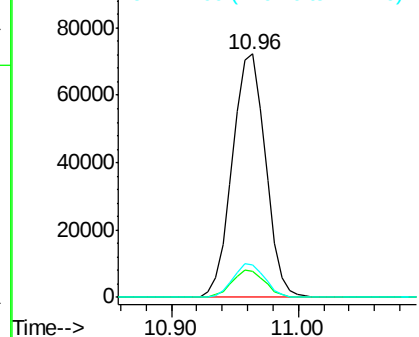



#30
4-Chloroaniline
Concen: 12.73 ng/ul
RT: 10.96 min Scan# 1382
Delta R.T. -0.11 min
Lab File: BG020278.D
Acq: 18 Dec 2015 16:57

Tgt Ion:127 Resp: 17541
Ion Ratio Lower Upper
127 100
129 79.4 25.7 38.5#

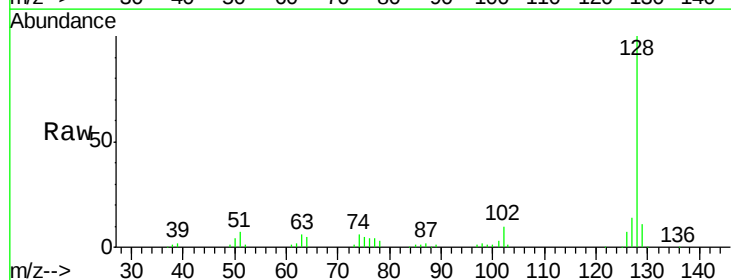

Abundance Ion 127.00 (126.70 to 127.70): E
Ion 129.00 (128.70 to 129.70): E



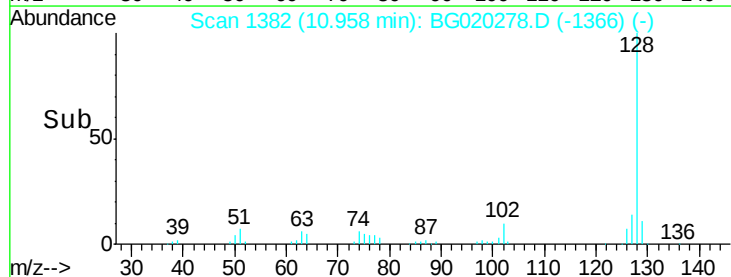
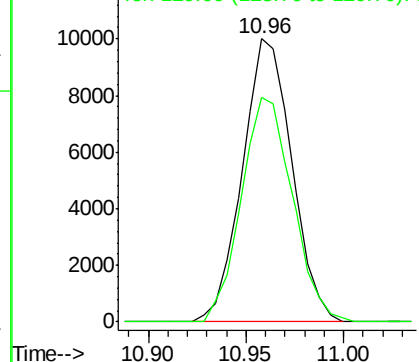


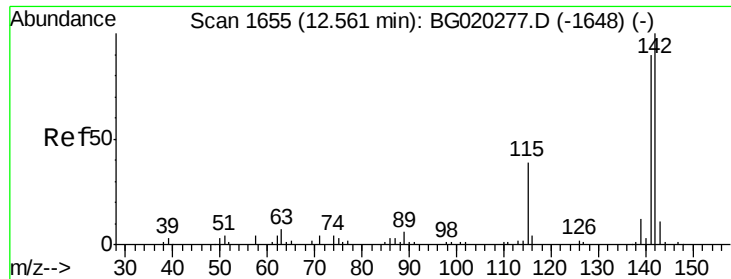

#34
 2-Methylnaphthalene
 Concen: 15.92 ng/ul
 RT: 12.56 min Scan# 1655
 Delta R.T. 0.00 min
 Lab File: BG020278.D
 Acq: 18 Dec 2015 16:57




Instrument :
 BNA_G
 ClientSampleId :
 D9N40DL2


Tgt Ion:142 Resp: 43432
 Ion Ratio Lower Upper
 142 100
 141 91.4 74.9 112.3

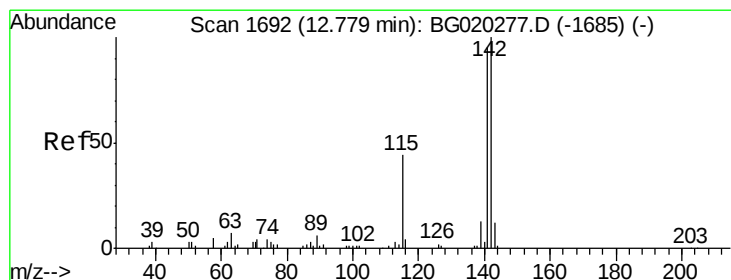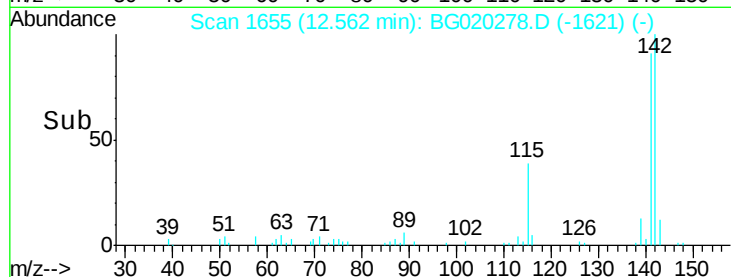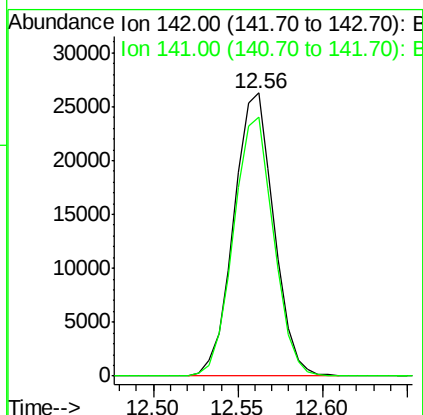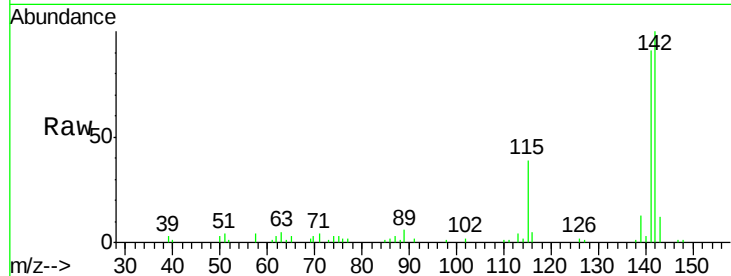

#35
 1-Methylnaphthalene
 Concen: 8.39 ng/ul
 RT: 12.78 min Scan# 1692
 Delta R.T. 0.00 min
 Lab File: BG020278.D
 Acq: 18 Dec 2015 16:57

Tgt Ion:142 Resp: 21995
 Ion Ratio Lower Upper
 142 100
 141 93.1 73.0 109.6
 116 3.8 3.0 4.6

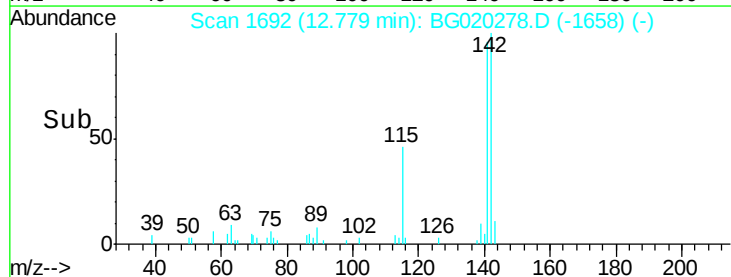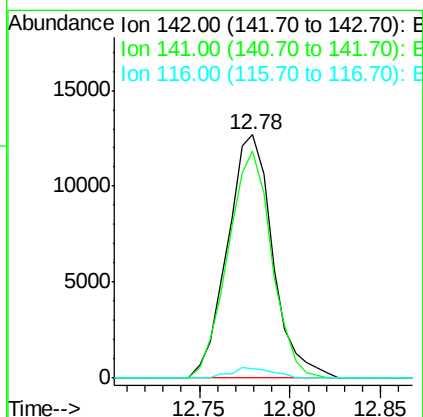


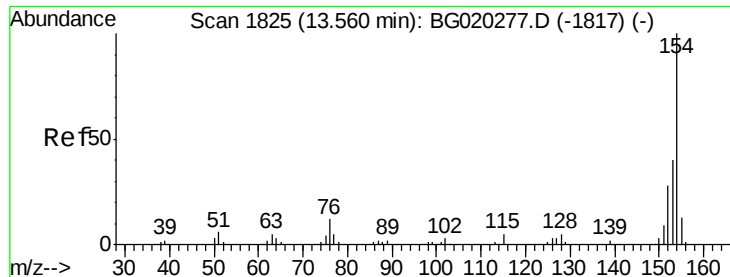




#41
 1,1'-Biphenyl
 Concen: 5.10 ng/ul
 RT: 13.56 min Scan# 1825
 Delta R.T. 0.00 min
 Lab File: BG020278.D
 Acq: 18 Dec 2015 16:57

Instrument :
 BNA_G
 ClientSampleId :
 D9N40DL2

Tgt Ion:154 Resp: 19584
 Ion Ratio Lower Upper
 154 100
 153 42.5 35.5 53.3
 76 10.7 10.4 15.6

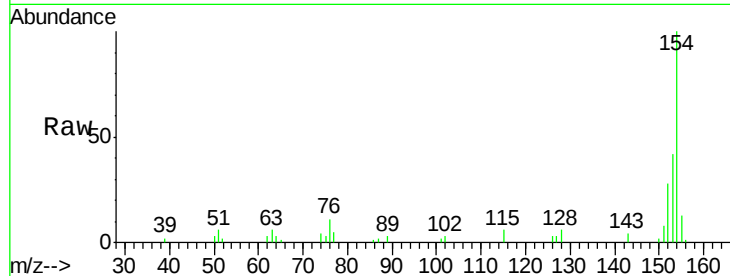


Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 76.00 (75.70 to 76.70): BGC

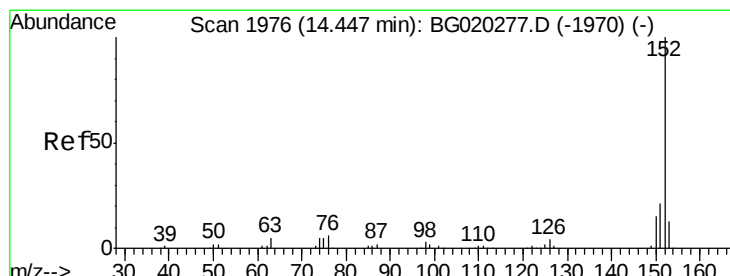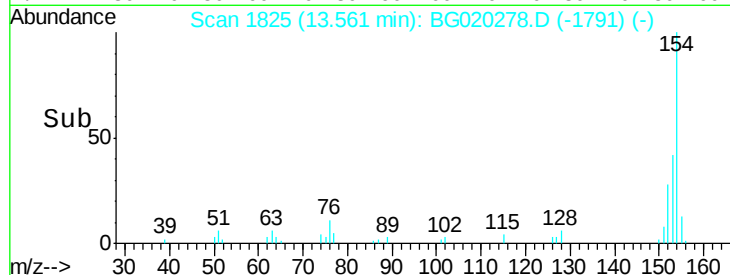
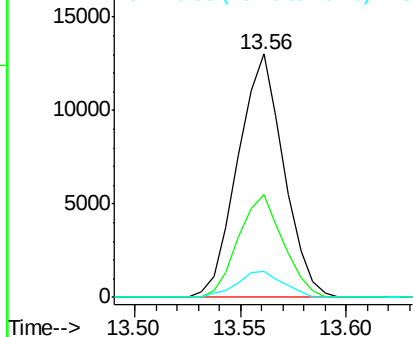



#48
 Acenaphthylene
 Concen: 1.31 ng/ul
 RT: 14.45 min Scan# 1976
 Delta R.T. 0.00 min
 Lab File: BG020278.D
 Acq: 18 Dec 2015 16:57

Tgt Ion:152 Resp: 6645
 Ion Ratio Lower Upper
 152 100
 151 20.4 16.4 24.6
 153 16.9 10.4 15.6#

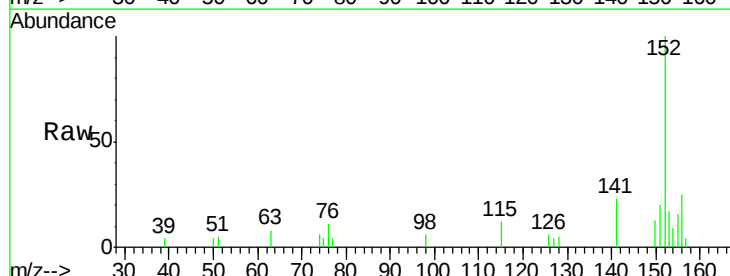

Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 151.00 (150.70 to 151.70): E
 Ion 153.00 (152.70 to 153.70): E

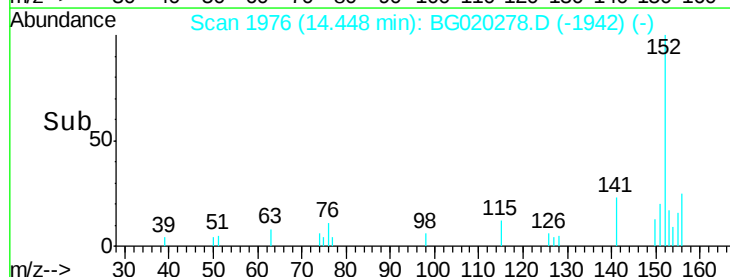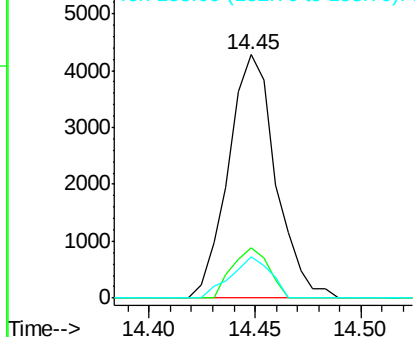

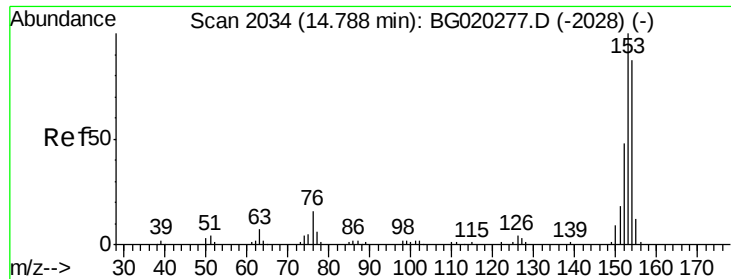

#50

Acenaphthene

Concen: 25.84 ng/ul

RT: 14.79 min Scan# 2034

Delta R.T. 0.00 min

Lab File: BG020278.D

Acq: 18 Dec 2015 16:57

Instrument :

BNA_G

ClientSampleId :

D9N40DL2


Tgt Ion:153 Resp: 88433

Ion Ratio Lower Upper

153 100

152 48.1 37.6 56.4




154 86.0 67.9 101.9

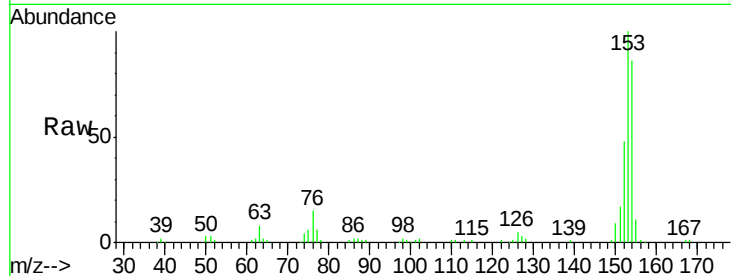

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

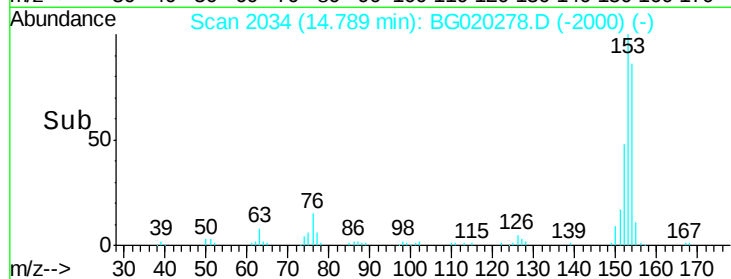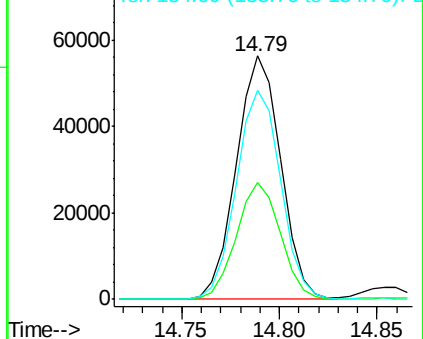

#54

Dibenzofuran

Concen: 18.63 ng/ul

RT: 15.12 min Scan# 2091

Delta R.T. 0.00 min

Lab File: BG020278.D


Acq: 18 Dec 2015 16:57

Tgt Ion:168 Resp: 94846

Ion Ratio Lower Upper



168 100


139 37.8 30.5 45.7



Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

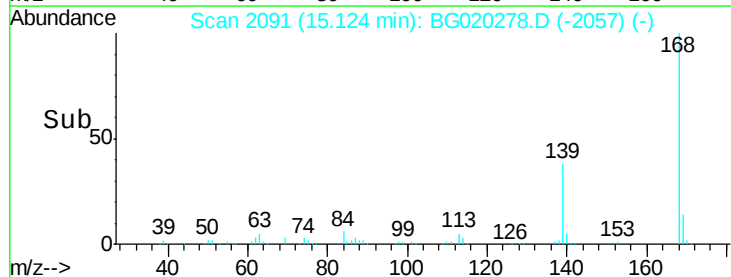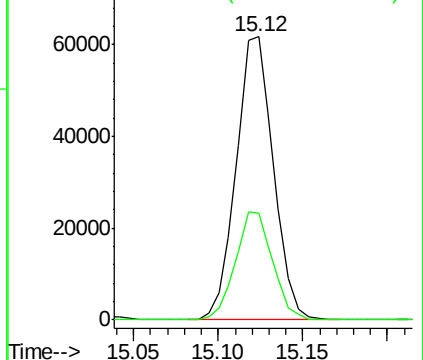

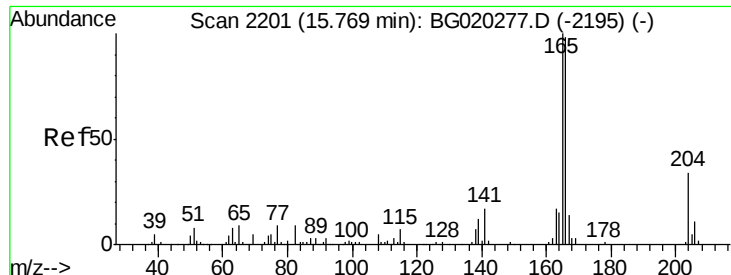

#59

Fluorene

Concen: 22.21 ng/ul

RT: 15.77 min Scan# 2201

Delta R.T. 0.00 min

Lab File: BG020278.D

Acq: 18 Dec 2015 16:57

Instrument :

BNA_G

ClientSampleId :

D9N40DL2


Tgt Ion:166 Resp: 90810

Ion Ratio Lower Upper

166 100

165 102.9 81.4 122.0




167 13.6 11.2 16.8

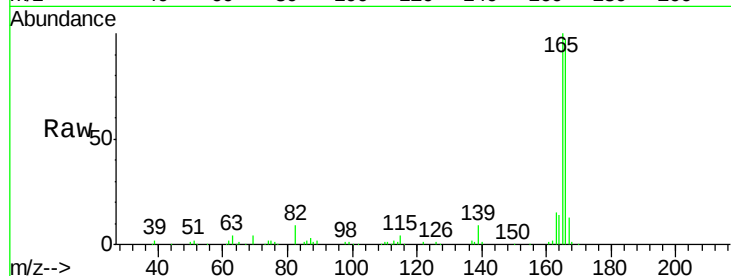

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

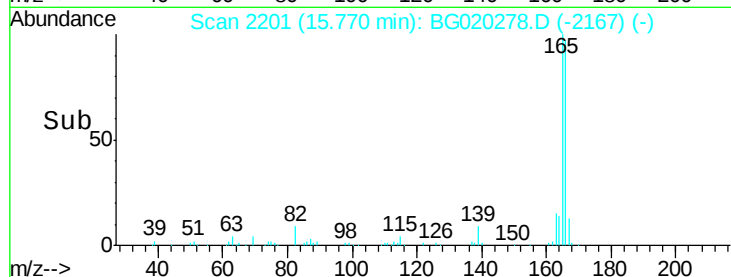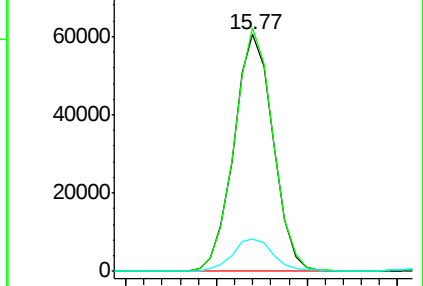

#61

4-Nitroaniline

Concen: 1.20 ng/ul

RT: 15.76 min Scan# 2200

Delta R.T. -0.02 min

Lab File: BG020278.D

Acq: 18 Dec 2015 16:57


Tgt Ion:138 Resp: 1096

Ion Ratio Lower Upper

138 100

92 0.0 45.2 67.8#



108 0.0 75.4 113.0#




Abundance Ion 138.00 (137.70 to 138.70): E

Ion 92.00 (91.70 to 92.70): BG

Ion 108.00 (107.70 to 108.70): E

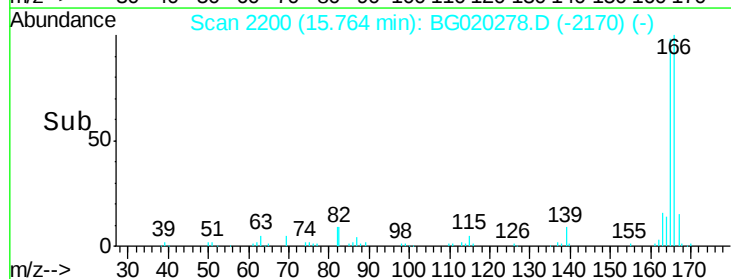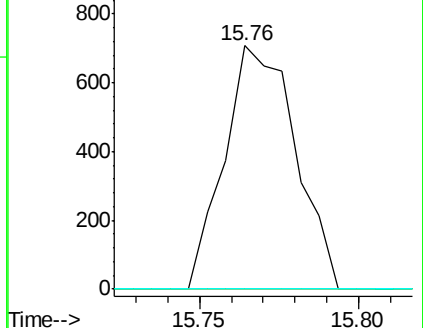

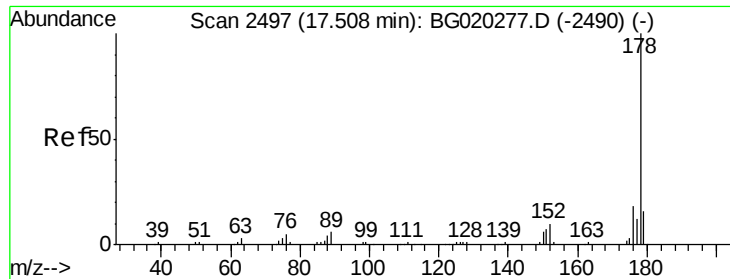

#70

Phenanthrene

Concen: 63.05 ng/ul

RT: 17.52 min Scan# 2498

Delta R.T. 0.01 min

Lab File: BG020278.D

Acq: 18 Dec 2015 16:57

Instrument :

BNA_G

ClientSampleId :

D9N40DL2


Tgt Ion:178 Resp: 448063

Ion Ratio Lower Upper

178 100

179 16.3 12.9 19.3




176 19.2 15.3 22.9

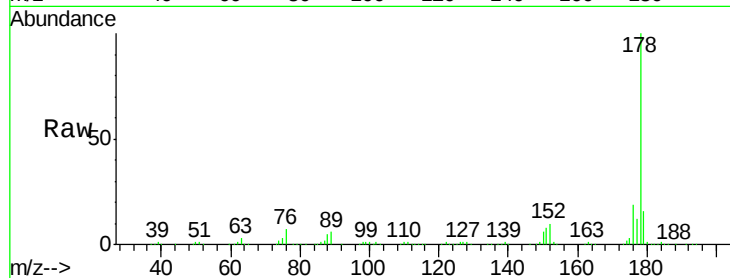

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

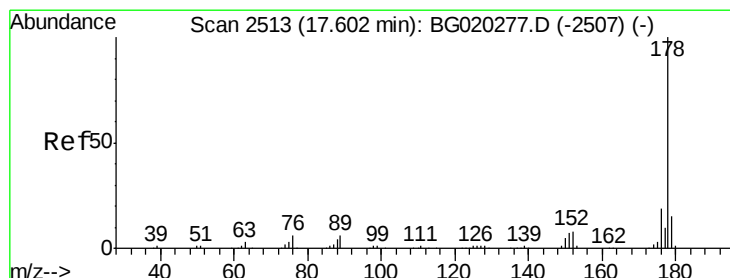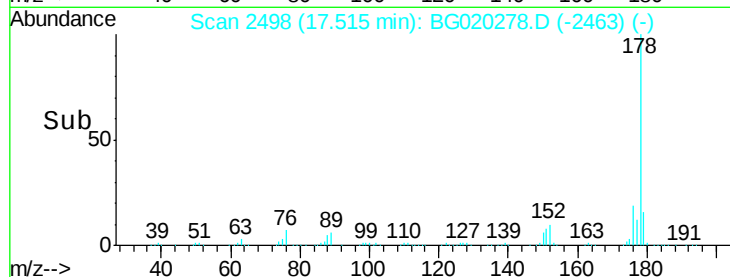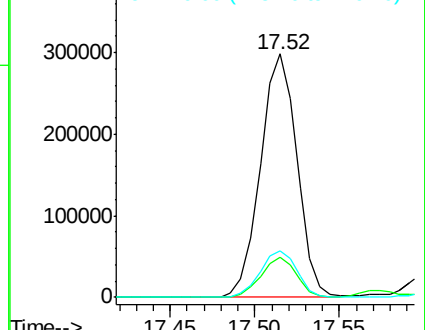

#72

Anthracene

Concen: 7.01 ng/ul

RT: 17.60 min Scan# 2513

Delta R.T. 0.00 min

Lab File: BG020278.D

Acq: 18 Dec 2015 16:57


Tgt Ion:178 Resp: 50562

Ion Ratio Lower Upper

178 100

179 17.0 12.3 18.5



176 18.3 14.3 21.5

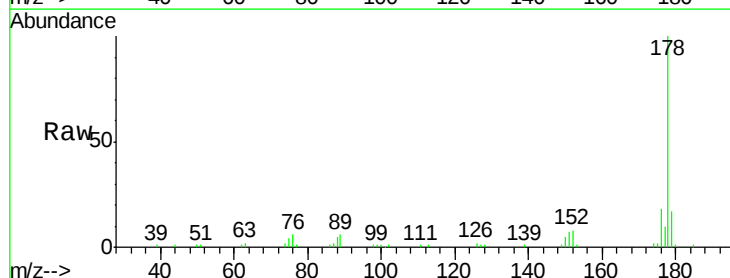


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

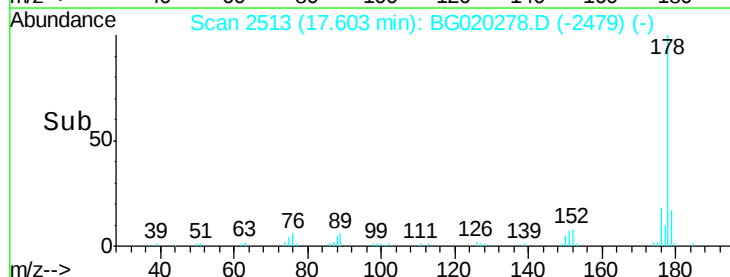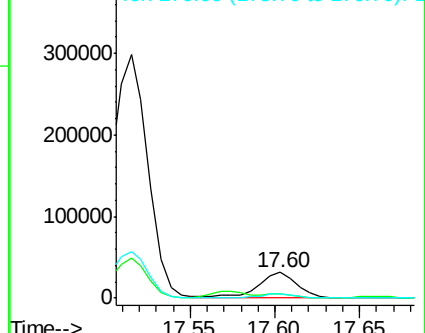

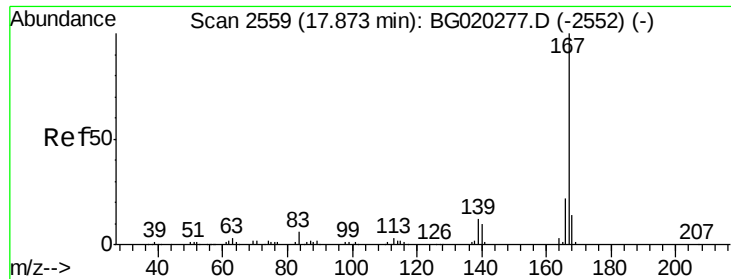

#75

Carbazole

Concen: 5.72 ng/ul

RT: 17.87 min Scan# 2559

Delta R.T. 0.00 min

Lab File: BG020278.D

Acq: 18 Dec 2015 16:57

Instrument :

BNA_G

ClientSampleId :

D9N40DL2


Tgt Ion:167 Resp: 34665

Ion Ratio Lower Upper

167 100

166 19.7 17.0 25.6




139 10.3 10.1 15.1

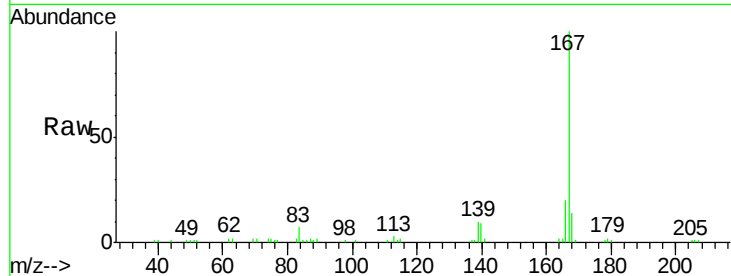

Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

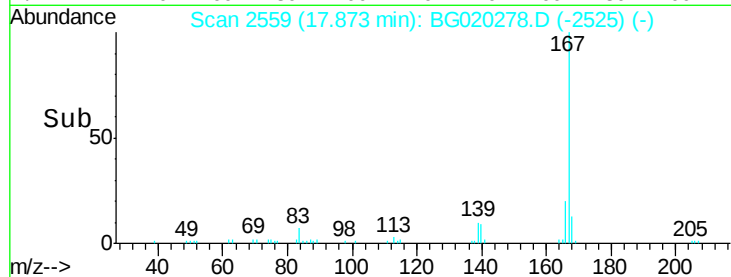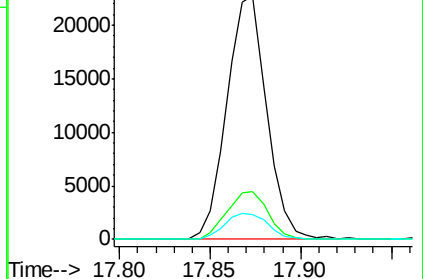

#77

Fluoranthene

Concen: 30.43 ng/ul

RT: 19.52 min Scan# 2839

Delta R.T. 0.00 min

Lab File: BG020278.D

Acq: 18 Dec 2015 16:57


Tgt Ion:202 Resp: 252739

Ion Ratio Lower Upper

202 100

101 6.6 6.2 9.4



100 5.8 5.1 7.7




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B



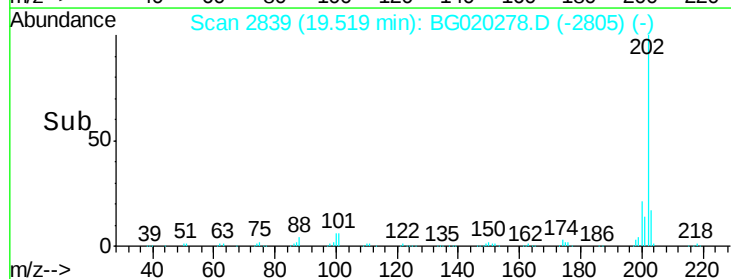
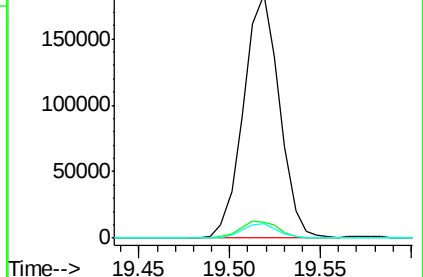


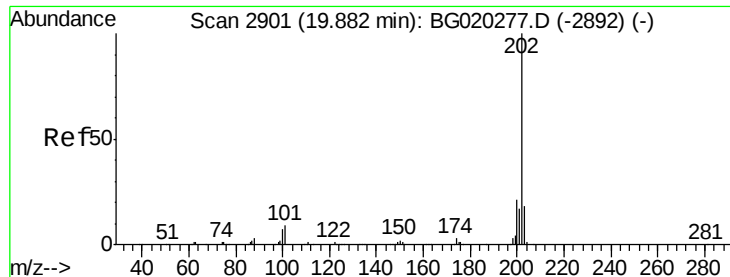

#80
 Pyrene
 Concen: 16.49 ng/u1
 RT: 19.88 min Scan# 2900
 Delta R.T. -0.01 min
 Lab File: BG020278.D
 Acq: 18 Dec 2015 16:57




Instrument :
 BNA_G
 ClientSampleId :
 D9N40DL2


Tgt Ion	Ratio	Lower	Upper
202	100		
101	7.8	7.0	10.4
100	7.7	6.4	9.6

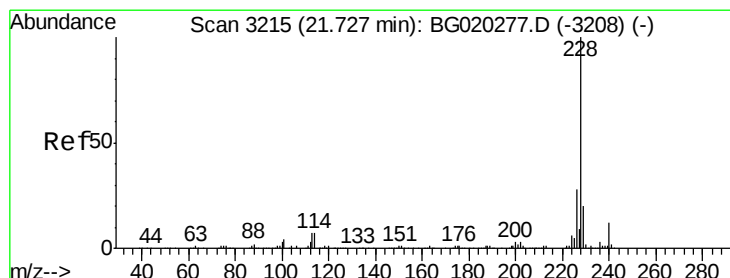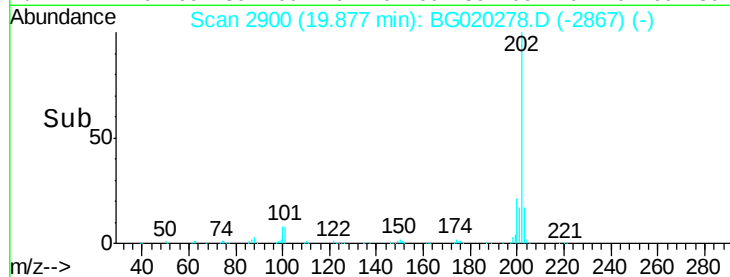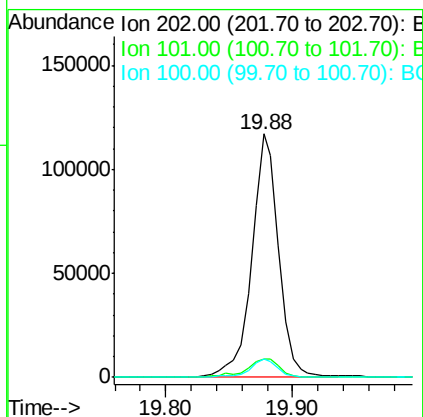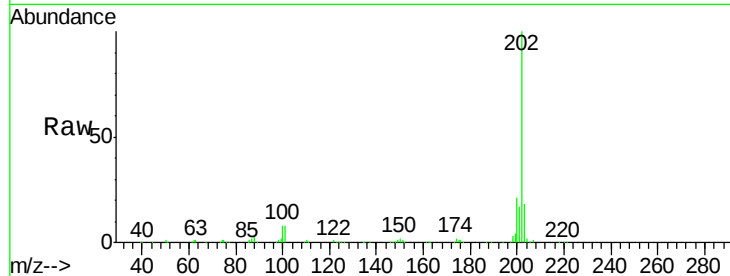

#83
 Benzo(a)anthracene
 Concen: 3.75 ng/u1
 RT: 21.72 min Scan# 3214
 Delta R.T. -0.01 min
 Lab File: BG020278.D
 Acq: 18 Dec 2015 16:57

Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.3	15.8	23.8
226	25.8	21.8	32.6


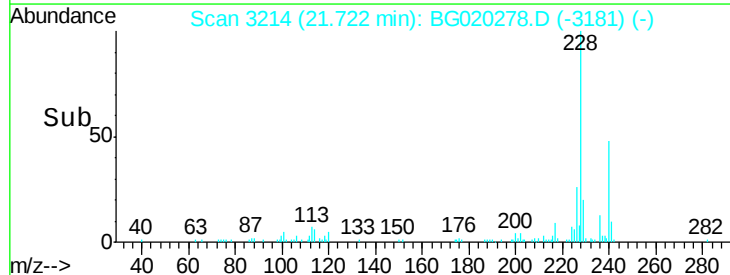
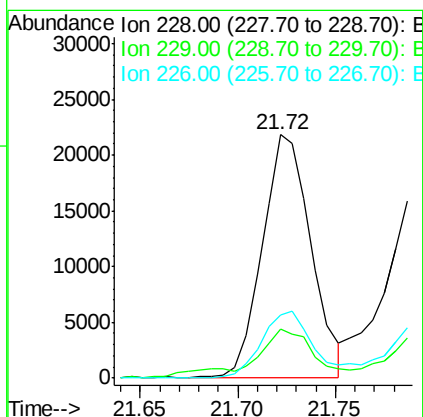
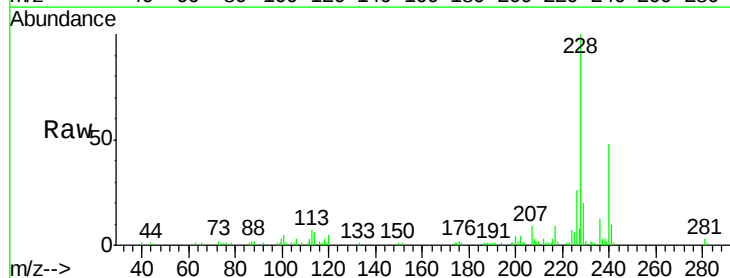


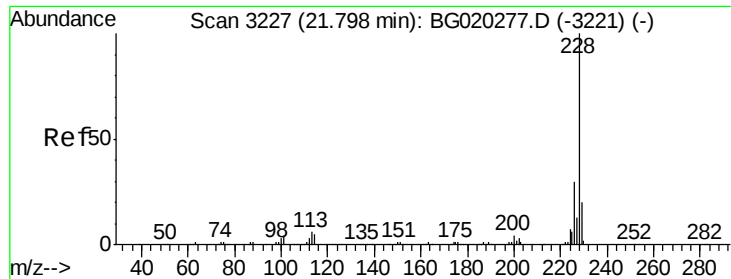

#85
Chrysene
Concen: 3.98 ng/ul
RT: 21.72 min Scan# 3214
Delta R.T. -0.08 min
Lab File: BG020278.D
Acq: 18 Dec 2015 16:57




Instrument :
BNA_G
ClientSampleId :
D9N40DL2


Tgt Ion: 228 Resp: 37780
Ion Ratio Lower Upper
228 100
226 25.8 23.9 35.9
229 20.3 15.6 23.4

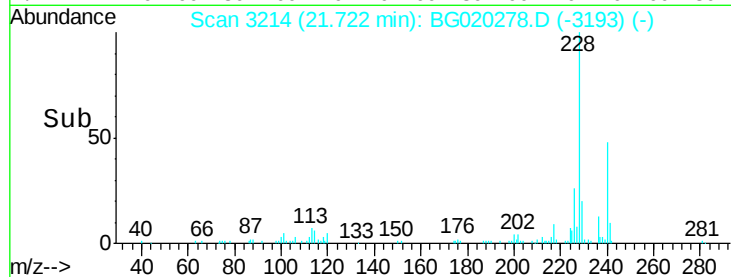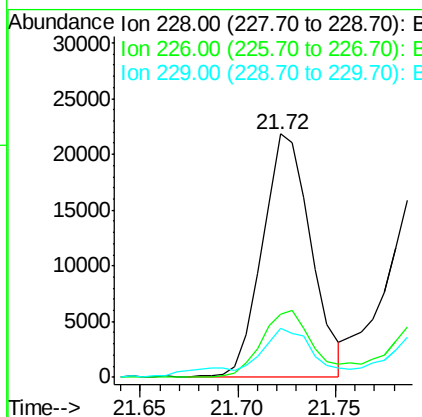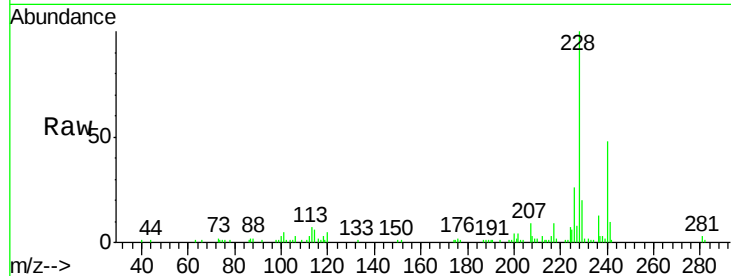

#88
Benzo(b)fluoranthene
Concen: 1.60 ng/ul
RT: 23.98 min Scan# 3598
Delta R.T. 0.00 min
Lab File: BG020278.D
Acq: 18 Dec 2015 16:57

Tgt Ion: 252 Resp: 15192
Ion Ratio Lower Upper
252 100
253 25.5 16.7 25.1#
125 10.2 6.2 9.2#

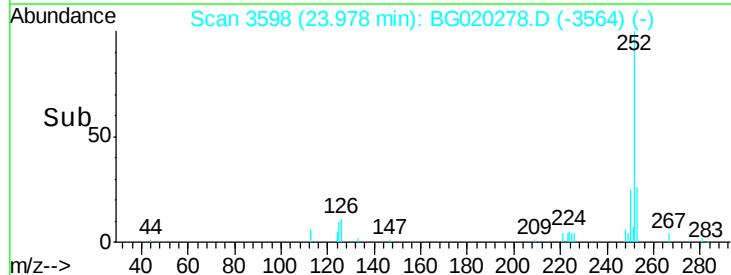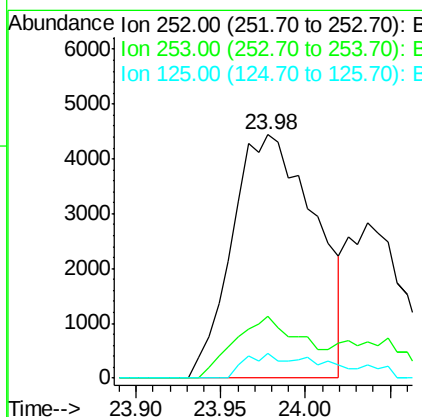

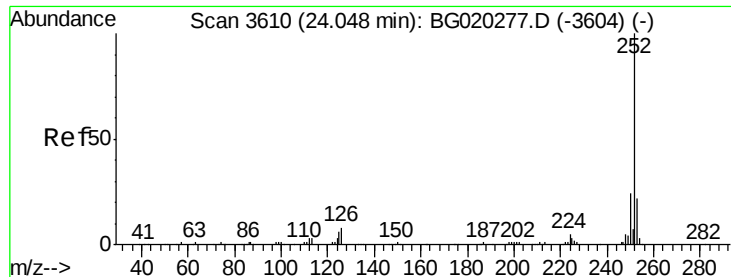

#89

Benzo(k)fluoranthene

Concen: 1.67 ng/ul

RT: 23.98 min Scan# 3598

Delta R.T. -0.07 min

Lab File: BG020278.D

Acq: 18 Dec 2015 16:57

Instrument :

BNA_G

ClientSampleId :

D9N40DL2


Tgt Ion:252 Resp: 15192

Ion Ratio Lower Upper

252 100

253 25.5 17.9 26.9




125 10.2 5.8 8.6#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

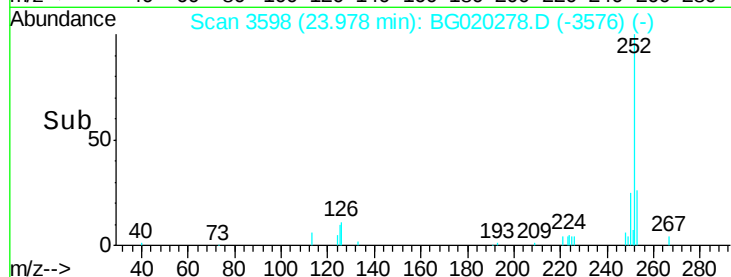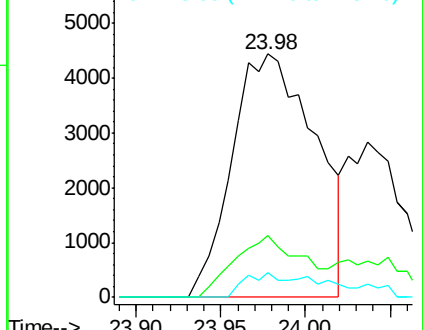

#91

Benzo(a)pyrene

Concen: 1.03 ng/ul

RT: 24.87 min Scan# 3749

Delta R.T. 0.00 min

Lab File: BG020278.D

Acq: 18 Dec 2015 16:57


Tgt Ion:252 Resp: 9296

Ion Ratio Lower Upper

252 100

253 21.9 17.0 25.4

125 8.1 6.2 9.4



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

