

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121915\
 Data File : BG020306.D
 Acq On : 19 Dec 2015 11:20
 Operator : UM/SJ
 Sample : PB87277BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK77

Quant Time: Dec 20 04:51:28 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Dec 20 04:48:33 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	16895	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	70895	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.72	164	51151	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.46	188	128521	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	171644	20.00	ng/ul	0.00
86) Perylene-d12	25.01	264	152361	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.47	96	2295	7.50	ng/uL	0.00
5) Phenol-d5	7.24	99	49576	33.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.41	67	31748	35.71	ng/ul	0.00
9) 2-Chlorophenol-d4	7.62	132	39434	36.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.79	113	43314	34.00	ng/ul	0.00
19) Nitrobenzene-d5	9.25	128	21077	38.14	ng/ul	0.00
22) 2-Nitrophenol-d4	9.98	143	24379	39.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	44704	35.89	ng/ul	0.00
29) 4-Chloroaniline-d4	11.04	131	48642	34.76	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	164971	39.87	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	184229	38.27	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	25258	34.04	ng/ul	0.00
58) Fluorene-d10	15.71	176	144079	38.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	23184	30.43	ng/ul	0.00
71) Anthracene-d10	17.57	188	238561	40.28	ng/ul	0.00
79) Pyrene-d10	19.85	212	294325	36.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	329825	43.40	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.79	70	1062	1.01 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121915\
Data File : BG020306.D
Acq On : 19 Dec 2015 11:20
Operator : UM/SJ
Sample : PB87277BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK77

Quant Time: Dec 20 04:51:28 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Dec 20 04:48:33 2015
Response via : Initial Calibration

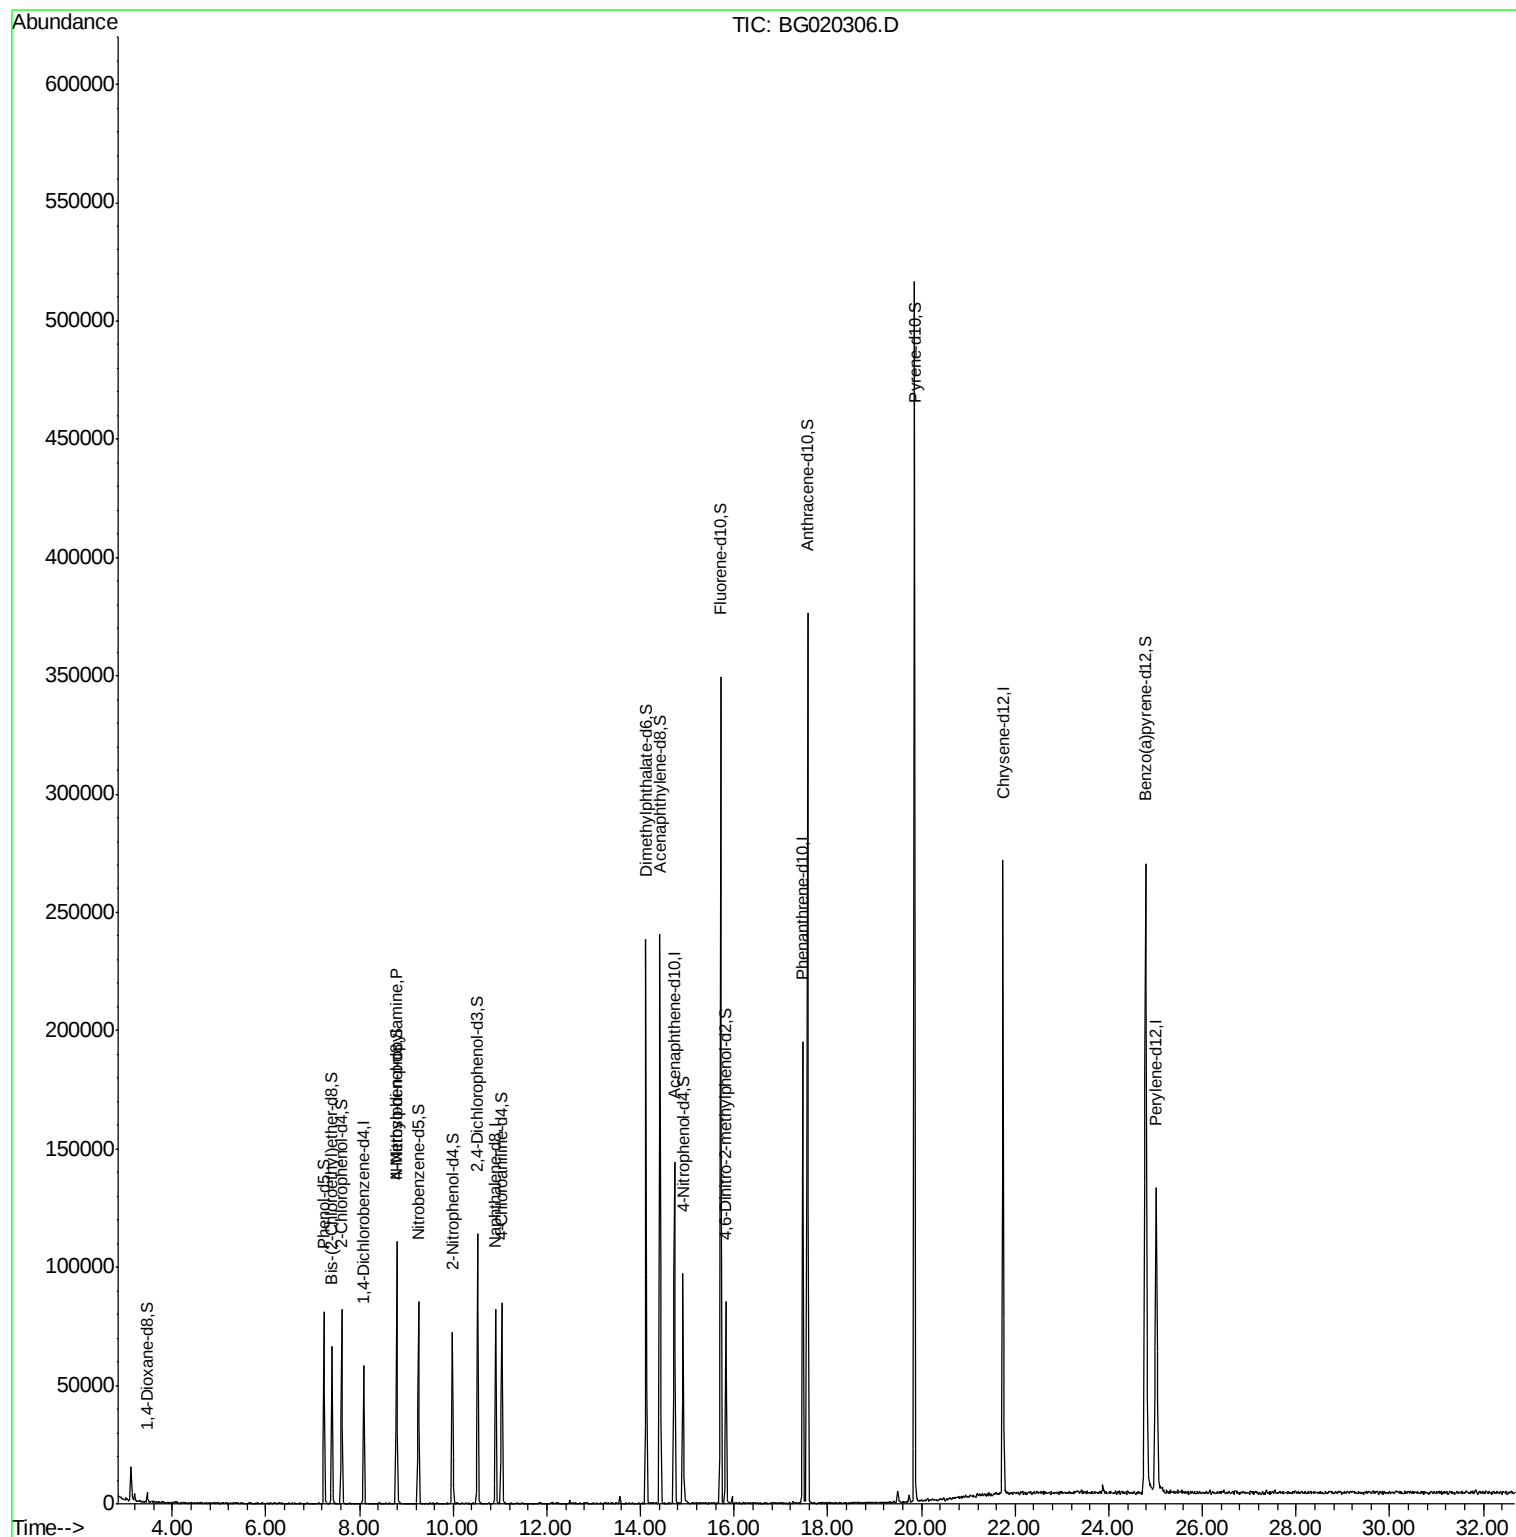

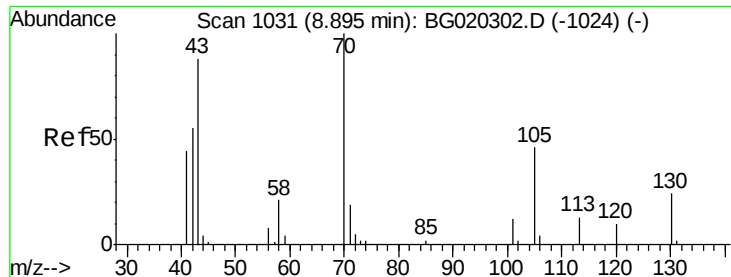

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.01 ng/ul
 RT: 8.79 min Scan# 1013
 Delta R.T. -0.10 min
 Lab File: BG020306.D
 Acq: 19 Dec 2015 11:20

Instrument :
 BNA_G
 ClientSampleId :
 SBLK77

Tgt Ion:	70	Resp:	1062
Ion	Ratio	Lower	Upper
70	100		
42	343.6	44.3	66.5#
101	0.0	7.6	11.4#
130	0.0	17.0	25.4#

