

(QT Reviewed)


```
Data Path   : Z:\HPCHEM1\BNA G\DATA\BG121915\  
Data File  : BG020277.D  
Acq On     : 18 Dec 2015  16:17  
Operator   : UM/SJ  
Sample     : SSTDCCC020  
Misc       :  
ALS Vial   : 2      Sample Multiplier: 1
```

Instrument :
BNA_G
LabSampleId :
SSTD02005

Quant Time: Dec 19 00:43:38 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 18 23:45:43 2015
Response via : Initial Calibration

Manual Integrations

apatel
12/22/2015 12:34:34 PM

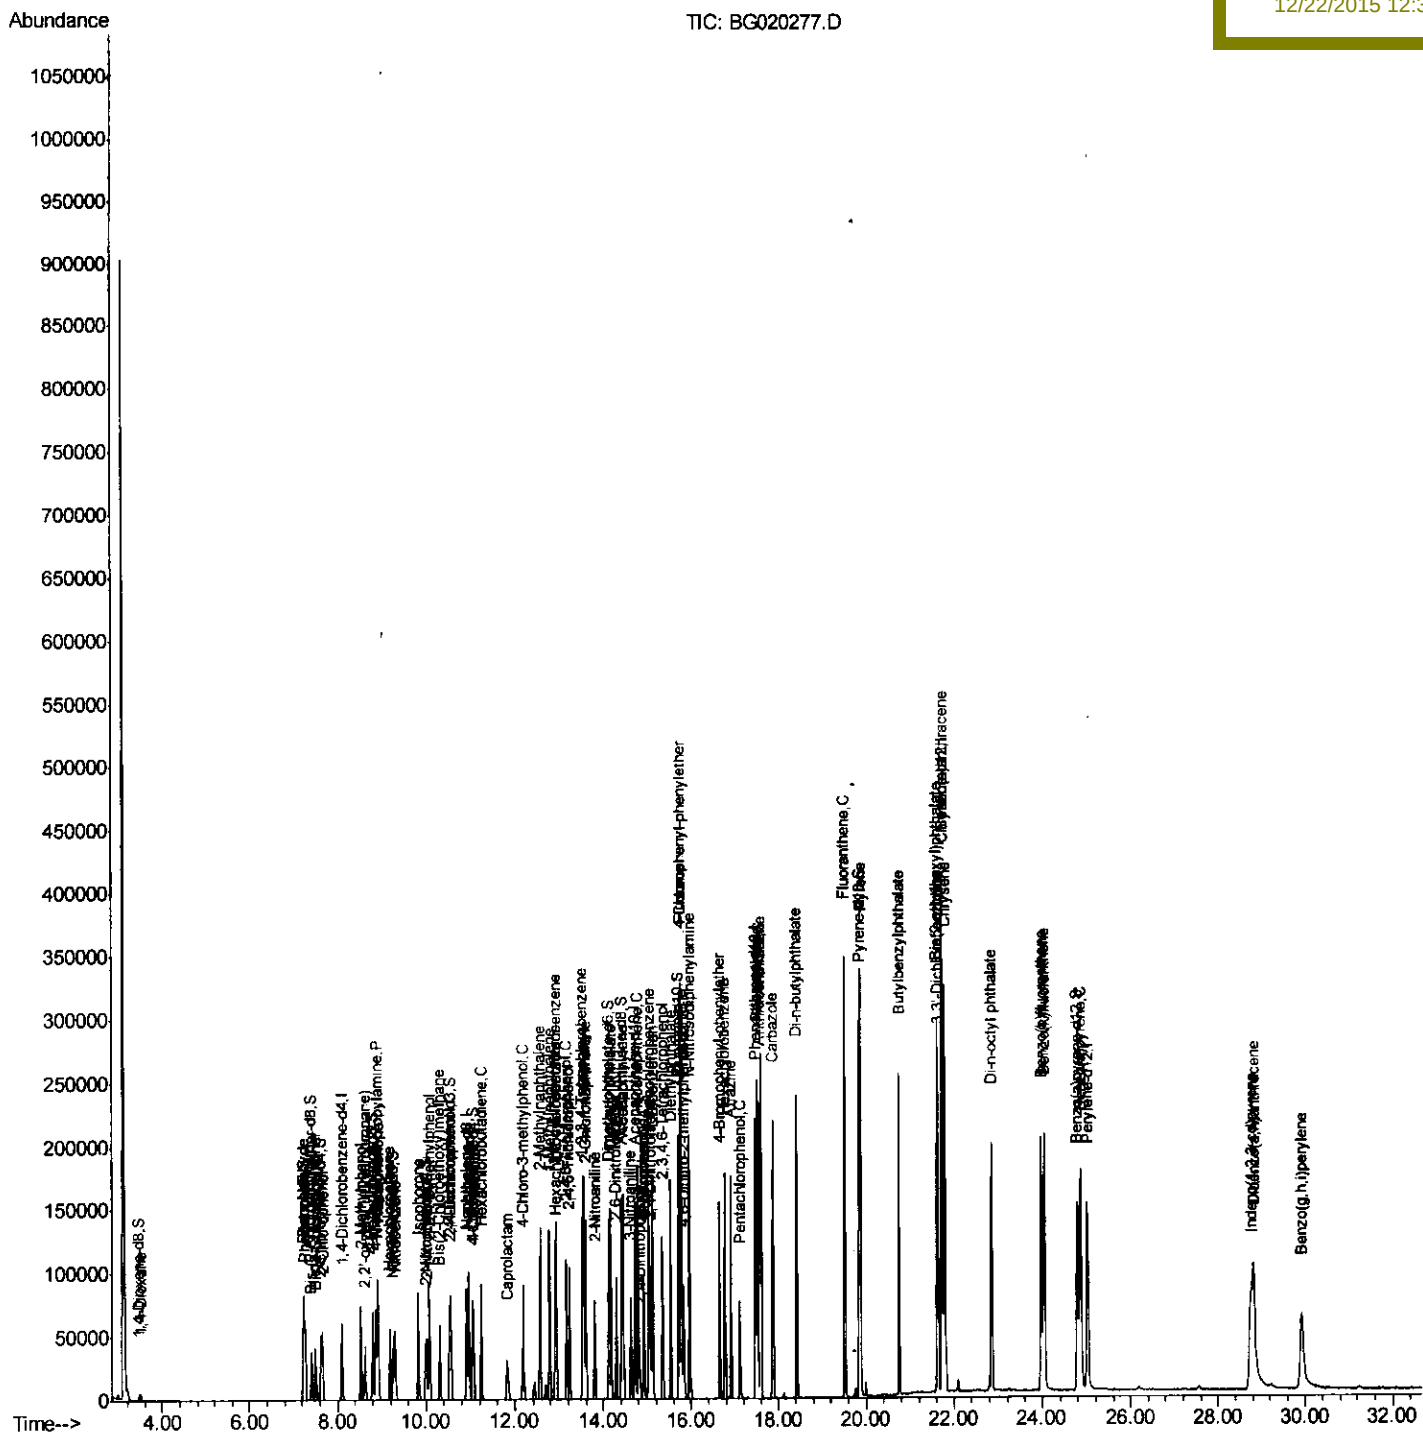

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121915\
Data File : BG020277.D
Acq On : 18 Dec 2015 16:17
Operator : UM/SJ
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
LabSampleId :
SSTD02005

Quant Time: Dec 18 23:50:00 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 18 23:45:43 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

apatel
12/22/2015 12:34:34 PM

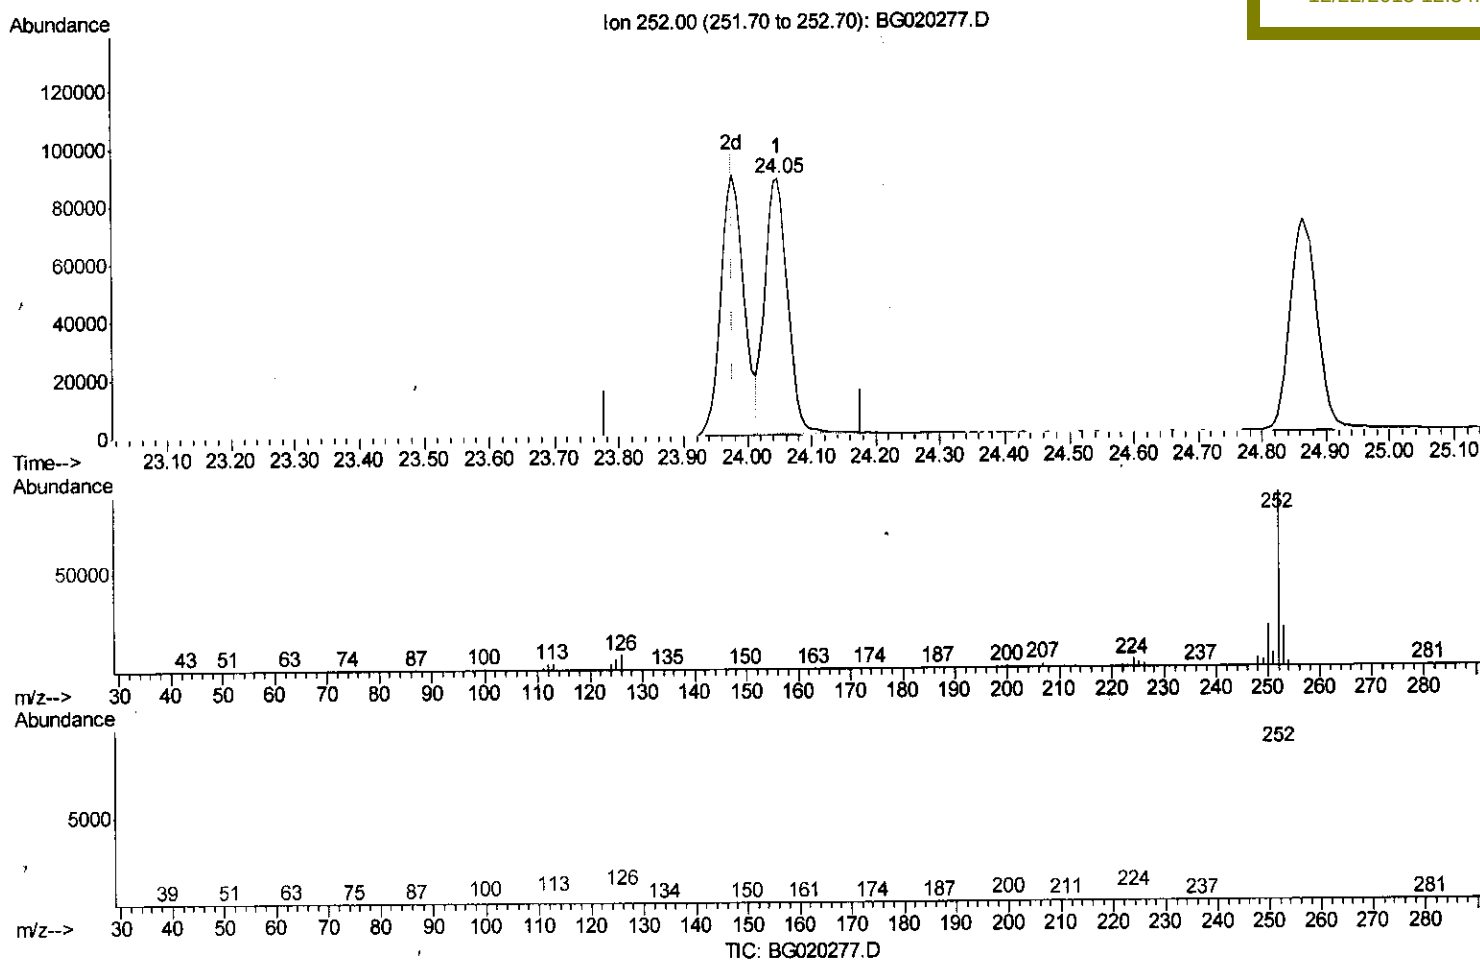

(88) Benzo(b)fluoranthene

24.048min (+0.070) 21.13ng/ui

response 215955

Ion	Exp%	Act%
252.00	100	100
253.00	20.90	22.43
125.00	7.70	6.34
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121915\
 Data File : BG020277.D
 Acq On : 18 Dec 2015 16:17
 Operator : UM/SJ
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleID :
 SSTD02005

Quant Time: Dec 18 23:50:00 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 18 23:45:43 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 12/22/2015 12:34:34 PM

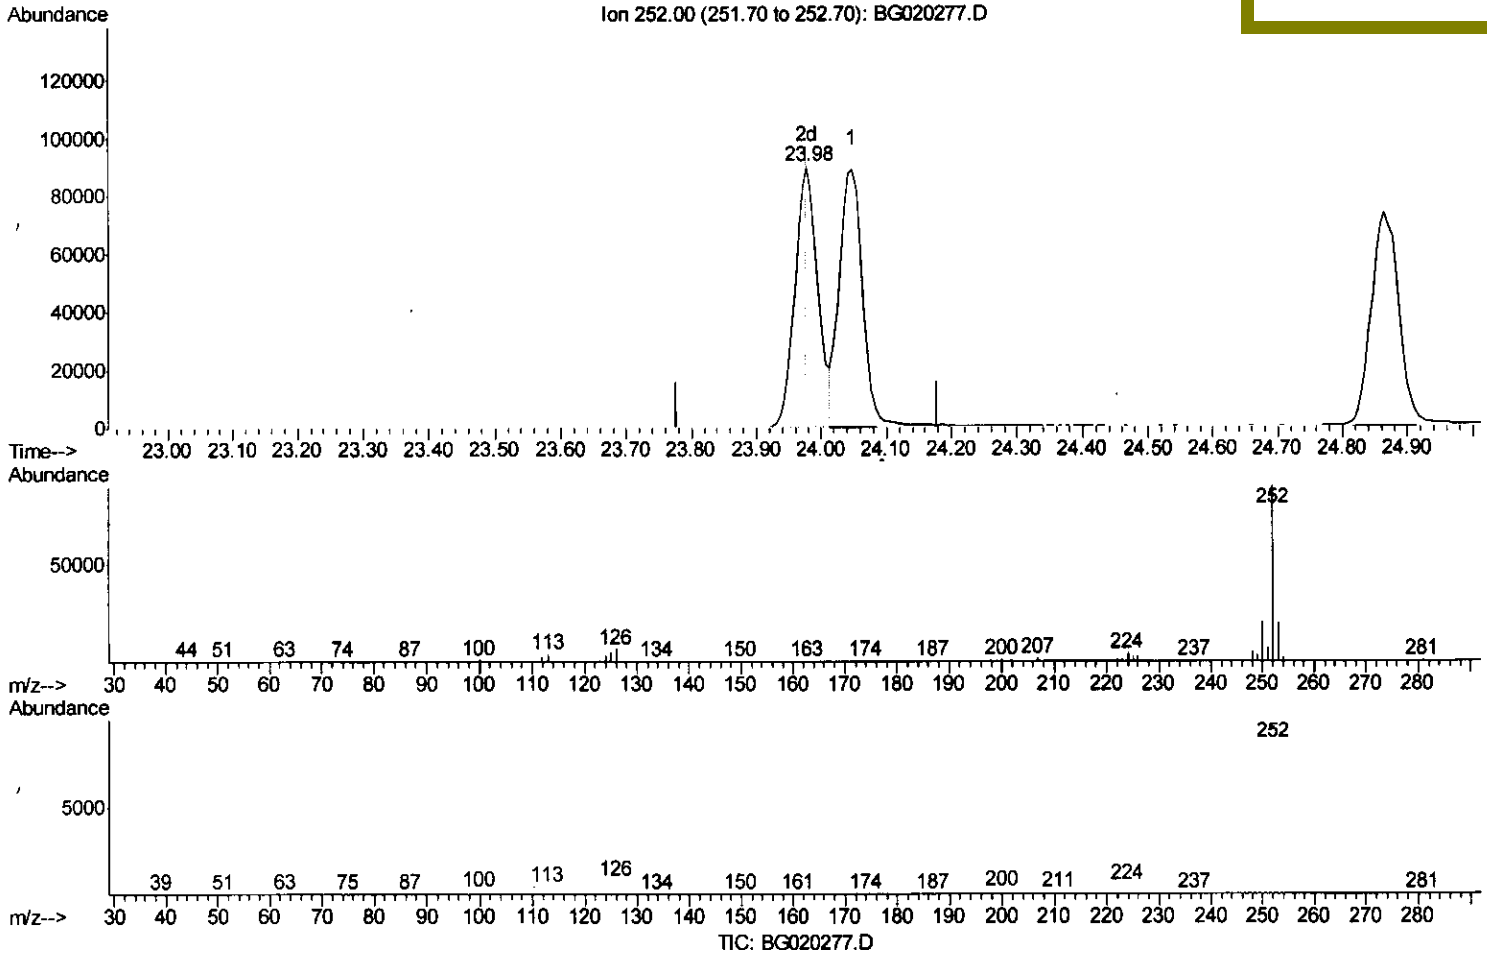

(88) Benzo(b)fluoranthene

23.977min (-0.001) 21.72ng/ul m U.M
 response 221994 12/22/15

Ion	Exp%	Act%
252.00	100	100
253.00	20.90	22.03
125.00	7.70	5.92#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121915\
 Data File : BG020277.D
 Acq On : 18 Dec 2015 16:17
 Operator : UM/SJ
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTD02005

Quant Time: Dec 19 00:43:38 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 18 23:45:43 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 12/22/2015 12:34:34 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	18155	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	78319	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	56928	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	147260	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	187721	20.00	ng/ul	0.00
86) Perylene-d12	25.02	264	169790	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.47	96	2723	8.28	ng/uL	0.00
5) Phenol-d5	7.24	99	32243	20.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.41	67	18946	19.83	ng/ul	0.00
9) 2-Chlorophenol-d4	7.62	132	25092	21.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	27837	20.33	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	12498	20.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.98	143	15107	22.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	29615	21.52	ng/ul	0.00
29) 4-Chloroaniline-d4	11.04	131	34521	22.33	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	97999	21.28	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	114765	21.42	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	16283	19.72	ng/ul	0.00
58) Fluorene-d10	15.72	176	86693	20.76	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	16630	19.05	ng/ul	0.00
71) Anthracene-d10	17.57	188	146171	21.54	ng/ul	0.00
79) Pyrene-d10	19.85	212	169402	19.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	187820	22.18	ng/ul	0.00

Target Compounds

					Ovalue	
2) 1,4-Dioxane	3.50	88	3432	7.07	ng/uL#	86
4) Benzaldehyde	7.23	77	20985	20.25	ng/ul	98
6) Phenol	7.27	94	34133	19.91	ng/ul	99
8) Bis(2-Chloroethyl)ether	7.51	93	24168	20.55	ng/ul	96
10) 2-Chlorophenol	7.66	128	25941	21.27	ng/ul	98
11) 2-Methylphenol	8.53	108	25620	19.59	ng/ul	86
12) 2,2'-oxybis(1-Chloropropan	8.62	45	33290	19.65	ng/ul	98
14) Acetophenone	8.92	105	43728	20.40	ng/ul	96
15) N-Nitroso-di-n-propylamine	8.90	70	22631	19.94	ng/ul#	97
16) 4-Methylphenol	8.86	108	28827	19.91	ng/ul	95
17) Hexachloroethane	9.18	117	10711	20.90	ng/ul	95
20) Nitrobenzene	9.30	77	33390	20.64	ng/ul	98
21) Isophorone	9.82	82	62985	20.39	ng/ul	97
23) 2-Nitrophenol	10.02	139	16199	22.24	ng/ul	98
24) 2,4-Dimethylphenol	10.06	107	34629	20.93	ng/ul	98
25) Bis(2-Chloroethoxy)methane	10.31	93	34823	20.81	ng/ul	96
27) 2,4-Dichlorophenol	10.55	162	30710	21.73	ng/ul	96
28) Naphthalene	10.96	128	87900	21.49	ng/ul	97
30) 4-Chloroaniline	11.06	127	34985	22.17	ng/ul	94
31) Hexachlorobutadiene	11.25	225	23916	22.70	ng/ul	97
32) Caprolactam	11.82	113	9753	19.55	ng/ul	99
33) 4-Chloro-3-methylphenol	12.18	107	33937	20.20	ng/ul	93
34) 2-Methylnaphthalene	12.56	142	67248	21.53	ng/ul	96

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121915\
 Data File : BG020277.D
 Acq On : 18 Dec 2015 16:17
 Operator : UM/SJ
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTD02005

Quant Time: Dec 19 00:43:38 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 18 23:45:43 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 12/22/2015 12:34:34 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	12.78	142	62524	20.82	ng/ul	96
37) 1,2,4,5-Tetrachlorobenzene	12.93	216	47542	22.25	ng/ul	99
38) Hexachlorocyclopentadiene	12.90	237	18537	14.04	ng/ul	94
39) 2,4,6-Trichlorophenol	13.16	196	28990	21.15	ng/ul	99
40) 2,4,5-Trichlorophenol	13.23	196	31775	20.86	ng/ul	96
41) 1,1'-Biphenyl	13.56	154	93047	21.66	ng/ul	94
42) 2-Chloronaphthalene	13.61	162	73756	21.45	ng/ul	98
43) 2-Nitroaniline	13.81	65	22698	19.42	ng/ul	90
45) Dimethylphthalate	14.17	163	100296	21.33	ng/ul	99
46) 2,6-Dinitrotoluene	14.29	165	21396	21.99	ng/ul	97
48) Acenaphthylene	14.45	152	120013	21.09	ng/ul	99
49) 3-Nitroaniline	14.62	138	20890	22.12	ng/ul	96
50) Acenaphthene	14.79	153	80811	21.10	ng/ul	98
51) 2,4-Dinitrophenol	14.84	184	8482	15.32	ng/ul	93
53) 4-Nitrophenol	14.93	109	15364	19.34	ng/ul	94
54) Dibenzofuran	15.12	168	121632	21.35	ng/ul	100
55) 2,4-Dinitrotoluene	15.08	165	31316	21.93	ng/ul	89
56) 2,3,4,6-Tetrachlorophenol	15.35	232	30919	21.11	ng/ul	98
57) Diethylphthalate	15.53	149	103020	21.11	ng/ul	98
59) Fluorene	15.77	166	98295	21.49	ng/ul	100
60) 4-Chlorophenyl-phenylether	15.76	204	56061	21.73	ng/ul	96
61) 4-Nitroaniline	15.79	138	22248	21.79	ng/ul	95
64) 4,6-Dinitro-2-methylphenol	15.84	198	16625	17.74	ng/ul#	98
65) N-Nitrosodiphenylamine	15.97	169	87380	21.34	ng/ul	98
66) 4-Bromophenyl-phenylether	16.66	248	38938	22.53	ng/ul	96
67) Hexachlorobenzene	16.77	284	41759	22.50	ng/ul#	89
68) Atrazine	16.92	200	37891	21.70	ng/ul	99
69) Pentachlorophenol	17.11	266	16455	14.70	ng/ul	96
70) Phenanthrene	17.51	178	172526	21.42	ng/ul	98
72) Anthracene	17.60	178	175254	21.45	ng/ul	99
73) 1,2,3,4-Tetrachlorobenzene	13.53	216	51081	22.14	ng/uL	95
74) Pentachlorobenzene	15.04	250	47947	22.41	ng/uL	96
75) Carbazole	17.87	167	151293	22.04	ng/ul	99
76) Di-n-butylphthalate	18.42	149	173750	21.78	ng/ul	99
77) Fluoranthene	19.52	202	220364	23.41	ng/ul	98
80) Pyrene	19.88	202	222560	19.59	ng/ul	99
81) Butylbenzylphthalate	20.76	149	78845	19.97	ng/ul	93
82) 3,3'-Dichlorobenzidine	21.64	252	79645	23.22	ng/ul	97
83) Benzo(a)anthracene	21.73	228	233922	21.36	ng/ul	99
84) Bis(2-ethylhexyl)phthalate	21.62	149	109223	19.35	ng/ul	99
85) Chrysene	21.80	228	221972	21.52	ng/ul	99
87) Di-n-octyl phthalate	22.85	149	139956	20.36	ng/ul	100
88) Benzo(b)fluoranthene	23.98	252	221994m	21.72	ng/ul	99
89) Benzo(k)fluoranthene	24.05	252	216697	22.10	ng/ul	99
91) Benzo(a)pyrene	24.86	252	215889	22.29	ng/ul	98
92) Indeno(1,2,3-cd)pyrene	28.75	276	218561	18.95	ng/ul	95
93) Dibenzo(a,h)anthracene	28.82	278	185897	19.41	ng/ul	97
94) Benzo(a,h,i)perylene	29.93	276	152088	16.08	ng/ul	98

U.M
 12/22/15

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121915\
Data File : BG020277.D
Acq On : 18 Dec 2015 16:17
Operator : UM/SJ
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 19 00:43:38 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 18 23:45:43 2015
Response via : Initial Calibration

Instrument :
BNA_G
LabSampleId :
SSTD02005

Manual Integrations
APPROVED

apatel
12/22/2015 12:34:34 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						