

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121915\
 Data File : BG020324.D
 Acq On : 19 Dec 2015 23:01
 Operator : UM/SJ
 Sample : G4866-06
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E43L8

Quant Time: Dec 20 05:59:07 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Dec 20 05:53:46 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	24715	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	108184	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.72	164	77470	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.46	188	190845	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	237852	20.00	ng/ul	0.00
86) Perylene-d12	25.01	264	224778	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	2528	5.65	ng/uL	0.00
5) Phenol-d5	7.24	99	64764	29.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.40	67	41903	32.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.62	132	51894	32.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.79	113	55492	29.77	ng/ul	0.00
19) Nitrobenzene-d5	9.25	128	29131	34.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.98	143	34513	36.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	63061	33.18	ng/ul	0.00
29) 4-Chloroaniline-d4	11.04	131	74232	34.77	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	221018	35.27	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	254326	34.88	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	30642	27.27	ng/ul	0.00
58) Fluorene-d10	15.71	176	199940	35.18	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	34261	30.28	ng/ul	0.00
71) Anthracene-d10	17.56	188	313817	35.69	ng/ul	0.00
79) Pyrene-d10	19.85	212	390785	35.25	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	443248	39.53	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.17	163	111187	17.37	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121915\
Data File : BG020324.D
Acq On : 19 Dec 2015 23:01
Operator : UM/SJ
Sample : G4866-06
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E43L8

Quant Time: Dec 20 05:59:07 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Dec 20 05:53:46 2015
Response via : Initial Calibration

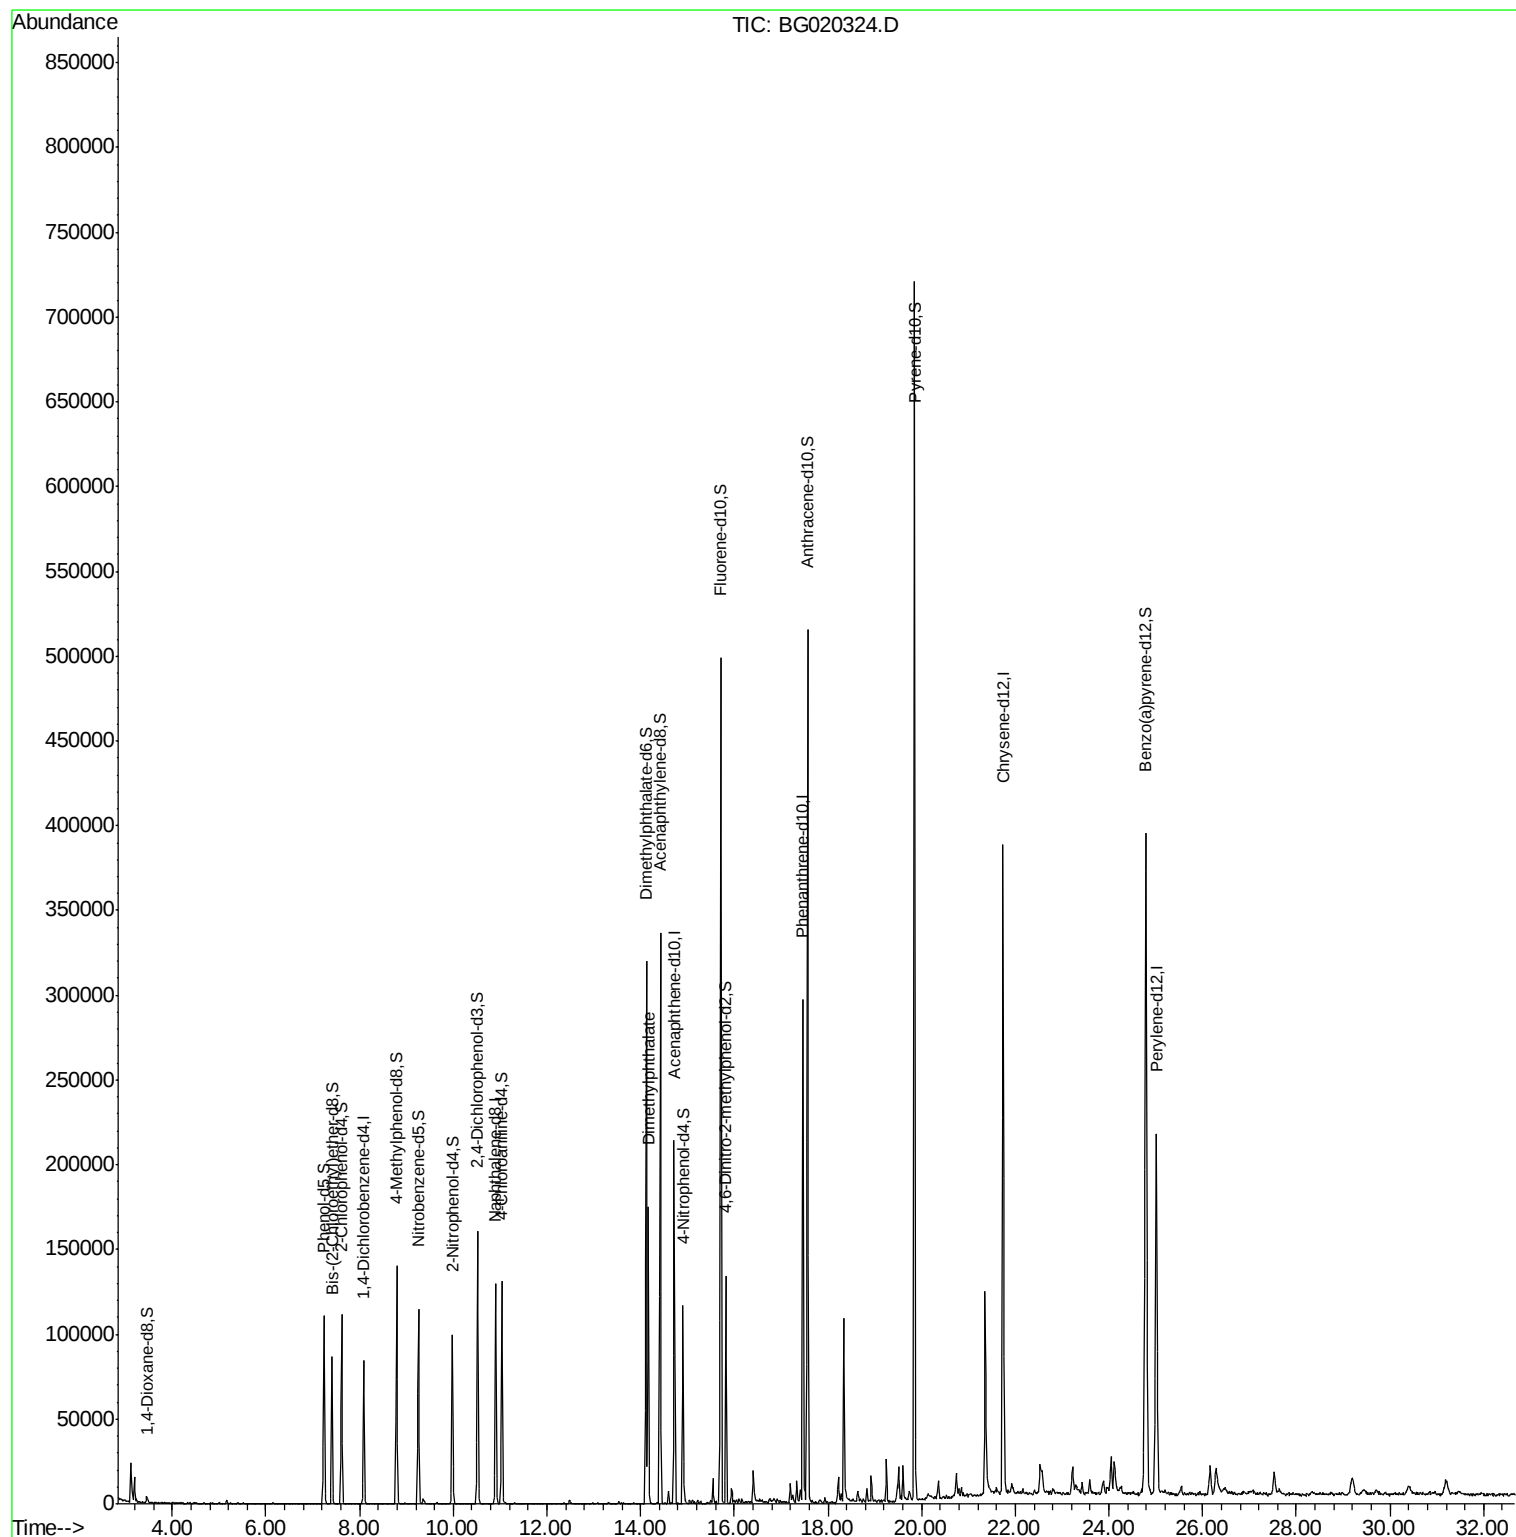

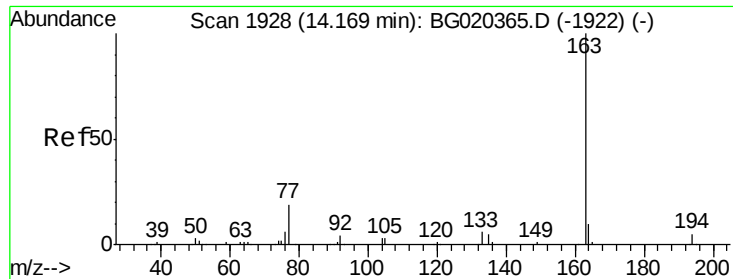

#45

Dimethylphthalate

Concen: 17.37 ng/ul

RT: 14.17 min Scan# 1928

Delta R.T. 0.00 min

Lab File: BG020324.D

Acq: 19 Dec 2015 23:01

Instrument :

BNA_G

ClientSampleId :

E43L8


Tot Ion:163 Resp: 111187

Ion Ratio Lower Upper

163 100

194 5.4 3.5 5.3#

164 10.9 7.7 11.5

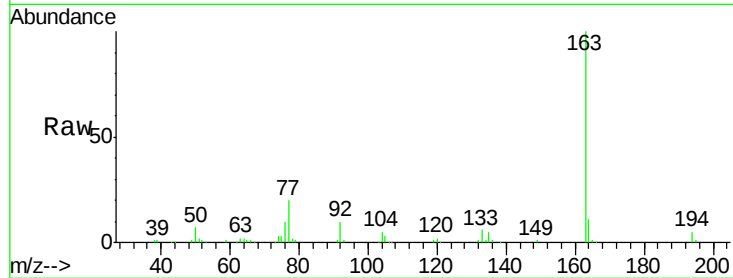

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

