

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121915\
 Data File : BG020303.D
 Acq On : 19 Dec 2015 9:24
 Operator : UM/SJ
 Sample : PB87276BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	42	47	55	rBV2	13253	24683	3.26%	0.380%
2	3.187	56	59	66	rVB3	3328	4652	0.61%	0.072%
3	3.387	89	93	94	rVB	750	838	0.11%	0.013%
4	3.463	102	106	112	rVB	4435	5673	0.75%	0.087%
5	7.241	742	749	761	rVB	81971	136018	17.97%	2.095%
6	7.412	771	778	788	rVB	63730	104448	13.80%	1.609%
7	7.617	807	813	822	rVB	83412	137697	18.19%	2.121%
8	8.093	888	894	902	rVB	52546	88140	11.65%	1.358%
9	8.792	1005	1013	1023	rBB	107808	183827	24.29%	2.831%
10	9.256	1083	1092	1101	rBB	83183	143858	19.01%	2.216%
11	9.979	1209	1215	1222	rBV	71455	125755	16.62%	1.937%
12	10.520	1300	1307	1317	rBV	113313	197508	26.10%	3.042%
13	10.907	1366	1373	1381	rBB	79510	138170	18.26%	2.128%
14	11.037	1389	1395	1409	rVB	87547	155028	20.48%	2.388%
15	12.482	1636	1641	1645	rBB2	1656	2284	0.30%	0.035%
16	14.121	1914	1920	1927	rBV	241376	337448	44.59%	5.198%
17	14.415	1962	1970	1978	rBV	242475	386757	51.10%	5.957%
18	14.721	2016	2022	2031	rVB2	138562	226380	29.91%	3.487%
19	14.909	2047	2054	2063	rBV	94688	154646	20.43%	2.382%
20	14.997	2068	2069	2073	rVV	1200	1176	0.16%	0.018%
21	15.044	2075	2077	2083	rVB2	745	1208	0.16%	0.019%
22	15.714	2184	2191	2198	rBV	336058	521958	68.97%	8.040%
23	15.819	2204	2209	2218	rBV	86128	124520	16.45%	1.918%
24	15.954	2228	2232	2235	rVB2	3001	3904	0.52%	0.060%
25	17.253	2450	2453	2460	rBV2	802	1493	0.20%	0.023%
26	17.464	2482	2489	2499	rBV2	204999	304135	40.19%	4.685%
27	17.564	2499	2506	2515	rVB2	395909	597876	79.00%	9.209%
28	18.892	2728	2732	2734	rBV2	611	799	0.11%	0.012%
29	19.480	2827	2832	2835	rBV	4112	5709	0.75%	0.088%
30	19.515	2835	2838	2843	rVB	1547	2285	0.30%	0.035%
31	19.738	2872	2876	2882	rBV	3896	5304	0.70%	0.082%
32	19.850	2886	2895	2906	rBV	530632	755491	99.82%	11.637%
33	20.144	2942	2945	2947	rBV2	628	884	0.12%	0.014%
34	20.526	3005	3010	3012	rBV3	1016	1763	0.23%	0.027%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121915\
 Data File : BG020303.D
 Acq On : 19 Dec 2015 9:24
 Operator : UM/SJ
 Sample : PB87276BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

35	20.602	3018	3023	3024	rBV3	879	1051	0.14%	0.016%
36	20.614	3024	3025	3028	rBV3	1032	908	0.12%	0.014%
37	20.755	3047	3049	3052	rVB2	912	758	0.10%	0.012%
38	21.101	3106	3108	3110	rBV3	834	1047	0.14%	0.016%
39	21.425	3161	3163	3164	rBV2	1260	849	0.11%	0.013%
40	21.742	3210	3217	3229	rVB	269199	423529	55.96%	6.524%
41	22.171	3289	3290	3293	rBV3	1027	1227	0.16%	0.019%
42	22.588	3360	3361	3366	rVB4	1439	885	0.12%	0.014%
43	22.882	3409	3411	3415	rBV5	1052	1317	0.17%	0.020%
44	23.123	3451	3452	3454	rBV	1183	967	0.13%	0.015%
45	23.228	3469	3470	3473	rBV2	1621	1796	0.24%	0.028%
46	23.346	3487	3490	3491	rBV2	1103	1296	0.17%	0.020%
47	23.463	3508	3510	3513	rBV4	1521	1302	0.17%	0.020%
48	23.880	3575	3581	3587	rVB7	3331	6494	0.86%	0.100%
49	24.233	3639	3641	3642	rVB2	1296	863	0.11%	0.013%
50	24.468	3679	3681	3684	rBV4	824	814	0.11%	0.013%
51	24.668	3713	3715	3717	rVB	944	881	0.12%	0.014%
52	24.703	3720	3721	3723	rVB	1581	824	0.11%	0.013%
53	24.791	3723	3736	3750	rBV	259960	756816	100.00%	11.657%
54	25.014	3764	3774	3791	rVB2	124419	362280	47.87%	5.580%
55	25.473	3850	3852	3855	rVB2	1190	820	0.11%	0.013%
56	25.614	3875	3876	3878	rVB2	1342	865	0.11%	0.013%
57	25.649	3878	3882	3883	rBV2	1142	1495	0.20%	0.023%
58	25.802	3905	3908	3913	rBV5	1053	1889	0.25%	0.029%
59	25.866	3917	3919	3922	rVB3	1139	995	0.13%	0.015%
60	25.913	3925	3927	3928	rVV	1464	799	0.11%	0.012%
61	25.960	3931	3935	3938	rBV4	1398	2055	0.27%	0.032%
62	26.037	3946	3948	3951	rBV3	1496	1516	0.20%	0.023%
63	26.084	3954	3956	3958	rVB3	1331	1206	0.16%	0.019%
64	26.507	4026	4028	4031	rBV3	775	799	0.11%	0.012%
65	26.560	4035	4037	4039	rBV3	843	821	0.11%	0.013%
66	27.018	4113	4115	4117	rBV3	920	1000	0.13%	0.015%
67	27.177	4140	4142	4145	rBV4	789	904	0.12%	0.014%
68	27.400	4178	4180	4183	rVB4	935	759	0.10%	0.012%
69	27.506	4196	4198	4201	rVB3	948	913	0.12%	0.014%
70	27.529	4201	4202	4203	rBV	1296	851	0.11%	0.013%
71	27.588	4210	4212	4215	rVB4	1482	1472	0.19%	0.023%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121915\
 Data File : BG020303.D
 Acq On : 19 Dec 2015 9:24
 Operator : UM/SJ
 Sample : PB87276BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

72	27.623	4217	4218	4221	rVB3	1618	1079	0.14%	0.017%
73	27.664	4221	4225	4226	rBV4	1160	1540	0.20%	0.024%
74	27.911	4265	4267	4269	rVB3	1718	1090	0.14%	0.017%
75	27.946	4269	4273	4275	rBV4	1063	1644	0.22%	0.025%
76	28.128	4303	4304	4306	rBV2	955	789	0.10%	0.012%
77	28.158	4307	4309	4312	rVV3	964	1005	0.13%	0.015%
78	28.428	4354	4355	4358	rVB2	957	802	0.11%	0.012%
79	28.452	4358	4359	4360	rBV	1395	774	0.10%	0.012%
80	28.751	4409	4410	4412	rBV2	1234	877	0.12%	0.014%
81	28.769	4412	4413	4415	rBV2	1043	878	0.12%	0.014%
82	28.951	4442	4444	4446	rBV3	980	1209	0.16%	0.019%
83	29.045	4458	4460	4464	rBV5	1256	1842	0.24%	0.028%
84	29.145	4475	4477	4480	rBV4	1060	819	0.11%	0.013%
85	29.215	4487	4489	4492	rBV2	1184	840	0.11%	0.013%
86	29.456	4528	4530	4532	rBV3	1050	771	0.10%	0.012%
87	30.913	4777	4778	4781	rBV2	1117	1010	0.13%	0.016%
88	31.002	4792	4793	4796	rBV3	954	1031	0.14%	0.016%
89	31.148	4816	4818	4819	rBV2	987	766	0.10%	0.012%
90	31.231	4830	4832	4834	rVB3	1272	829	0.11%	0.013%
91	31.366	4853	4855	4857	rBV3	976	962	0.13%	0.015%
92	31.718	4912	4915	4917	rBV3	843	1182	0.16%	0.018%
93	31.959	4954	4956	4959	rVB3	959	965	0.13%	0.015%
94	32.147	4986	4988	4991	rBV4	1590	2243	0.30%	0.035%


Sum of corrected areas: 6492325

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121915\
Data File : BG020303.D
Acq On : 19 Dec 2015 9:24
Operator : UM/SJ
Sample : PB87276BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK76

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

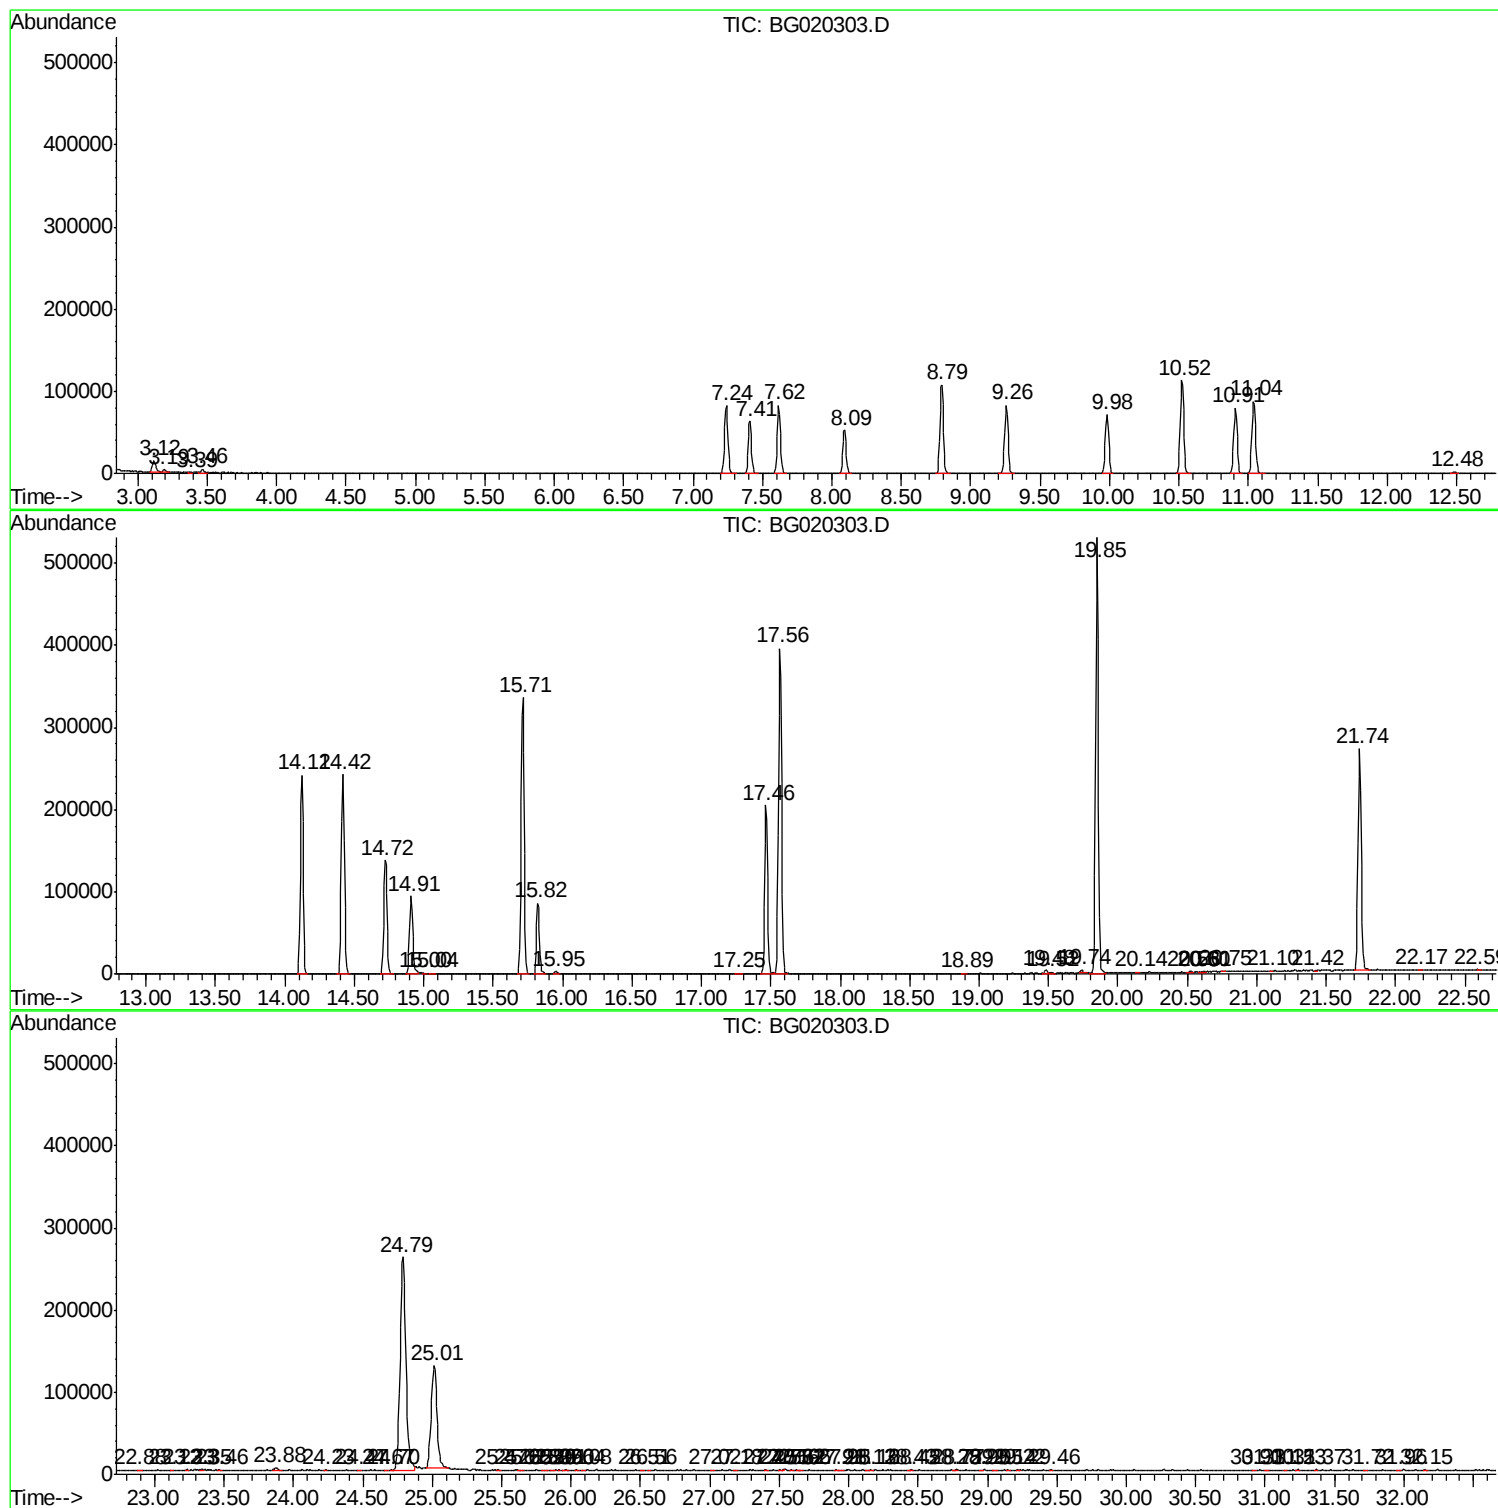

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121915\
Data File : BG020303.D
Acq On : 19 Dec 2015 9:24
Operator : UM/SJ
Sample : PB87276BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK76

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121915\
Data File : BG020303.D
Acq On : 19 Dec 2015 9:24
Operator : UM/SJ
Sample : PB87276BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK76

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc