


Data Path : Z:\HPCHEM1\BNA G\DATA\BG121915\
 Data File : BG020267.D
 Acq On : 18 Dec 2015 9:44
 Operator : UM/SJ
 Sample : DFTPP10
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP10

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION
 Last Update : Mon Dec 21 07:46:34 2015

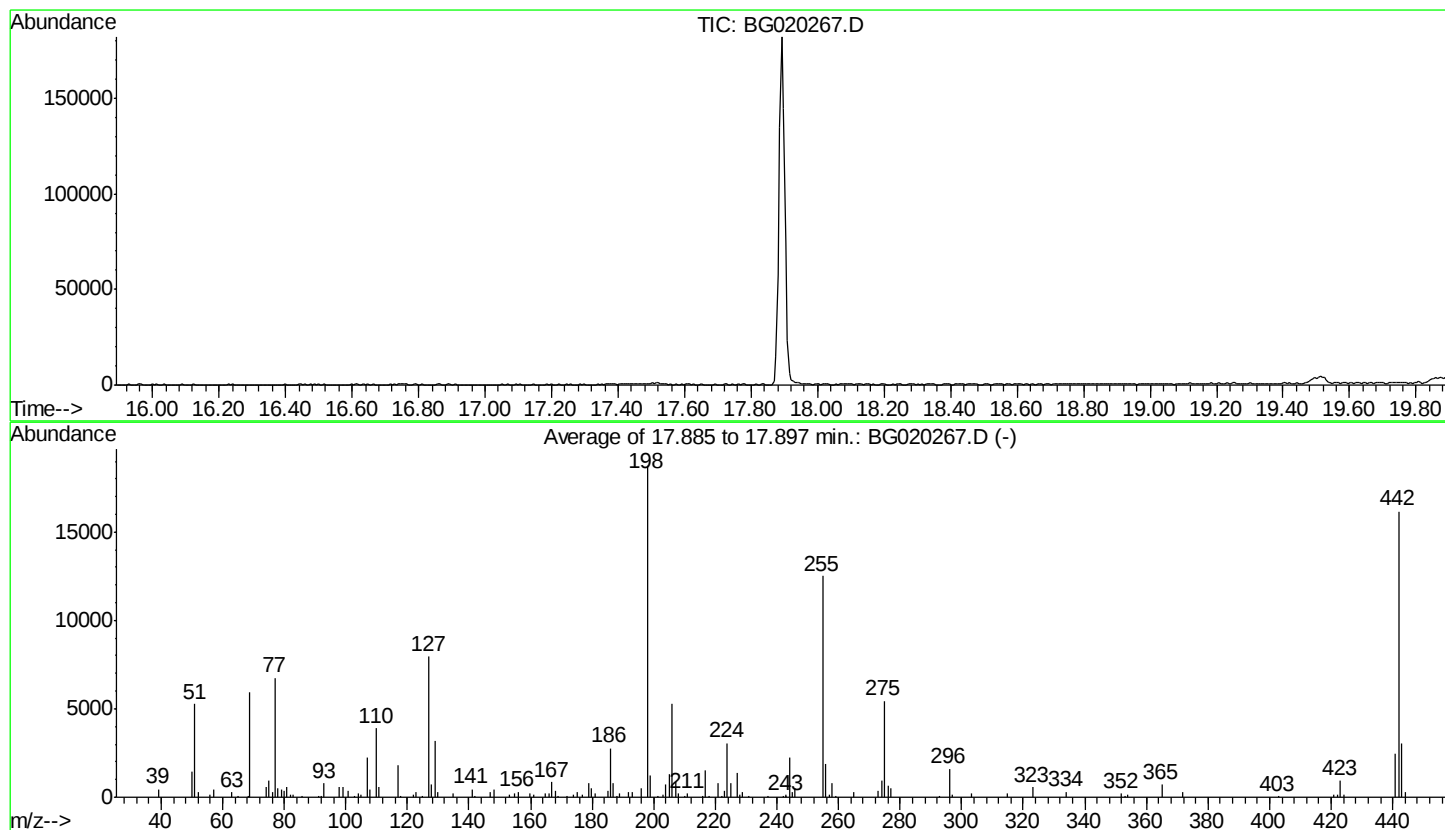

AutoFind: Scans 2561, 2562, 2563; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	5262	PASS
68	69	0.00	2	1.1	67	PASS
69	198	0.00	100	31.8	5963	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.4	7945	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18749	PASS
199	198	5	9	6.6	1242	PASS
275	198	10	60	29.1	5449	PASS
365	198	1	100	3.8	711	PASS
441	442	0.01	24	15.1	2439	PASS
442	198	50	100	86.3	16175	PASS
443	442	15	24	19.0	3071	PASS

Scan 2556 (17.856 min): BG020267.D
DFTPP10

m/z	Abundance
39.90	153.0
43.90	198.0

Instrument :
BNA_G
ClientSampleId :
DFTPP10

m/z	Abundance
39.00	437.0
43.90	156.0
50.00	1491.0
51.00	5421.0
52.00	252.0
55.90	178.0
57.00	473.0
62.90	172.0
65.00	177.0
68.90	6017.0
74.00	540.0
74.90	956.0
76.10	392.0
77.00	6711.0
78.00	463.0
79.00	473.0
79.90	404.0
81.00	710.0
82.90	154.0
92.90	781.0
97.90	480.0
98.90	528.0
100.90	355.0
103.90	320.0
105.00	186.0
107.00	2380.0
108.00	398.0
109.90	3780.0
110.90	581.0
117.00	1681.0
121.80	173.0
122.90	248.0
127.00	7428.0
128.00	713.0
128.90	3063.0
130.00	288.0
134.90	235.0
140.90	510.0
142.00	176.0
147.00	189.0
147.90	421.0
154.90	258.0
156.00	292.0
164.90	201.0
166.10	197.0
166.90	824.0
167.90	355.0
173.90	162.0
175.00	261.0
178.90	714.0
179.90	501.0
181.00	178.0
184.90	340.0
186.00	2472.0
186.90	701.0
188.90	277.0
192.00	235.0
193.00	193.0
195.90	496.0
197.90	16800.0
198.90	1195.0
203.00	158.0
203.90	525.0
205.00	1111.0
206.00	4770.0
207.00	796.0
207.90	174.0
211.00	188.0
216.90	1157.0
221.00	734.0
222.80	266.0
224.00	2545.0
225.00	611.0
226.90	1171.0
228.90	297.0
242.80	186.0
243.90	2157.0
244.90	250.0
245.90	431.0
254.90	11042.0
255.90	1496.0
256.90	162.0
257.90	738.0
264.90	263.0
272.90	335.0
273.90	762.0
274.90	4479.0
276.00	616.0
276.90	376.0
296.00	1224.0
314.80	191.0
323.00	549.0

Instrument :
BNA_G
ClientSampleId :
DFTPP10

333.90	283.0
352.00	223.0
354.00	177.0
364.90	639.0
371.90	217.0
422.90	735.0
441.00	1634.0
442.00	11830.0
442.90	1985.0
443.90	268.0

Instrument :
BNA_G
ClientSampleId :
DFTPP10

m/z	Abundance
39.00	482.0
40.00	170.0
43.90	158.0
50.00	1678.0
51.00	6108.0
52.00	411.0
55.90	260.0
56.90	416.0
62.90	383.0
68.90	7253.0
74.00	848.0
75.00	1129.0
76.00	282.0
77.00	8192.0
78.00	532.0
78.90	443.0
79.90	389.0
80.90	612.0
82.00	171.0
83.00	183.0
85.90	203.0
91.90	159.0
92.90	870.0
98.00	760.0
98.90	648.0
100.90	372.0
102.90	179.0
103.90	161.0
105.00	248.0
107.00	2532.0
108.00	462.0
109.90	4736.0
110.90	710.0
116.90	2148.0
117.90	210.0
121.90	217.0
122.90	309.0
127.00	9281.0
127.90	751.0
128.90	3789.0
129.90	272.0
135.00	262.0
141.00	523.0
146.90	367.0
147.90	485.0
152.90	274.0
154.90	298.0
156.00	375.0
159.90	283.0
160.90	258.0
164.80	173.0
165.90	190.0
167.00	1000.0
168.00	417.0
171.90	175.0
174.00	290.0
174.90	406.0
176.90	400.0
178.90	928.0
179.90	564.0
180.90	255.0
184.90	354.0
186.00	3467.0
187.00	1012.0
188.00	192.0
189.00	247.0
191.90	363.0
193.00	281.0
196.00	526.0
197.90	21608.0
198.90	1272.0
201.30	154.0
202.80	167.0
203.90	874.0
205.00	1685.0
206.00	6400.0
206.90	956.0
207.80	262.0
209.90	153.0
210.90	238.0
215.90	171.0
216.90	1918.0
217.90	290.0
220.90	885.0
222.90	354.0
224.00	3842.0
224.90	1115.0
226.90	1608.0
227.90	296.0
228.90	303.0
230.90	175.0
236.90	151.0

Instrument :
BNA_G
ClientSampleId :
DFTPP10

241.90	193.0
243.00	232.0
243.90	2403.0
244.90	360.0
245.90	641.0
254.90	14266.0
255.90	2256.0
257.00	178.0
257.90	752.0
258.90	162.0
264.90	283.0
273.00	376.0
273.90	1205.0
274.90	6518.0
275.90	779.0
276.90	624.0
292.80	201.0
295.90	1977.0
296.90	270.0
303.00	337.0
314.90	195.0
322.90	621.0
334.00	336.0
352.00	205.0
353.90	190.0
364.90	748.0
371.90	298.0
421.00	228.0
422.00	217.0
423.00	1091.0
424.00	218.0
441.00	2897.0
442.00	18400.0
443.00	3704.0
444.00	396.0

Instrument :
BNA_G
ClientSampleId :
DFTPP10

m/z	Abundance
39.00	398.0
39.90	159.0
44.00	269.0
50.00	1184.0
51.00	4259.0
52.00	228.0
56.90	314.0
63.00	294.0
68.10	202.0
68.90	4619.0
74.00	434.0
75.00	845.0
75.90	236.0
77.00	5314.0
78.00	471.0
79.00	409.0
79.90	191.0
80.90	450.0
81.90	187.0
91.00	184.0
91.90	171.0
92.90	726.0
97.90	449.0
98.90	517.0
100.90	302.0
104.00	268.0
106.90	1906.0
108.00	363.0
109.90	3155.0
110.90	471.0
116.90	1540.0
122.80	236.0
125.00	171.0
126.90	7128.0
128.00	633.0
128.90	2622.0
130.00	238.0
134.90	231.0
140.90	367.0
146.90	220.0
148.00	392.0
153.00	186.0
154.90	200.0
155.90	313.0
159.90	273.0
160.90	180.0
165.00	233.0
165.90	226.0
166.90	779.0
167.90	275.0
168.80	167.0
174.90	201.0
178.90	737.0
179.90	475.0
181.00	211.0
185.00	351.0
185.90	2414.0
186.90	672.0
188.80	215.0
191.90	202.0
192.90	308.0
196.00	523.0
197.90	17840.0
198.90	1261.0
202.80	216.0
204.00	750.0
204.90	1158.0
206.00	4658.0
206.90	819.0
207.90	219.0
210.90	177.0
216.90	1456.0
220.90	776.0
221.90	246.0
223.00	479.0
223.90	2790.0
225.00	733.0
226.90	1344.0
227.90	202.0
228.80	340.0
242.90	152.0
244.00	2071.0
244.90	274.0
245.90	511.0
254.90	12181.0
255.90	1808.0
257.90	841.0
264.90	306.0
272.90	317.0
273.90	936.0
274.90	5352.0
275.90	631.0

Instrument :
BNA_G
ClientSampleId :
DFTPP10

276.90	468.0
295.90	1613.0
297.00	209.0
303.00	221.0
314.80	251.0
323.00	524.0
333.90	354.0
351.90	225.0
352.90	204.0
364.90	746.0
372.00	295.0
402.90	171.0
420.90	244.0
421.90	222.0
422.90	958.0
423.90	261.0
440.90	2787.0
442.00	18296.0
443.00	3525.0
444.00	313.0

Instrument :
BNA_G
ClientSampleId :
DFTPP10