


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121916\
Data File : BG025313.D
Acq On : 19 Dec 2016 10:38
Operator : UM/SJ
Sample : DFTPP22
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP22

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG113016.M
Title : SVOA CALIBRATION
Last Update : Tue Dec 20 18:35:08 2016

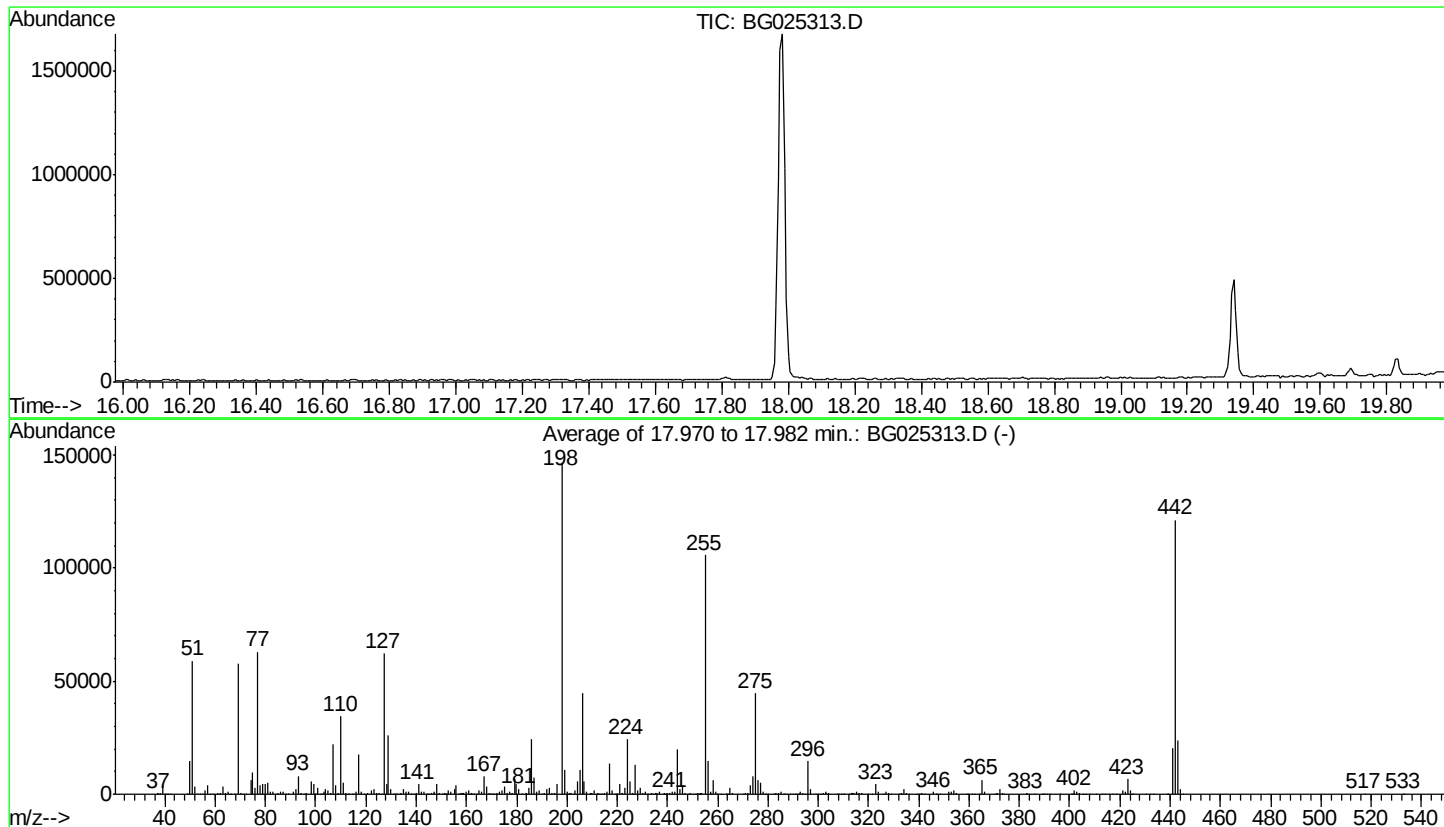

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	59040	PASS
68	69	0.00	2	0.5	281	PASS
69	198	0.00	100	39.2	57538	PASS
70	69	0.00	2	0.9	498	PASS
127	198	10	80	42.5	62290	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	146709	PASS
199	198	5	9	7.3	10728	PASS
275	198	10	60	30.3	44522	PASS
365	198	1	100	4.3	6292	PASS
441	442	0.01	100	16.9	20538	PASS
442	198	50	100	82.8	121429	PASS
443	442	15	24	19.6	23804	PASS