
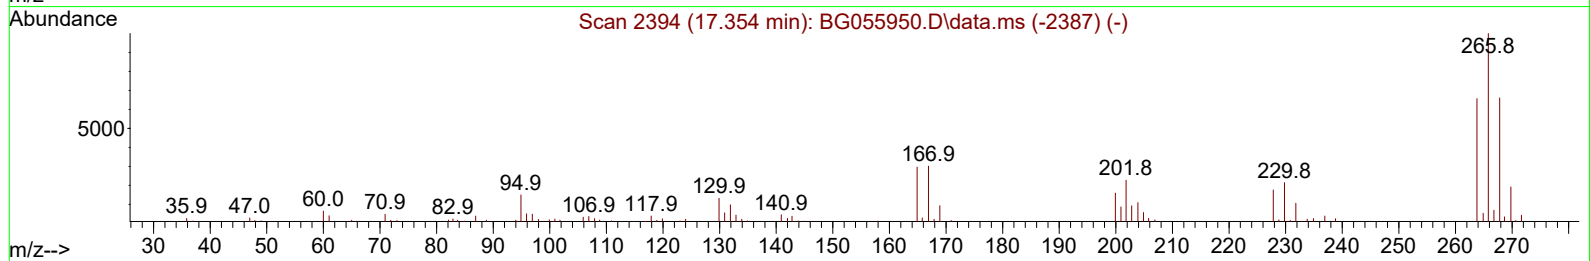
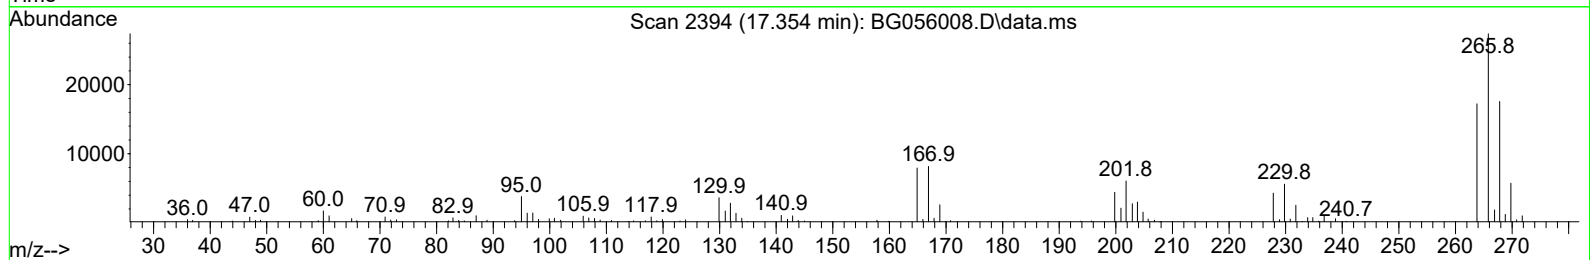


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121922\
Data File : BG056008.D
Acq On : 19 Dec 2022 9:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 06:16:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 01:01:12 2022
Response via : Initial Calibration

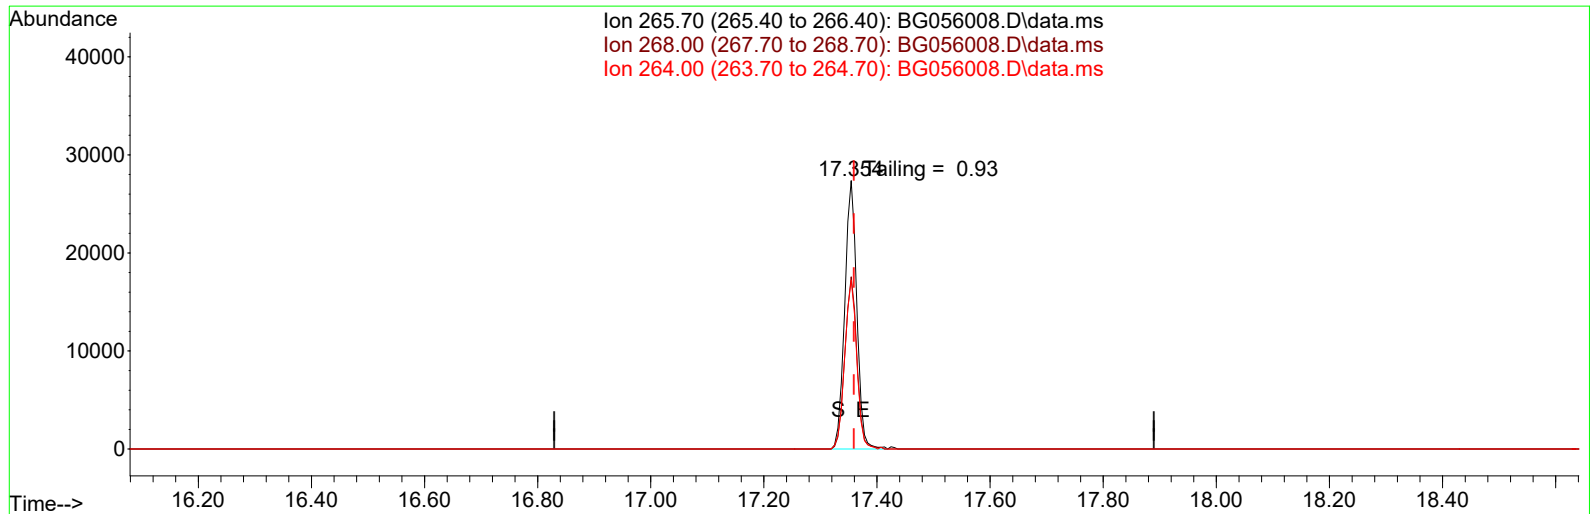

TIC: BG056008.D\data.ms

(70) Pentachlorophenol (C)




17.354min (-0.005) 56926.48 ng

response 40530

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	64.17
264.00	65.70	62.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121922\
 Data File : BG056008.D
 Acq On : 19 Dec 2022 9:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 06:16:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 20 01:01:12 2022
 Response via : Initial Calibration

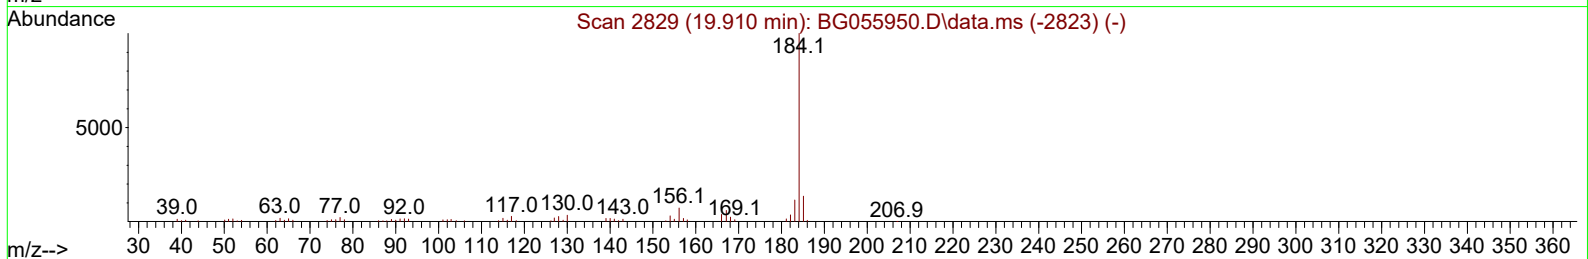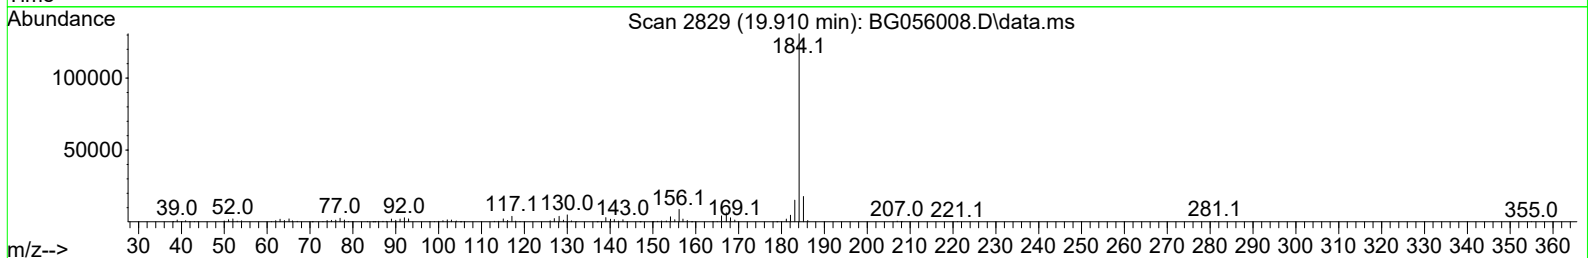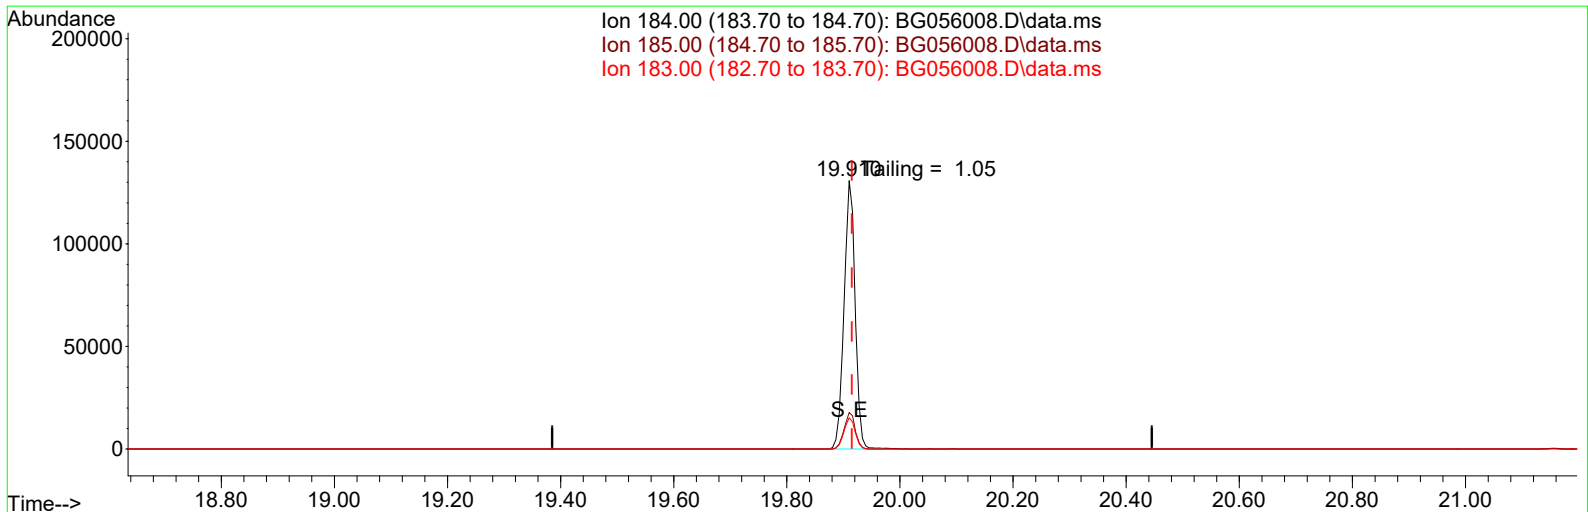

TIC: BG056008.D\data.ms

(77) Benzidine

19.910min (-0.005) 0.00 ng

response 178099

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.59
183.00	11.50	11.62
0.00	0.00	0.00