


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121922\
Data File : BG056008.D
Acq On : 19 Dec 2022 9:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Dec 20 01:01:12 2022

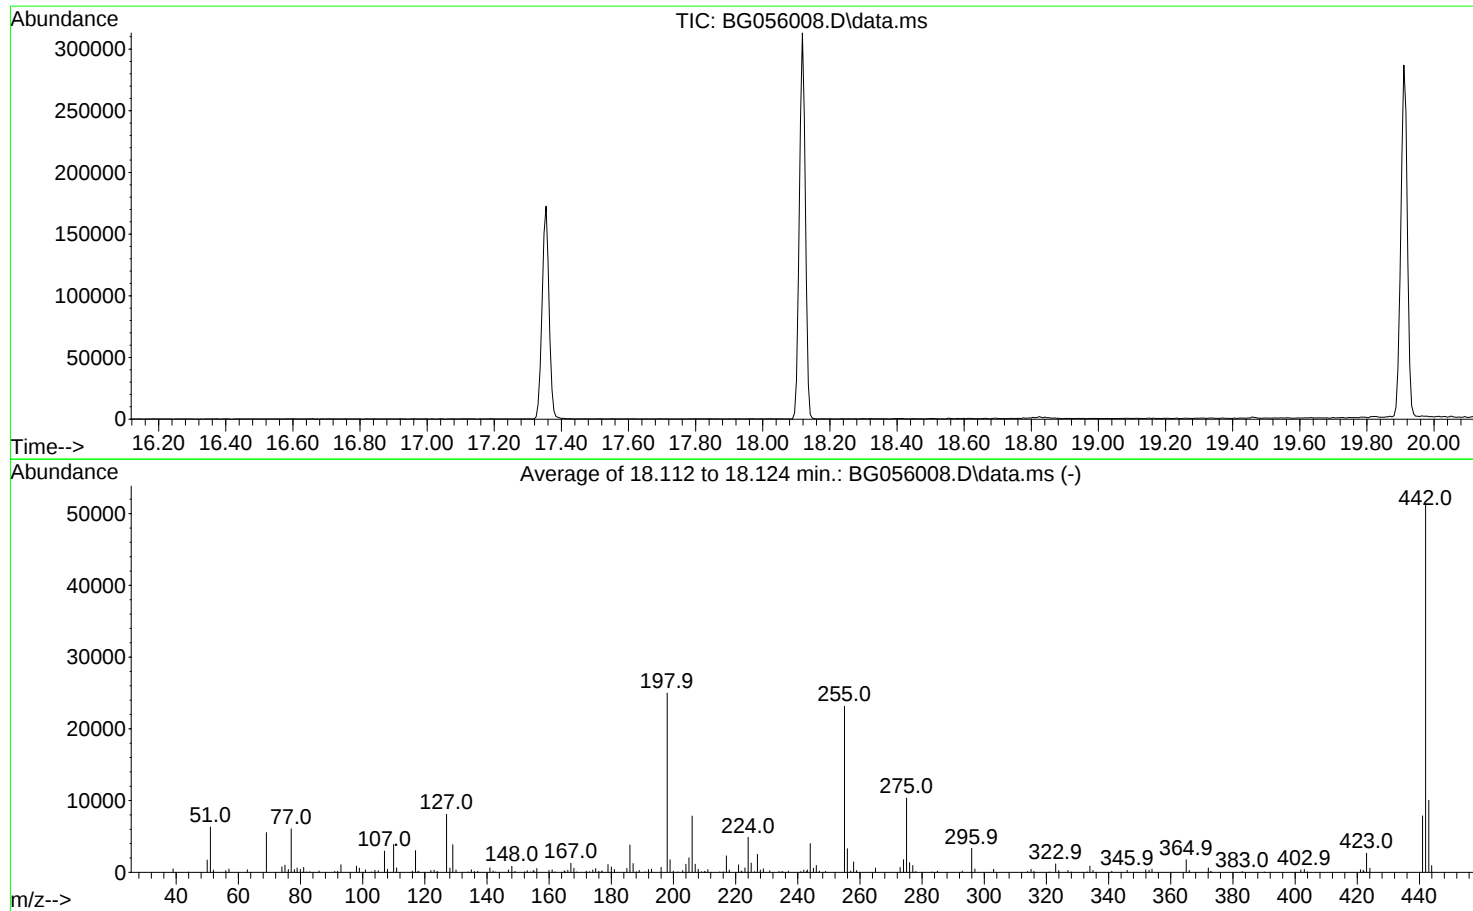




AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	6311	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	22.2	5550	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.4	8093	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	24989	PASS
199	198	5	9	7.0	1751	PASS
275	198	10	60	41.4	10338	PASS
365	198	1	100	7.0	1752	PASS
441	198	0.01	100	31.5	7860	PASS
442	442	50	100	100.0	51280	PASS
443	442	15	24	19.5	10020	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121922\
Data File : BG056008.D
Acq On : 19 Dec 2022 9:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 20 06:16:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 01:01:12 2022
Response via : Initial Calibration

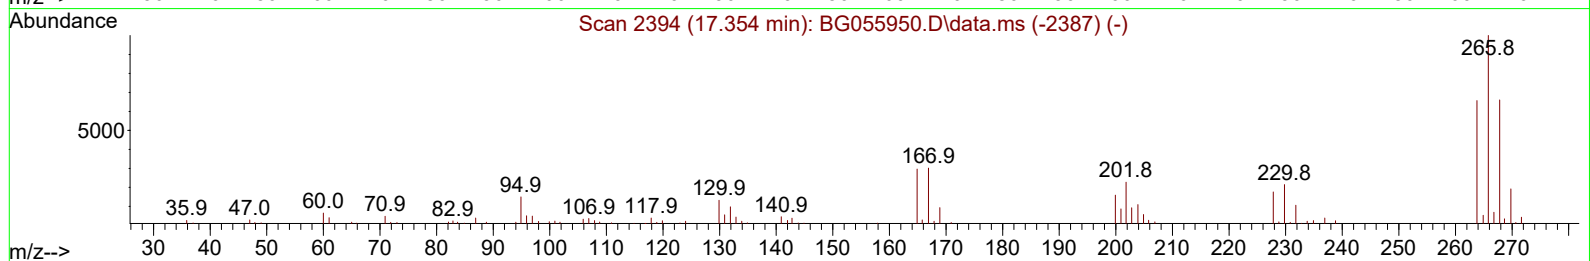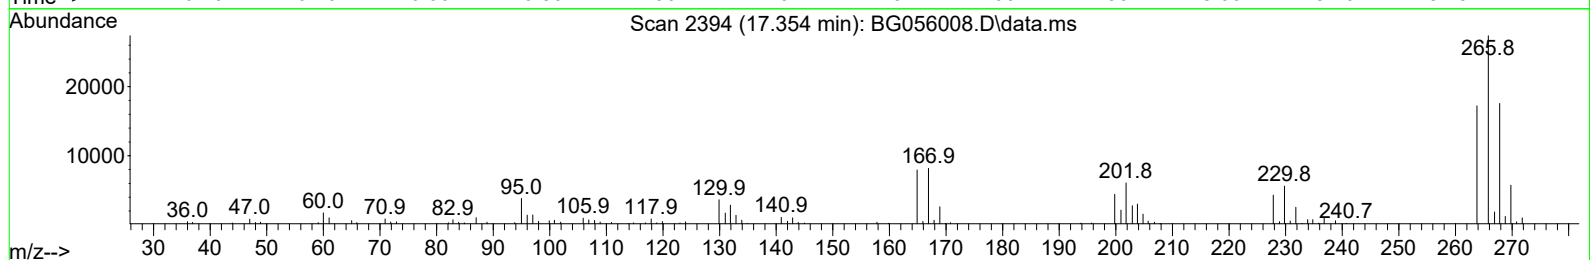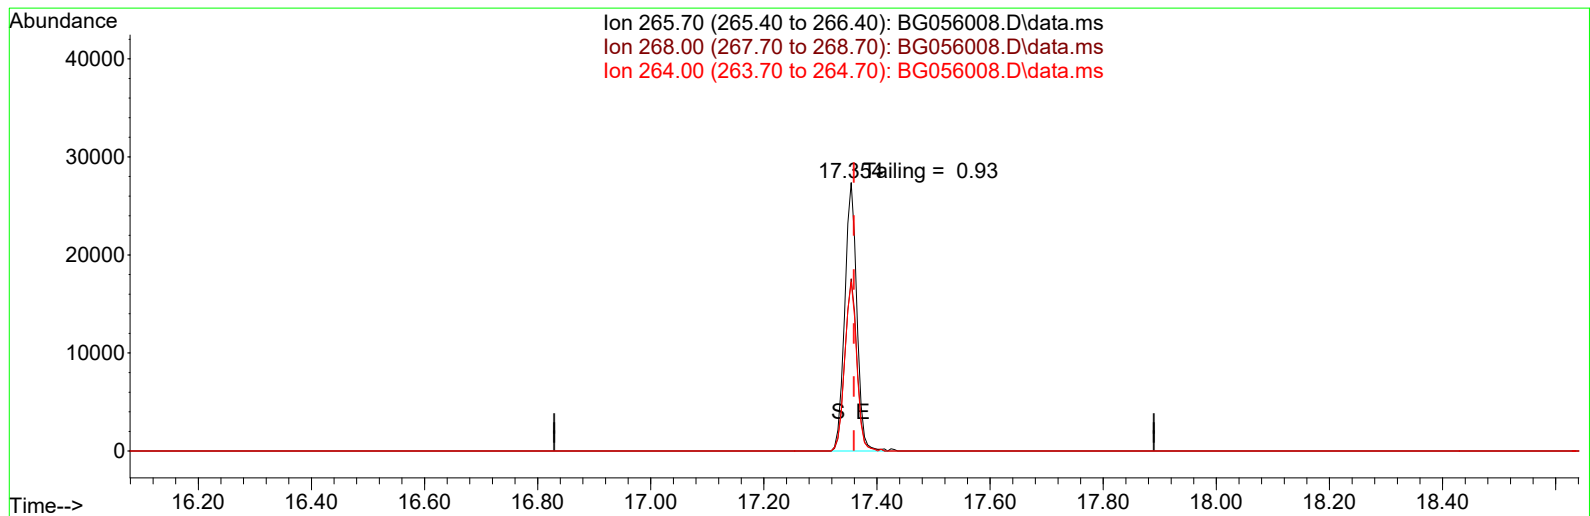

TIC: BG056008.D\data.ms

(70) Pentachlorophenol (C)

17.354min (-0.005) 56926.48 ng




response 40530

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	64.17
264.00	65.70	62.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121922\
Data File : BG056008.D
Acq On : 19 Dec 2022 9:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 20 06:16:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 01:01:12 2022
Response via : Initial Calibration

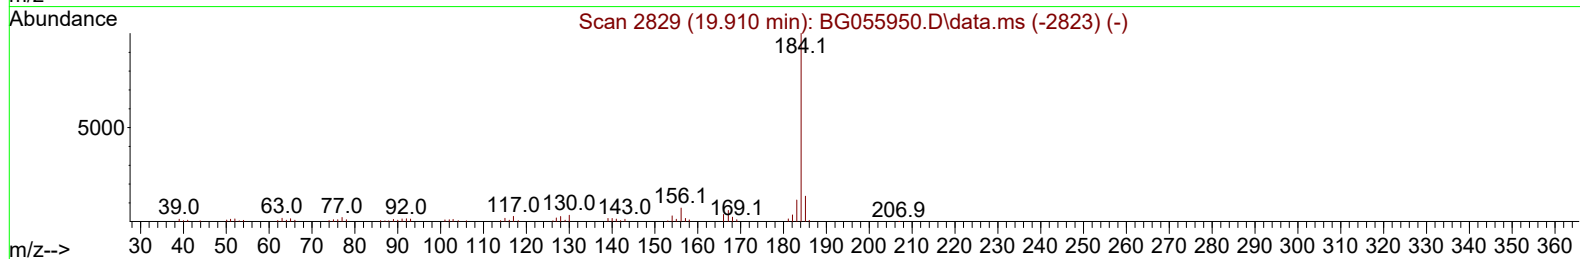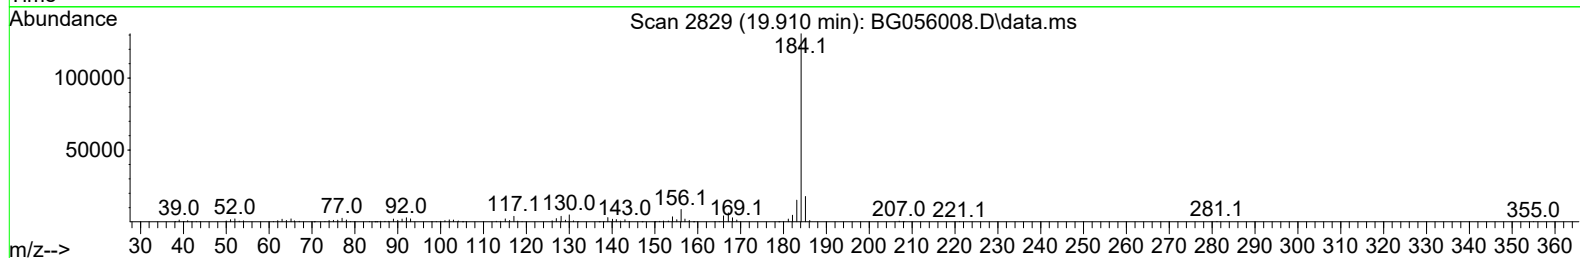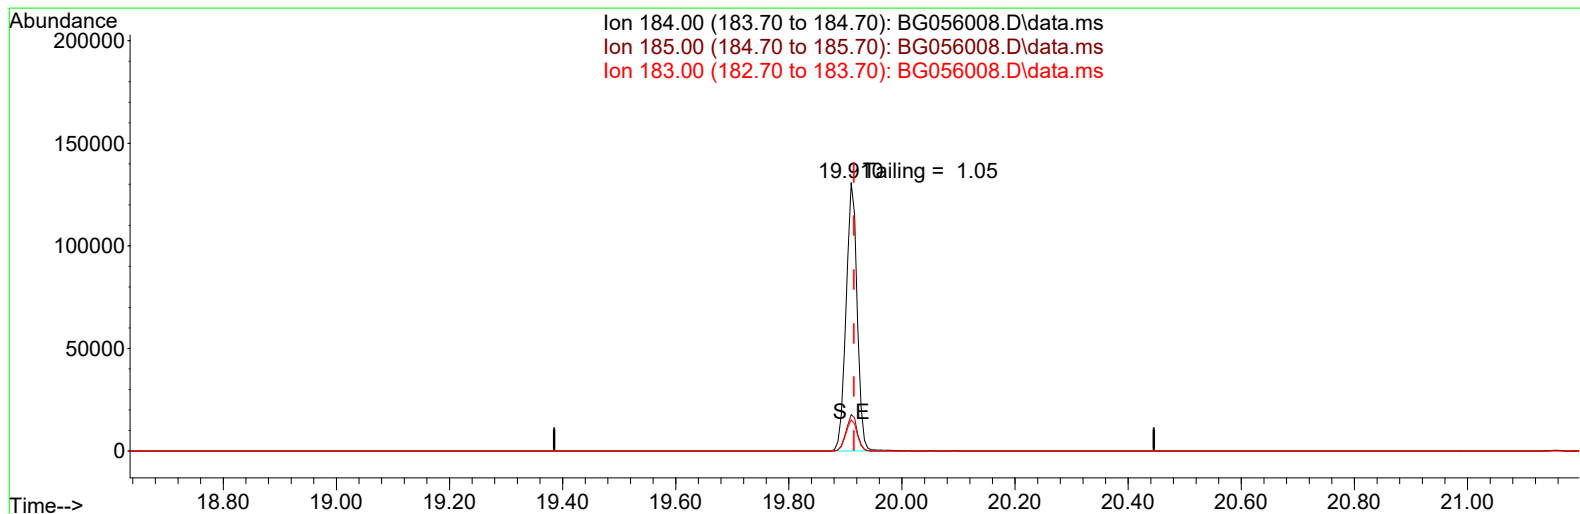

TIC: BG056008.D\data.ms

(77) Benzidine

19.910min (-0.005) 0.00 ng

response 178099

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.59
183.00	11.50	11.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/19/2022	BNA_G	BG056008.D
Compound Name	Response	Retention Time
DDT	89795	21.156
DDD	2508	20.692
DDE	0	20.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2508	92303	2.72

Instrument :
BNA_G
ClientSampleId :
DFTPP