

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG121923\  
 Data File : BG060083.D  
 Acq On : 19 Dec 2023 13:19  
 Operator : MA/JU  
 Sample : PB157746BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB157746BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG121323.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060083.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.520       | 407           | 414         | 424          | rBV      | 902038         | 1397903       | 16.82%          | 5.760%        |
| 2         | 7.112       | 677           | 685         | 692          | rBV      | 926788         | 1505066       | 18.11%          | 6.202%        |
| 3         | 7.947       | 822           | 827         | 835          | rVB      | 158917         | 268847        | 3.24%           | 1.108%        |
| 4         | 9.110       | 1016          | 1025        | 1037         | rVB      | 547115         | 976059        | 11.75%          | 4.022%        |
| 5         | 10.755      | 1298          | 1305        | 1313         | rBV      | 207753         | 377179        | 4.54%           | 1.554%        |
| 6         | 13.211      | 1716          | 1723        | 1731         | rVB      | 2086149        | 3157118       | 38.00%          | 13.009%       |
| 7         | 14.592      | 1951          | 1958        | 1965         | rBV      | 429208         | 666606        | 8.02%           | 2.747%        |
| 8         | 16.078      | 2204          | 2211        | 2218         | rBV      | 2486734        | 3633680       | 43.73%          | 14.973%       |
| 9         | 17.336      | 2419          | 2425        | 2433         | rVB      | 729043         | 1119649       | 13.48%          | 4.614%        |
| 10        | 19.962      | 2866          | 2872        | 2878         | rBV      | 6292093        | 8308659       | 100.00%         | 34.236%       |
| 11        | 21.607      | 3147          | 3152        | 3159         | rVB      | 898876         | 1450634       | 17.46%          | 5.977%        |
| 12        | 24.798      | 3688          | 3695        | 3705         | rVB2     | 511896         | 1407463       | 16.94%          | 5.799%        |




Sum of corrected areas: 24268863

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG121923\  
Data File : BG060083.D  
Acq On : 19 Dec 2023 13:19  
Operator : MA/JU  
Sample : PB157746BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB157746BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG121323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

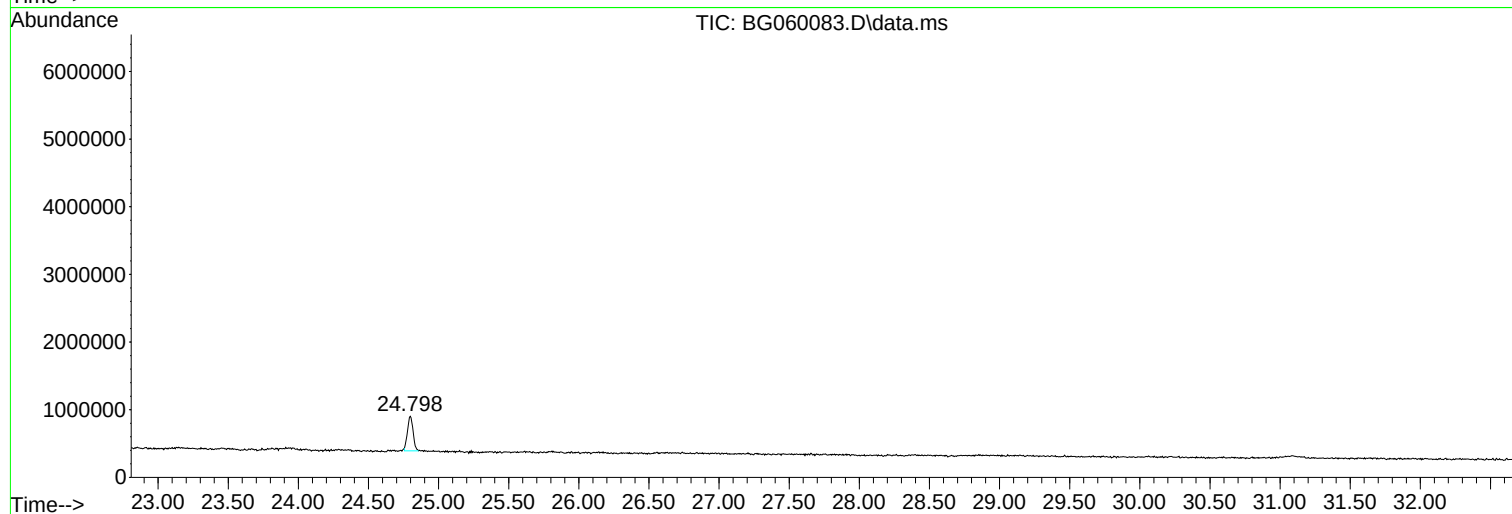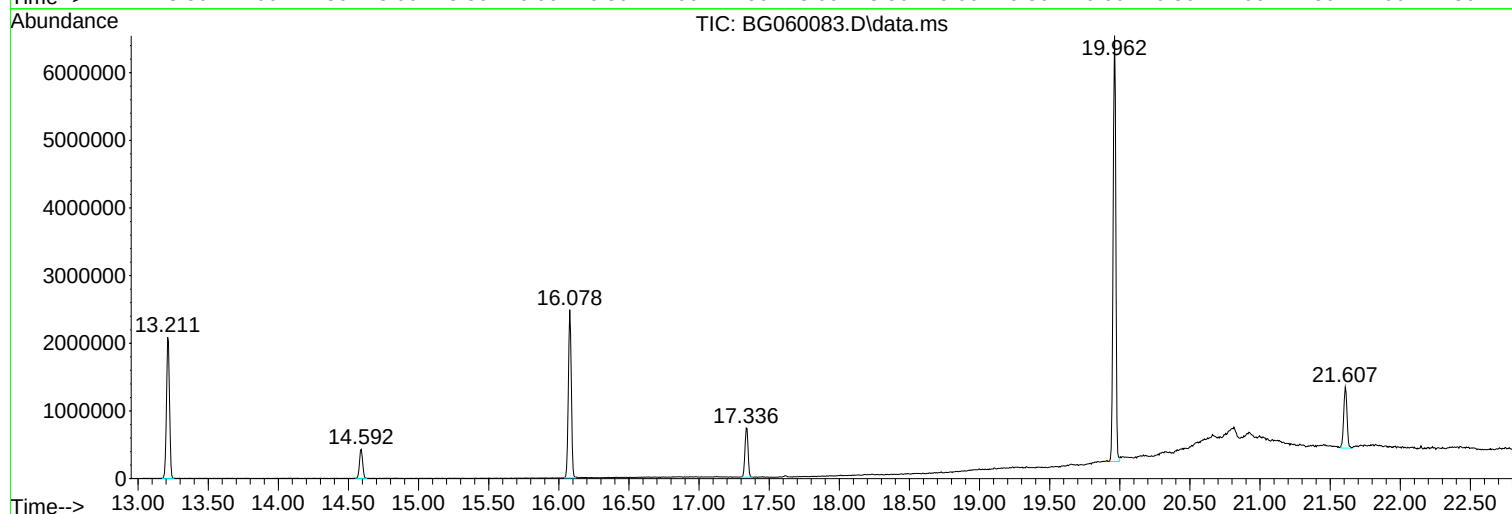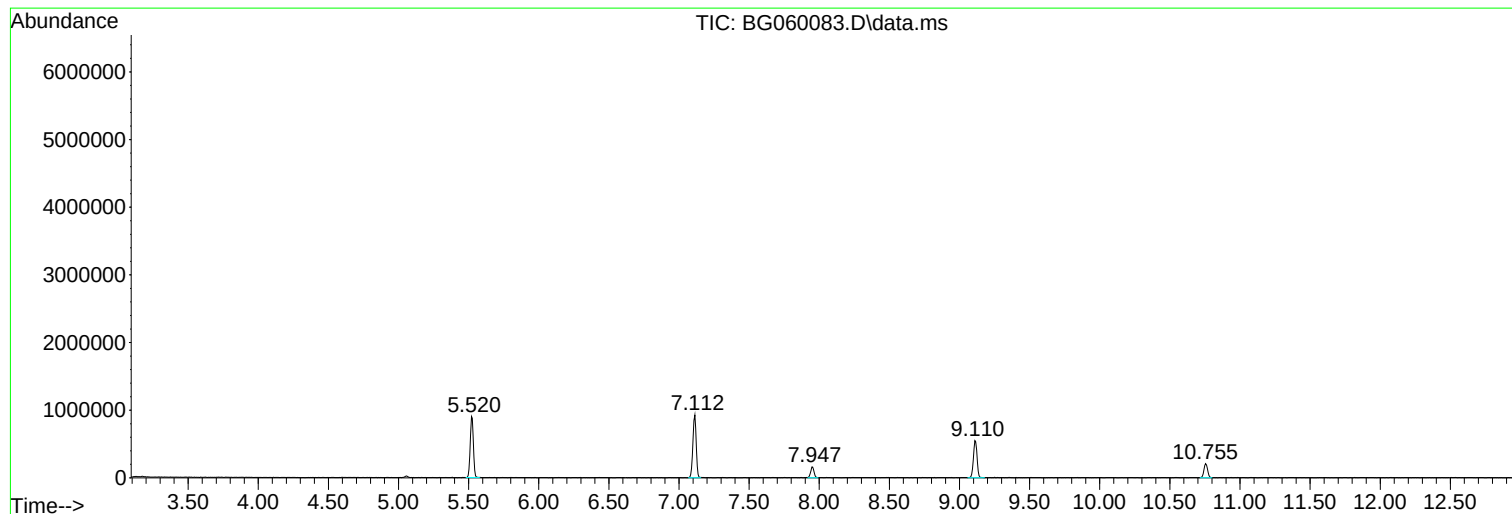

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG121923\  
Data File : BG060083.D  
Acq On : 19 Dec 2023 13:19  
Operator : MA/JU  
Sample : PB157746BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB157746BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG121323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG121923\  
Data File : BG060083.D  
Acq On : 19 Dec 2023 13:19  
Operator : MA/JU  
Sample : PB157746BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB157746BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG121323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|