
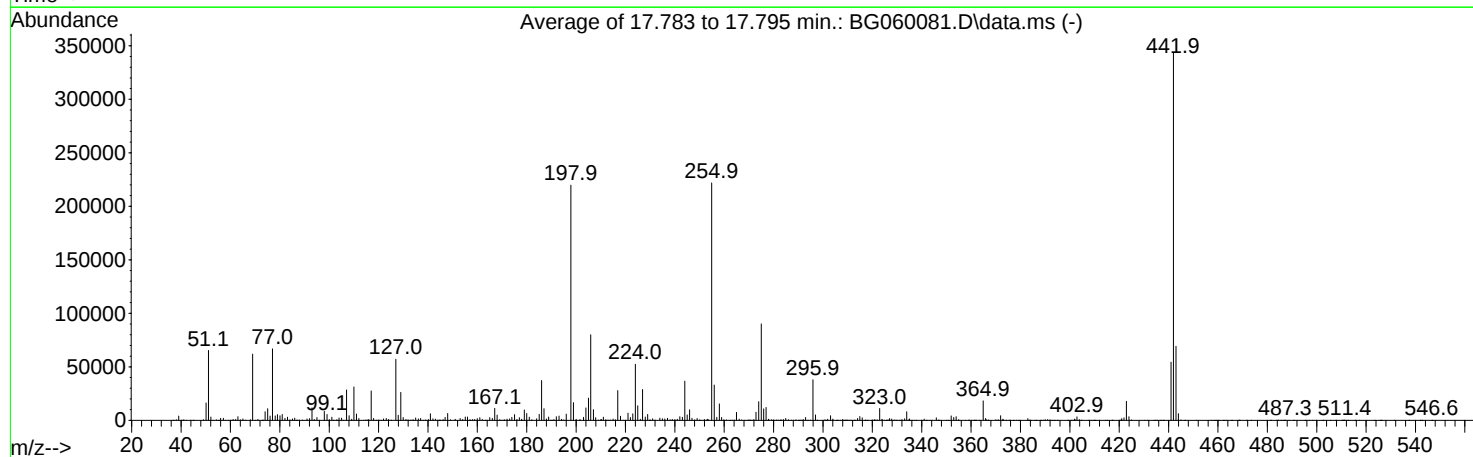


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121923\
 Data File : BG060081.D
 Acq On : 19 Dec 2023 11:14
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 19 04:37:23 2023

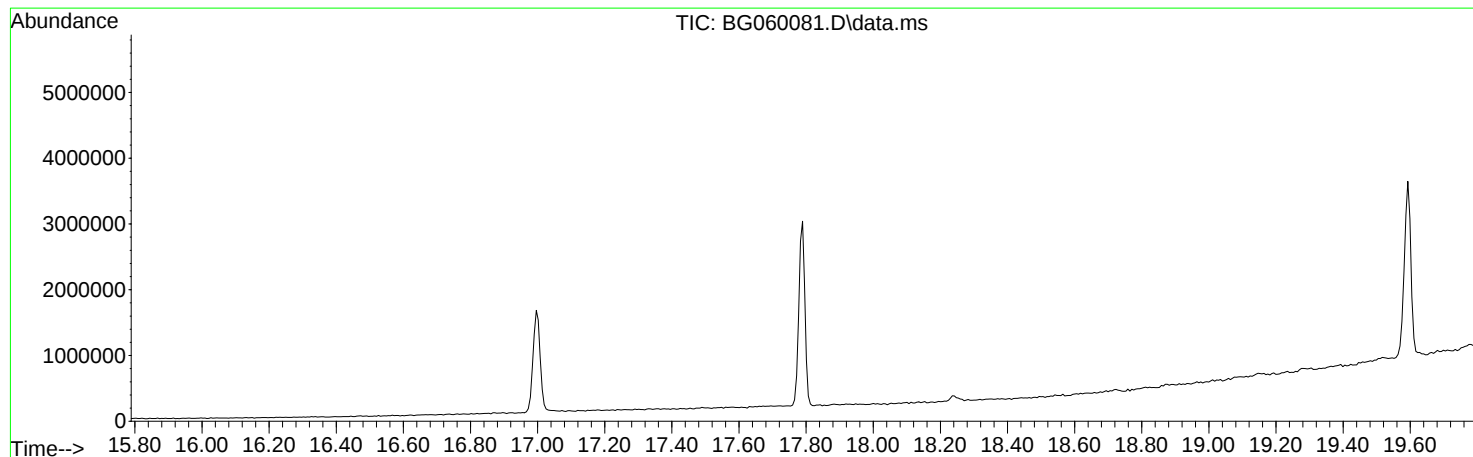




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	65326	PASS
68	69	0.00	2	1.0	628	PASS
69	198	0.00	100	28.1	61879	PASS
70	69	0.00	2	0.4	217	PASS
127	198	10	80	26.0	57156	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	219819	PASS
199	198	5	9	7.6	16661	PASS
275	198	10	60	41.0	90229	PASS
365	198	1	100	8.3	18233	PASS
441	198	0.01	100	24.8	54429	PASS
442	442	50	100	100.0	343723	PASS
443	442	15	24	20.2	69299	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121923\
Data File : BG060081.D
Acq On : 19 Dec 2023 11:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 20 01:44:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 04:37:23 2023
Response via : Initial Calibration

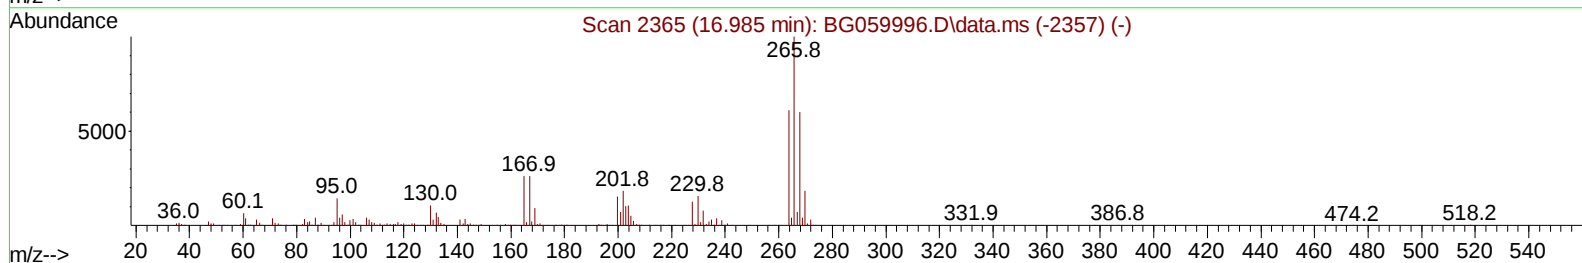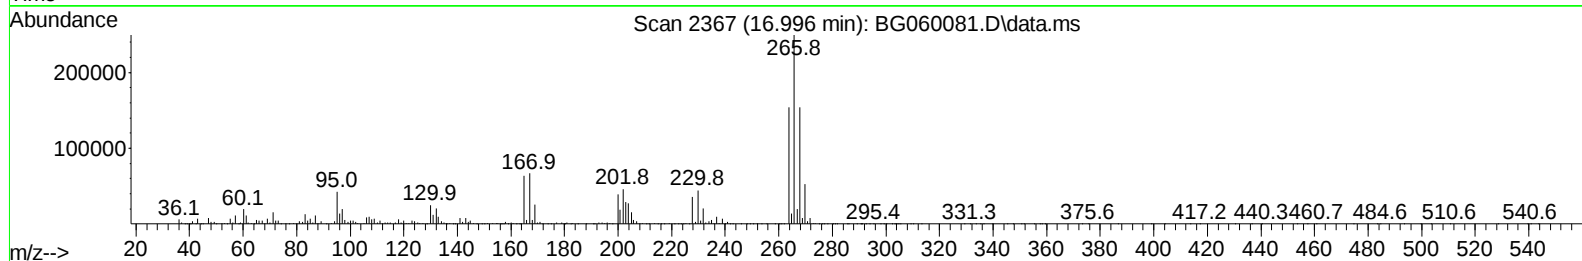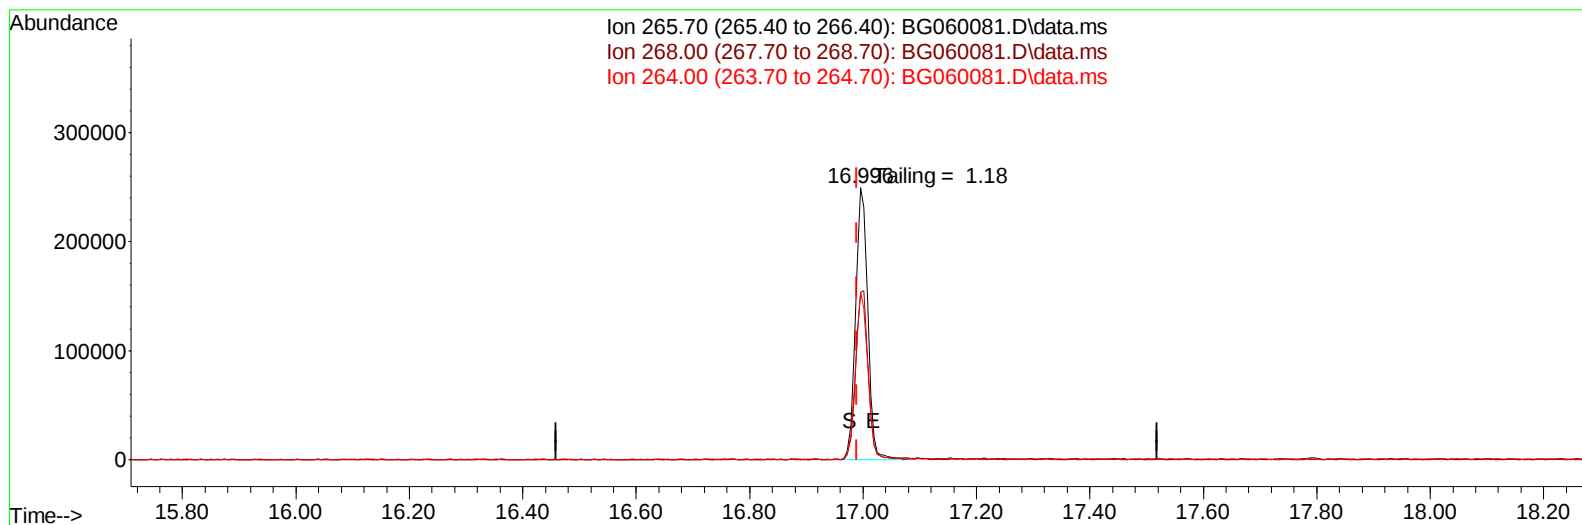

TIC: BG060081.D\data.ms

(70) Pentachlorophenol (C)

16.996min (+ 0.007) 561236.75 ng




response 371811

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	61.69
264.00	61.00	61.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121923\
Data File : BG060081.D
Acq On : 19 Dec 2023 11:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 20 01:44:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 04:37:23 2023
Response via : Initial Calibration

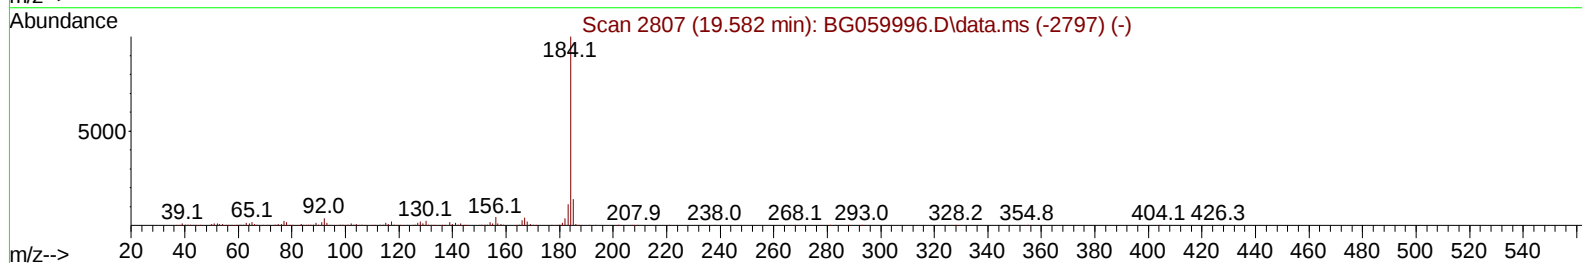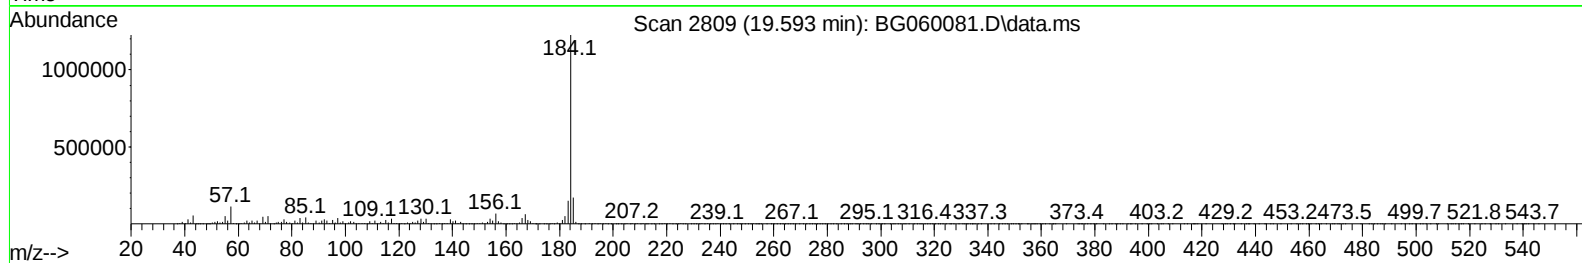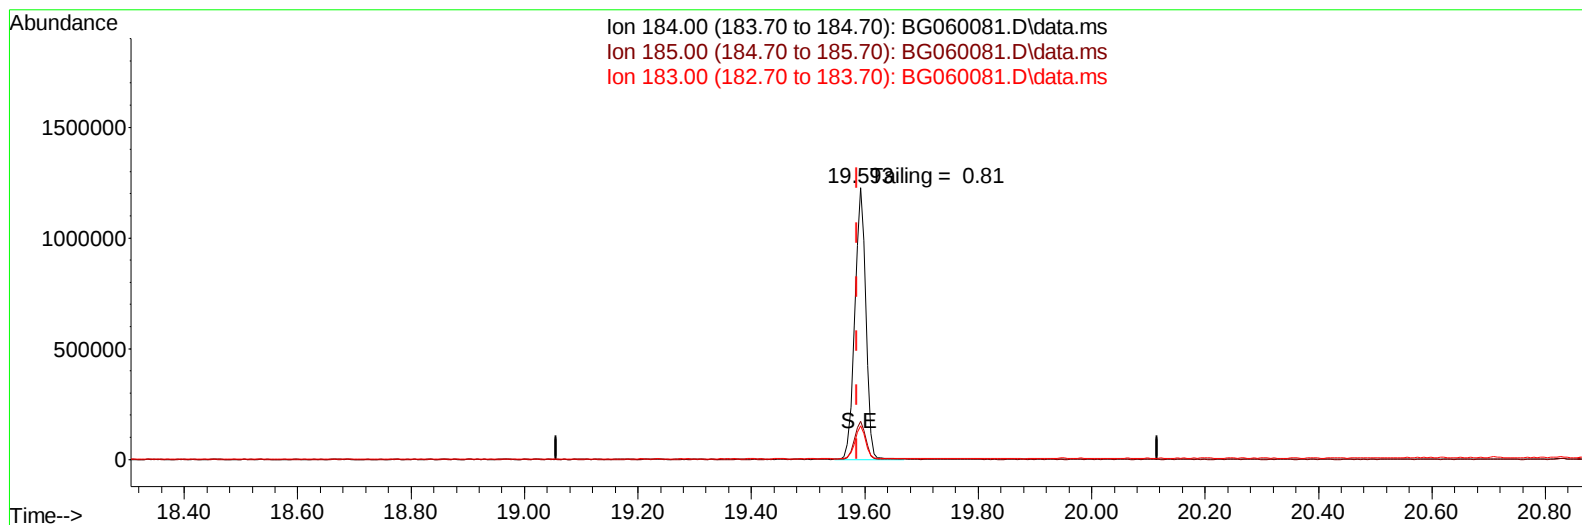

TIC: BG060081.D\data.ms

(77) Benzidine**19.593min (+ 0.007) 136993.41 ng****response 1659342**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.09
183.00	11.20	12.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/19/2023	BNA_G	<u>BG060081.D</u>
Compound Name	Response	Retention Time
DDT	964257	20.827
DDD	30106	20.38
DDE	0	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30106	994363	3.03

Instrument :
BNA_G
ClientSampleId :
DFTPP