

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
 Data File : BG020336.D
 Acq On : 20 Dec 2015 10:58
 Operator : UM/SJ
 Sample : PB87396BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK96

Quant Time: Dec 21 00:39:05 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 21 00:36:38 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	17999	20.00	ng/ul	0.00
18) Naphthalene-d8	10.90	136	79370	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.72	164	56191	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	132611	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	163783	20.00	ng/ul	0.00
86) Perylene-d12	25.01	264	155408	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.46	96	2160	6.63	ng/uL	0.00
5) Phenol-d5	7.24	99	54496	34.34	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.41	67	34239	36.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.62	132	44304	38.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.79	113	47936	35.32	ng/ul	0.00
19) Nitrobenzene-d5	9.25	128	23723	38.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.98	143	27865	40.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	51326	36.81	ng/ul	0.00
29) 4-Chloroaniline-d4	11.03	131	66620	42.53	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	173475	38.17	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	200035	37.83	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	28234	34.64	ng/ul	0.00
58) Fluorene-d10	15.71	176	153566	37.25	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	24668	31.38	ng/ul	0.00
71) Anthracene-d10	17.56	188	245317	40.15	ng/ul	0.00
79) Pyrene-d10	19.85	212	287993	37.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	319465	41.21	ng/ul	0.00


Target Compounds					Ovalue
15) N-Nitroso-di-n-propylamine	8.78	70	1235	1.10 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
Data File : BG020336.D
Acq On : 20 Dec 2015 10:58
Operator : UM/SJ
Sample : PB87396BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK96

Quant Time: Dec 21 00:39:05 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 21 00:36:38 2015
Response via : Initial Calibration

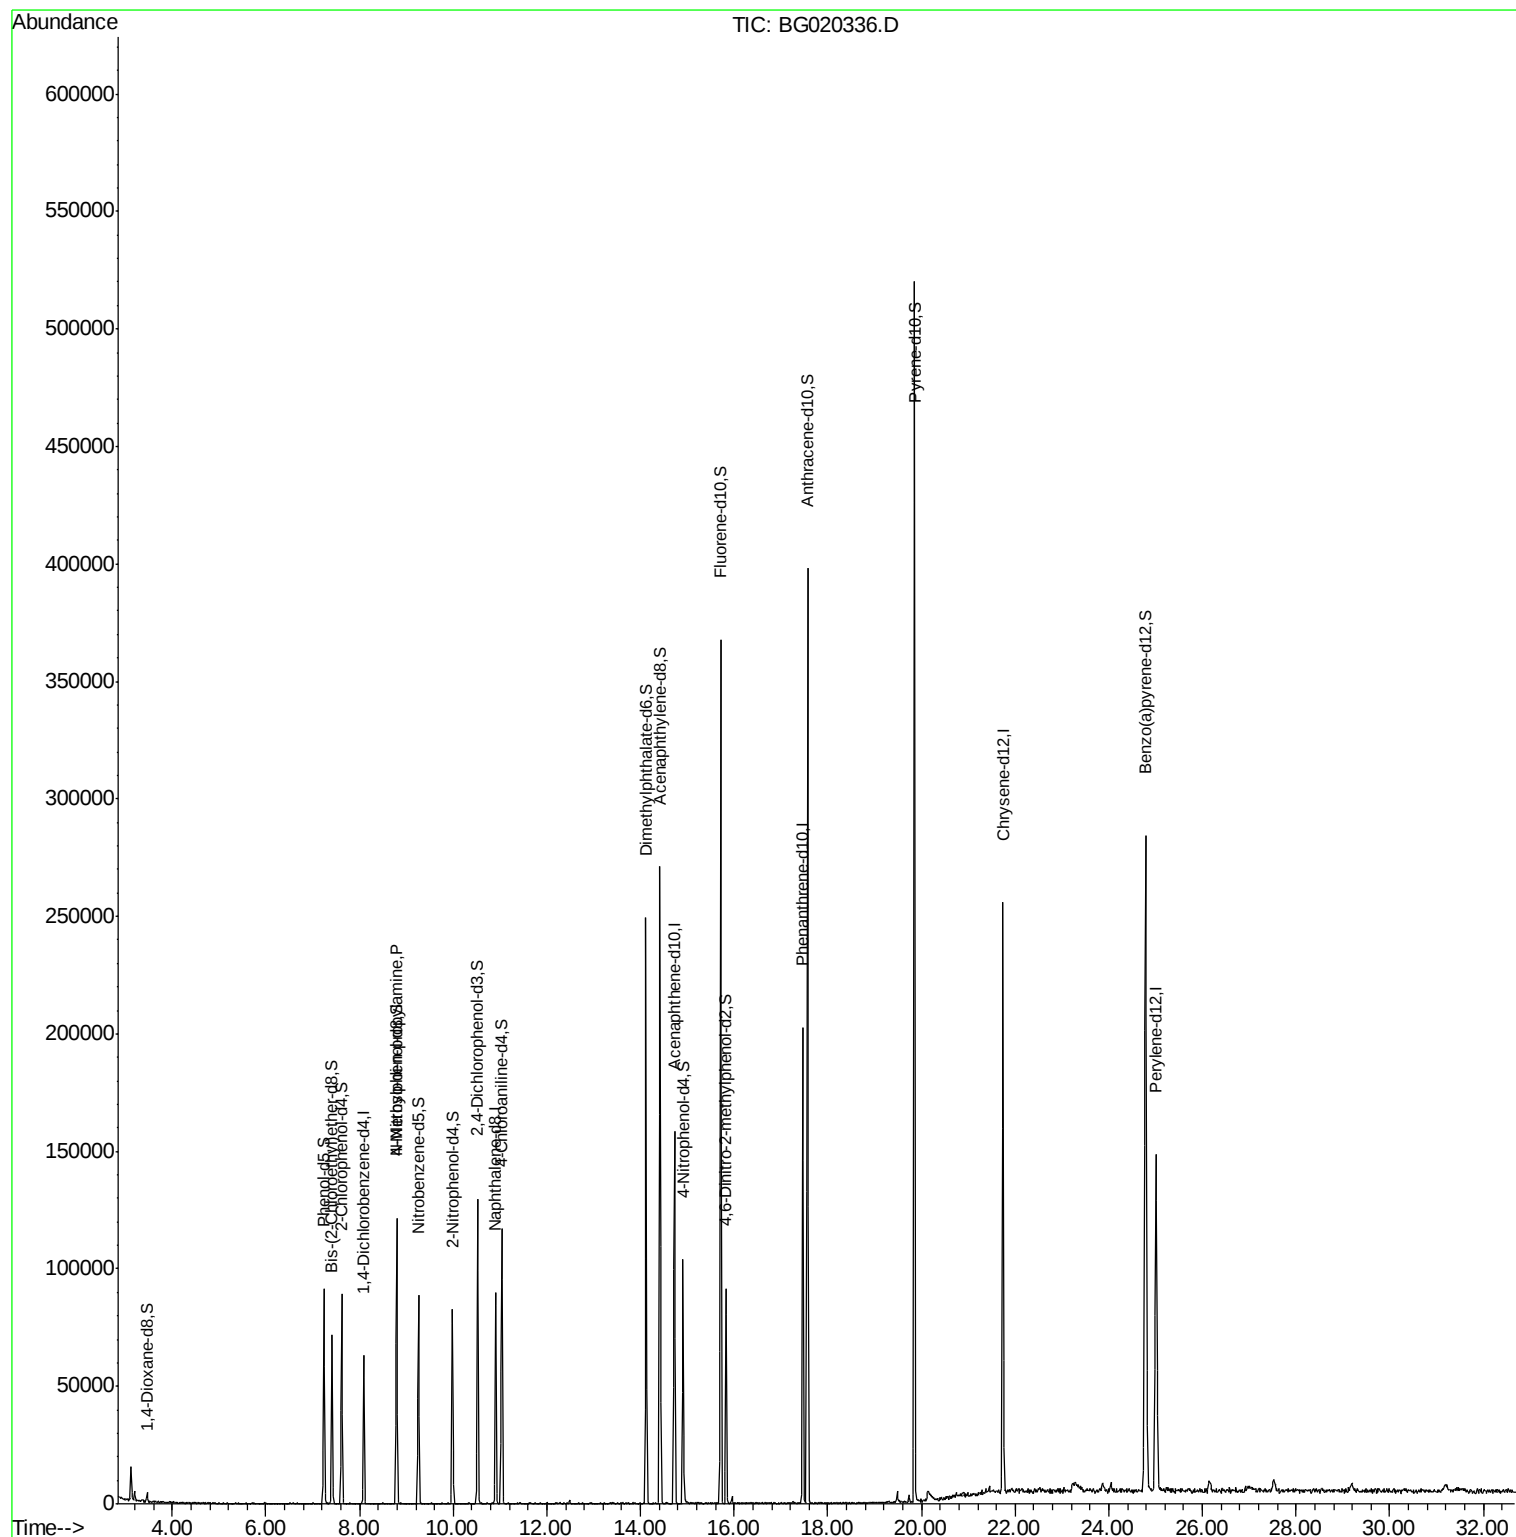

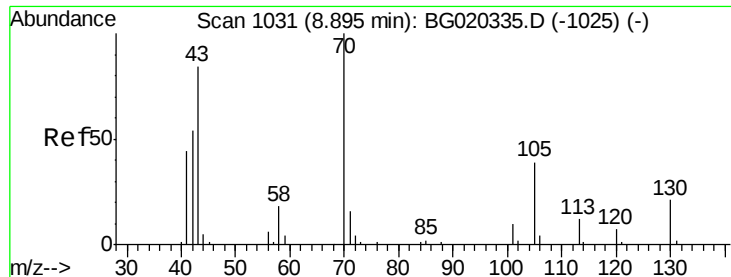

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.10 ng/ul
 RT: 8.78 min Scan# 1012
 Delta R.T. -0.11 min
 Lab File: BG020336.D
 Acq: 20 Dec 2015 10:58

Instrument :
 BNA_G
 ClientSampleId :
 SBLK96

Tot Ion:	70	Resp:	1235
Ion	Ratio	Lower	Upper
70	100		
42	273.1	44.3	66.5#
101	0.0	7.6	11.4#
130	0.0	17.0	25.4#

