

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
 Data File : BG020344.D
 Acq On : 20 Dec 2015 16:09
 Operator : UM/SJ
 Sample : G4803-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04D0

Quant Time: Dec 21 00:40:20 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 21 00:36:38 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	18584	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	78990	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	51355	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	118722	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	149742	20.00	ng/ul	0.00
86) Perylene-d12	25.02	264	144637	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	601	1.79	ng/uL	0.00
5) Phenol-d5	7.26	99	14555	8.88	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	7.41	67	35601	36.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	39699	33.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.81	113	28025	20.00	ng/ul	0.02
19) Nitrobenzene-d5	9.27	128	24973	40.56	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	30123	43.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	52419	37.77	ng/ul	0.01
29) 4-Chloroaniline-d4	11.05	131	4227	2.71	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	170863	41.13	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	199322	41.24	ng/ul	0.00
52) 4-Nitrophenol-d4	14.94	143	5878	7.89	ng/ul	0.03
58) Fluorene-d10	15.72	176	149837	39.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	22053	31.33	ng/ul	0.00
71) Anthracene-d10	17.57	188	232737	42.54	ng/ul	0.00
79) Pyrene-d10	19.85	212	279833	40.10	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.80	264	306793	42.53	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
33) 4-Chloro-3-methylphenol	12.24	107	2155	1.27	ng/ul#	26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
Data File : BG020344.D
Acq On : 20 Dec 2015 16:09
Operator : UM/SJ
Sample : G4803-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04D0

Quant Time: Dec 21 00:40:20 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 21 00:36:38 2015
Response via : Initial Calibration

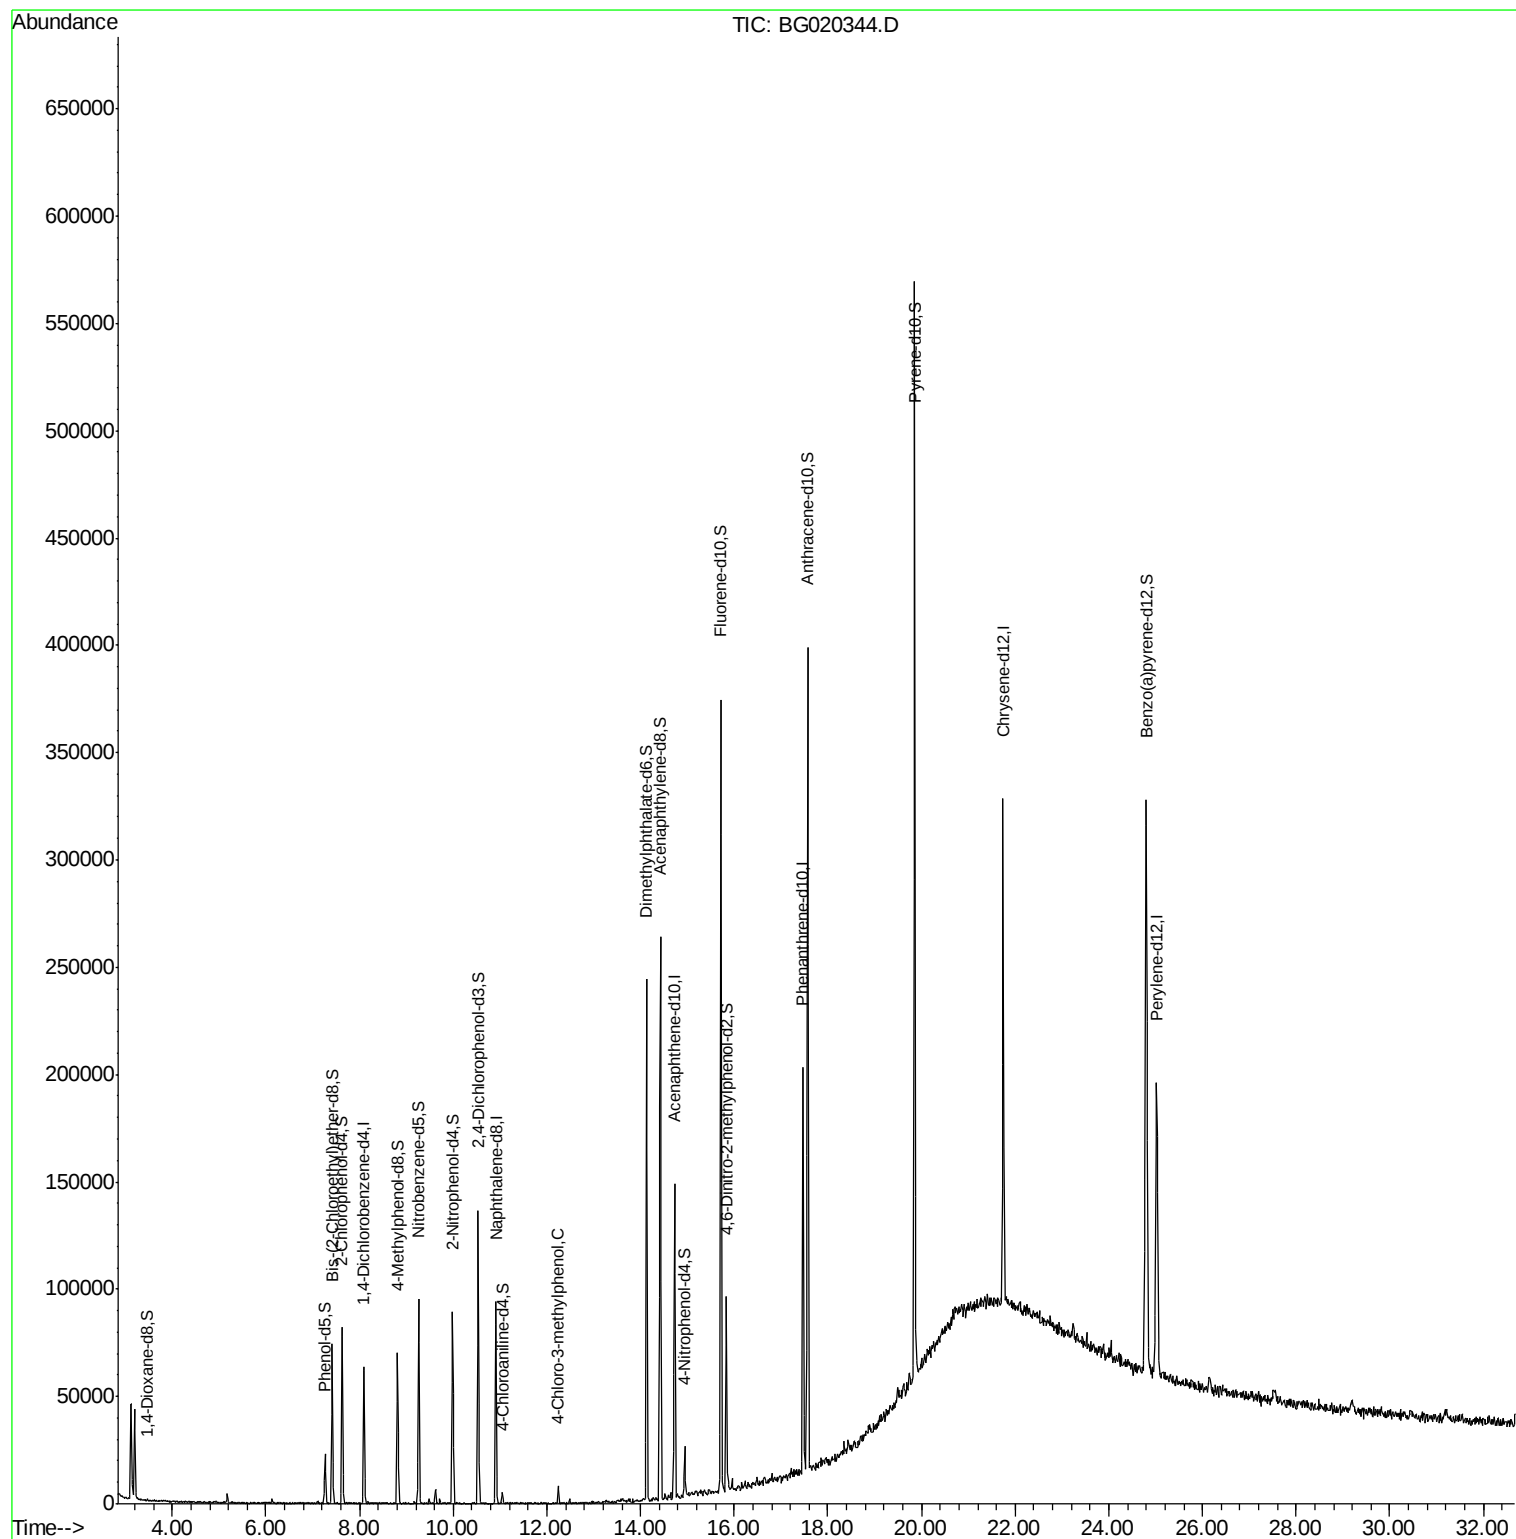

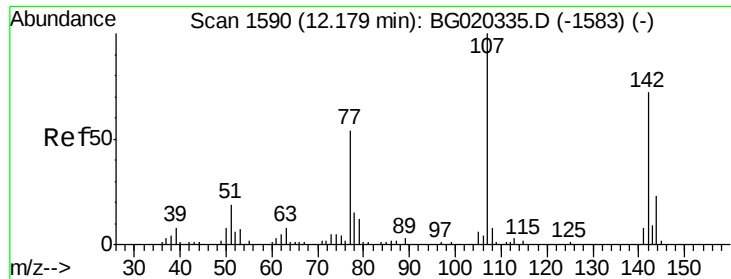

#33
 4-Chloro-3-methylphenol
 Concen: 1.27 ng/ul
 RT: 12.24 min Scan# 1601
 Delta R.T. 0.07 min
 Lab File: BG020344.D
 Acq: 20 Dec 2015 16:09

Instrument :
 BNA_G
 ClientSampleId :
 C04D0

Tot Ion:107 Resp: 2155
 Ion Ratio Lower Upper
 107 100
 144 0.0 18.7 28.1#
 142 0.0 52.8 79.2#

