

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
 Data File : BG020345.D
 Acq On : 20 Dec 2015 16:48
 Operator : UM/SJ
 Sample : G4803-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04B2

Quant Time: Dec 21 00:40:28 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 21 00:36:38 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	20629	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	89238	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	59854	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.57	188	49045	20.00	ng/ul	0.10
78) Chrysene-d12	21.74	240	173079	20.00	ng/ul	0.00
86) Perylene-d12	25.02	264	165370	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.26	99	3198	1.76	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	7.41	67	7061	6.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	8246	6.23	ng/ul	0.01
13) 4-Methylphenol-d8	8.81	113	5510	3.54	ng/ul	0.02
19) Nitrobenzene-d5	9.26	128	4727	6.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	5485	7.09	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.54	165	10154	6.48	ng/ul	0.02
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
44) Dimethylphthalate-d6	14.12	166	35045	7.24	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	40593	7.21	ng/ul	0.00
52) 4-Nitrophenol-d4	14.95	143	918	1.06	ng/ul	0.04
58) Fluorene-d10	15.72	176	31351	7.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	2630	9.05	ng/ul	0.00
71) Anthracene-d10	17.57	188	48784	21.59	ng/ul	0.00
79) Pyrene-d10	19.85	212	57829	7.17	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	59636	7.23	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.17	163	42766	8.65	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
Data File : BG020345.D
Acq On : 20 Dec 2015 16:48
Operator : UM/SJ
Sample : G4803-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04B2

Quant Time: Dec 21 00:40:28 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 21 00:36:38 2015
Response via : Initial Calibration

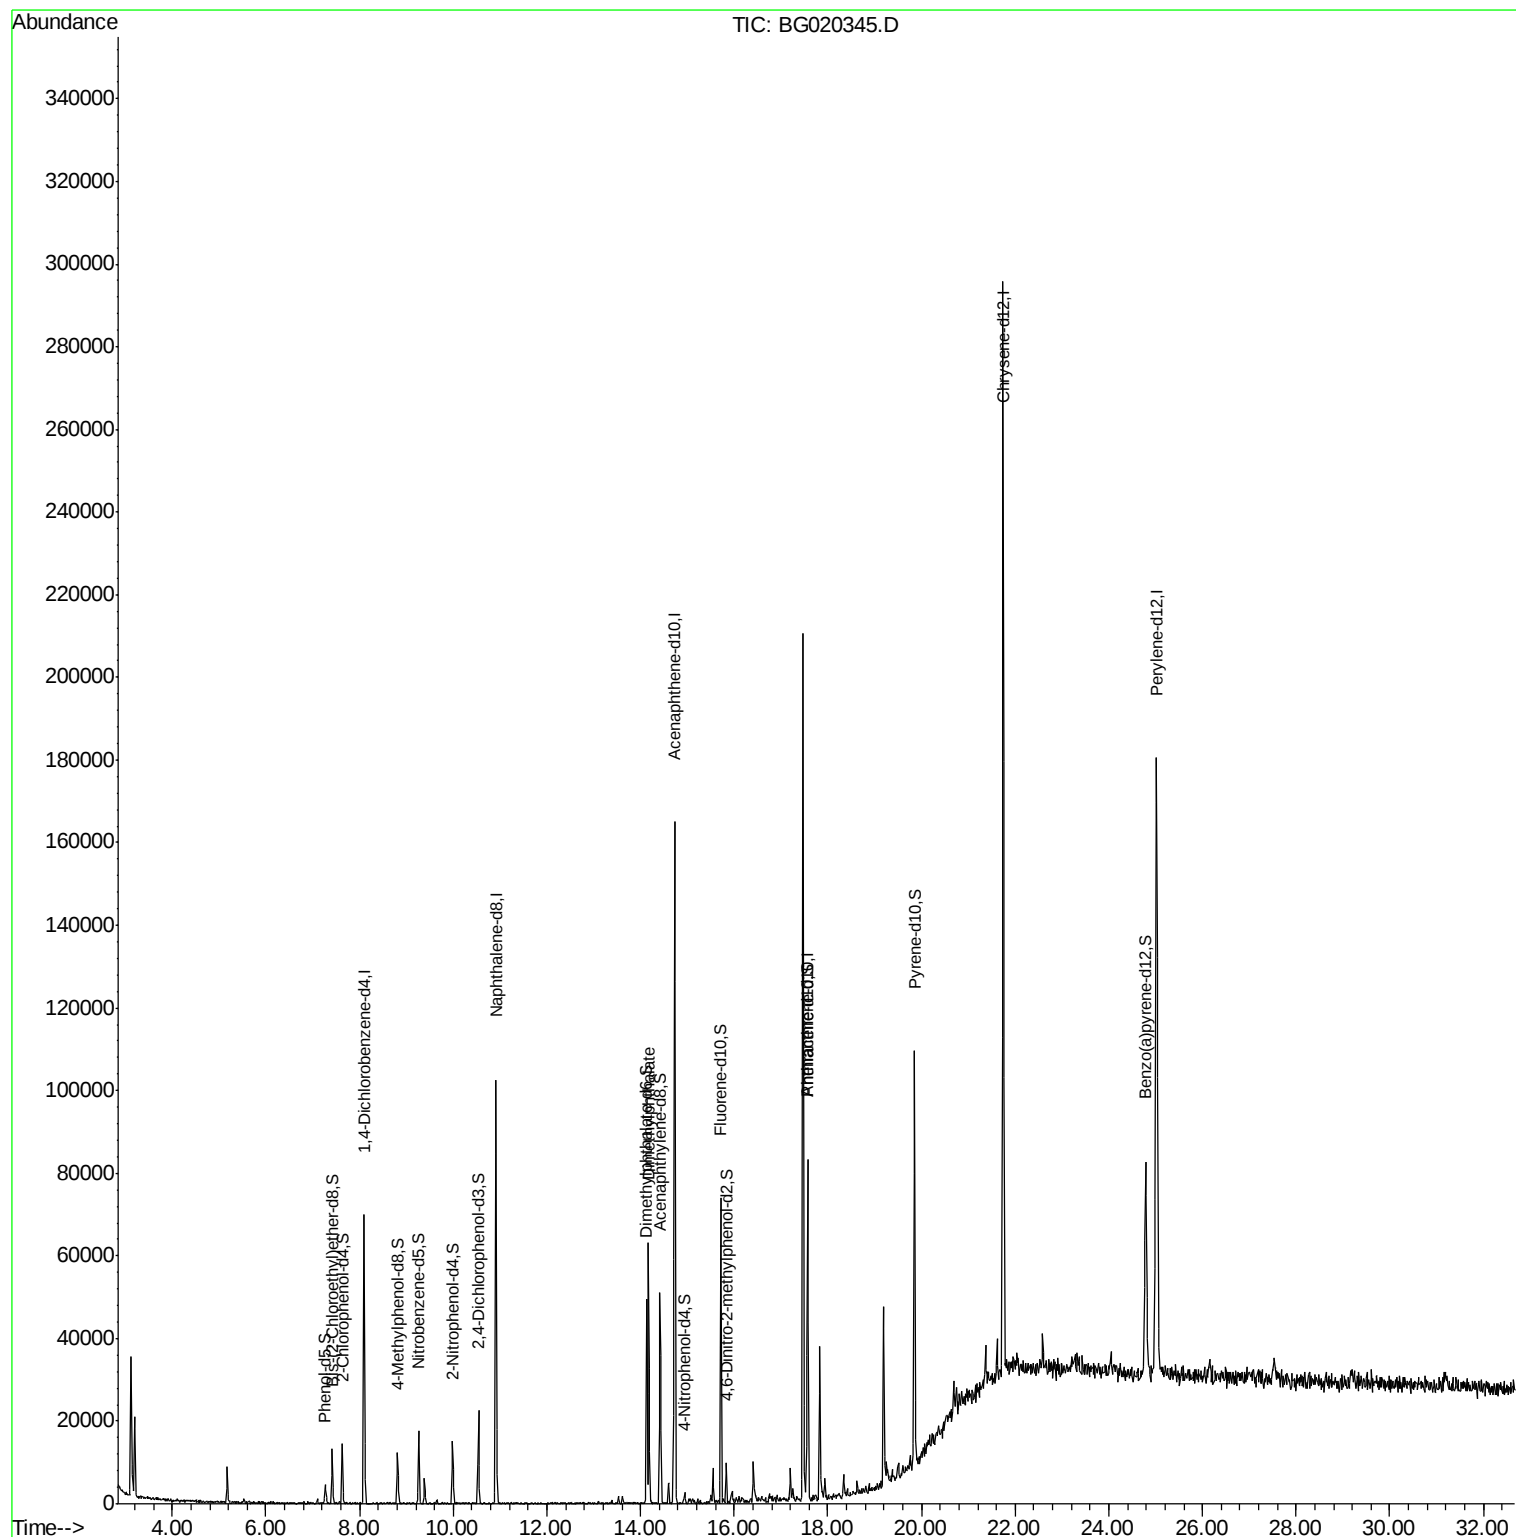

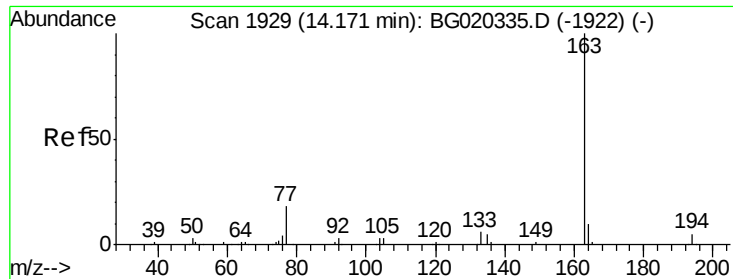

#45

Dimethylphthalate

Concen: 8.65 ng/ul

RT: 14.17 min Scan# 1929

Delta R.T. 0.00 min

Lab File: BG020345.D

Acq: 20 Dec 2015 16:48

Instrument :

BNA_G

ClientSampleId :

C04B2


Tot Ion:163 Resp: 42766

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 10.3 7.7 11.5

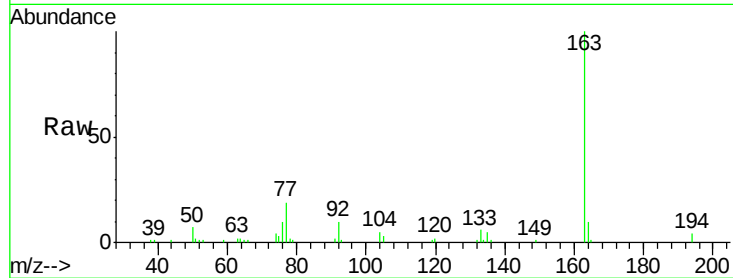

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

