

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
 Data File : BG020352.D
 Acq On : 20 Dec 2015 21:21
 Operator : UM/SJ
 Sample : G4803-20
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04C1

Quant Time: Dec 21 02:00:43 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 21 01:58:00 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	17180	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	75120	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	52068	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	124789	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	157634	20.00	ng/ul	0.00
86) Perylene-d12	25.01	264	147031	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.46	96	310	1.00	ng/uL	0.00
5) Phenol-d5	7.26	99	10344	6.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.41	67	28335	31.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	31306	28.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	20622	15.92	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	21093	36.02	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	24259	37.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	42370	32.10	ng/ul	0.00
29) 4-Chloroaniline-d4	11.05	131	1818	1.23	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	145808	34.62	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	177958	36.32	ng/ul	0.00
52) 4-Nitrophenol-d4	14.94	143	3646	4.83	ng/ul	0.00
58) Fluorene-d10	15.71	176	135879	35.57	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	19675	26.60	ng/ul	0.00
71) Anthracene-d10	17.57	188	208589	36.28	ng/ul	0.00
79) Pyrene-d10	19.85	212	247459	33.68	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	271822	37.06	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.17	163	27901	6.49	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
Data File : BG020352.D
Acq On : 20 Dec 2015 21:21
Operator : UM/SJ
Sample : G4803-20
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04C1

Quant Time: Dec 21 02:00:43 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 21 01:58:00 2015
Response via : Initial Calibration

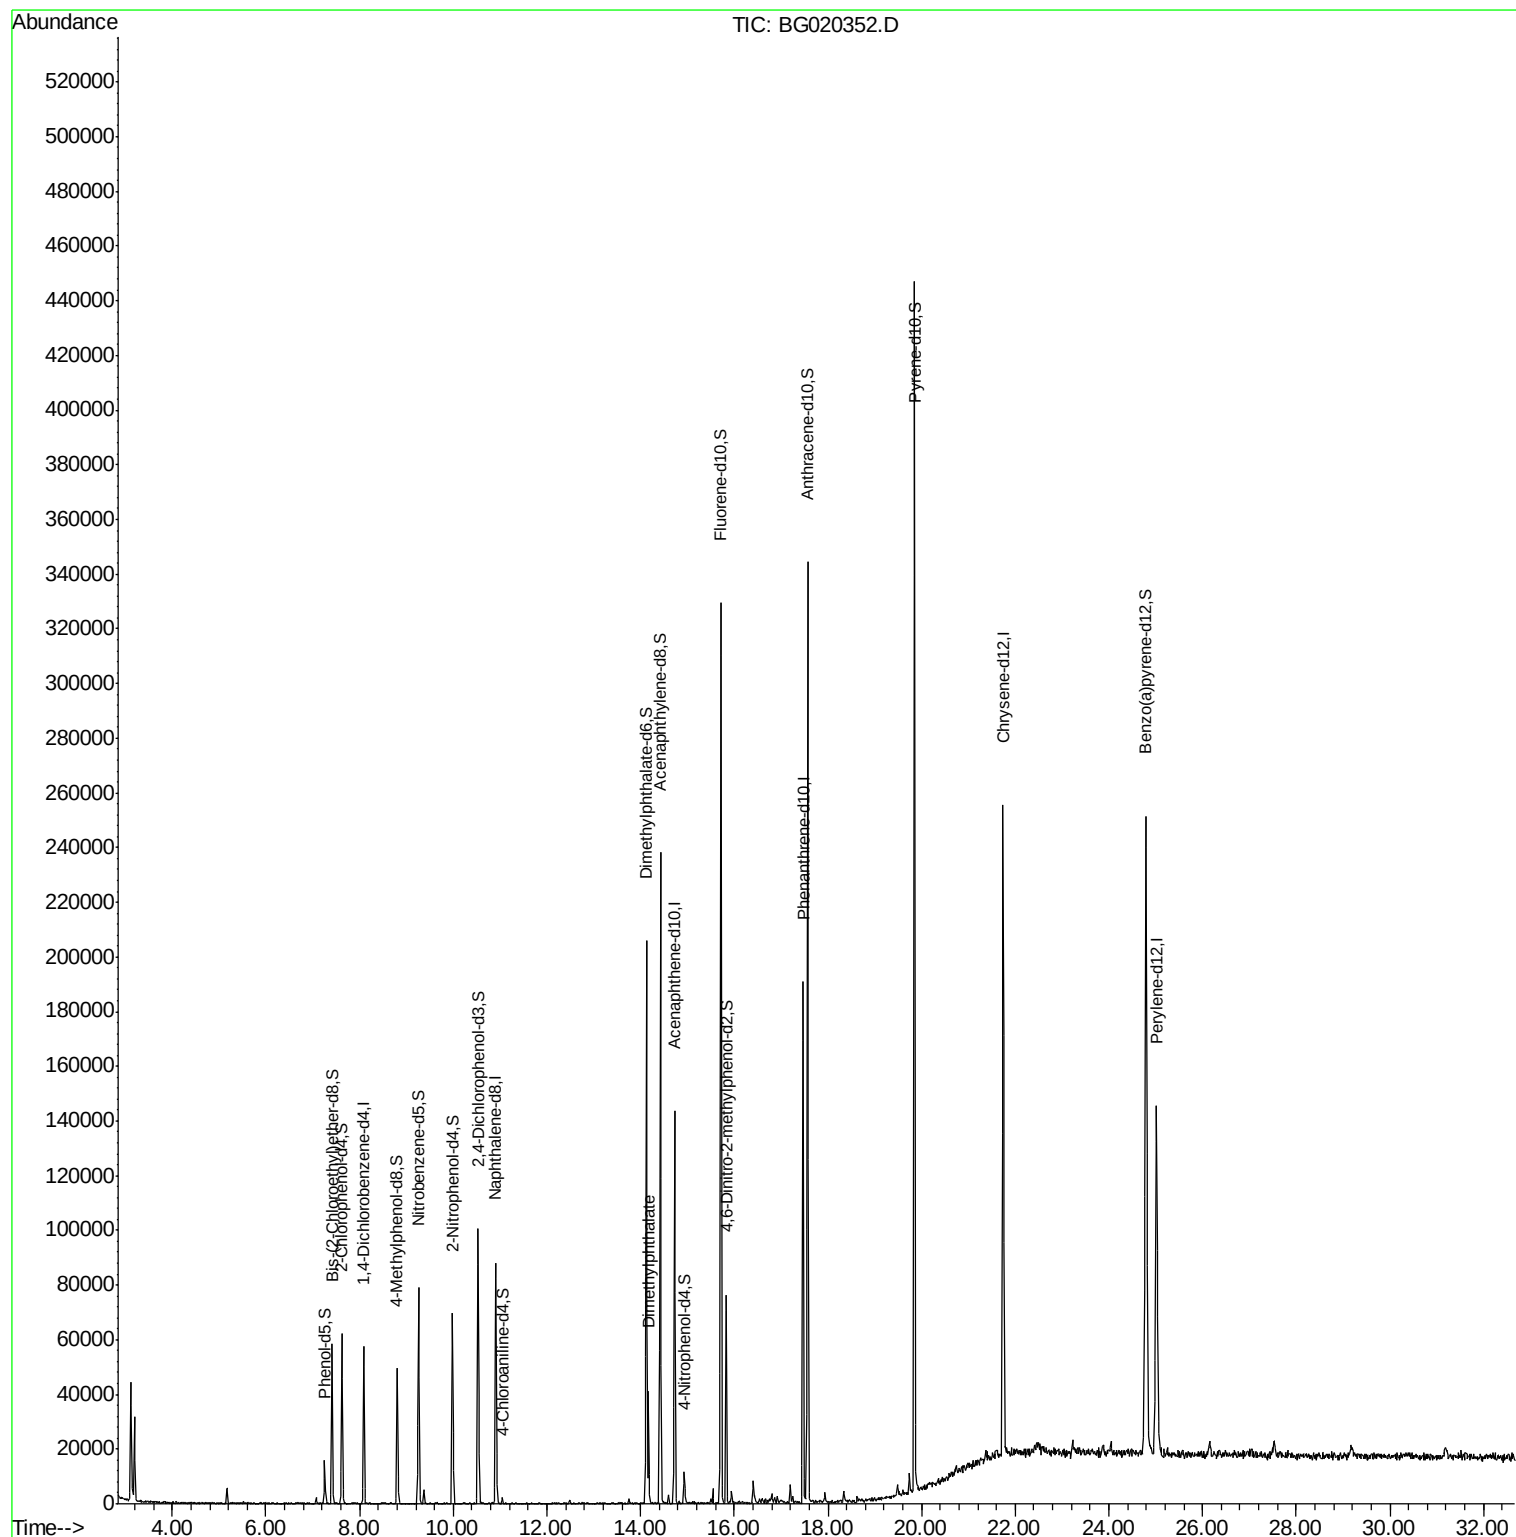

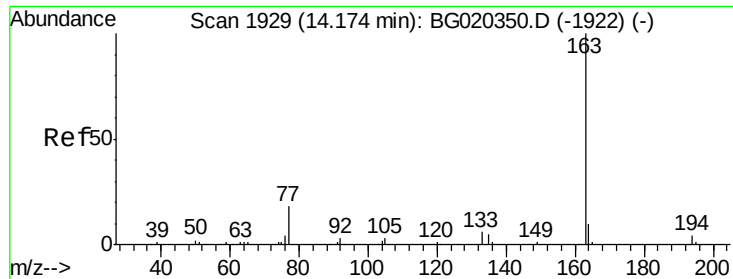

#45

Dimethylphthalate

Concen: 6.49 ng/ul

RT: 14.17 min Scan# 1928

Delta R.T. -0.01 min

Lab File: BG020352.D

Acq: 20 Dec 2015 21:21

Instrument :

BNA_G

ClientSampleId :

C04C1

Tot Ion:163 Resp: 27901

Ion Ratio Lower Upper

163 100

194 5.9 3.5 5.3#

164 10.3 7.7 11.5

