

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
 Data File : BG020354.D
 Acq On : 20 Dec 2015 22:38
 Operator : UM/SJ
 Sample : PB87360BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK60

Quant Time: Dec 21 02:01:00 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 21 01:58:00 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	18002	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	79719	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	54771	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	133597	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	169642	20.00	ng/ul	0.00
86) Perylene-d12	25.01	264	151915	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.46	96	2318	7.11	ng/uL	0.00
5) Phenol-d5	7.26	99	59215	37.30	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.41	67	34974	36.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.62	132	47085	40.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	52074	38.36	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	25338	40.77	ng/ul	0.00
22) 2-Nitrophenol-d4	9.98	143	29638	42.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	53799	38.41	ng/ul	0.00
29) 4-Chloroaniline-d4	11.05	131	61005	38.77	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	176246	39.78	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	208135	40.38	ng/ul	0.00
52) 4-Nitrophenol-d4	14.93	143	25836	32.52	ng/ul	0.00
58) Fluorene-d10	15.71	176	159987	39.81	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	23996	30.30	ng/ul	0.00
71) Anthracene-d10	17.57	188	261840	42.54	ng/ul	0.00
79) Pyrene-d10	19.85	212	308400	39.01	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	336804	44.45	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.80	70	1252	1.11	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
Data File : BG020354.D
Acq On : 20 Dec 2015 22:38
Operator : UM/SJ
Sample : PB87360BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK60

Quant Time: Dec 21 02:01:00 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 21 01:58:00 2015
Response via : Initial Calibration

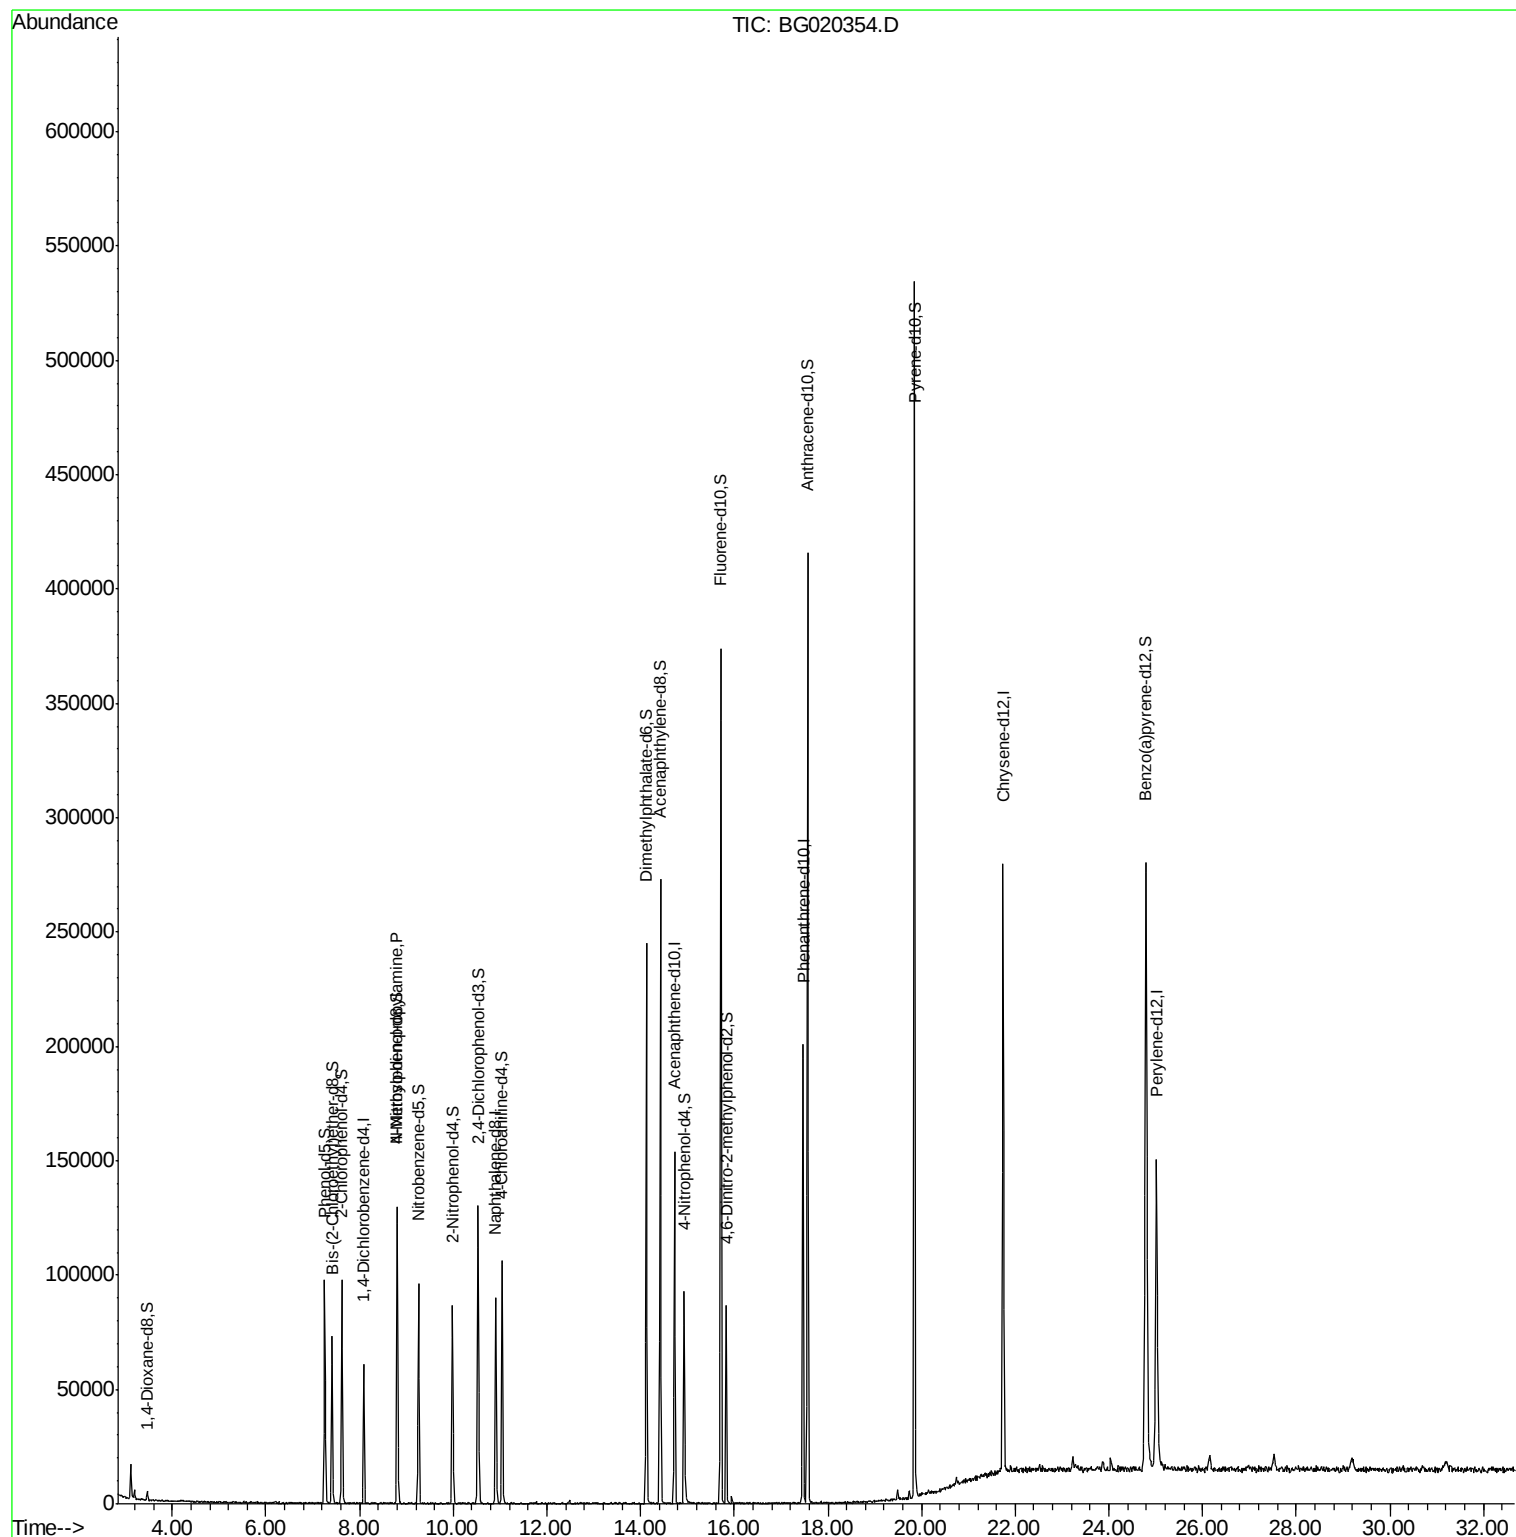

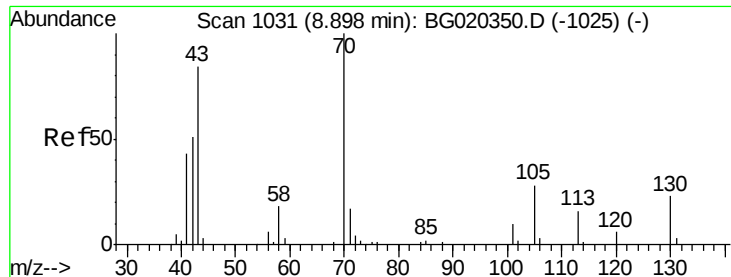

#15

N-Nitroso-di-n-propylamine

Concen: 1.11 ng/ul

RT: 8.80 min Scan# 1015

Delta R.T. -0.09 min

Lab File: BG020354.D

Acq: 20 Dec 2015 22:38

Instrument :

BNA_G

ClientSampleId :

SBLK60

Tot Ion: 70 Resp: 1252


Ion Ratio Lower Upper

70 100

42 321.6 44.3 66.5#

101 0.0 7.6 11.4#

130 0.0 17.0 25.4#

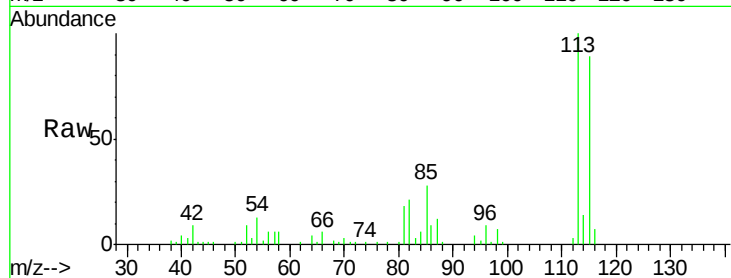


Abundance Ion 70.00 (69.70 to 70.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 101.00 (100.70 to 101.70): BGC

Ion 130.00 (129.70 to 130.70): BGC

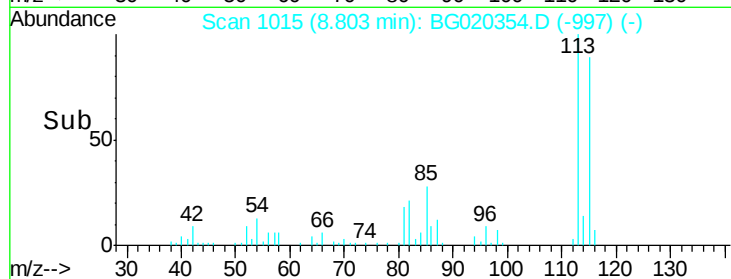

Time-->