

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122015\
 Data File : BG020371.D
 Acq On : 21 Dec 2015 9:39
 Operator : UM/SJ
 Sample : G4848-20
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9N67

Quant Time: Dec 22 00:23:16 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 21 07:46:34 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	19670	20.00	ng/ul	0.00
18) Naphthalene-d8	10.90	136	88995	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.72	164	63028	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	153212	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	189308	20.00	ng/ul	0.00
86) Perylene-d12	25.01	264	175874	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	2017	5.66	ng/uL	0.00
5) Phenol-d5	7.25	99	51329	29.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.41	67	31151	30.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.62	132	41762	33.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	46143	31.11	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	22782	32.84	ng/ul	0.00
22) 2-Nitrophenol-d4	9.98	143	26656	34.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	49159	31.44	ng/ul	0.00
29) 4-Chloroaniline-d4	11.04	131	62740	35.72	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	169158	33.18	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	195767	33.00	ng/ul	0.00
52) 4-Nitrophenol-d4	14.93	143	24265	26.54	ng/ul	0.00
58) Fluorene-d10	15.71	176	153685	33.24	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	23009	25.33	ng/ul	0.00
71) Anthracene-d10	17.57	188	242985	34.42	ng/ul	0.00
79) Pyrene-d10	19.85	212	290422	32.92	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	315312	35.94	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.17	163	62577	12.02	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122015\
Data File : BG020371.D
Acq On : 21 Dec 2015 9:39
Operator : UM/SJ
Sample : G4848-20
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9N67

Quant Time: Dec 22 00:23:16 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 21 07:46:34 2015
Response via : Initial Calibration

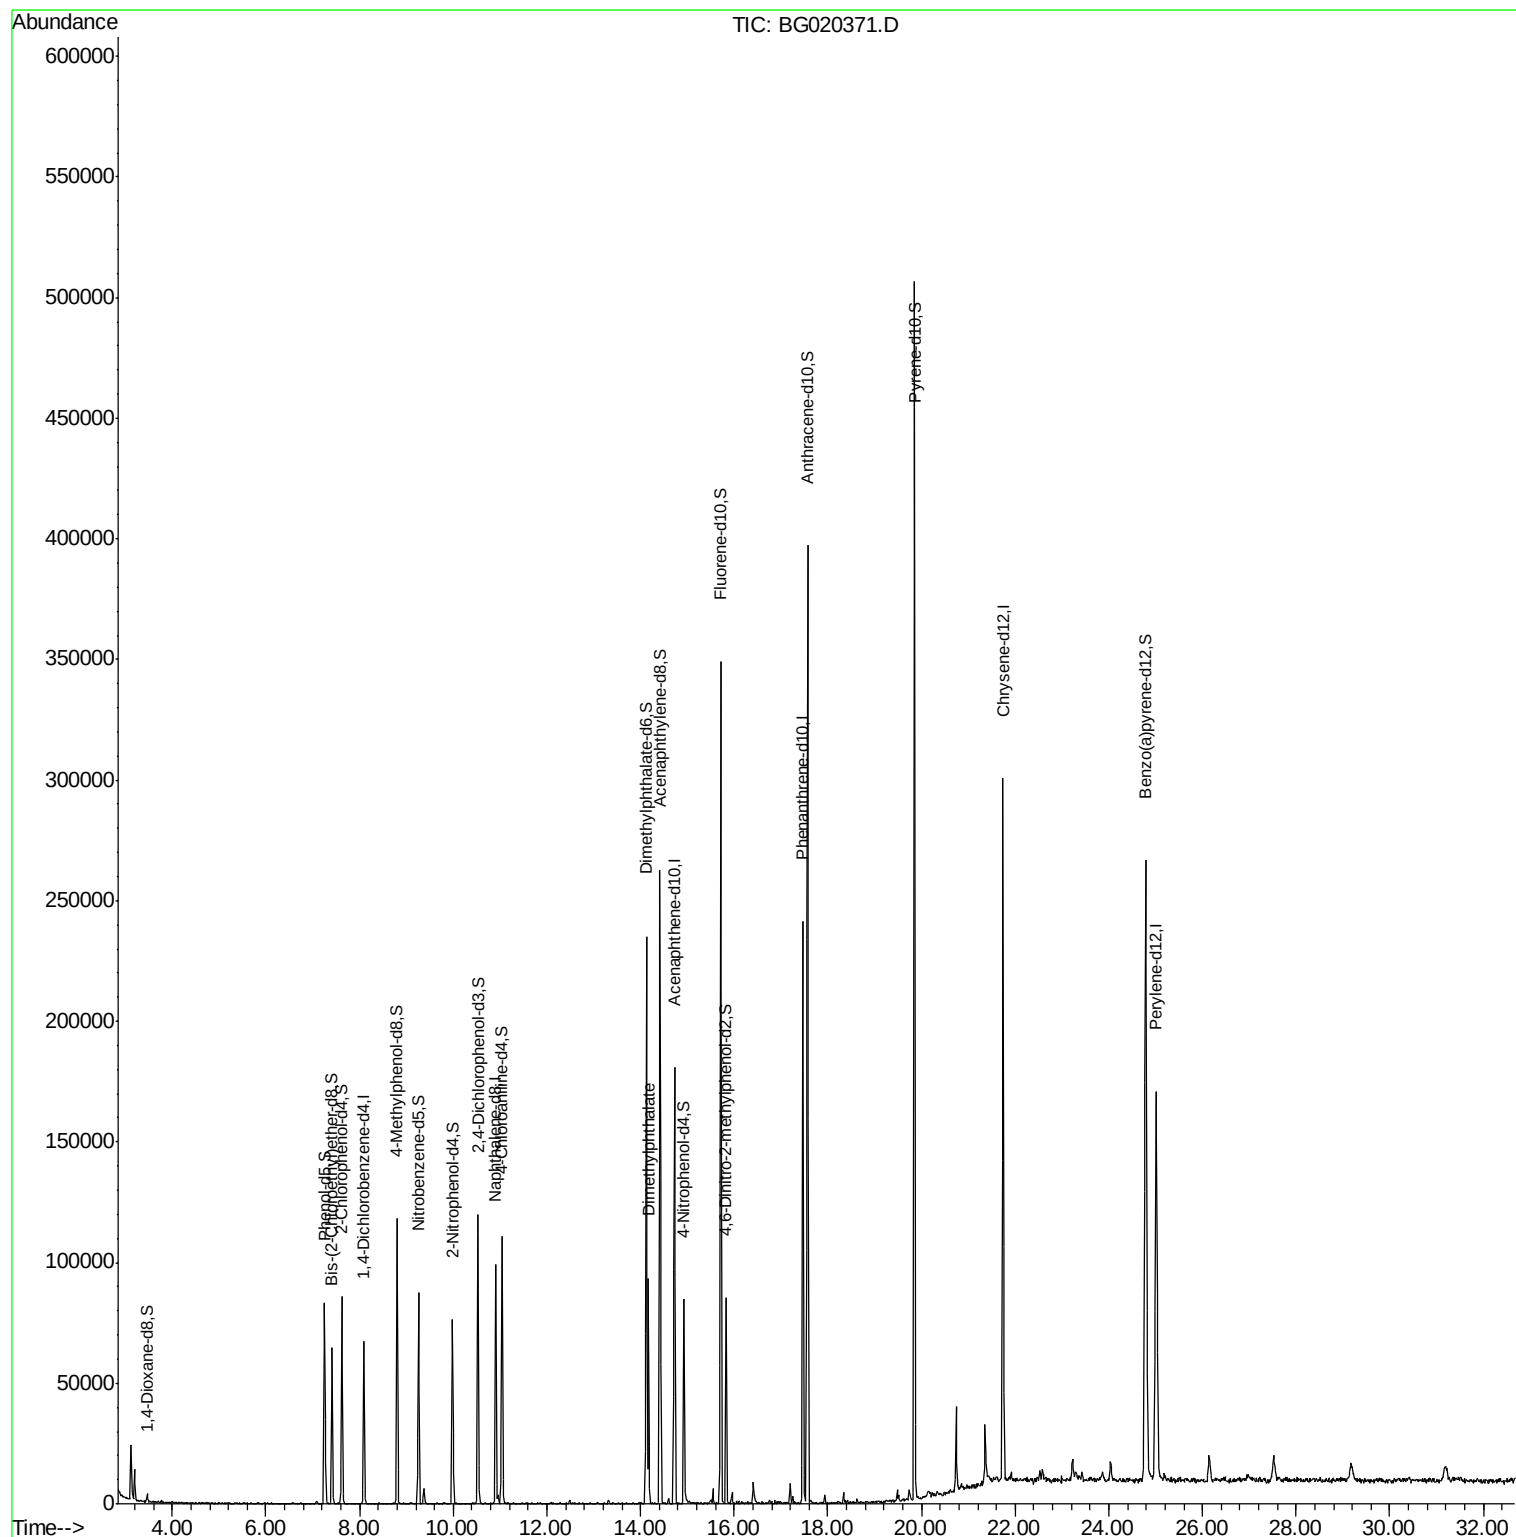

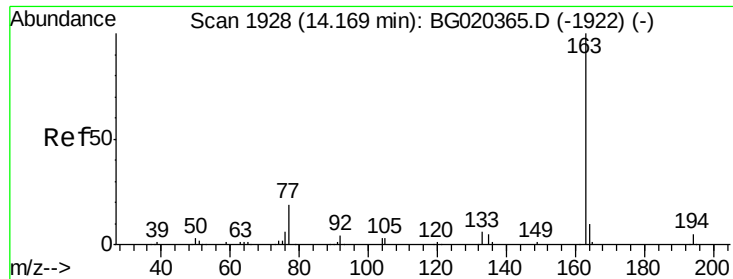

#45

Dimethylphthalate

Concen: 12.02 ng/ul

RT: 14.17 min Scan# 1928

Delta R.T. -0.00 min

Lab File: BG020371.D

Acq: 21 Dec 2015 9:39

Instrument :

BNA_G

ClientSampleId :

D9N67


Tgt Ion:163 Resp: 62577

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 9.4 7.7 11.5

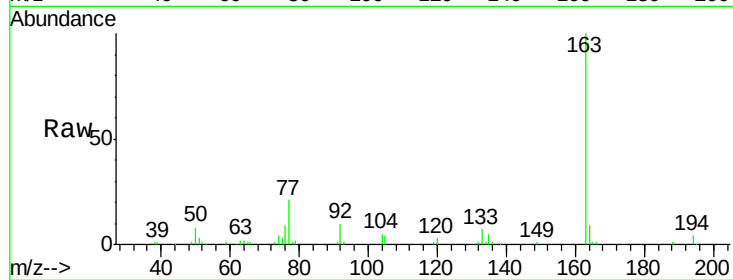

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

