

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
 Data File : BG020336.D
 Acq On : 20 Dec 2015 10:58
 Operator : UM/SJ
 Sample : PB87396BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.114	43	47	56	rVV	14605	28179	3.67%	0.407%
2	3.190	56	60	65	rVB2	4166	5790	0.75%	0.084%
3	3.467	100	107	113	rVB2	3935	6288	0.82%	0.091%
4	7.239	743	749	760	rBV	91570	154133	20.07%	2.226%
5	7.409	772	778	785	rBB	71900	114549	14.91%	1.654%
6	7.615	807	813	821	rVB	89567	153696	20.01%	2.219%
7	8.091	888	894	901	rBB	63030	103125	13.43%	1.489%
8	8.790	1006	1013	1024	rBB	121681	205518	26.76%	2.968%
9	9.254	1085	1092	1102	rVB	88817	157550	20.51%	2.275%
10	9.982	1209	1216	1223	rBB	82743	143628	18.70%	2.074%
11	10.523	1301	1308	1317	rBV	129945	222089	28.92%	3.207%
12	10.905	1366	1373	1381	rBB	89786	160444	20.89%	2.317%
13	11.034	1386	1395	1403	rBV	116954	215126	28.01%	3.106%
14	12.485	1636	1642	1647	rBB2	1612	2561	0.33%	0.037%
15	14.119	1914	1920	1926	rBV	249418	354535	46.16%	5.119%
16	14.418	1964	1971	1979	rBV	271088	414075	53.91%	5.979%
17	14.724	2016	2023	2030	rBV2	158426	250913	32.67%	3.623%
18	14.906	2048	2054	2066	rBV	104000	165374	21.53%	2.388%
19	15.711	2184	2191	2200	rBB	367584	547695	71.31%	7.908%
20	15.823	2204	2210	2218	rBV	91763	135944	17.70%	1.963%
21	15.952	2227	2232	2239	rBV	3372	4809	0.63%	0.069%
22	17.468	2483	2490	2500	rBV	202459	307974	40.10%	4.447%
23	17.568	2500	2507	2518	rVB	398171	601646	78.34%	8.687%
24	19.483	2829	2833	2836	rBV	4532	5942	0.77%	0.086%
25	19.512	2836	2838	2842	rVB3	1411	1483	0.19%	0.021%
26	19.736	2870	2876	2880	rBV	3443	4893	0.64%	0.071%
27	19.847	2888	2895	2904	rBV	519561	734703	95.66%	10.609%
28	20.129	2940	2943	2944	rBV2	2576	2122	0.28%	0.031%
29	20.335	2977	2978	2983	rVB2	1214	1460	0.19%	0.021%
30	20.740	3044	3047	3052	rVV4	2438	4371	0.57%	0.063%
31	20.782	3052	3054	3058	rVV4	1433	2044	0.27%	0.030%
32	20.905	3070	3075	3076	rVV4	1575	2316	0.30%	0.033%
33	21.445	3165	3167	3171	rVB4	2759	3470	0.45%	0.050%
34	21.534	3180	3182	3188	rVB5	1367	1783	0.23%	0.026%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
 Data File : BG020336.D
 Acq On : 20 Dec 2015 10:58
 Operator : UM/SJ
 Sample : PB87396BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

35	21.645	3199	3201	3206	rVB5	1662	1869	0.24%	0.027%
36	21.739	3210	3217	3225	rVV	251413	411969	53.64%	5.949%
37	21.863	3236	3238	3242	rBV5	1164	1622	0.21%	0.023%
38	22.098	3277	3278	3281	rBV2	1628	1809	0.24%	0.026%
39	22.309	3313	3314	3317	rBV3	1511	1252	0.16%	0.018%
40	22.339	3317	3319	3323	rVB2	1397	1545	0.20%	0.022%
41	22.938	3420	3421	3424	rVB3	1939	1799	0.23%	0.026%
42	22.967	3424	3426	3428	rBV3	1921	1924	0.25%	0.028%
43	23.008	3431	3433	3436	rVB4	1545	1393	0.18%	0.020%
44	23.032	3436	3437	3443	rBV5	2302	3152	0.41%	0.046%
45	23.120	3450	3452	3456	rVB5	1428	1707	0.22%	0.025%
46	23.214	3464	3468	3469	rBV4	3644	3790	0.49%	0.055%
47	23.661	3541	3544	3552	rVB5	1764	4324	0.56%	0.062%
48	23.719	3552	3554	3557	rBV3	1045	1432	0.19%	0.021%
49	23.854	3574	3577	3578	rBV3	2762	2625	0.34%	0.038%
50	24.037	3604	3608	3609	rBV4	3714	5089	0.66%	0.073%
51	24.242	3641	3643	3646	rVB4	1587	1532	0.20%	0.022%
52	24.283	3649	3650	3655	rBV4	1605	1597	0.21%	0.023%
53	24.512	3686	3689	3692	rVB4	1524	1823	0.24%	0.026%
54	24.789	3724	3736	3747	rBV	279236	768015	100.00%	11.090%
55	25.006	3762	3773	3785	rBV2	143203	395118	51.45%	5.705%
56	25.218	3807	3809	3811	rBV2	2356	1791	0.23%	0.026%
57	25.364	3831	3834	3839	rBV6	1588	2351	0.31%	0.034%
58	25.429	3844	3845	3846	rBV	2377	1409	0.18%	0.020%
59	25.840	3912	3915	3916	rVB3	1439	1276	0.17%	0.018%
60	26.046	3949	3950	3953	rVB3	1700	1247	0.16%	0.018%
61	26.081	3953	3956	3958	rVB2	2080	2014	0.26%	0.029%
62	26.105	3958	3960	3961	rBV	1627	1680	0.22%	0.024%
63	26.146	3961	3967	3970	rVV6	4537	10150	1.32%	0.147%
64	26.193	3973	3975	3978	rVB3	1763	1395	0.18%	0.020%
65	26.410	4009	4012	4013	rBV2	1755	1937	0.25%	0.028%
66	26.504	4026	4028	4031	rBV3	1321	1530	0.20%	0.022%
67	26.716	4062	4064	4066	rBV3	2053	1292	0.17%	0.019%
68	26.751	4068	4070	4074	rBV3	906	1346	0.18%	0.019%
69	26.822	4079	4082	4083	rBV2	1484	1333	0.17%	0.019%
70	26.833	4083	4084	4088	rVB3	1417	1613	0.21%	0.023%
71	26.916	4096	4098	4101	rVB3	1807	1443	0.19%	0.021%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
 Data File : BG020336.D
 Acq On : 20 Dec 2015 10:58
 Operator : UM/SJ
 Sample : PB87396BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

72	27.239	4151	4153	4155	rBV3	1730	1765	0.23%	0.025%
73	27.462	4187	4191	4192	rBV3	1609	1877	0.24%	0.027%
74	27.515	4194	4200	4203	rBV6	4431	8908	1.16%	0.129%
75	27.732	4235	4237	4241	rVB4	1210	1467	0.19%	0.021%
76	27.767	4241	4243	4246	rBV3	1094	1370	0.18%	0.020%
77	27.985	4277	4280	4281	rBV2	1611	1457	0.19%	0.021%
78	28.085	4294	4297	4298	rBV3	1465	1566	0.20%	0.023%
79	28.326	4335	4338	4340	rBV3	1202	1385	0.18%	0.020%
80	28.367	4343	4345	4349	rVV4	1519	1593	0.21%	0.023%
81	28.402	4349	4351	4355	rVV5	1179	1666	0.22%	0.024%
82	28.637	4389	4391	4394	rVB4	1104	1271	0.17%	0.018%
83	28.990	4448	4451	4455	rBV5	1601	2345	0.31%	0.034%
84	29.042	4458	4460	4461	rBV2	1584	1259	0.16%	0.018%
85	29.060	4461	4463	4467	rVB4	1429	1302	0.17%	0.019%
86	29.119	4470	4473	4475	rBV3	2464	2915	0.38%	0.042%
87	29.254	4494	4496	4499	rVB4	1423	1361	0.18%	0.020%
88	29.424	4523	4525	4528	rBV4	1082	1300	0.17%	0.019%
89	29.988	4619	4621	4624	rVB3	1603	1555	0.20%	0.022%
90	30.253	4662	4666	4669	rBV2	1560	2954	0.38%	0.043%
91	30.682	4736	4739	4742	rBV4	1070	1761	0.23%	0.025%
92	31.046	4799	4801	4803	rBV3	1234	1372	0.18%	0.020%
93	31.428	4865	4866	4870	rBV4	1611	1532	0.20%	0.022%
94	31.910	4947	4948	4951	rBV3	1649	1470	0.19%	0.021%
95	32.015	4962	4966	4971	rBV4	1260	2813	0.37%	0.041%
96	32.315	5015	5017	5019	rVV2	1408	1383	0.18%	0.020%
97	32.350	5021	5023	5027	rVB4	1620	1479	0.19%	0.021%
98	32.521	5051	5052	5056	rVB3	1796	1283	0.17%	0.019%
99	32.574	5056	5061	5063	rBV4	1194	1917	0.25%	0.028%
100	32.609	5066	5067	5073	rVB4	1165	1729	0.23%	0.025%


Sum of corrected areas: 6925476

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
Data File : BG020336.D
Acq On : 20 Dec 2015 10:58
Operator : UM/SJ
Sample : PB87396BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK96

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

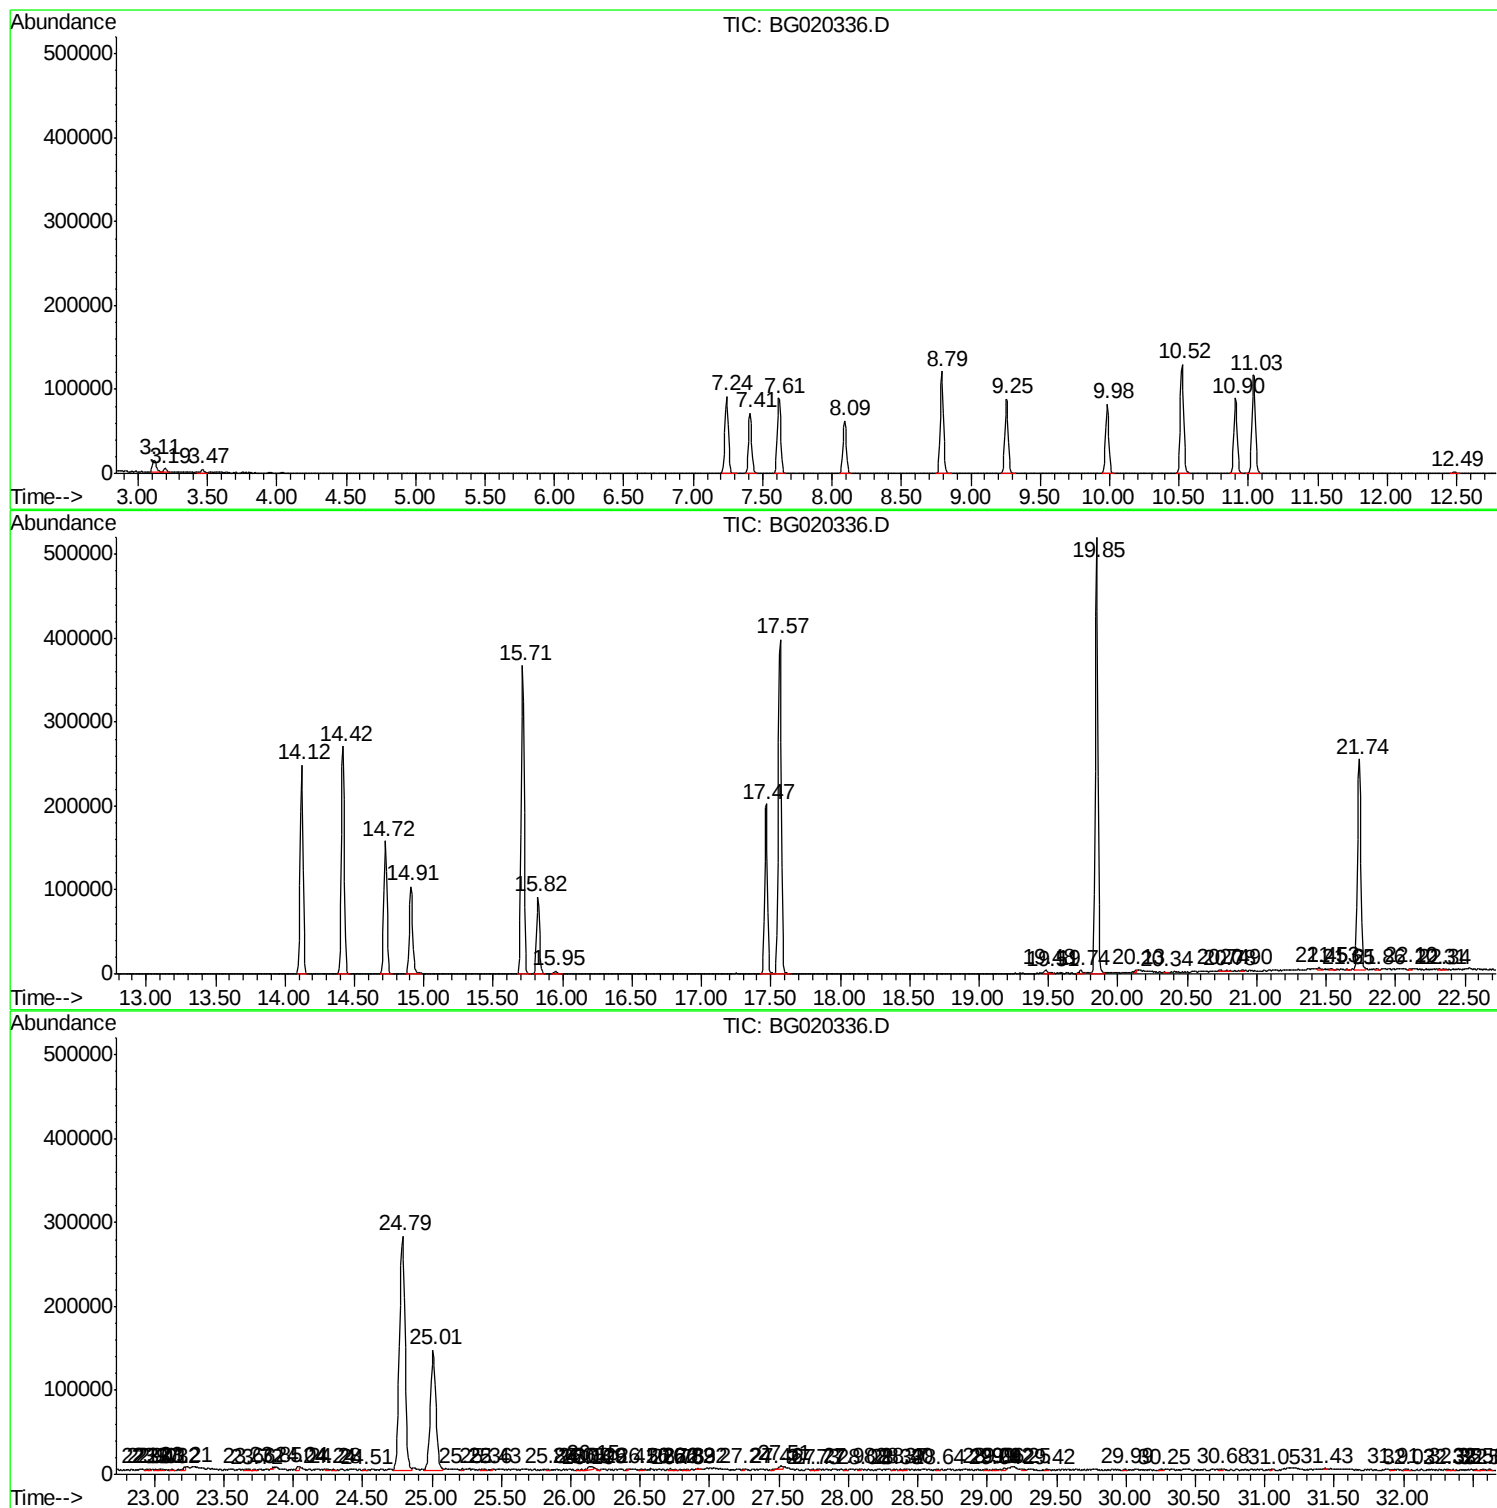

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122015\
Data File : BG020336.D
Acq On : 20 Dec 2015 10:58
Operator : UM/SJ
Sample : PB87396BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK96

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122015\
Data File : BG020336.D
Acq On : 20 Dec 2015 10:58
Operator : UM/SJ
Sample : PB87396BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK96

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc