

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
 Data File : BG020337.D
 Acq On : 20 Dec 2015 11:37
 Operator : UM/SJ
 Sample : PB87425BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.114	41	47	56	rBV2	14872	29175	3.56%	0.403%
2	3.196	56	61	64	rVB2	4053	5481	0.67%	0.076%
3	3.467	103	107	113	rBV2	4611	6739	0.82%	0.093%
4	7.239	743	749	758	rVB	99070	165217	20.13%	2.279%
5	7.409	770	778	786	rBB	77086	125843	15.34%	1.736%
6	7.621	805	814	823	rBB	96950	168340	20.52%	2.322%
7	8.091	888	894	902	rBB	61358	101690	12.39%	1.403%
8	8.790	1006	1013	1024	rBB2	131055	224988	27.42%	3.104%
9	9.254	1085	1092	1100	rBB	98896	174750	21.30%	2.411%
10	9.983	1209	1216	1225	rVB	89008	156677	19.09%	2.162%
11	10.523	1301	1308	1317	rBB	135136	240740	29.34%	3.321%
12	10.905	1366	1373	1382	rBB	90728	160205	19.52%	2.210%
13	11.034	1389	1395	1403	rBV	127078	232404	28.32%	3.206%
14	12.486	1637	1642	1647	rBB	1710	2452	0.30%	0.034%
15	14.119	1914	1920	1926	rBV	270801	378137	46.08%	5.217%
16	14.419	1963	1971	1978	rBV	281834	451040	54.97%	6.223%
17	14.724	2016	2023	2031	rVB2	145135	243811	29.71%	3.364%
18	14.906	2048	2054	2066	rBV	110787	174071	21.21%	2.402%
19	15.711	2184	2191	2198	rBV	402625	590794	72.00%	8.151%
20	15.823	2205	2210	2218	rBV	98251	142427	17.36%	1.965%
21	15.952	2225	2232	2237	rBV2	3007	5150	0.63%	0.071%
22	17.462	2479	2489	2496	rBV2	196707	303894	37.04%	4.193%
23	17.562	2500	2506	2514	rVB2	420175	652073	79.47%	8.996%
24	19.483	2826	2833	2836	rBV	4868	6634	0.81%	0.092%
25	19.736	2871	2876	2880	rBV	3986	5824	0.71%	0.080%
26	19.848	2888	2895	2904	rBV	568480	793908	96.75%	10.953%
27	20.059	2928	2931	2934	rVB2	1101	1193	0.15%	0.016%
28	20.171	2948	2950	2953	rVB3	1425	1289	0.16%	0.018%
29	20.306	2968	2973	2977	rBV3	879	1875	0.23%	0.026%
30	20.664	3033	3034	3039	rVB3	1140	1159	0.14%	0.016%
31	20.799	3055	3057	3059	rBV3	1520	1022	0.12%	0.014%
32	21.117	3110	3111	3116	rVB3	1009	1075	0.13%	0.015%
33	21.170	3116	3120	3121	rBV4	1452	1300	0.16%	0.018%
34	21.322	3144	3146	3148	rVB3	1751	1378	0.17%	0.019%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
 Data File : BG020337.D
 Acq On : 20 Dec 2015 11:37
 Operator : UM/SJ
 Sample : PB87425BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

35	21.546	3183	3184	3187	rBV2	1406	1296	0.16%	0.018%
36	21.739	3210	3217	3224	rBV	243199	396042	48.27%	5.464%
37	21.839	3232	3234	3239	rVB4	1631	1848	0.23%	0.025%
38	21.986	3257	3259	3264	rVB6	1557	2168	0.26%	0.030%
39	22.033	3264	3267	3268	rBV2	1155	1340	0.16%	0.018%
40	22.098	3276	3278	3283	rVB4	1077	1359	0.17%	0.019%
41	22.198	3294	3295	3298	rVB3	1307	1270	0.15%	0.018%
42	22.539	3351	3353	3355	rVB4	2162	1635	0.20%	0.023%
43	22.797	3395	3397	3399	rBV3	1207	1318	0.16%	0.018%
44	22.821	3399	3401	3403	rVV2	1261	1089	0.13%	0.015%
45	22.956	3422	3424	3426	rVB3	1240	1056	0.13%	0.015%
46	23.009	3431	3433	3436	rVB3	1264	1414	0.17%	0.020%
47	23.067	3440	3443	3444	rBV3	1212	1031	0.13%	0.014%
48	23.220	3467	3469	3472	rVB3	1614	1865	0.23%	0.026%
49	23.526	3519	3521	3523	rVB2	1248	1081	0.13%	0.015%
50	23.573	3527	3529	3531	rBV4	1878	1727	0.21%	0.024%
51	23.637	3538	3540	3541	rBV2	1319	1063	0.13%	0.015%
52	23.672	3544	3546	3549	rVB3	1877	1446	0.18%	0.020%
53	23.784	3563	3565	3569	rBV4	915	1218	0.15%	0.017%
54	23.872	3574	3580	3586	rVV6	4137	8773	1.07%	0.121%
55	24.037	3604	3608	3609	rBV3	2290	2596	0.32%	0.036%
56	24.495	3683	3686	3689	rVB4	1487	1835	0.22%	0.025%
57	24.624	3705	3708	3711	rVB3	1321	1681	0.20%	0.023%
58	24.789	3725	3736	3750	rVV	288281	820556	100.00%	11.321%
59	24.883	3750	3752	3755	rBV3	1324	1395	0.17%	0.019%
60	25.012	3761	3774	3788	rBV2	129692	380238	46.34%	5.246%
61	25.177	3799	3802	3803	rBV2	1618	1656	0.20%	0.023%
62	25.253	3813	3815	3816	rBV2	1754	1109	0.14%	0.015%
63	25.335	3828	3829	3832	rBV2	1908	1371	0.17%	0.019%
64	25.429	3843	3845	3846	rVB	1954	1068	0.13%	0.015%
65	25.465	3850	3851	3857	rVB4	1125	1582	0.19%	0.022%
66	25.506	3857	3858	3861	rBV3	1873	1203	0.15%	0.017%
67	25.905	3925	3926	3928	rVB2	2232	1344	0.16%	0.019%
68	26.076	3953	3955	3957	rBV2	1779	1815	0.22%	0.025%
69	26.264	3984	3987	3992	rBV6	1768	1809	0.22%	0.025%
70	26.581	4039	4041	4044	rVB3	1287	1134	0.14%	0.016%
71	26.939	4100	4102	4105	rVB3	1273	1073	0.13%	0.015%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
Data File : BG020337.D
Acq On : 20 Dec 2015 11:37
Operator : UM/SJ
Sample : PB87425BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK25

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Title : SVOA CALIBRATION

72	26.992	4109	4111	4114	rVB4	1122	1067	0.13%	0.015%
73	27.480	4192	4194	4196	rBV2	1538	1067	0.13%	0.015%
74	27.515	4196	4200	4202	rBV5	2967	4789	0.58%	0.066%
75	27.685	4227	4229	4231	rBV3	1311	1233	0.15%	0.017%
76	27.879	4260	4262	4265	rVB3	1017	1051	0.13%	0.015%
77	27.926	4268	4270	4272	rVB2	1293	1099	0.13%	0.015%
78	28.238	4321	4323	4324	rBV2	1145	1147	0.14%	0.016%
79	28.291	4330	4332	4334	rVB3	1742	1340	0.16%	0.018%
80	28.308	4334	4335	4337	rBV2	1708	1133	0.14%	0.016%
81	28.355	4342	4343	4345	rVB2	2086	1056	0.13%	0.015%
82	28.502	4365	4368	4370	rBV4	1288	1407	0.17%	0.019%
83	29.430	4524	4526	4529	rVV3	1151	1142	0.14%	0.016%
84	29.724	4574	4576	4577	rBV2	1401	1035	0.13%	0.014%
85	29.777	4583	4585	4586	rBV2	1479	1130	0.14%	0.016%
86	30.323	4676	4678	4682	rBV5	1436	2054	0.25%	0.028%
87	30.447	4696	4699	4700	rBV2	1164	1387	0.17%	0.019%
88	30.517	4708	4711	4713	rBV2	1449	1461	0.18%	0.020%
89	30.611	4725	4727	4729	rVB2	2058	1686	0.21%	0.023%
90	30.629	4729	4730	4732	rBV2	1871	1144	0.14%	0.016%
91	30.870	4770	4771	4773	rBV2	1444	1167	0.14%	0.016%
92	30.911	4775	4778	4779	rBV2	1002	1075	0.13%	0.015%
93	31.046	4800	4801	4803	rBV2	1479	1207	0.15%	0.017%
94	31.093	4808	4809	4812	rBV3	1273	1283	0.16%	0.018%
95	31.170	4819	4822	4823	rBV3	1350	1835	0.22%	0.025%
96	31.369	4852	4856	4860	rBV4	1591	1889	0.23%	0.026%
97	31.481	4873	4875	4878	rBV3	1054	1155	0.14%	0.016%
98	32.198	4993	4997	5001	rBV4	958	1442	0.18%	0.020%
99	32.251	5005	5006	5008	rBV2	1155	1070	0.13%	0.015%
100	32.368	5024	5026	5030	rBV4	1703	2459	0.30%	0.034%


Sum of corrected areas: 7248269

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122015\
Data File : BG020337.D
Acq On : 20 Dec 2015 11:37
Operator : UM/SJ
Sample : PB87425BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK25

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

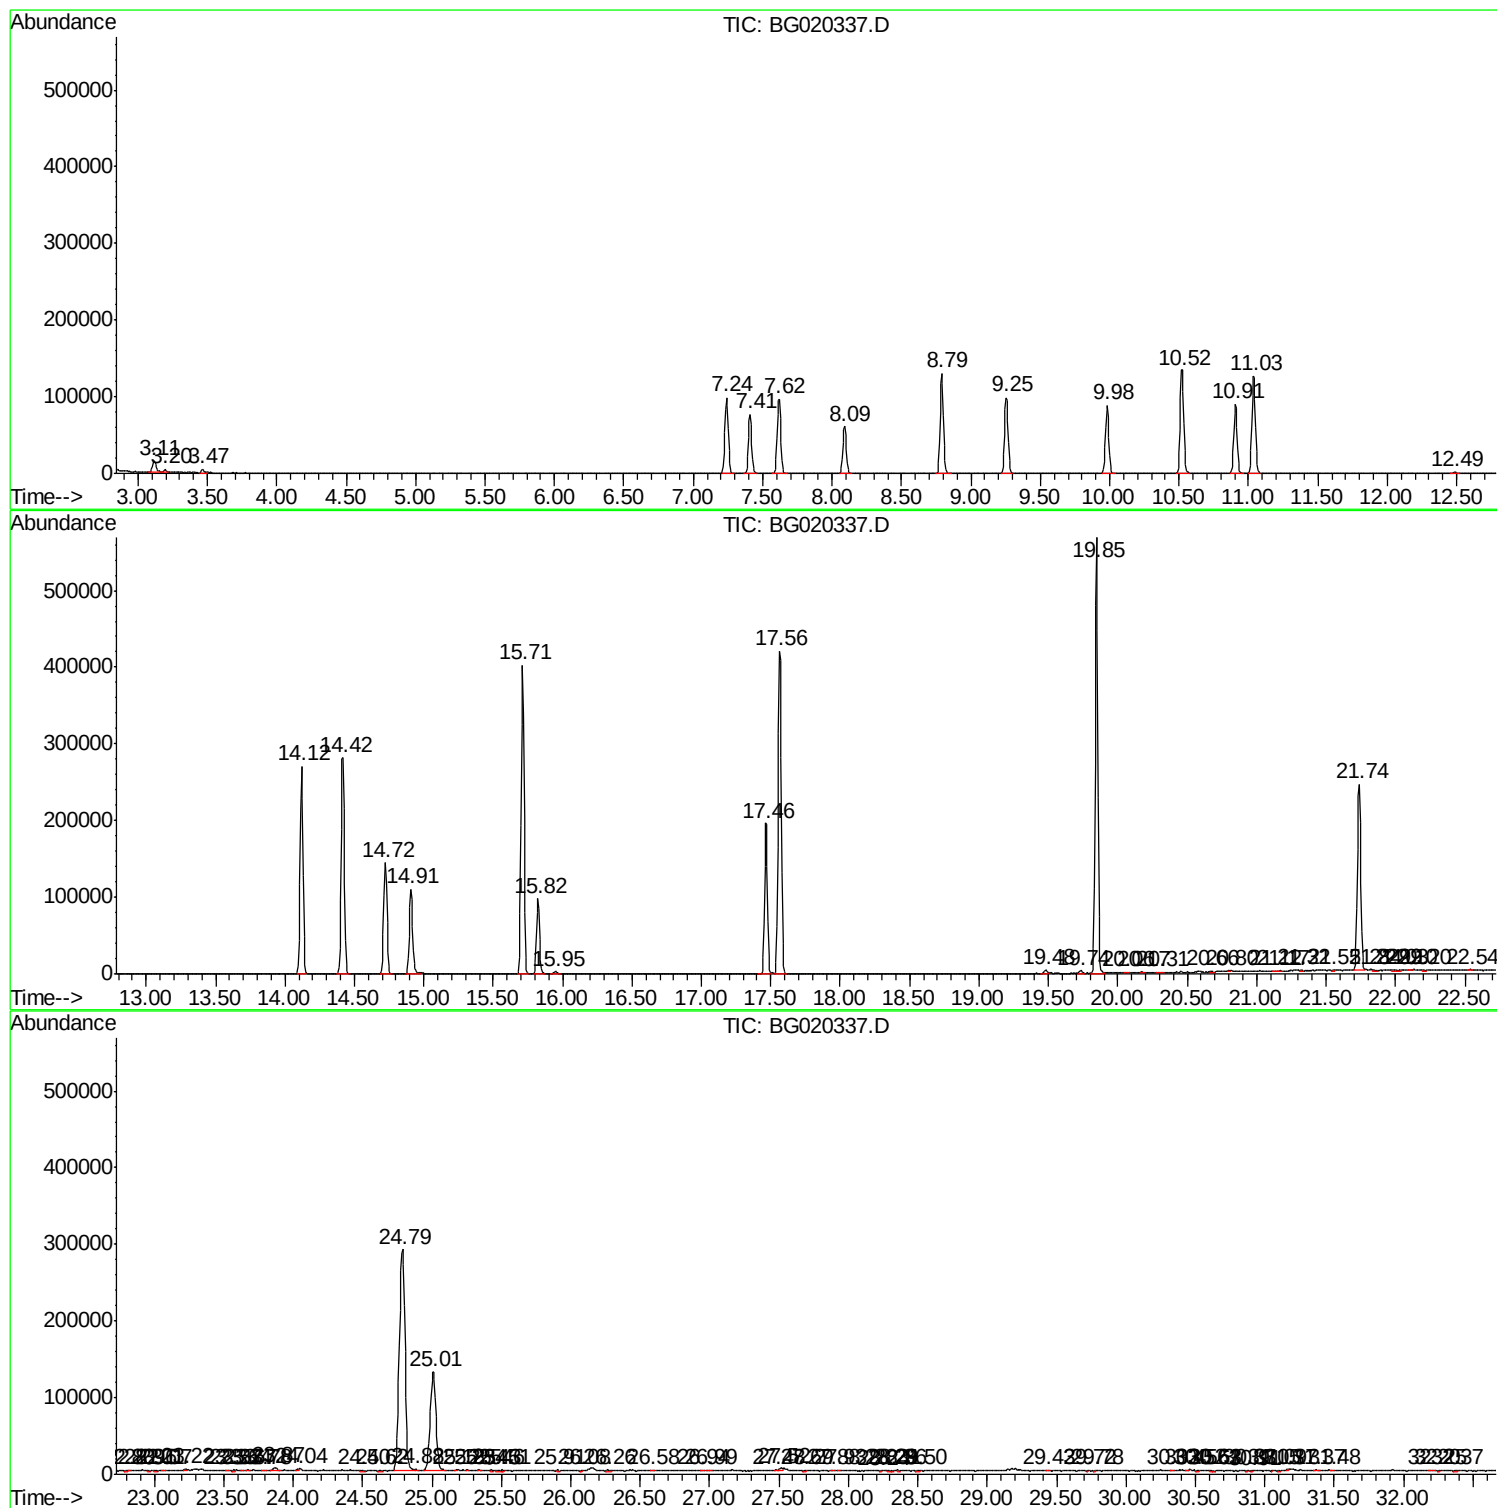

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122015\
Data File : BG020337.D
Acq On : 20 Dec 2015 11:37
Operator : UM/SJ
Sample : PB87425BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK25

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122015\
Data File : BG020337.D
Acq On : 20 Dec 2015 11:37
Operator : UM/SJ
Sample : PB87425BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK25

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc