






Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

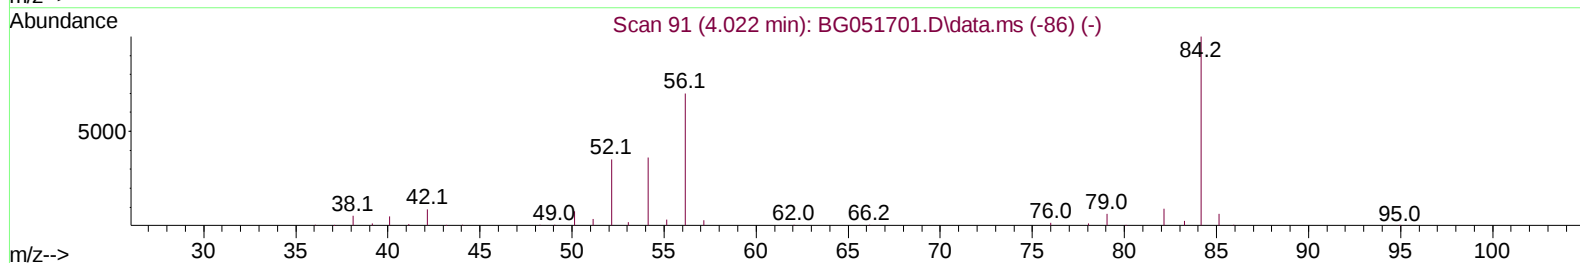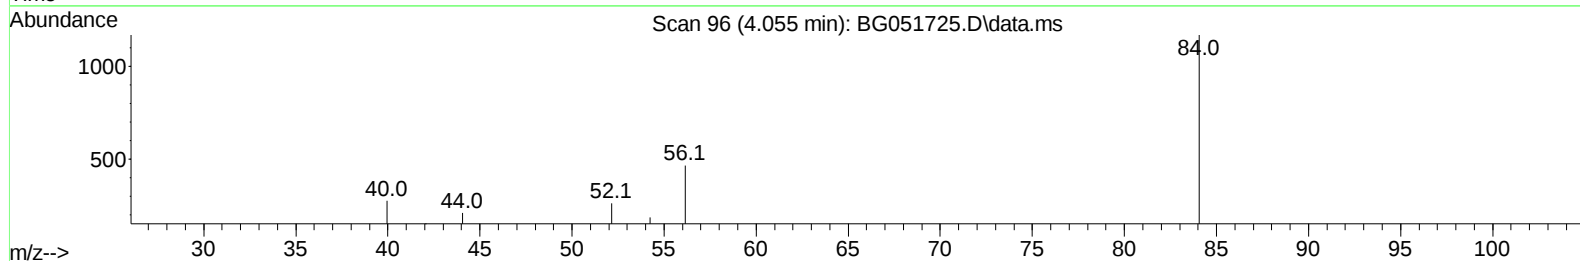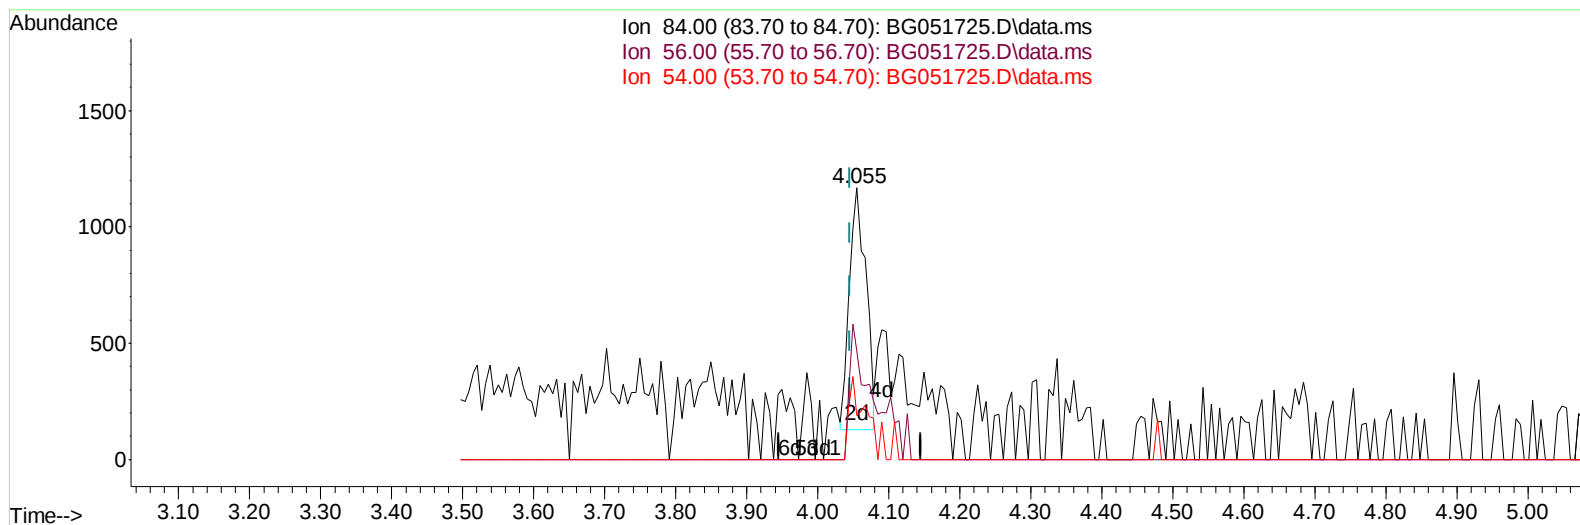

TIC: BG051725.D\data.ms

#### (4) Pyridine-d5 (S)

4.055min (+ 0.010) 0.48 ng/ul m

response 1708

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 84.00 | 100.00 | 100.00 |
| 56.00 | 68.00  | 39.90# |
| 54.00 | 31.50  | 16.10# |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

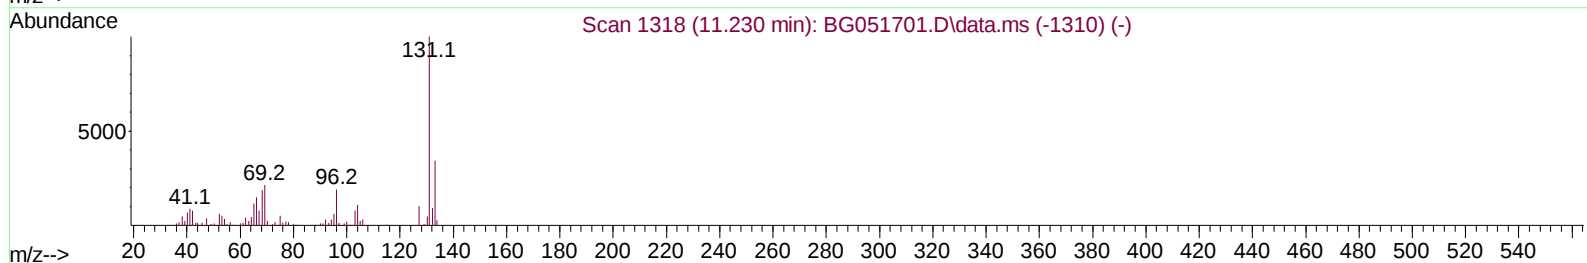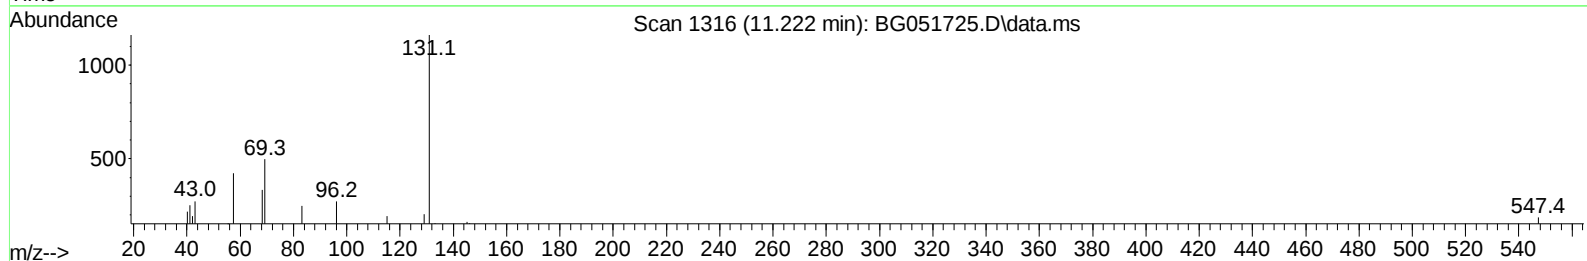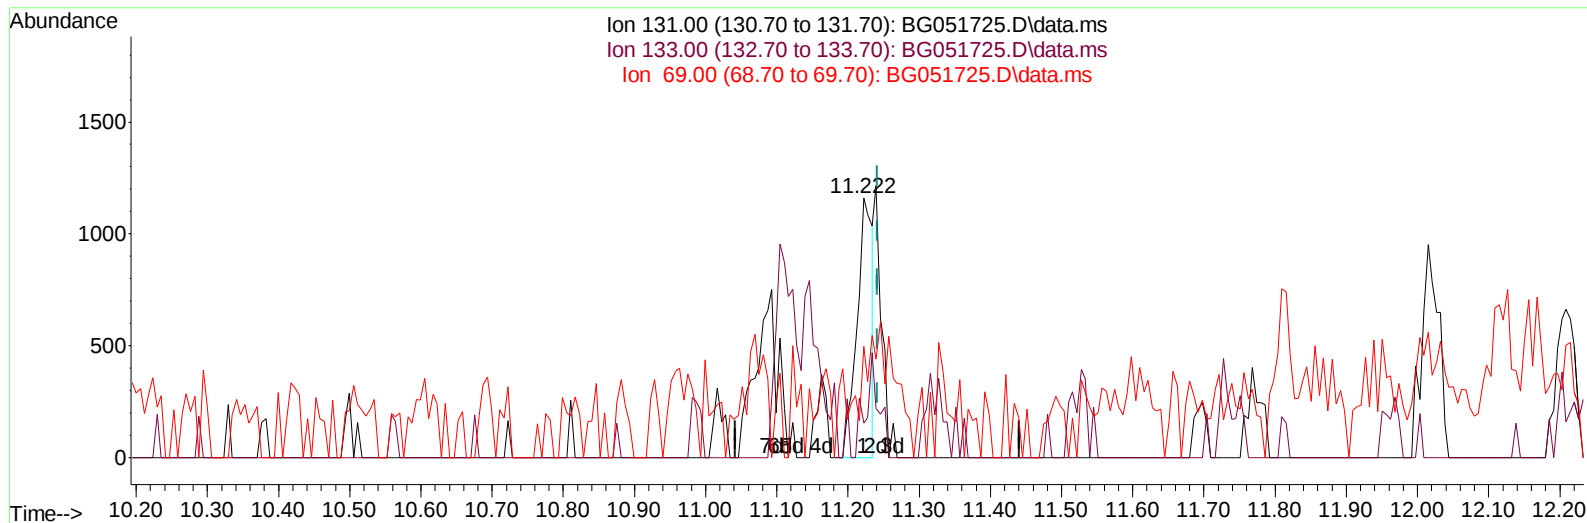

TIC: BG051725.D\data.ms

**(31) 4-Chloroaniline-d4 (S)**

**11.222min (-0.020) 0.37 ng/u1**

**response 1752**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 131.00 | 100.00 | 100.00 |
| 133.00 | 33.20  | 13.26# |
| 69.00  | 21.30  | 42.72# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

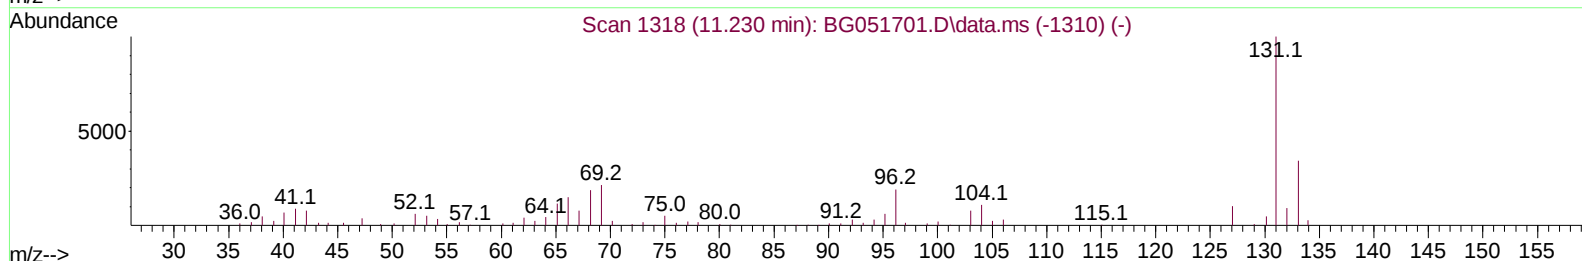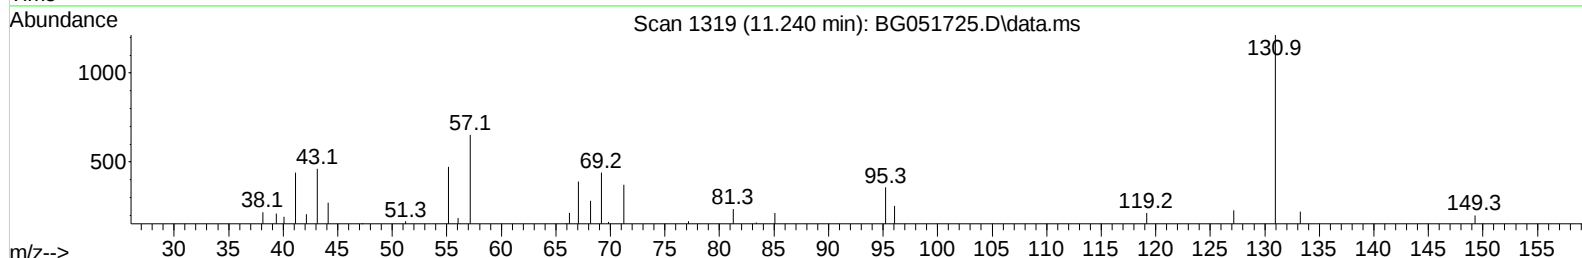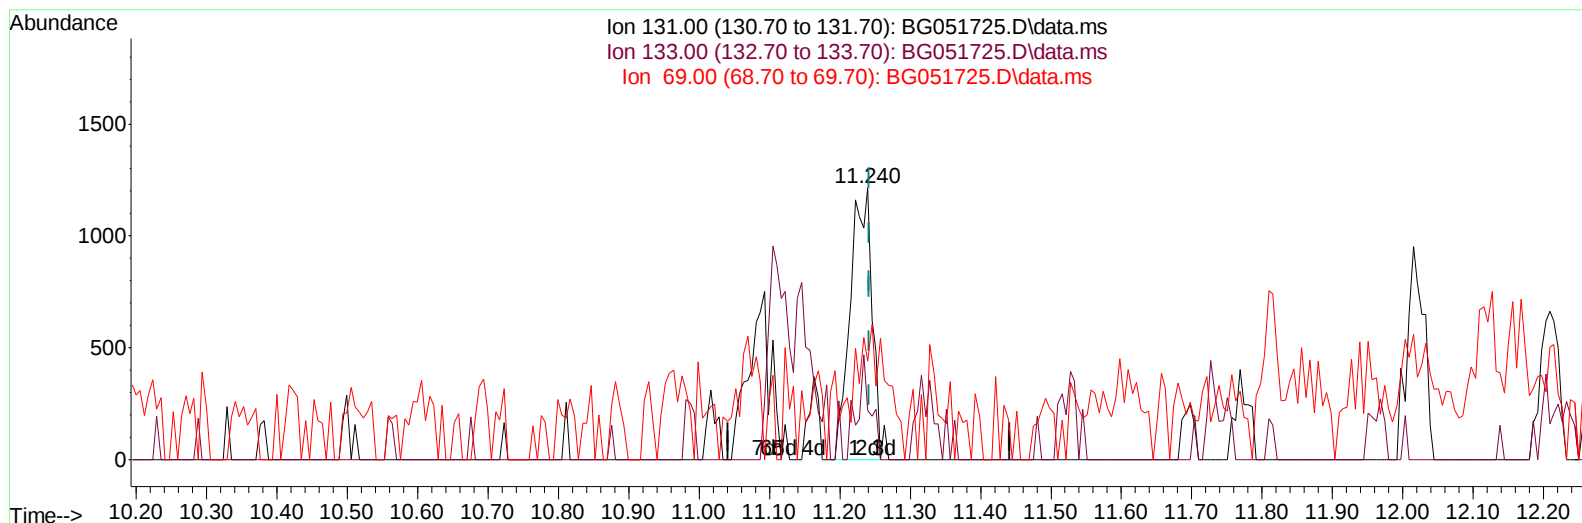

TIC: BG051725.D\data.ms

**(31) 4-Chloroaniline-d4 (S)**

11.240min (-0.002) 0.55 ng/ul m

response 2569

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 131.00 | 100.00 | 100.00 |
| 133.00 | 33.20  | 18.04# |
| 69.00  | 21.30  | 36.16# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
Data File : BG051725.D  
Acq On : 21 Dec 2021 20:59  
Operator : CG/JU  
Sample : M5153-05DL 10X  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Dec 14 14:19:57 2021  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
Supervised By :mohammad ahmed 12/28/2021

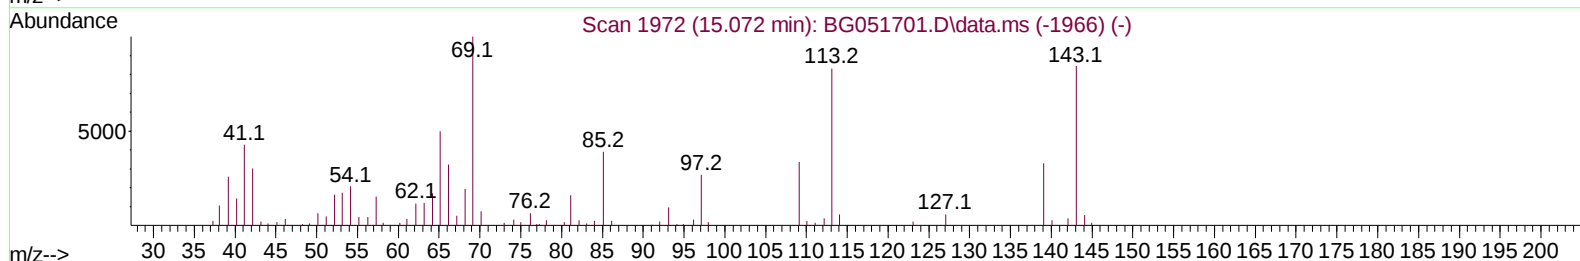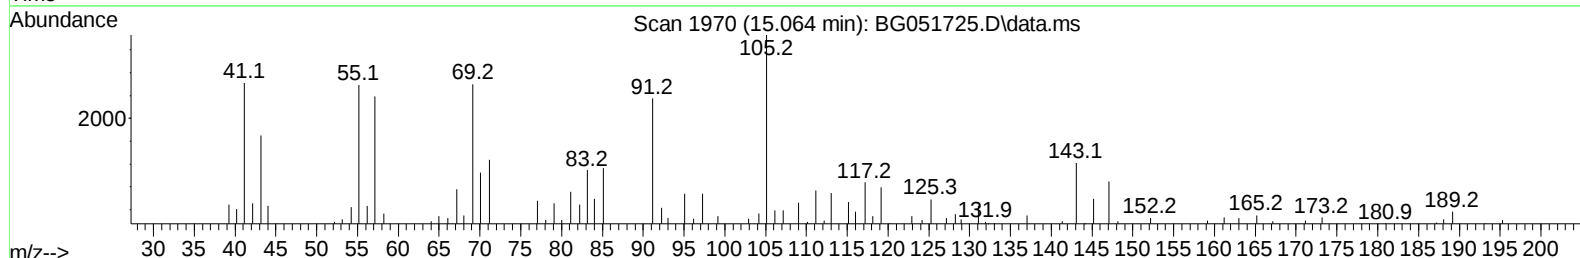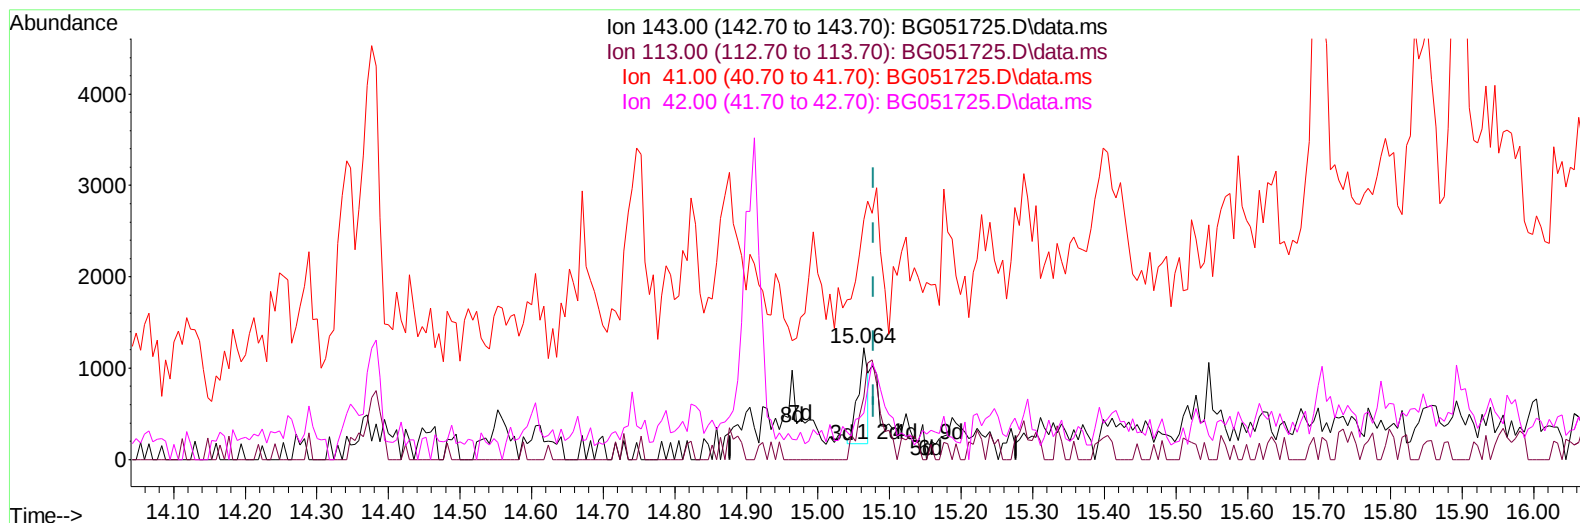

TIC: BG051725.D\data.ms

**(54) 4-Nitrophenol-d4 (S)**

**15.064min (-0.014) 0.58 ng/u1**

**response 1017**

| Ion    | Exp%   | Act%    |
|--------|--------|---------|
| 143.00 | 100.00 | 100.00  |
| 113.00 | 80.30  | 56.27#  |
| 41.00  | 44.40  | 214.91# |
| 42.00  | 29.70  | 41.93#  |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

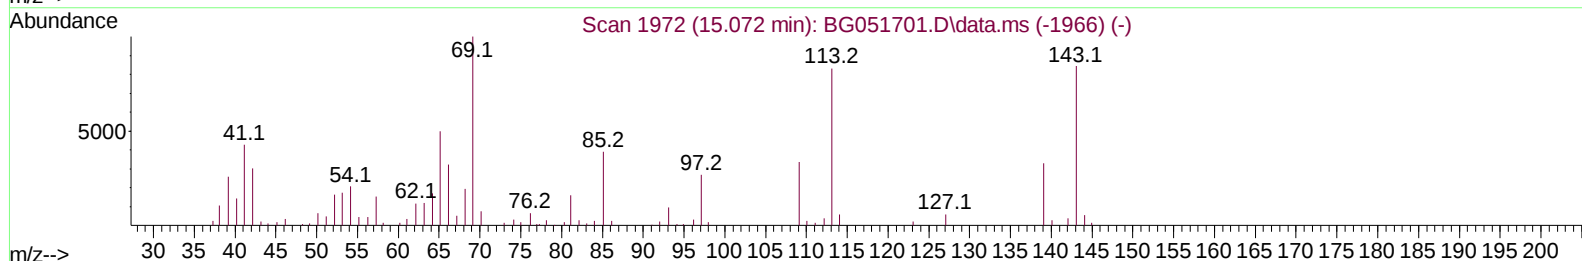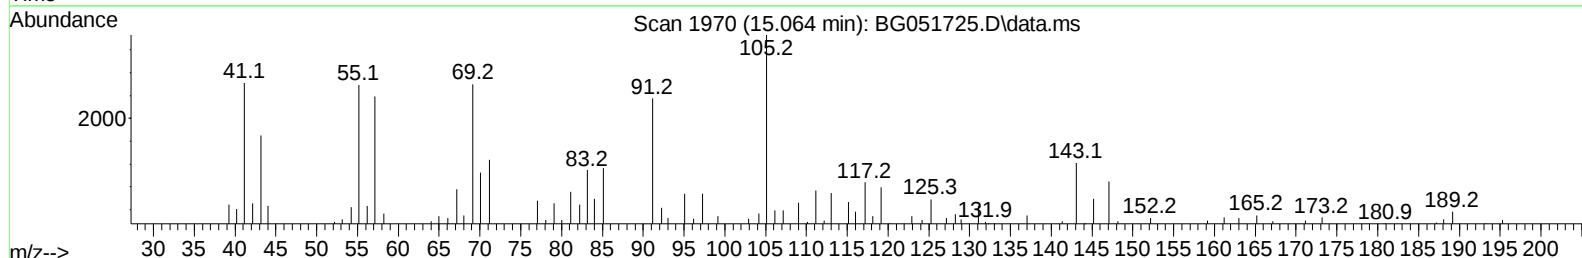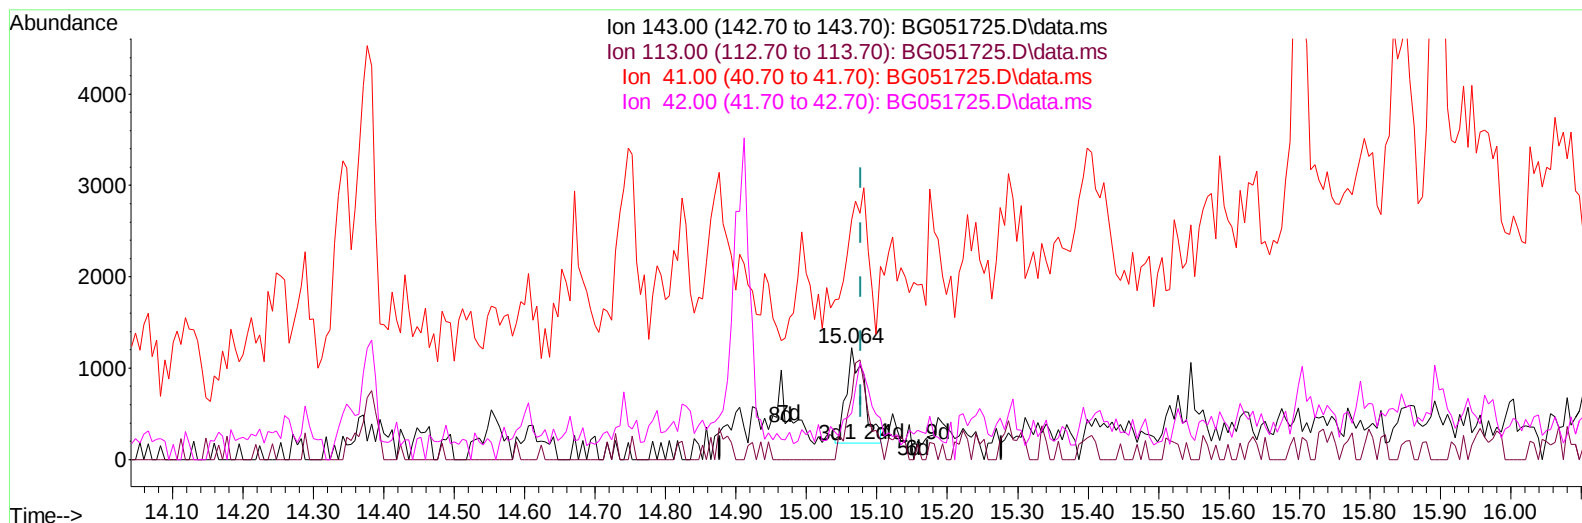

TIC: BG051725.D\data.ms

**(54) 4-Nitrophenol-d4 (S)**

**15.064min (-0.014) 1.04 ng/ul m**

**response 1832**

| Ion    | Exp%   | Act%    |
|--------|--------|---------|
| 143.00 | 100.00 | 100.00  |
| 113.00 | 80.30  | 56.27#  |
| 41.00  | 44.40  | 214.91# |
| 42.00  | 29.70  | 41.93#  |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
Data File : BG051725.D  
Acq On : 21 Dec 2021 20:59  
Operator : CG/JU  
Sample : M5153-05DL 10X  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Dec 14 14:19:57 2021  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
Supervised By :mohammad ahmed 12/28/2021

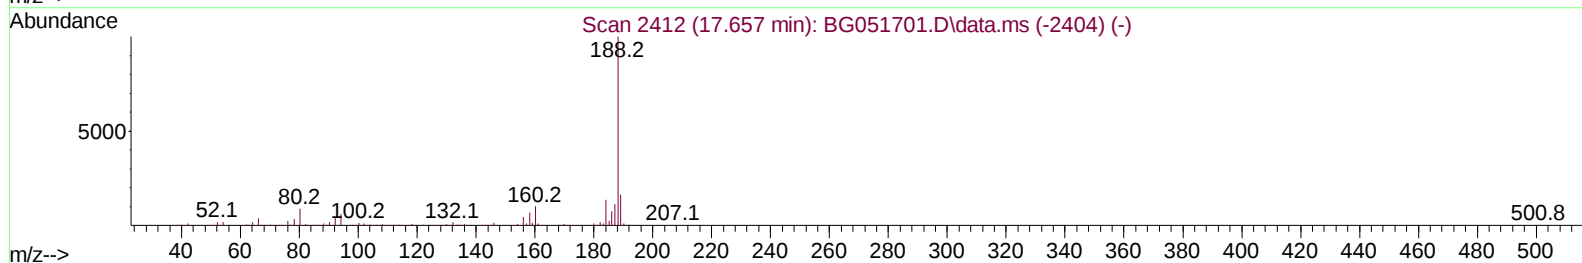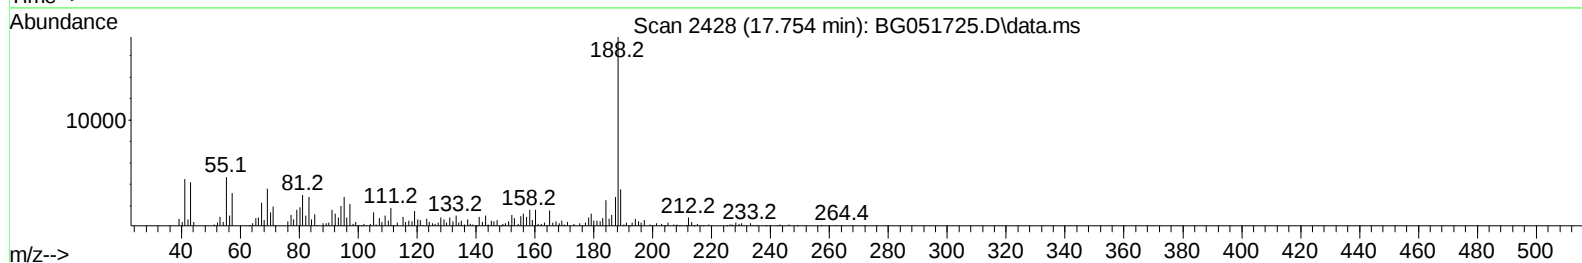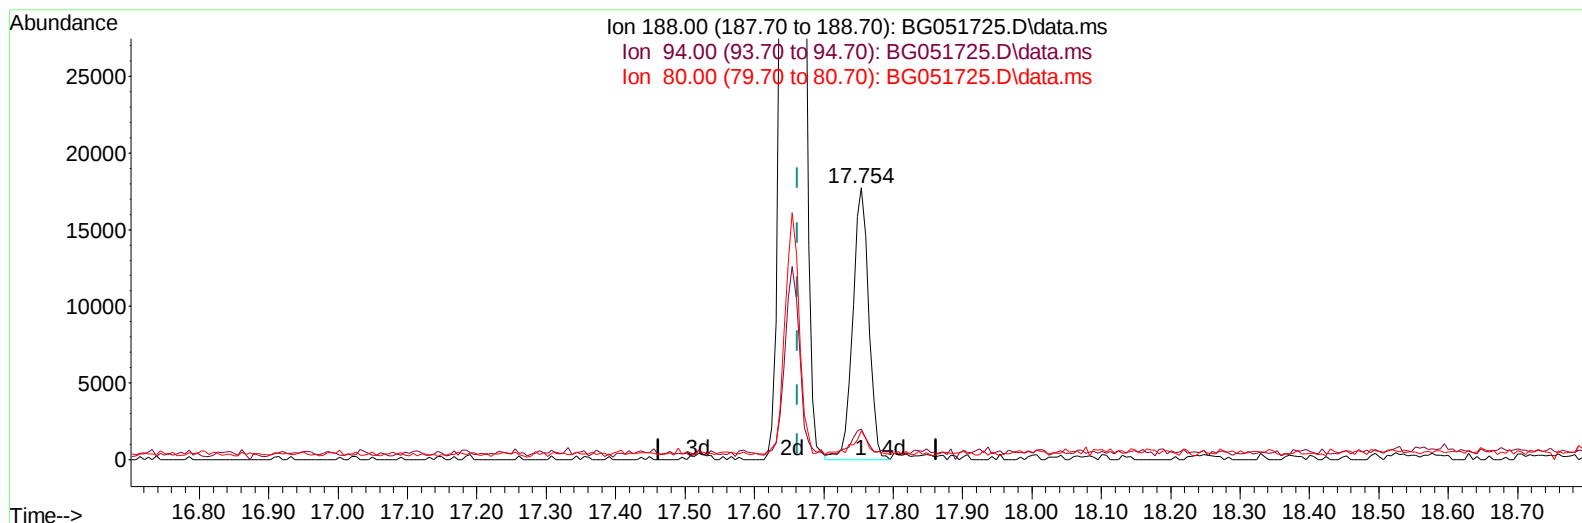

TIC: BG051725.D\data.ms

(64) Phenanthrene-d10 (I)

17.754min (+ 0.092) 20.00 ng/u1

response 28274

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 188.00 | 100.00 | 100.00 |
| 94.00  | 9.50   | 11.28  |
| 80.00  | 11.40  | 10.54  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

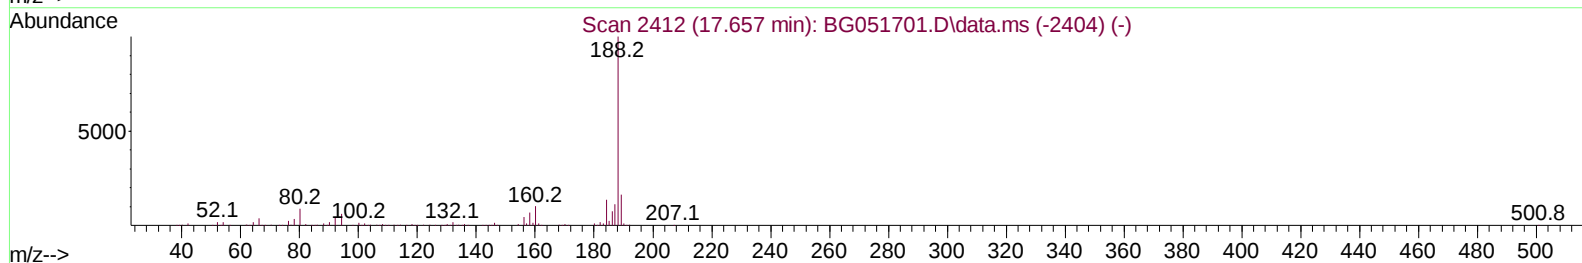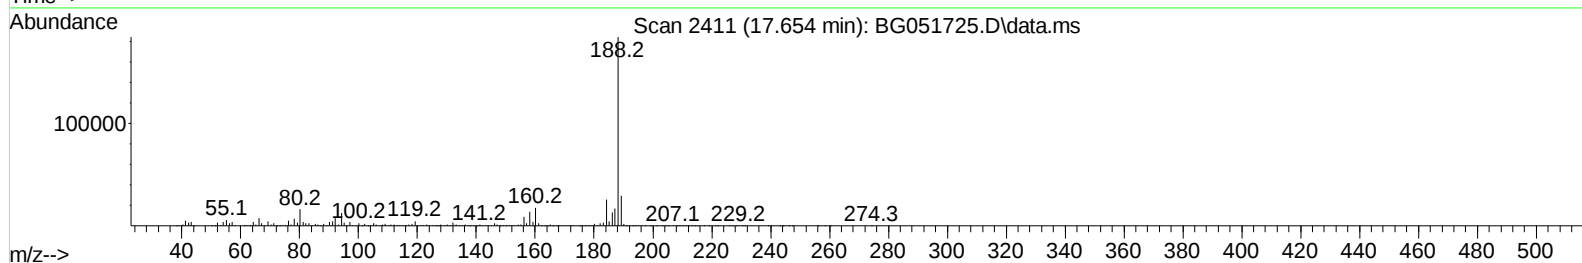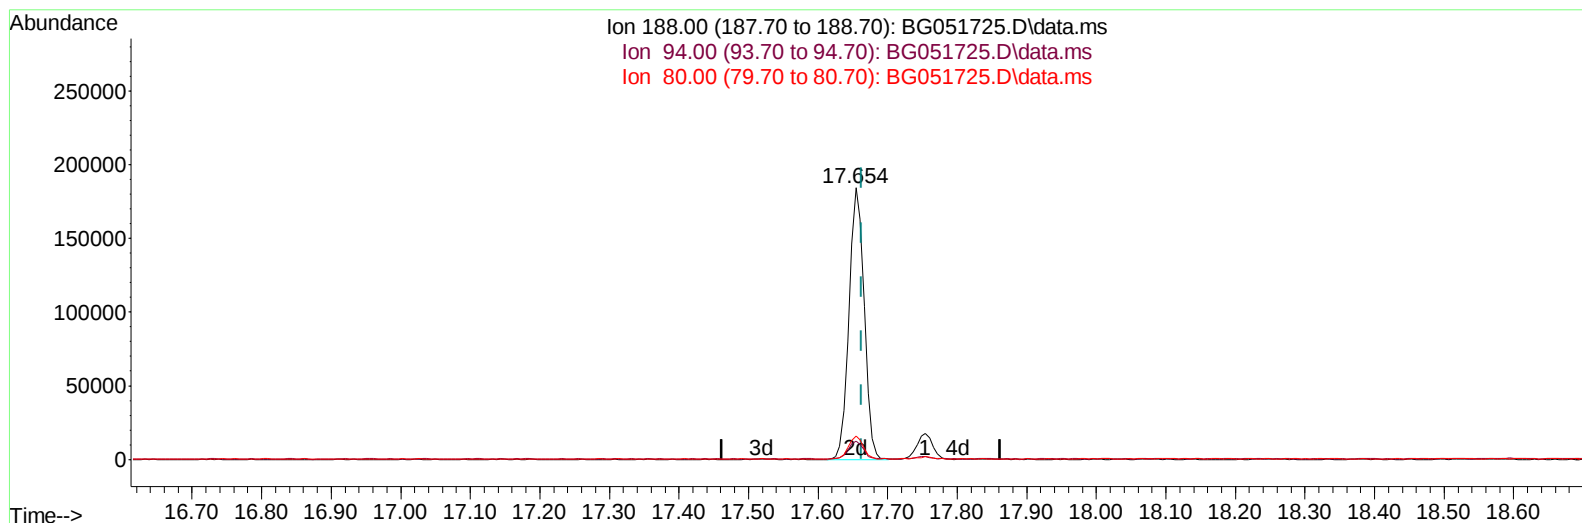

TIC: BG051725.D\data.ms

**(64) Phenanthrene-d10 (I)**

**17.654min (-0.008) 20.00 ng/ul m**

**response 277156**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 188.00 | 100.00 | 100.00 |
| 94.00  | 9.50   | 6.85#  |
| 80.00  | 11.40  | 8.74#  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :

BNA\_G




ClientSampleId :

BGL70DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

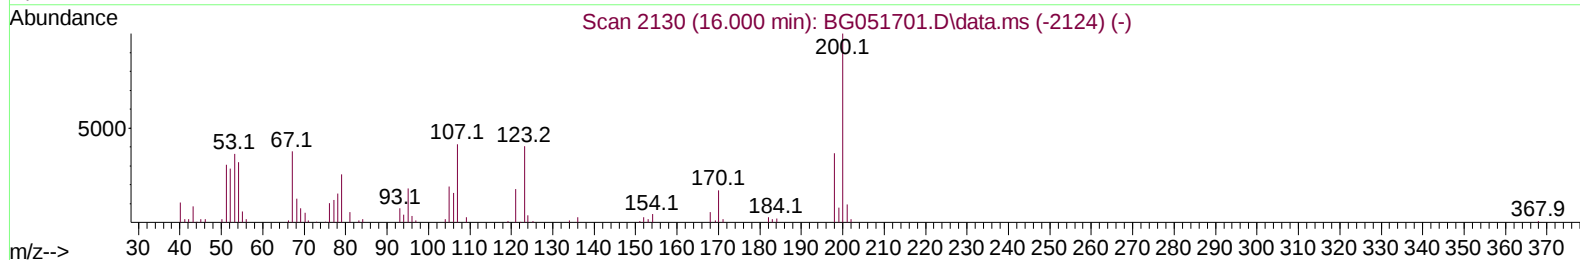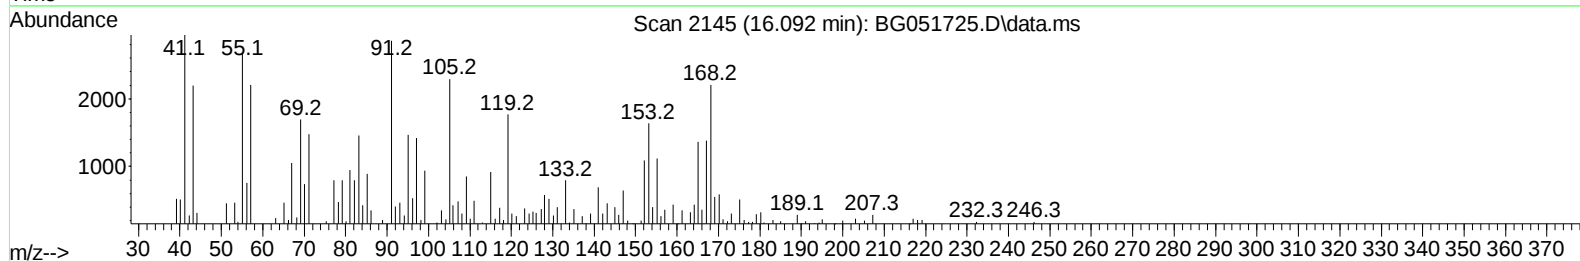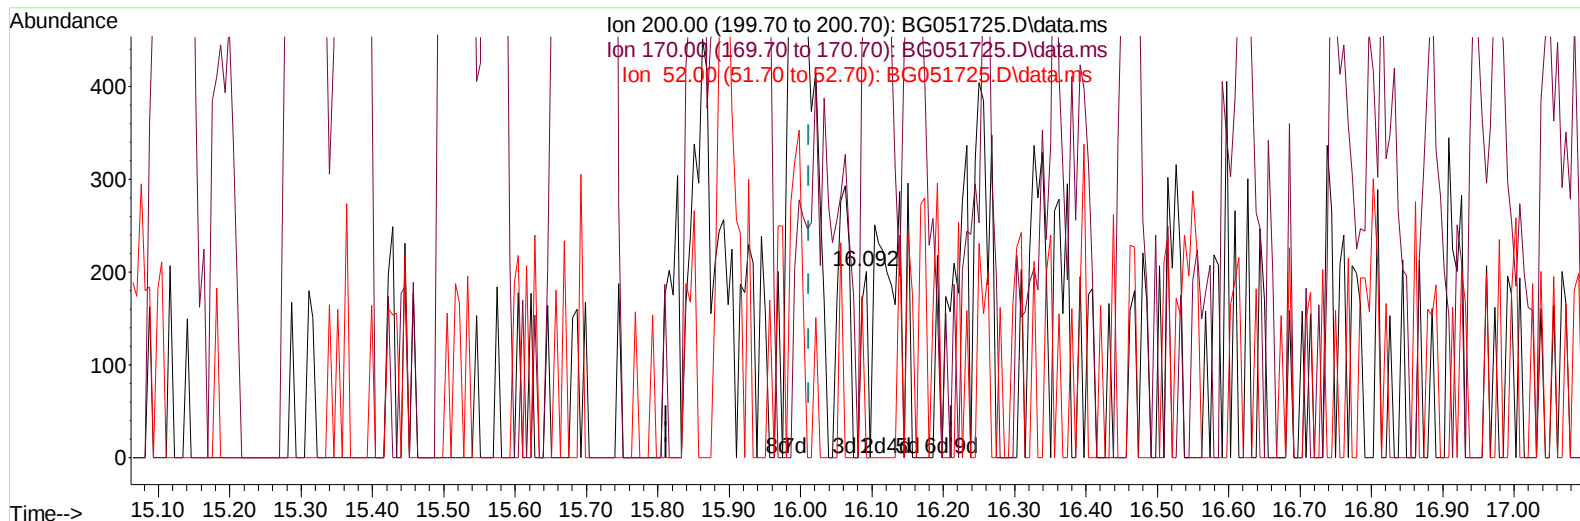

TIC: BG051725.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

16.092min (+ 0.080) 0.09 ng/u1

response 130

| Ion    | Exp%   | Act%    |
|--------|--------|---------|
| 200.00 | 100.00 | 100.00  |
| 170.00 | 19.80  | 291.54# |
| 52.00  | 47.40  | 0.00#   |
| 0.00   | 0.00   | 0.00    |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

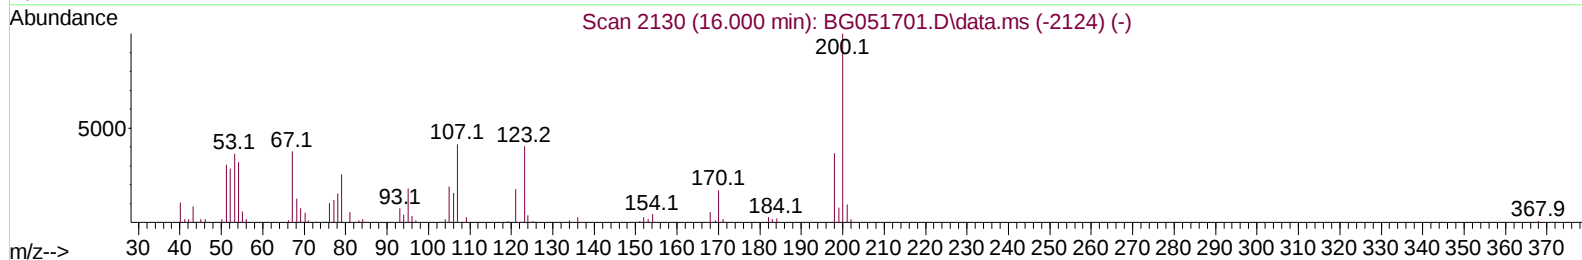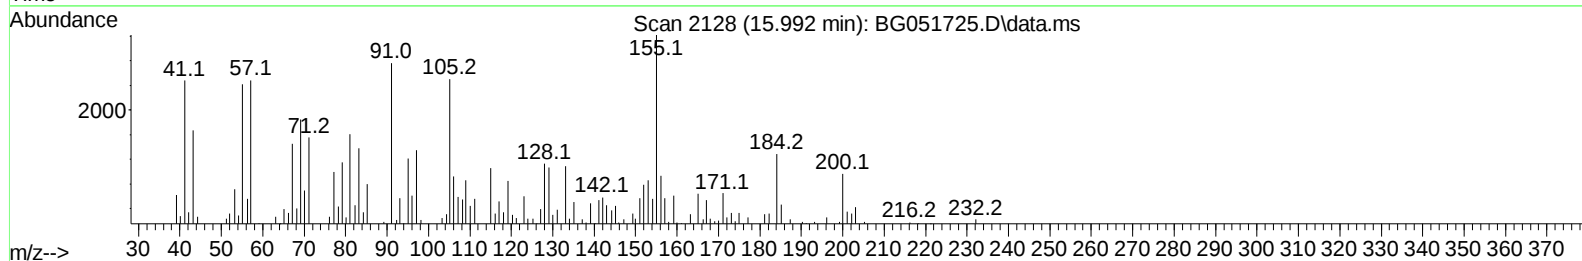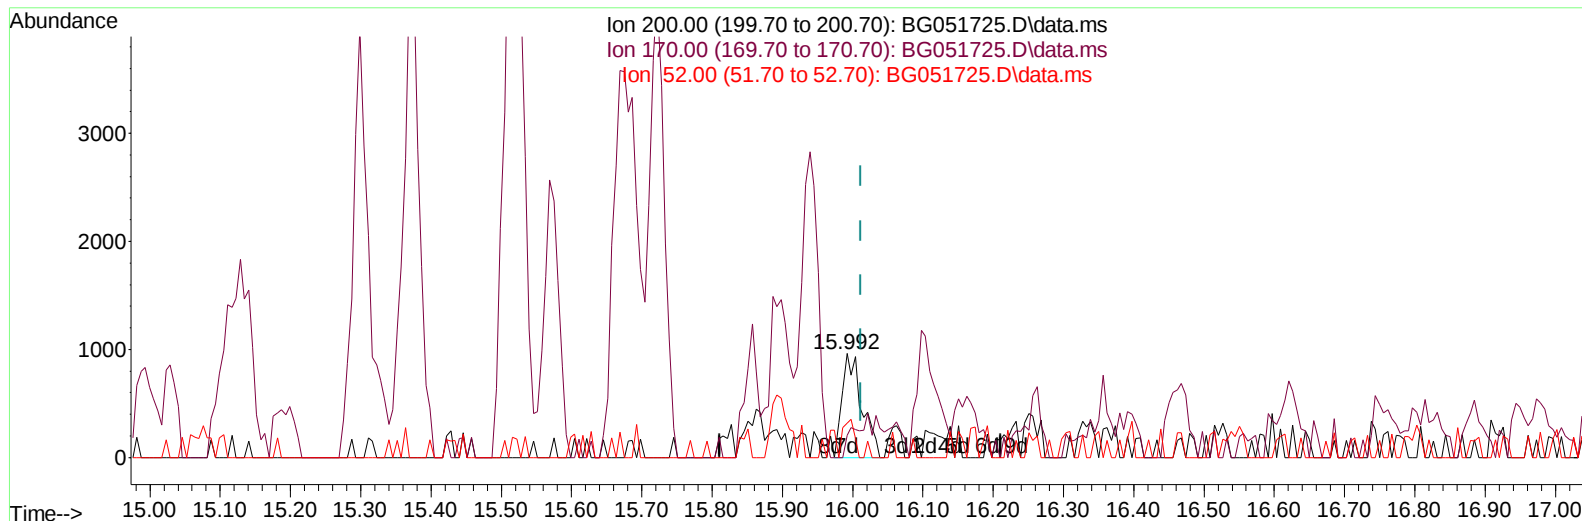

TIC: BG051725.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.992min (-0.020) 1.29 ng/ul m

response 1867

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 200.00 | 100.00 | 100.00 |
| 170.00 | 19.80  | 21.18  |
| 52.00  | 47.40  | 33.13# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

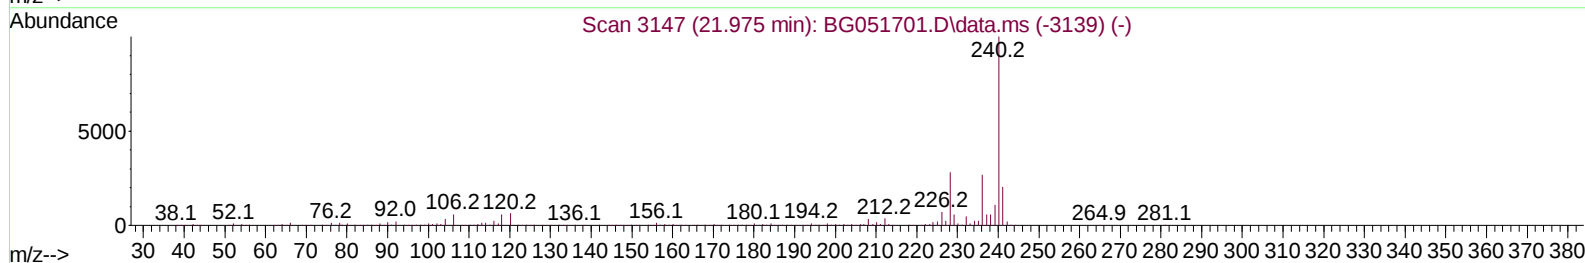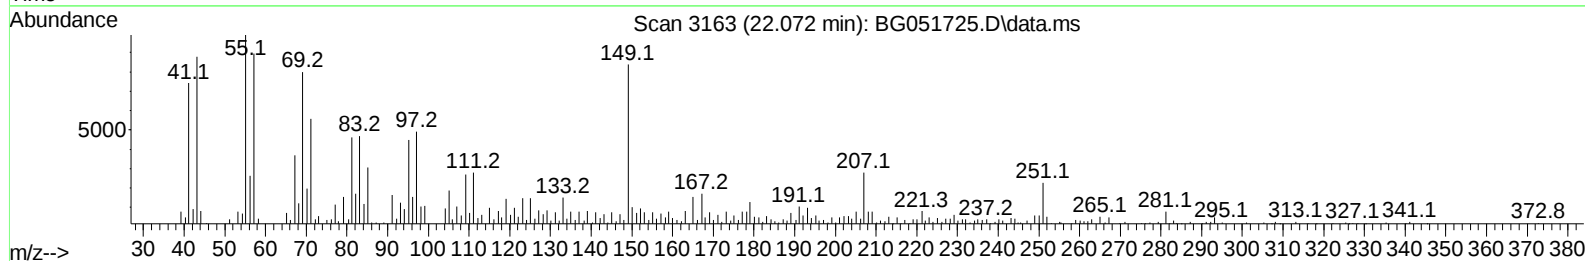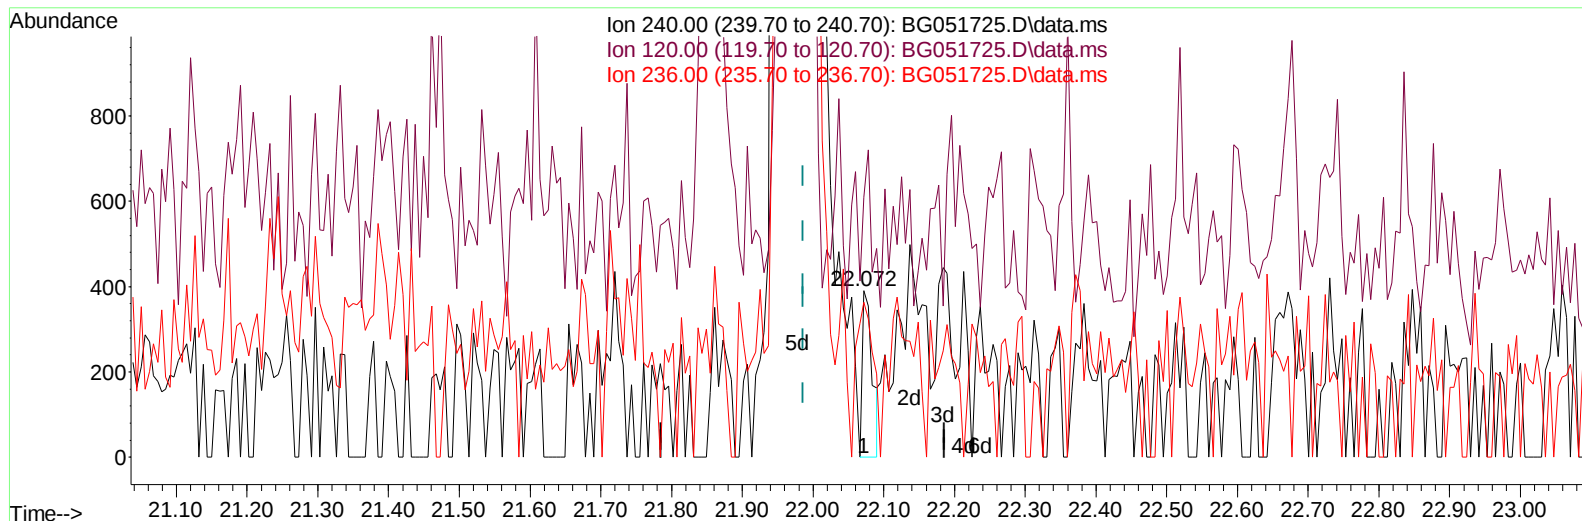

TIC: BG051725.D\data.ms

**(79) Chrysene-d12 (I)**

**22.072min (+ 0.086) 20.00 ng/ul**

**response 380**

| Ion    | Exp%   | Act%    |
|--------|--------|---------|
| 240.00 | 100.00 | 100.00  |
| 120.00 | 9.50   | 155.75# |
| 236.00 | 26.70  | 93.09#  |
| 0.00   | 0.00   | 0.00    |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

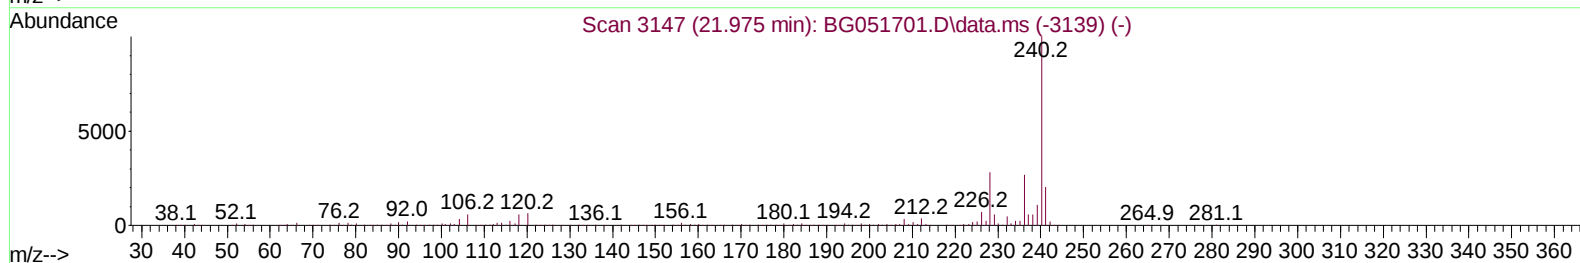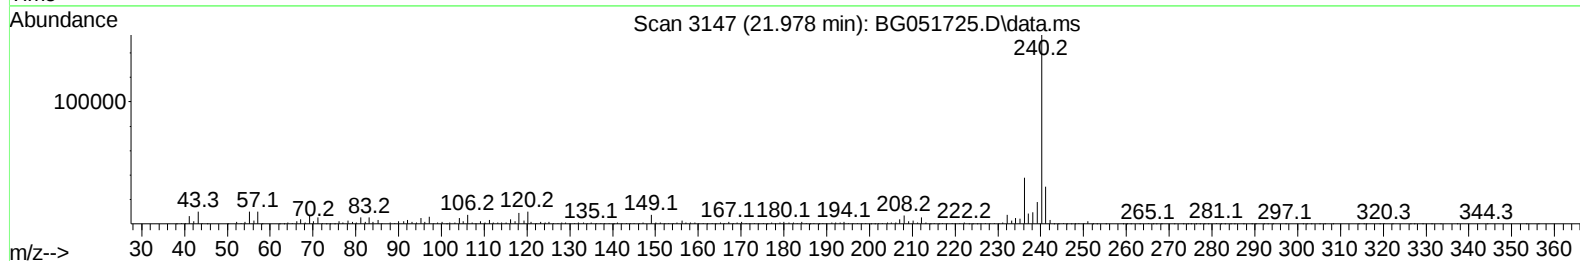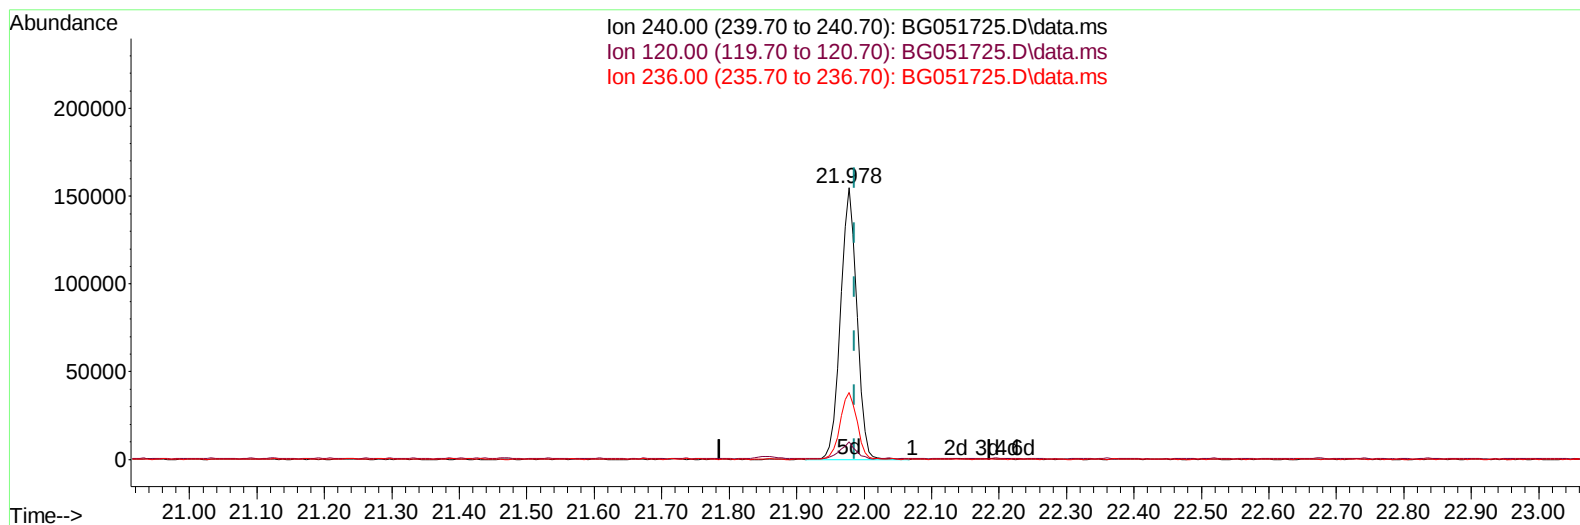

TIC: BG051725.D\data.ms

**(79) Chrysene-d12 (I)**

**21.978min (-0.008) 20.00 ng/ul m**

**response 261105**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 240.00 | 100.00 | 100.00 |
| 120.00 | 9.50   | 6.56#  |
| 236.00 | 26.70  | 24.56  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

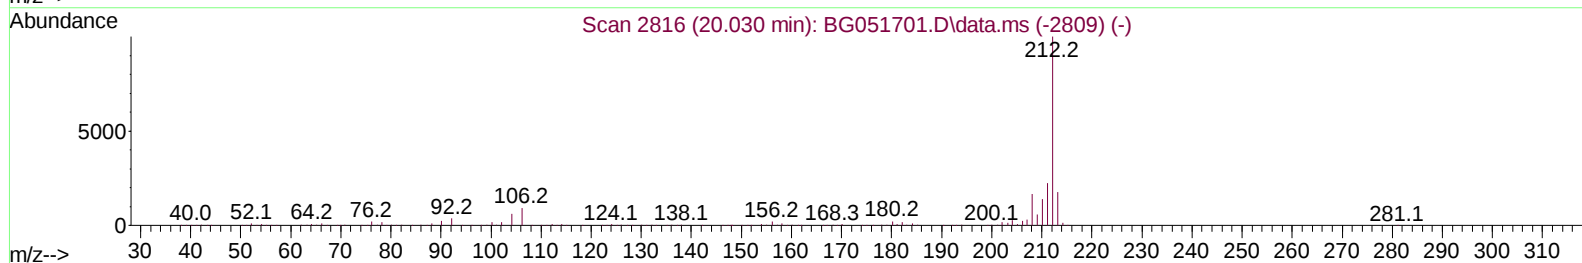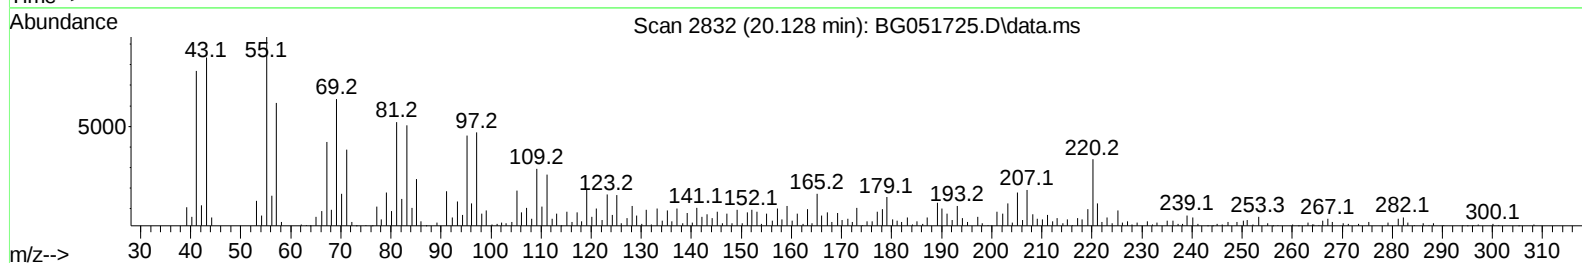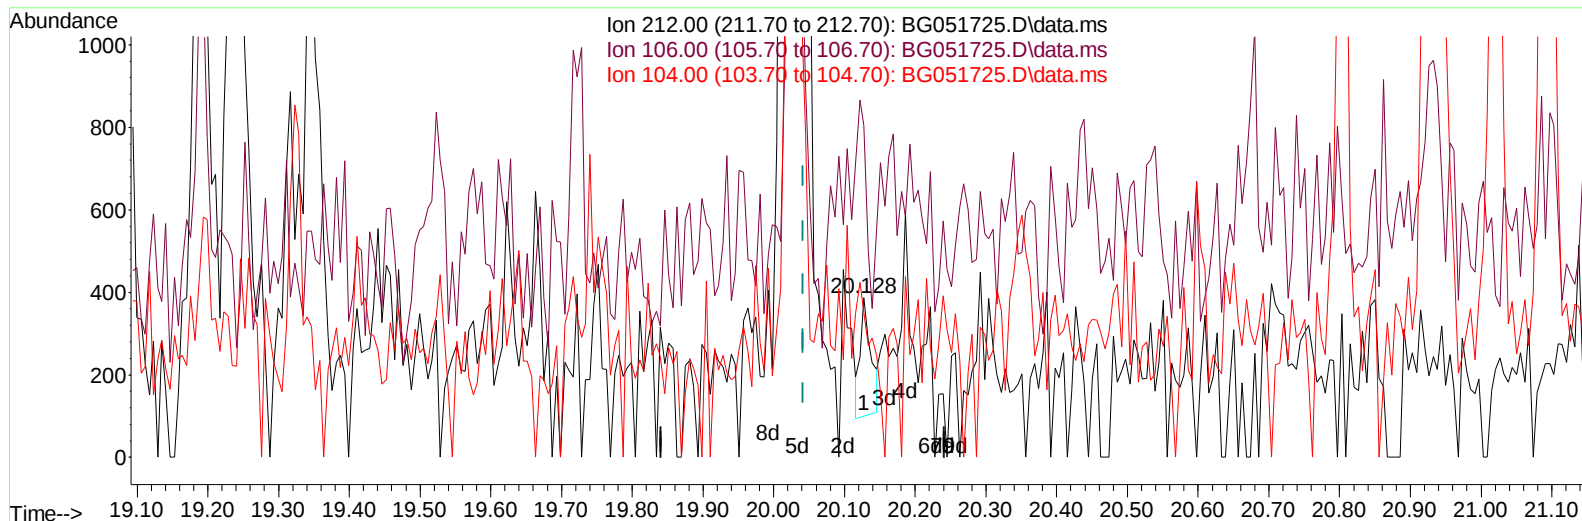

TIC: BG051725.D\data.ms

**(81) Pyrene-d10 (S)**

**20.128min (+ 0.086) 0.02 ng/u1**

**response 299**

| Ion    | Exp%   | Act%    |
|--------|--------|---------|
| 212.00 | 100.00 | 100.00  |
| 106.00 | 14.20  | 207.75# |
| 104.00 | 9.50   | 90.70#  |
| 0.00   | 0.00   | 0.00    |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

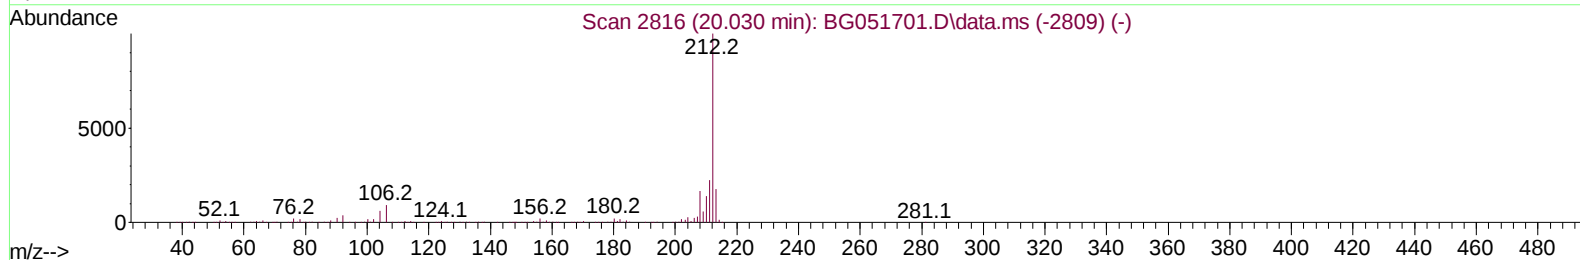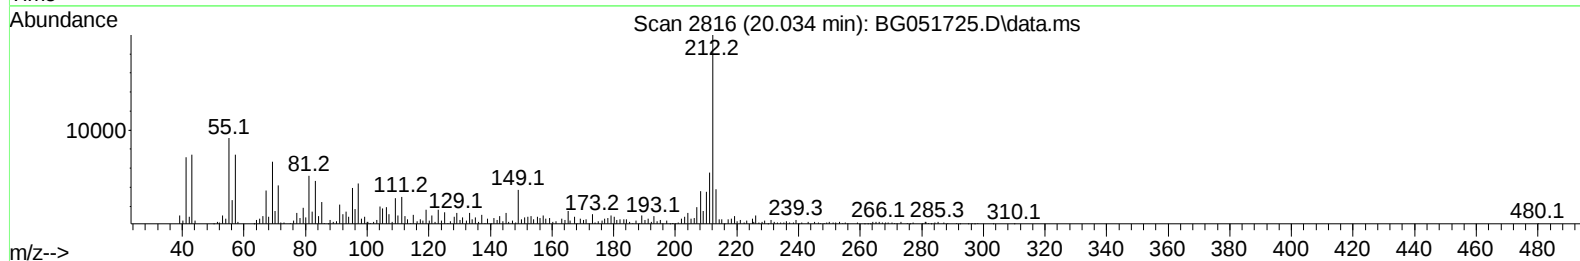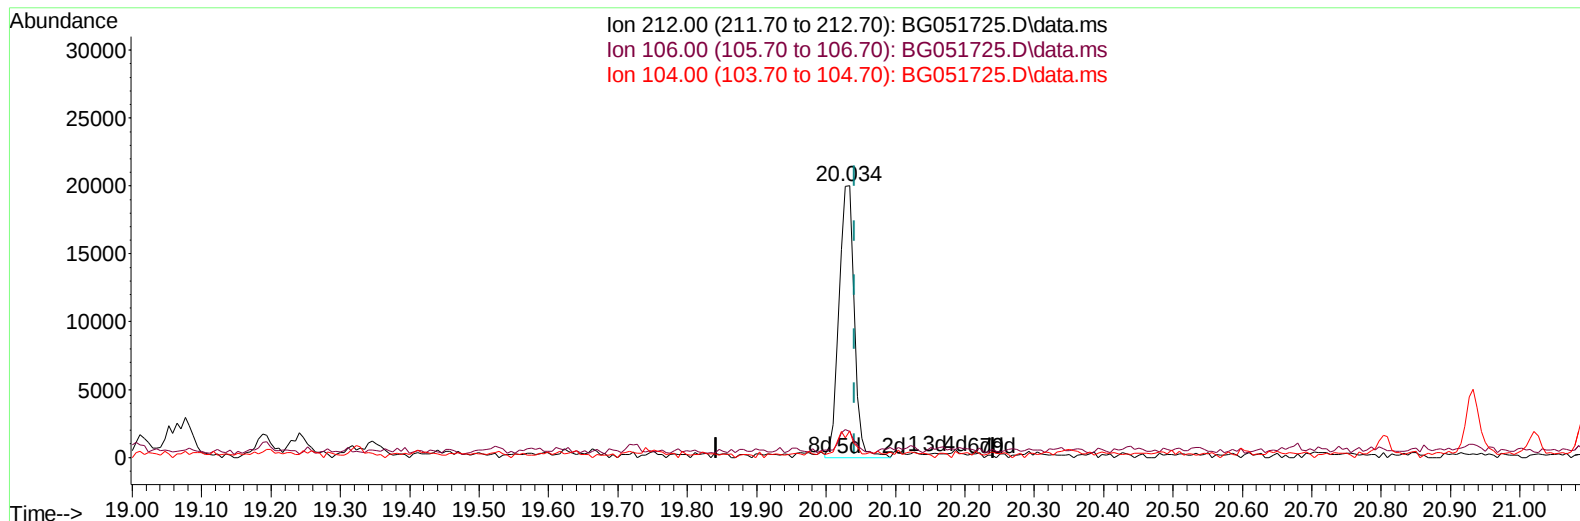

TIC: BG051725.D\data.ms

**(81) Pyrene-d10 (S)**

**20.034min (-0.008) 1.94 ng/ul m**

**response 30558**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 212.00 | 100.00 | 100.00 |
| 106.00 | 14.20  | 9.64#  |
| 104.00 | 9.50   | 9.79   |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

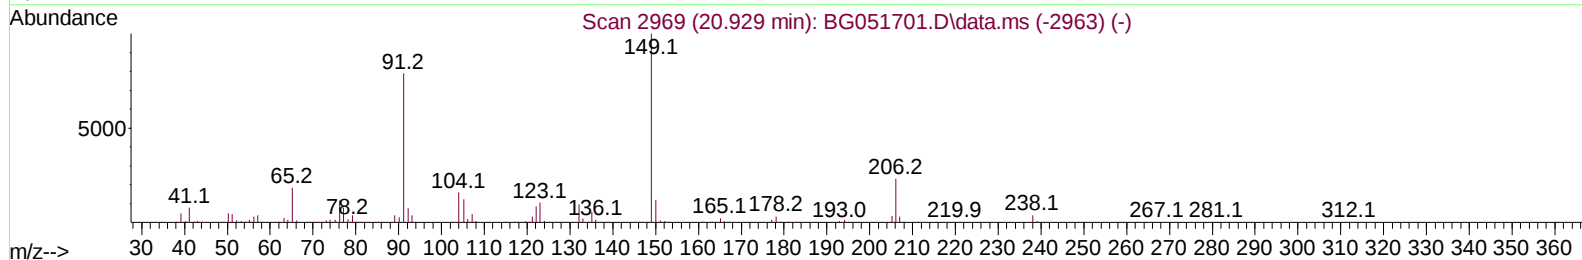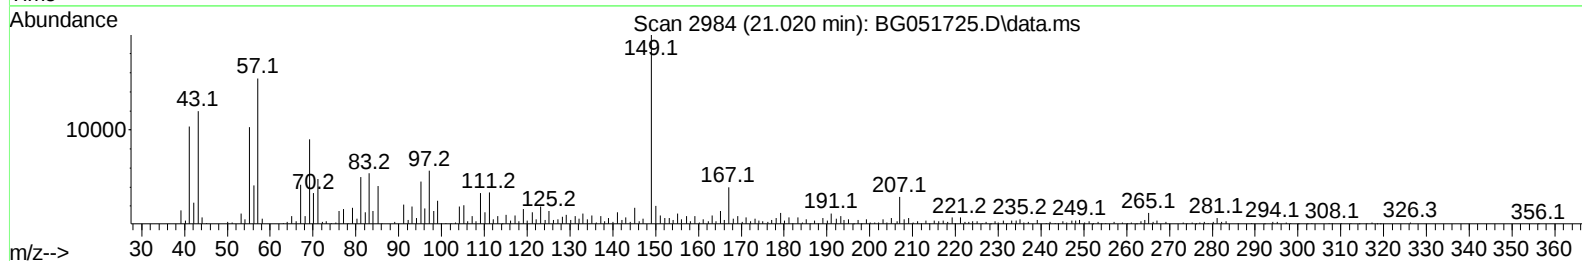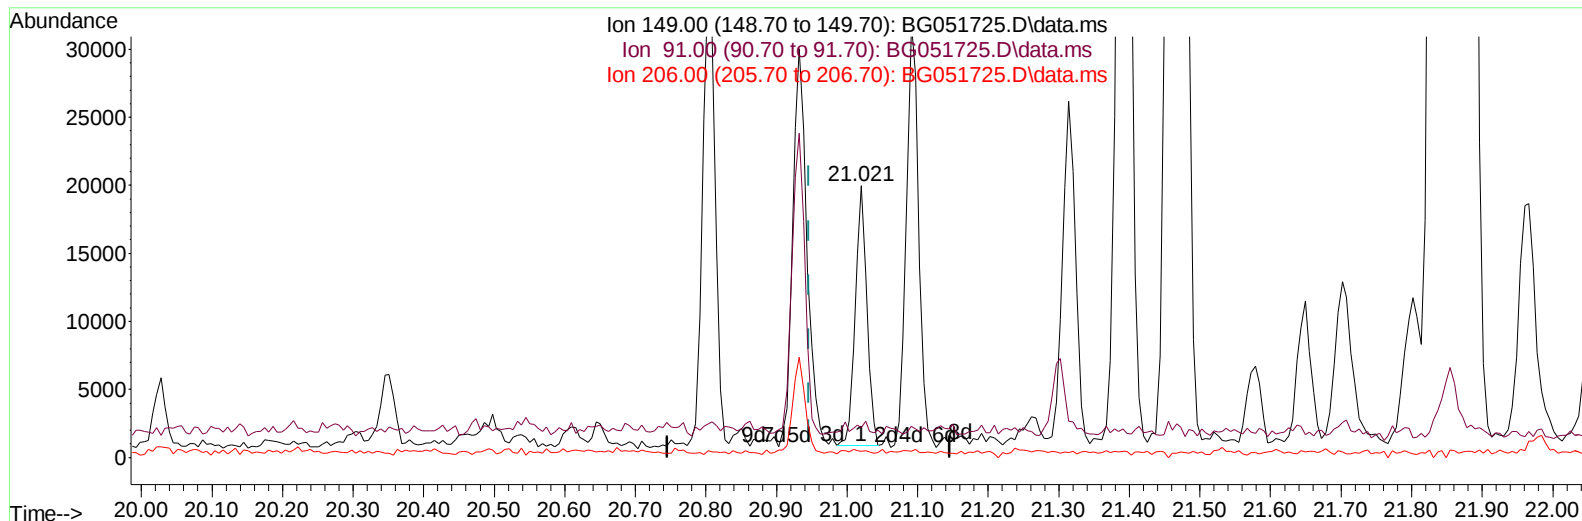

TIC: BG051725.D\data.ms

**(83) Butylbenzylphthalate**

**21.020min (+ 0.074) 3.69 ng/u1**

**response 22095**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 149.00 | 100.00 | 100.00 |
| 91.00  | 81.50  | 11.01# |
| 206.00 | 20.20  | 2.22#  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

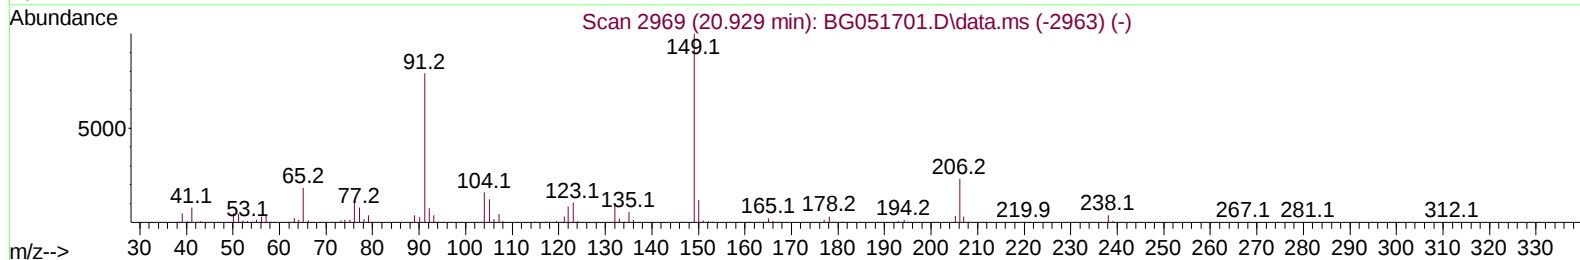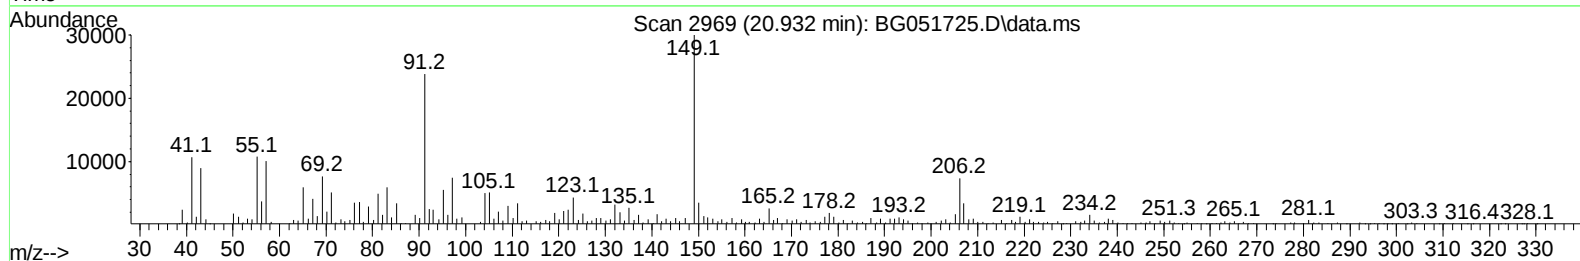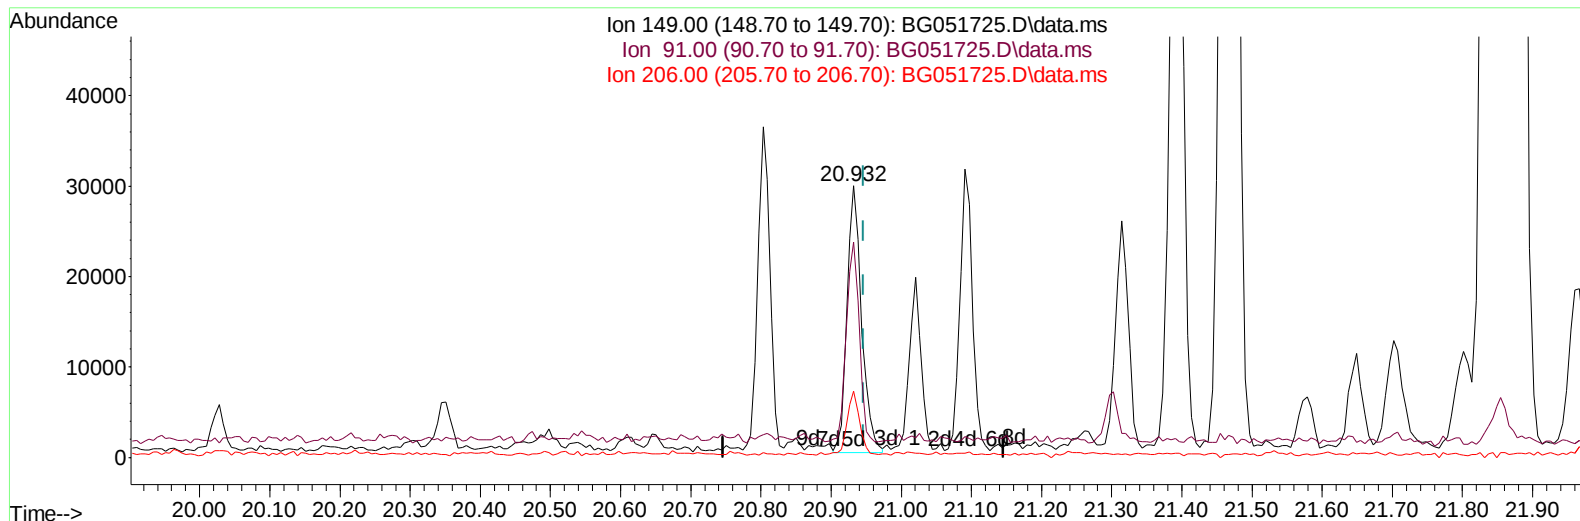

TIC: BG051725.D\data.ms

**(83) Butylbenzylphthalate**

20.932min (-0.014) 7.05 ng/ul m

response 42194

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 149.00 | 100.00 | 100.00 |
| 91.00  | 81.50  | 79.45  |
| 206.00 | 20.20  | 24.52# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

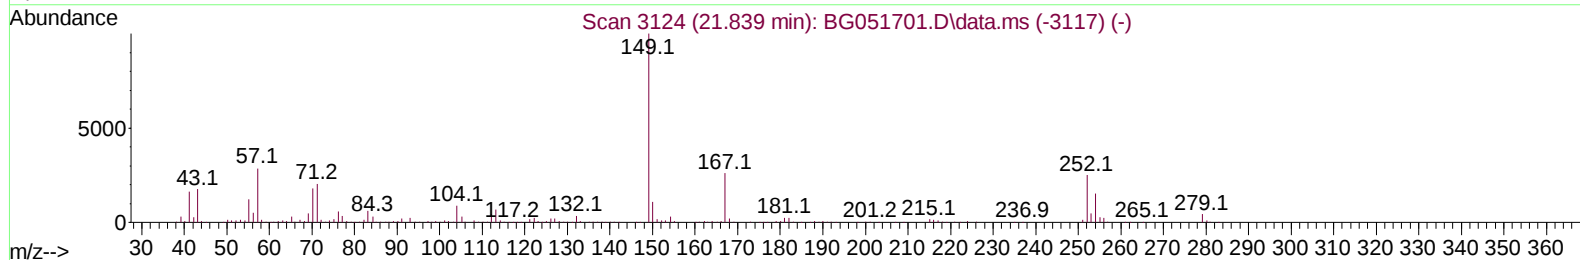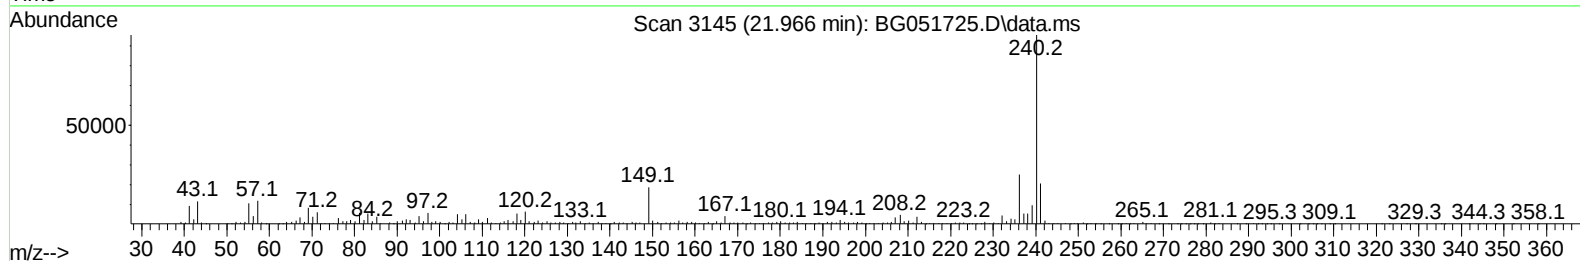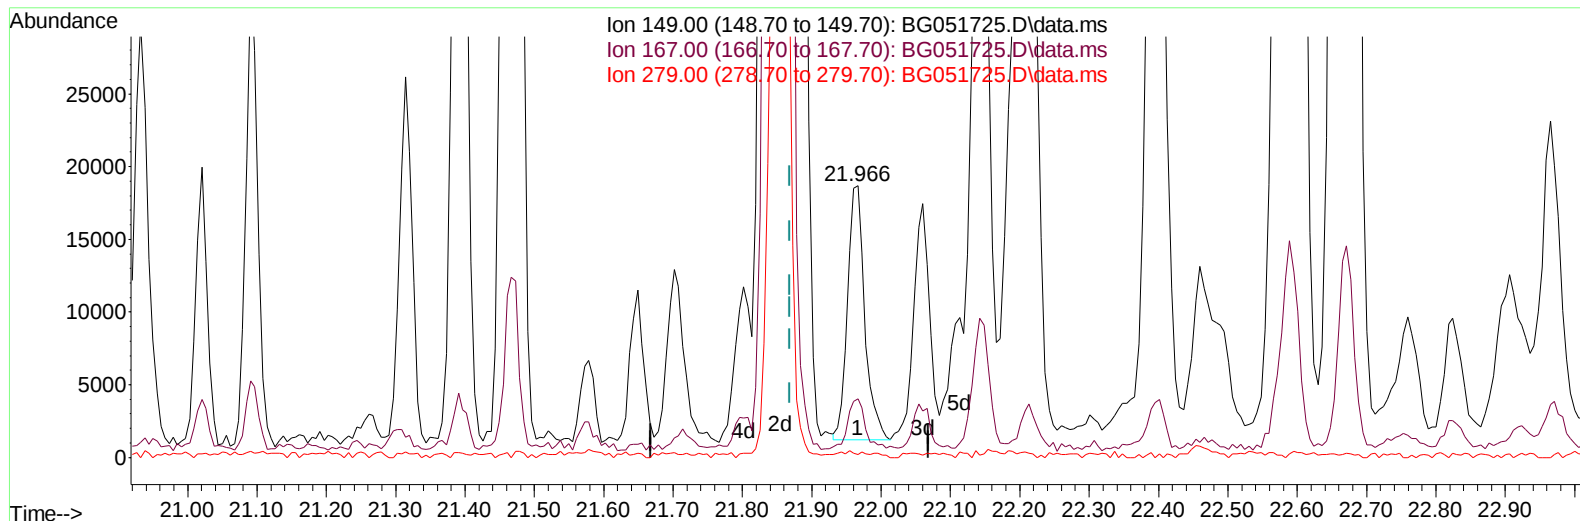

TIC: BG051725.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.966min (+ 0.098) 3.57 ng/u1

response 29925

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 149.00 | 100.00 | 100.00 |
| 167.00 | 26.40  | 21.63  |
| 279.00 | 3.40   | 1.17#  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

Manual IntegrationsAPPROVED

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

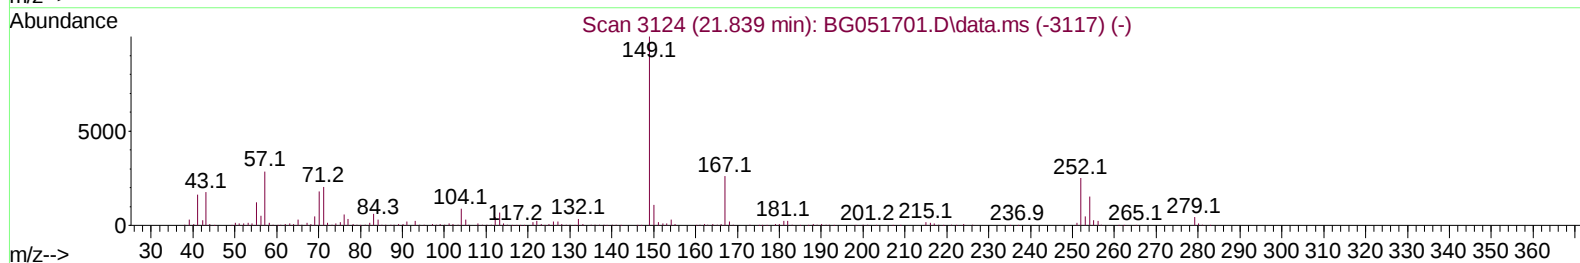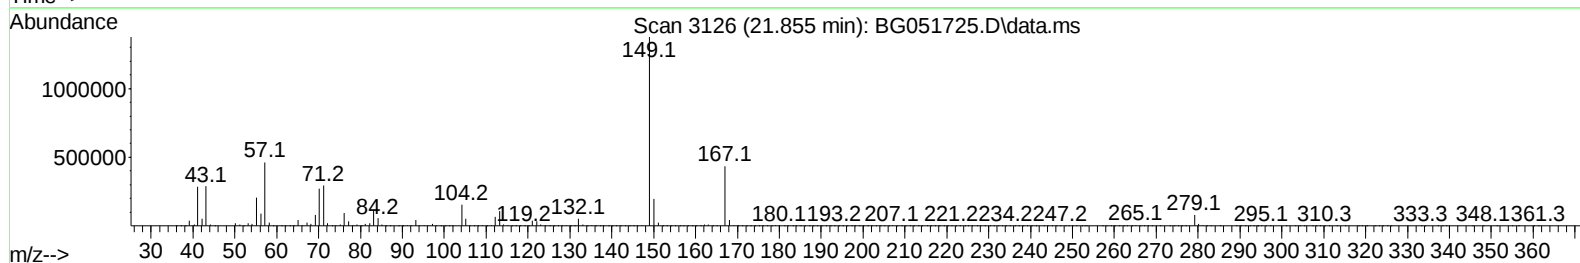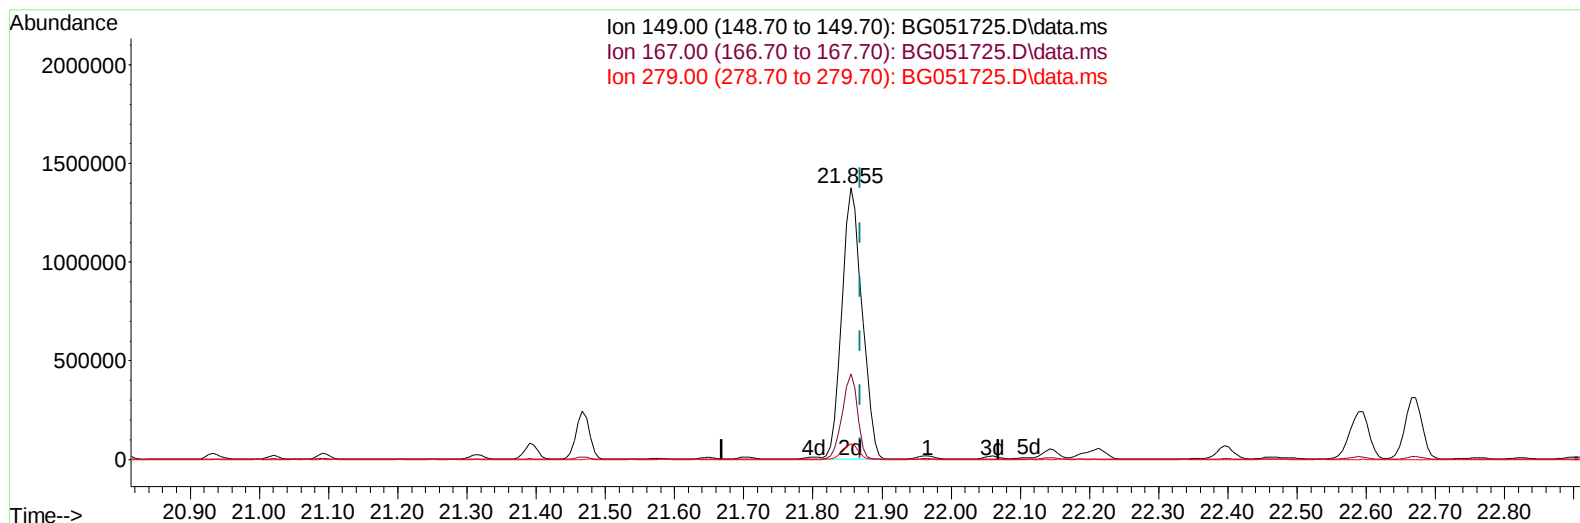

TIC: BG051725.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.855min (-0.014) 332.22 ng/ul m

response 2785813

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 149.00 | 100.00 | 100.00 |
| 167.00 | 26.40  | 31.58  |
| 279.00 | 3.40   | 5.84#  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
 Data File : BG051725.D  
 Acq On : 21 Dec 2021 20:59  
 Operator : CG/JU  
 Sample : M5153-05DL 10X  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 BGL70DL

## Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/22/2021  
 Supervised By :mohammad ahmed 12/28/2021

Quant Time: Dec 21 23:12:44 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Dec 14 14:19:57 2021  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon | Response | Conc    | Units | Dev(Min) |
|-------------------------------|--------|------|----------|---------|-------|----------|
| -----                         |        |      |          |         |       |          |
| Internal Standards            |        |      |          |         |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 8.273  | 152  | 48967    | 20.000  | ng/ul | -0.01    |
| 20) Naphthalene-d8            | 11.110 | 136  | 204628   | 20.000  | ng/ul | #-0.01   |
| 38) Acenaphthene-d10          | 14.911 | 164  | 135179   | 20.000  | ng/ul | 0.00     |
| 64) Phenanthrene-d10          | 17.654 | 188  | 277156m  | 20.000  | ng/ul | 0.00     |
| 79) Chrysene-d12              | 21.978 | 240  | 261105m  | 20.000  | ng/ul | 0.00     |
| 88) Perylene-d12              | 25.485 | 264  | 270150   | 20.000  | ng/ul | 0.00     |
| System Monitoring Compounds   |        |      |          |         |       |          |
| 3) 1,4-Dioxane-d8             | 0.000  | 96   | 0d       | 0.000   | ng/uL |          |
| 4) Pyridine-d5                | 4.055  | 84   | 1708m    | 0.479   | ng/ul | 0.00     |
| 7) Phenol-d5                  | 7.404  | 99   | 7750     | 1.773   | ng/ul | -0.01    |
| 9) Bis-(2-Chloroethyl)eth...  | 7.580  | 67   | 5424     | 2.087   | ng/ul | -0.01    |
| 11) 2-Chlorophenol-d4         | 7.797  | 132  | 5638     | 1.854   | ng/ul | -0.01    |
| 15) 4-Methylphenol-d8         | 8.966  | 113  | 6162     | 1.823   | ng/ul | -0.01    |
| 21) Nitrobenzene-d5           | 9.442  | 128  | 3298     | 2.198   | ng/ul | -0.01    |
| 24) 2-Nitrophenol-d4          | 10.170 | 143  | 3045     | 1.857   | ng/ul | -0.01    |
| 28) 2,4-Dichlorophenol-d3     | 10.717 | 165  | 6583     | 1.851   | ng/ul | -0.01    |
| 31) 4-Chloroaniline-d4        | 11.240 | 131  | 2569m    | 0.549   | ng/ul | 0.00     |
| 46) Dimethylphthalate-d6      | 14.294 | 166  | 21276    | 1.966   | ng/ul | -0.02    |
| 49) Acenaphthylene-d8         | 14.606 | 160  | 25510    | 1.898   | ng/ul | 0.00     |
| 54) 4-Nitrophenol-d4          | 15.064 | 143  | 1832m    | 1.041   | ng/ul | -0.01    |
| 60) Fluorene-d10              | 15.898 | 176  | 17587    | 1.814   | ng/ul | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.992 | 200  | 1867m    | 1.293   | ng/ul | -0.02    |
| 73) Anthracene-d10            | 17.754 | 188  | 28274    | 2.139   | ng/ul | 0.00     |
| 81) Pyrene-d10                | 20.034 | 212  | 30558m   | 1.945   | ng/ul | 0.00     |
| 92) Benzo(a)pyrene-d12        | 25.232 | 264  | 26446    | 1.861   | ng/ul | -0.02    |
| Target Compounds              |        |      |          |         |       |          |
| 83) Butylbenzylphthalate      | 20.932 | 149  | 42194m   | 7.048   | ng/ul |          |
| 86) Bis(2-ethylhexyl)phtha... | 21.855 | 149  | 2785813m | 332.217 | ng/ul |          |
| 89) Di-n-octyl phthalate      | 23.171 | 149  | 1629270  | 111.972 | ng/ul | 100      |
| -----                         |        |      |          |         |       |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122021\  
Data File : BG051725.D  
Acq On : 21 Dec 2021 20:59  
Operator : CG/JU  
Sample : M5153-05DL 10X  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
BGL70DL

## Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/22/2021  
Supervised By :mohammad ahmed 12/28/2021

Quant Time: Dec 21 23:12:44 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG121421.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Dec 14 14:19:57 2021  
Response via : Initial Calibration

