

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051678.D
 Acq On : 20 Dec 2021 12:44
 Operator : CG/JU
 Sample : M5171-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL97

Quant Time: Dec 20 23:08:13 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 14 14:19:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.275	152	37267	20.000	ng/ul	-0.01
20) Naphthalene-d8	11.112	136	155002	20.000	ng/ul	#-0.01
38) Acenaphthene-d10	14.907	164	109778	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.651	188	247662	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.974	240	216810	20.000	ng/ul	#-0.01
88) Perylene-d12	25.464	264	226554	20.000	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.599	96	3199	3.565	ng/uL	0.00
4) Pyridine-d5	4.034	84	18512	6.828	ng/ul	-0.01
7) Phenol-d5	7.400	99	73068	21.959	ng/ul	-0.02
9) Bis-(2-Chloroethyl)eth...	7.576	67	43507	21.994	ng/ul	-0.02
11) 2-Chlorophenol-d4	7.799	132	53107	22.948	ng/ul	-0.01
15) 4-Methylphenol-d8	8.962	113	56703	22.046	ng/ul	-0.02
21) Nitrobenzene-d5	9.438	128	27982	24.623	ng/ul	-0.02
24) 2-Nitrophenol-d4	10.167	143	29697	23.905	ng/ul	-0.02
28) 2,4-Dichlorophenol-d3	10.719	165	59317	22.018	ng/ul	-0.01
31) 4-Chloroaniline-d4	11.230	131	65866	18.570	ng/ul	-0.01
46) Dimethylphthalate-d6	14.296	166	182783	20.803	ng/ul	-0.02
49) Acenaphthylene-d8	14.602	160	240765	22.063	ng/ul	-0.01
54) 4-Nitrophenol-d4	15.066	143	24719	17.300	ng/ul	-0.01
60) Fluorene-d10	15.894	176	168946	21.461	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.994	200	20352	15.773	ng/ul	-0.02
73) Anthracene-d10	17.751	188	263061	22.267	ng/ul	-0.01
81) Pyrene-d10	20.030	212	281119	21.544	ng/ul	-0.01
92) Benzo(a)pyrene-d12	25.223	264	259852	21.799	ng/ul	-0.03
Target Compounds						
					Qvalue	
8) Phenol	7.435	94	4137	1.250	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051678.D
Acq On : 20 Dec 2021 12:44
Operator : CG/JU
Sample : M5171-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL97

Quant Time: Dec 20 23:08:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 14 14:19:57 2021
Response via : Initial Calibration

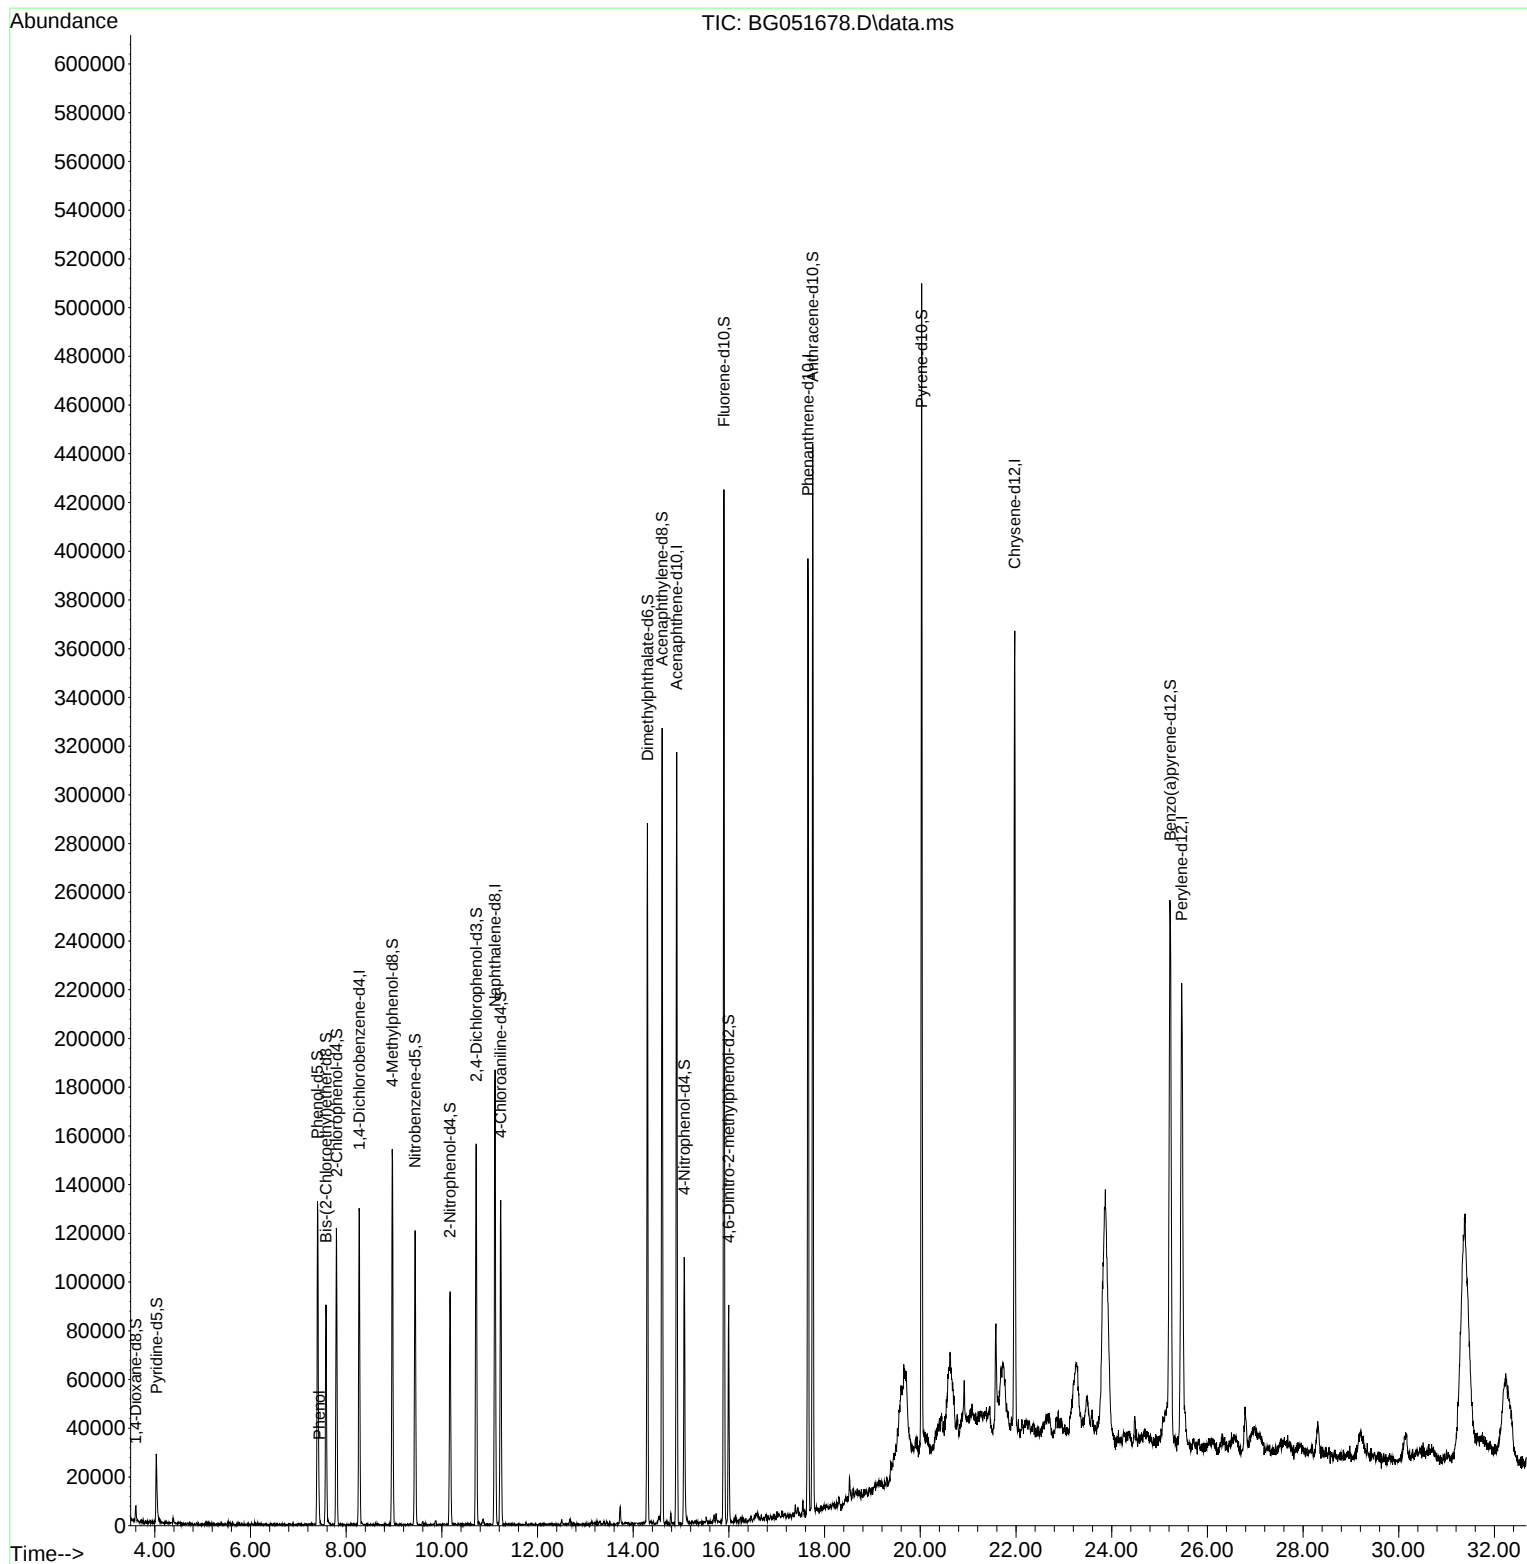

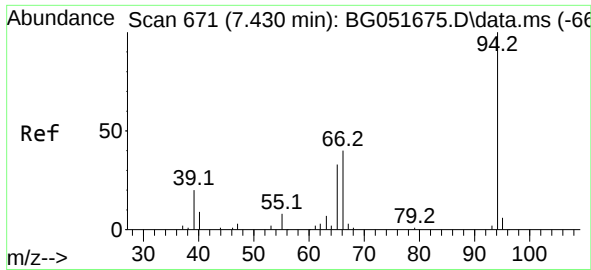

Phenol

Concen: 1.250 ng/ul

RT: 7.435 min Scan# 61

Delta R.T. -0.006 min

Lab File: BG051678.D

Acq: 20 Dec 2021 12:44

Instrument :

BNA_G

ClientSampleId :

BGL97

Tgt Ion: 94 Resp: 4137

Ion Ratio Lower Upper

94 100

65 26.8 25.1 37.7

66 51.7 31.6 47.4#

