

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051690.D
 Acq On : 20 Dec 2021 20:49
 Operator : CG/JU
 Sample : M5171-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLA7

Quant Time: Dec 20 23:12:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 14 14:19:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.270	152	37857	20.000	ng/u1	-0.02
20) Naphthalene-d8	11.107	136	164589	20.000	ng/u1	-0.02
38) Acenaphthene-d10	14.908	164	119383	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.651	188	260047	20.000	ng/u1	#-0.01
79) Chrysene-d12	21.975	240	215924	20.000	ng/u1	#-0.01
88) Perylene-d12	25.470	264	224191	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.600	96	1454	1.595	ng/uL	0.00
4) Pyridine-d5	4.040	84	7441	2.702	ng/u1	0.00
7) Phenol-d5	7.401	99	37193	11.003	ng/u1	-0.02
9) Bis-(2-Chloroethyl)eth...	7.571	67	21646	10.772	ng/u1	-0.02
11) 2-Chlorophenol-d4	7.794	132	25924	11.027	ng/u1	-0.02
15) 4-Methylphenol-d8	8.963	113	29779	11.397	ng/u1	-0.02
21) Nitrobenzene-d5	9.439	128	12978	10.755	ng/u1	-0.02
24) 2-Nitrophenol-d4	10.167	143	13948	10.574	ng/u1	-0.02
28) 2,4-Dichlorophenol-d3	10.714	165	29777	10.409	ng/u1	-0.02
31) 4-Chloroaniline-d4	11.231	131	36959	9.813	ng/u1	-0.01
46) Dimethylphthalate-d6	14.291	166	96254	10.073	ng/u1	-0.02
49) Acenaphthylene-d8	14.603	160	122136	10.292	ng/u1	-0.01
54) 4-Nitrophenol-d4	15.067	143	9631	6.198	ng/u1	-0.01
60) Fluorene-d10	15.895	176	84717	9.896	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.995	200	6218	4.589	ng/u1	-0.02
73) Anthracene-d10	17.751	188	143382	11.558	ng/u1	-0.01
81) Pyrene-d10	20.025	212	155689	11.980	ng/u1	-0.02
92) Benzo(a)pyrene-d12	25.229	264	137317	11.641	ng/u1	-0.02
Target Compounds						
83) Butylbenzylphthalate	20.929	149	5200	1.050	ng/u1	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051690.D
Acq On : 20 Dec 2021 20:49
Operator : CG/JU
Sample : M5171-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLA7

Quant Time: Dec 20 23:12:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 14 14:19:57 2021
Response via : Initial Calibration

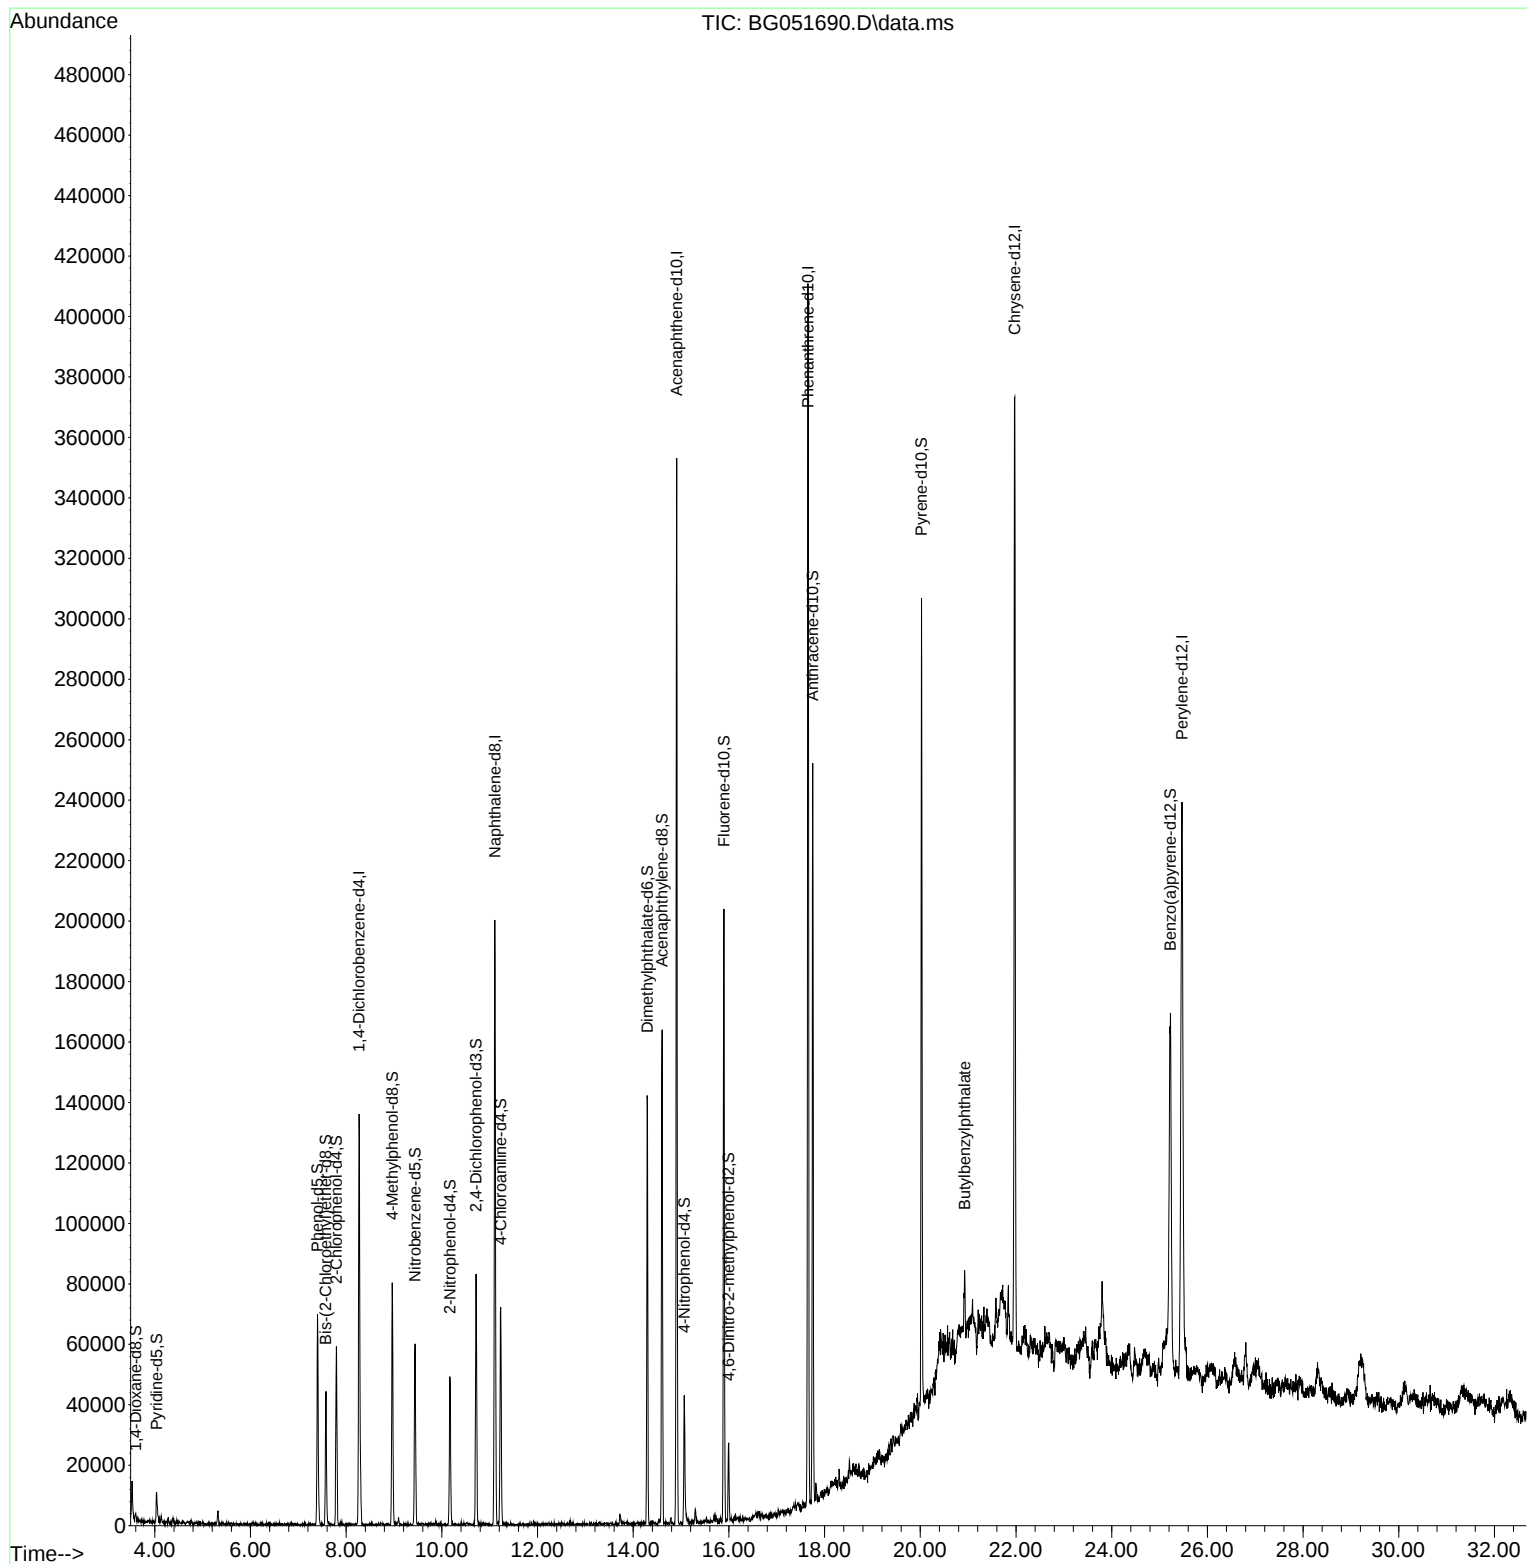

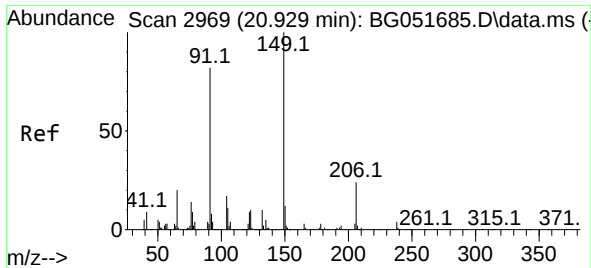

#83
 Butylbenzylphthalate
 Concen: 1.050 ng/ul
 RT: 20.929 min Scan# 2969
 Delta R.T. -0.017 min
 Lab File: BG051690.D
 Acq: 20 Dec 2021 20:49

Instrument :
 BNA_G
 ClientSampleId :
 BGLA7

Tgt Ion:	149	Resp:	5200
Ion	Ratio	Lower	Upper
149	100		
91	72.0	65.2	97.8
206	23.0	16.2	24.2

