

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051739.D
 Acq On : 22 Dec 2021 7:05
 Operator : CG/JU
 Sample : M5090-06
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3E1

Quant Time: Dec 22 07:48:46 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 14 14:19:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.276	152	39728	20.000	ng/ul	-0.01
20) Naphthalene-d8	11.113	136	169557	20.000	ng/ul	#-0.01
38) Acenaphthene-d10	14.908	164	123306	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.657	188	288813	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.980	240	281401	20.000	ng/ul	# 0.00
88) Perylene-d12	25.482	264	271184	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.599	96	4782	4.999	ng/uL	0.00
4) Pyridine-d5	4.034	84	11201	3.875	ng/ul	-0.01
7) Phenol-d5	7.406	99	28143	7.934	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.576	67	69871	33.134	ng/ul	-0.02
11) 2-Chlorophenol-d4	7.800	132	64750	26.246	ng/ul	-0.01
15) 4-Methylphenol-d8	8.969	113	46290	16.882	ng/ul	-0.01
21) Nitrobenzene-d5	9.439	128	43114	34.682	ng/ul	-0.02
24) 2-Nitrophenol-d4	10.173	143	44567	32.795	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.719	165	81692	27.721	ng/ul	-0.01
31) 4-Chloroaniline-d4	11.230	131	73850	19.033	ng/ul	-0.01
46) Dimethylphthalate-d6	14.297	166	299442	30.341	ng/ul	-0.02
49) Acenaphthylene-d8	14.602	160	364219	29.715	ng/ul	-0.01
54) 4-Nitrophenol-d4	15.072	143	9256	5.767	ng/ul	0.00
60) Fluorene-d10	15.895	176	262536	29.691	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	16.000	200	41060	27.287	ng/ul	-0.01
73) Anthracene-d10	17.757	188	454964	33.023	ng/ul	0.00
81) Pyrene-d10	20.030	212	548898	32.410	ng/ul	-0.01
92) Benzo(a)pyrene-d12	25.235	264	506182	35.475	ng/ul	-0.02
Target Compounds						
35) 4-Chloro-3-methylphenol	12.358	107	13051	4.154	ng/ul	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051739.D
Acq On : 22 Dec 2021 7:05
Operator : CG/JU
Sample : M5090-06
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3E1


Quant Time: Dec 22 07:48:46 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 14 14:19:57 2021
Response via : Initial Calibration

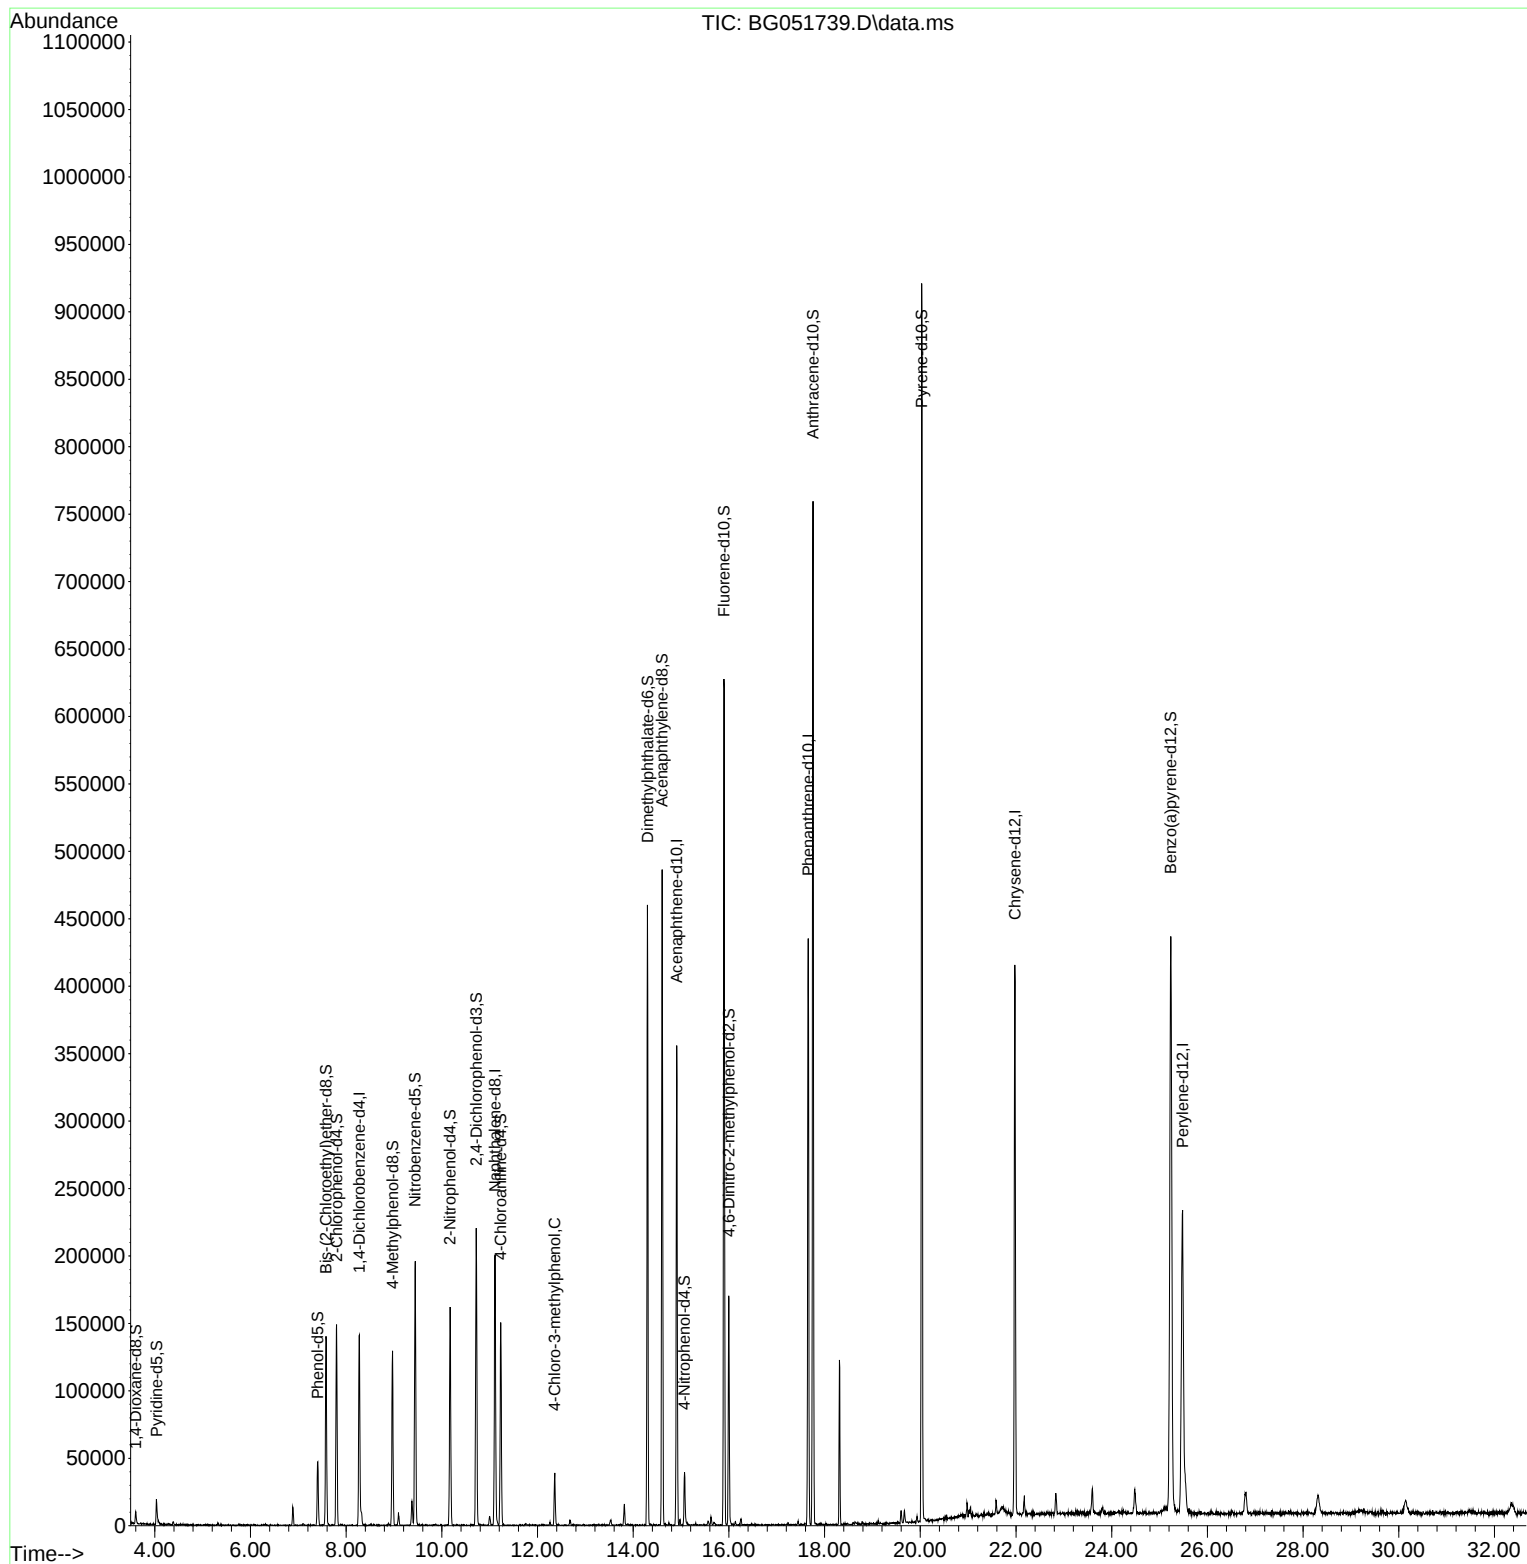

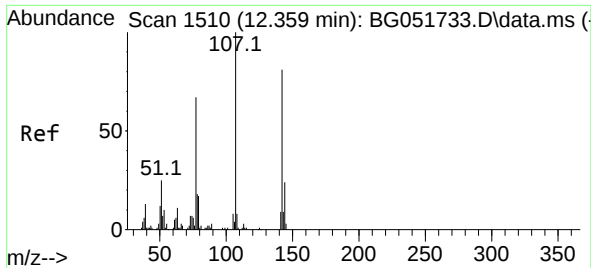

#35
 4-Chloro-3-methylphenol
 Concen: 4.154 ng/ul
 RT: 12.358 min Scan# 11
 Delta R.T. -0.011 min
 Lab File: BG051739.D
 Acq: 22 Dec 2021 7:05

Instrument :
 BNA_G
 ClientSampleId :
 BG3E1

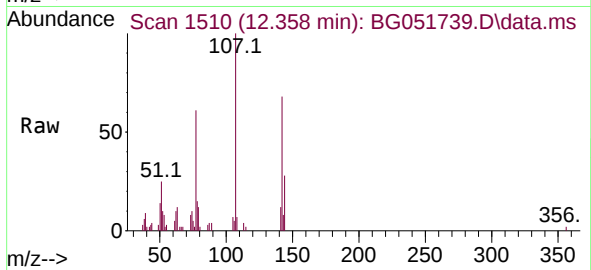

Tgt Ion:	107	Resp:	13051
Ion	Ratio	Lower	Upper
107	100		
144	27.9	19.8	29.6
142	68.4	56.2	84.4

