

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051686.D
 Acq On : 20 Dec 2021 18:08
 Operator : CG/JU
 Sample : PB141559BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK559

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051686.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.597	15	18	26	rVB	9797	14794	1.46%	0.133%
2	3.785	49	50	55	rBV4	1185	1227	0.12%	0.011%
3	4.026	86	91	102	rVV	106158	182633	18.06%	1.647%
4	4.097	102	103	112	rVV5	2213	4143	0.41%	0.037%
5	4.279	131	134	135	rVB	1273	1126	0.11%	0.010%
6	4.373	148	150	151	rBV	2499	1589	0.16%	0.014%
7	5.266	296	302	305	rVB2	832	1708	0.17%	0.015%
8	5.401	321	325	327	rVB2	908	1172	0.12%	0.011%
9	5.694	372	375	378	rBV	1060	1355	0.13%	0.012%
10	6.458	502	505	508	rBV	1009	1104	0.11%	0.010%
11	7.404	659	666	675	rVB	190486	314112	31.05%	2.832%
12	7.580	689	696	704	rVB	114771	200457	19.82%	1.807%
13	7.797	726	733	741	rVB	171755	288438	28.52%	2.601%
14	8.273	806	814	821	rVV	131775	222130	21.96%	2.003%
15	8.966	925	932	940	rBV2	223283	374016	36.98%	3.372%
16	9.442	1006	1013	1021	rVB	168865	297130	29.37%	2.679%
17	10.171	1130	1137	1144	rVB	145823	256156	25.32%	2.310%
18	10.276	1152	1155	1160	rBV	967	1424	0.14%	0.013%
19	10.323	1162	1163	1168	rBV2	860	1193	0.12%	0.011%
20	10.717	1221	1230	1239	rBV	227512	397269	39.27%	3.582%
21	11.111	1288	1297	1304	rBV	188133	333312	32.95%	3.005%
22	11.228	1309	1317	1327	rVV	175748	329692	32.59%	2.973%
23	11.868	1422	1426	1435	rVB3	1109	2713	0.27%	0.024%
24	12.685	1558	1565	1571	rVB3	3893	6588	0.65%	0.059%
25	14.295	1833	1839	1847	rVB	391529	586380	57.97%	5.287%
26	14.606	1884	1892	1900	rBV	434072	702717	69.47%	6.336%
27	14.911	1937	1944	1950	rBV	307927	489700	48.41%	4.415%
28	15.070	1964	1971	1985	rBV	179345	298202	29.48%	2.689%
29	15.305	2010	2011	2017	rBV	798	1144	0.11%	0.010%
30	15.405	2025	2028	2032	rBV2	869	1272	0.13%	0.011%
31	15.716	2080	2081	2086	rBV2	979	1065	0.11%	0.010%
32	15.898	2102	2112	2122	rVB	561020	868724	85.88%	7.833%
33	15.998	2122	2129	2137	rVV	116672	183224	18.11%	1.652%
34	16.057	2137	2139	2142	rVV2	1359	1403	0.14%	0.013%
35	16.139	2149	2153	2156	rVB2	2200	2593	0.26%	0.023%
36	16.280	2175	2177	2180	rBV4	927	1265	0.13%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051686.D
 Acq On : 20 Dec 2021 18:08
 Operator : CG/JU
 Sample : PB141559BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK559

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	16.427	2199	2202	2204	rVB2	1057	1263	0.12%	0.011%
38	16.468	2207	2209	2213	rVV	712	1120	0.11%	0.010%
39	16.580	2226	2228	2230	rBV	1004	1013	0.10%	0.009%
40	16.850	2271	2274	2276	rBV2	1382	1404	0.14%	0.013%
41	16.868	2276	2277	2280	rVV	1460	1228	0.12%	0.011%
42	16.962	2290	2293	2296	rVB	828	1167	0.12%	0.011%
43	17.026	2300	2304	2305	rBV	1208	1254	0.12%	0.011%
44	17.179	2327	2330	2332	rVB	1234	1033	0.10%	0.009%
45	17.220	2335	2337	2340	rBV3	1206	1234	0.12%	0.011%
46	17.320	2350	2354	2356	rVB3	1496	1288	0.13%	0.012%
47	17.349	2356	2359	2363	rVB3	1360	1663	0.16%	0.015%
48	17.390	2363	2366	2368	rBV	995	1359	0.13%	0.012%
49	17.437	2371	2374	2378	rBV4	2145	2653	0.26%	0.024%
50	17.555	2389	2394	2395	rVB3	1059	1334	0.13%	0.012%
51	17.578	2395	2398	2400	rBV2	1421	1766	0.17%	0.016%
52	17.655	2404	2411	2418	rVV	401391	595145	58.84%	5.366%
53	17.755	2421	2428	2434	rVB2	646418	946281	93.55%	8.532%
54	17.878	2448	2449	2451	rBV2	1144	1037	0.10%	0.009%
55	18.013	2469	2472	2475	rBV3	1626	1790	0.18%	0.016%
56	18.054	2475	2479	2483	rBV3	1156	1719	0.17%	0.015%
57	18.101	2486	2487	2491	rBV3	787	1233	0.12%	0.011%
58	18.154	2495	2496	2499	rVV3	1395	1400	0.14%	0.013%
59	18.189	2501	2502	2508	rVV4	1490	1880	0.19%	0.017%
60	18.295	2517	2520	2521	rBV2	2190	1864	0.18%	0.017%
61	18.313	2521	2523	2525	rVB3	2641	2327	0.23%	0.021%
62	18.330	2525	2526	2528	rBV2	1898	1173	0.12%	0.011%
63	18.454	2545	2547	2549	rVB3	1375	1054	0.10%	0.010%
64	18.483	2549	2552	2553	rBV3	2131	1910	0.19%	0.017%
65	18.636	2576	2578	2581	rVB4	1557	1631	0.16%	0.015%
66	18.659	2581	2582	2584	rBV2	1706	1432	0.14%	0.013%
67	18.700	2587	2589	2591	rVV3	1567	1155	0.11%	0.010%
68	18.777	2599	2602	2604	rBV4	2025	1187	0.12%	0.011%
69	18.865	2616	2617	2619	rBV2	2264	1800	0.18%	0.016%
70	18.900	2619	2623	2626	rVV4	2925	3553	0.35%	0.032%
71	18.929	2626	2628	2629	rVV2	1650	1133	0.11%	0.010%
72	18.965	2632	2634	2636	rBV3	2588	1852	0.18%	0.017%
73	18.988	2636	2638	2640	rBV3	2556	1907	0.19%	0.017%
74	19.053	2647	2649	2652	rBV4	2809	3789	0.37%	0.034%
75	19.117	2657	2660	2663	rBV4	2464	3485	0.34%	0.031%
76	19.164	2663	2668	2669	rBV5	4352	4930	0.49%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051686.D
 Acq On : 20 Dec 2021 18:08
 Operator : CG/JU
 Sample : PB141559BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK559

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	19.217	2675	2677	2680	rBV3	1739	1938	0.19%	0.017%
78	19.270	2684	2686	2688	rBV2	2228	2115	0.21%	0.019%
79	19.323	2692	2695	2697	rBV3	3080	3270	0.32%	0.029%
80	19.347	2697	2699	2700	rVB	2867	1428	0.14%	0.013%
81	19.370	2700	2703	2705	rBV4	1830	1959	0.19%	0.018%
82	19.399	2705	2708	2710	rBV3	3773	5456	0.54%	0.049%
83	19.464	2716	2719	2721	rBV3	3709	3585	0.35%	0.032%
84	19.564	2734	2736	2737	rBV2	2901	2305	0.23%	0.021%
85	19.593	2738	2741	2745	rVV4	8558	12758	1.26%	0.115%
86	19.670	2749	2754	2757	rVV2	8735	12379	1.22%	0.112%
87	19.728	2762	2764	2767	rBV4	3592	5082	0.50%	0.046%
88	19.805	2775	2777	2778	rBV2	3990	4059	0.40%	0.037%
89	19.952	2800	2802	2805	rBV4	3741	3494	0.35%	0.032%
90	20.028	2809	2815	2821	rVV	709556	1011519	100.00%	9.120%
91	20.275	2855	2857	2859	rBV3	5023	5102	0.50%	0.046%
92	21.867	3126	3128	3130	rBV3	7021	5903	0.58%	0.053%
93	21.972	3140	3146	3154	rVB	332046	560039	55.37%	5.049%
94	23.594	3418	3422	3426	rVB6	17689	25461	2.52%	0.230%
95	25.227	3690	3700	3712	rVB3	298960	912192	90.18%	8.224%
96	25.474	3732	3742	3750	rBV3	169838	519952	51.40%	4.688%
97	27.618	4105	4107	4109	rVB3	7990	5482	0.54%	0.049%
98	31.935	4840	4842	4846	rVB5	5507	5102	0.50%	0.046%




Sum of corrected areas: 11091196

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051686.D
Acq On : 20 Dec 2021 18:08
Operator : CG/JU
Sample : PB141559BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK559

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

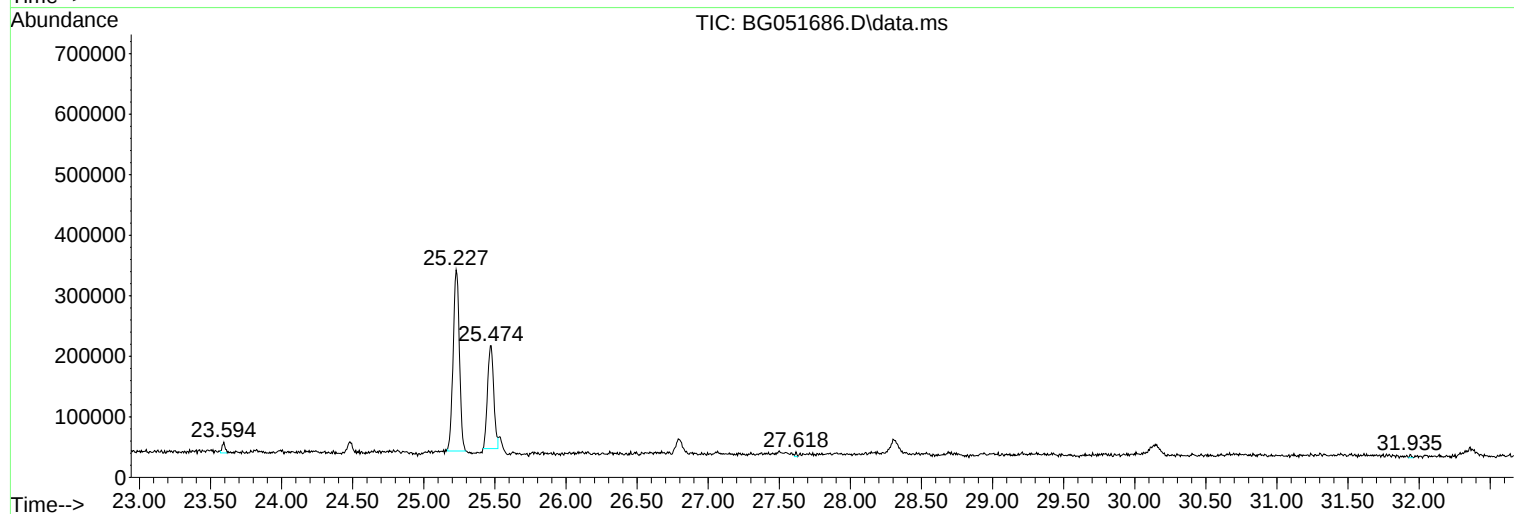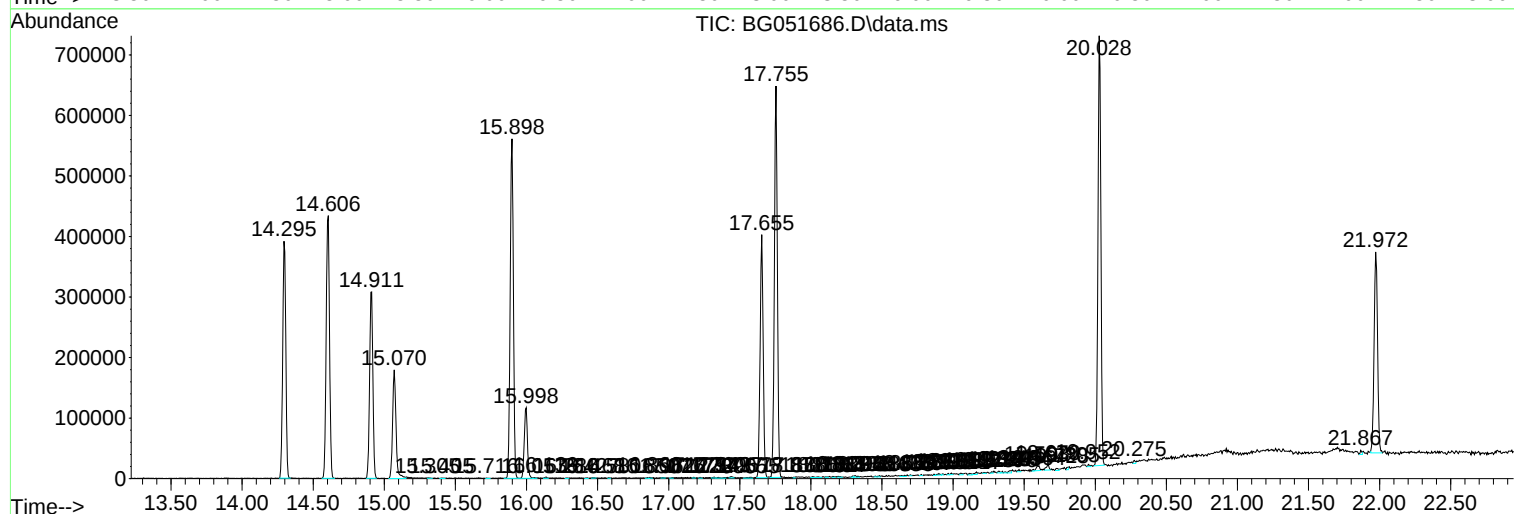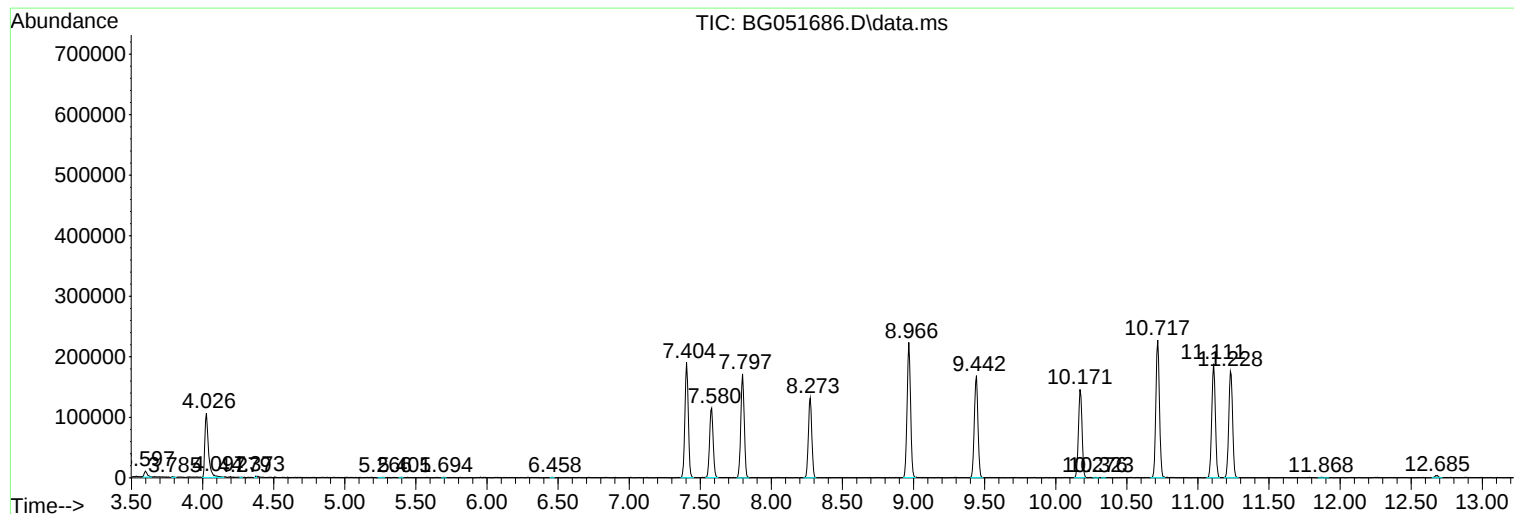

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051686.D
Acq On : 20 Dec 2021 18:08
Operator : CG/JU
Sample : PB141559BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK559

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051686.D
Acq On : 20 Dec 2021 18:08
Operator : CG/JU
Sample : PB141559BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK559

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
