

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051690.D
 Acq On : 20 Dec 2021 20:49
 Operator : CG/JU
 Sample : M5171-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051690.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.523	3	6	15	rVB4	13617	22512	3.61%	0.401%
2	3.600	15	19	23	rBV4	2900	5164	0.83%	0.092%
3	3.982	82	84	87	rVB2	1112	951	0.15%	0.017%
4	4.040	89	94	99	rVV	10261	19172	3.07%	0.341%
5	4.093	102	103	106	rVV	1465	1171	0.19%	0.021%
6	4.134	108	110	116	rVB5	2271	2789	0.45%	0.050%
7	4.234	124	127	128	rBV	960	1065	0.17%	0.019%
8	4.281	132	135	138	rBV2	2296	2321	0.37%	0.041%
9	4.381	147	152	154	rBV3	2468	3796	0.61%	0.068%
10	4.505	172	173	178	rBV2	973	1126	0.18%	0.020%
11	4.575	184	185	188	rBV	1097	1192	0.19%	0.021%
12	4.757	213	216	217	rBV2	1640	1506	0.24%	0.027%
13	4.974	250	253	256	rBV	701	987	0.16%	0.018%
14	5.004	256	258	261	rVB	1328	1248	0.20%	0.022%
15	5.321	306	312	316	rVB4	4730	7342	1.18%	0.131%
16	5.403	323	326	329	rBV	1013	904	0.14%	0.016%
17	5.597	355	359	360	rBV	990	1162	0.19%	0.021%
18	5.861	400	404	407	rVB	823	1014	0.16%	0.018%
19	6.032	430	433	436	rBV	856	1099	0.18%	0.020%
20	6.102	443	445	449	rVB2	1002	1073	0.17%	0.019%
21	6.132	449	450	454	rBV	807	915	0.15%	0.016%
22	6.361	486	489	491	rBV	822	1051	0.17%	0.019%
23	6.420	497	499	503	rBV	886	960	0.15%	0.017%
24	7.401	659	666	677	rBV	69728	121942	19.54%	2.172%
25	7.577	690	696	704	rBV	44156	73406	11.76%	1.307%
26	7.636	704	706	711	rVB2	1344	1851	0.30%	0.033%
27	7.683	711	714	717	rBV	738	1035	0.17%	0.018%
28	7.794	727	733	741	rVB	59057	103302	16.55%	1.840%
29	7.888	746	749	751	rVB	1267	1109	0.18%	0.020%
30	7.988	762	766	768	rBV	753	912	0.15%	0.016%
31	8.270	807	814	826	rVB2	135938	253757	40.66%	4.520%
32	8.963	924	932	940	rBV	80258	138650	22.22%	2.470%
33	9.040	942	945	948	rBV	970	1147	0.18%	0.020%
34	9.098	948	955	959	rVB	2434	3868	0.62%	0.069%
35	9.439	1006	1013	1020	rVB	59662	107840	17.28%	1.921%
36	9.598	1035	1040	1045	rBV2	710	1291	0.21%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051690.D
 Acq On : 20 Dec 2021 20:49
 Operator : CG/JU
 Sample : M5171-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLA7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	9.868	1085	1086	1090	rVB	1369	1382	0.22%	0.025%
38	10.167	1130	1137	1145	rVB3	49117	91536	14.67%	1.630%
39	10.714	1224	1230	1238	rVB	83020	143268	22.96%	2.552%
40	10.849	1250	1253	1254	rBV	824	940	0.15%	0.017%
41	11.107	1290	1297	1305	rBV	199848	352832	56.54%	6.284%
42	11.231	1311	1318	1325	rVB2	71864	132905	21.30%	2.367%
43	11.865	1425	1426	1431	rBV	1131	1088	0.17%	0.019%
44	11.912	1431	1434	1439	rVB	1156	1588	0.25%	0.028%
45	12.141	1470	1473	1478	rBV2	635	1227	0.20%	0.022%
46	12.282	1492	1497	1498	rBV	685	911	0.15%	0.016%
47	12.500	1532	1534	1535	rBV	1297	966	0.15%	0.017%
48	12.617	1548	1554	1556	rBV	723	1161	0.19%	0.021%
49	12.682	1564	1565	1569	rVB3	1529	1199	0.19%	0.021%
50	13.128	1638	1641	1645	rVB2	931	1190	0.19%	0.021%
51	13.293	1664	1669	1672	rBV2	1024	1799	0.29%	0.032%
52	13.510	1703	1706	1708	rBV2	813	1239	0.20%	0.022%
53	13.721	1738	1742	1747	rBV5	3401	5934	0.95%	0.106%
54	14.133	1808	1812	1815	rVB	937	1563	0.25%	0.028%
55	14.197	1820	1823	1825	rBV	827	1058	0.17%	0.019%
56	14.291	1833	1839	1846	rVB	141975	208457	33.40%	3.713%
57	14.526	1876	1879	1880	rBV	1486	1711	0.27%	0.030%
58	14.603	1885	1892	1898	rVV	163737	257680	41.29%	4.590%
59	14.791	1919	1924	1928	rBV2	2141	2771	0.44%	0.049%
60	14.820	1928	1929	1935	rVB2	817	969	0.16%	0.017%
61	14.908	1937	1944	1953	rVB	352703	527739	84.57%	9.400%
62	15.067	1965	1971	1981	rBV2	42774	75611	12.12%	1.347%
63	15.184	1988	1991	1995	rBV	1089	1337	0.21%	0.024%
64	15.237	1995	2000	2001	rVB	1195	1531	0.25%	0.027%
65	15.249	2001	2002	2005	rBV	1216	1077	0.17%	0.019%
66	15.296	2005	2010	2015	rVB3	4783	7963	1.28%	0.142%
67	15.331	2015	2016	2019	rBV3	1388	1081	0.17%	0.019%
68	15.531	2048	2050	2052	rVB	1584	1394	0.22%	0.025%
69	15.689	2075	2077	2080	rVB2	2134	2013	0.32%	0.036%
70	15.725	2082	2083	2088	rVB2	2278	2313	0.37%	0.041%
71	15.777	2090	2092	2094	rBV2	1106	913	0.15%	0.016%
72	15.795	2094	2095	2098	rBV2	1774	1984	0.32%	0.035%
73	15.895	2105	2112	2119	rVB	202758	319225	51.16%	5.686%
74	15.954	2119	2122	2124	rBV2	813	889	0.14%	0.016%
75	15.995	2124	2129	2134	rVV3	25594	37940	6.08%	0.676%
76	16.095	2145	2146	2148	rBV2	1093	969	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051690.D
 Acq On : 20 Dec 2021 20:49
 Operator : CG/JU
 Sample : M5171-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	16.136	2150	2153	2155	rVV3	2437	2324	0.37%	0.041%
78	16.236	2169	2170	2173	rBV3	1407	1073	0.17%	0.019%
79	16.289	2176	2179	2181	rVB3	1797	2002	0.32%	0.036%
80	16.336	2183	2187	2189	rBV3	1244	1640	0.26%	0.029%
81	16.430	2200	2203	2205	rVB3	1491	1728	0.28%	0.031%
82	16.459	2205	2208	2209	rBV2	830	1074	0.17%	0.019%
83	16.477	2209	2211	2214	rBV3	893	1013	0.16%	0.018%
84	16.670	2243	2244	2249	rBV4	1550	1827	0.29%	0.033%
85	16.741	2254	2256	2258	rBV2	1194	1212	0.19%	0.022%
86	16.764	2258	2260	2262	rBV2	1059	970	0.16%	0.017%
87	16.858	2273	2276	2277	rBV2	2520	2307	0.37%	0.041%
88	16.911	2283	2285	2288	rBV2	1198	1612	0.26%	0.029%
89	16.993	2298	2299	2302	rVB2	1469	1069	0.17%	0.019%
90	17.029	2303	2305	2309	rBV5	2334	3065	0.49%	0.055%
91	17.193	2332	2333	2335	rBV2	1502	1286	0.21%	0.023%
92	17.446	2370	2376	2378	rBV5	2555	6117	0.98%	0.109%
93	17.487	2382	2383	2386	rVB3	2227	1481	0.24%	0.026%
94	17.651	2405	2411	2418	rVB	403534	624033	100.00%	11.115%
95	17.751	2422	2428	2437	rBV	245195	365852	58.63%	6.516%
96	17.816	2437	2439	2444	rVV7	5900	7796	1.25%	0.139%
97	18.515	2556	2558	2563	rBV6	6152	8914	1.43%	0.159%
98	20.025	2810	2815	2823	rBV	266935	390618	62.60%	6.957%
99	21.975	3141	3147	3155	rVB2	315768	573997	91.98%	10.224%
100	25.470	3734	3742	3753	rVB2	181198	521414	83.56%	9.287%




Sum of corrected areas: 5614407

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051690.D
Acq On : 20 Dec 2021 20:49
Operator : CG/JU
Sample : M5171-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

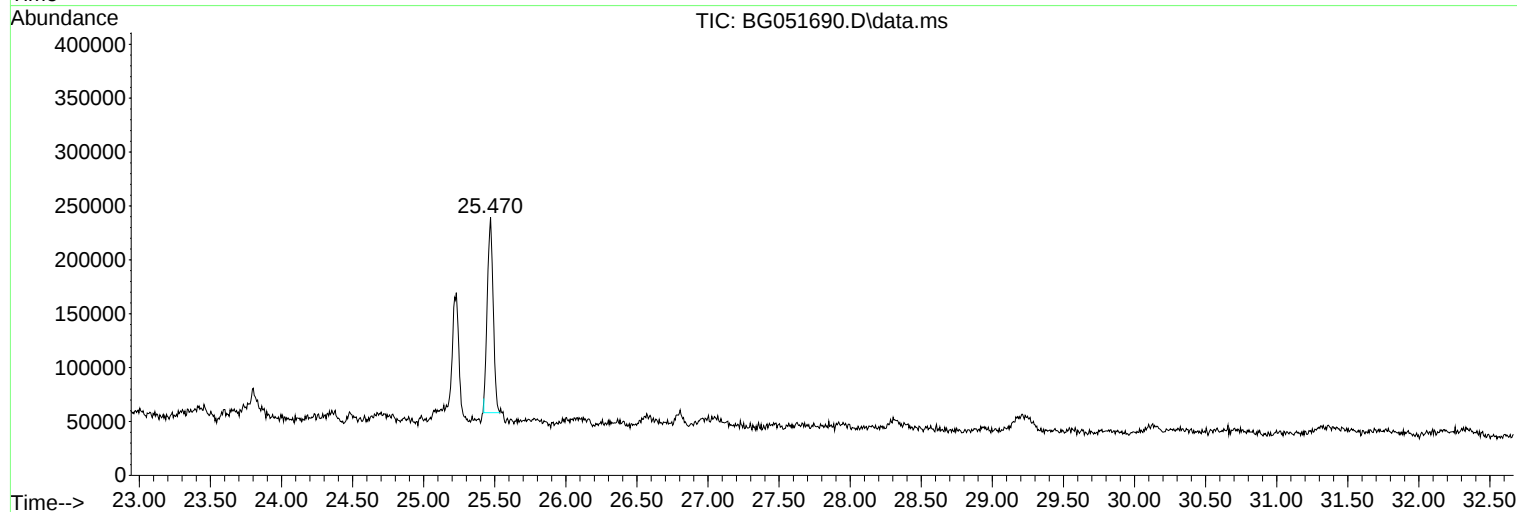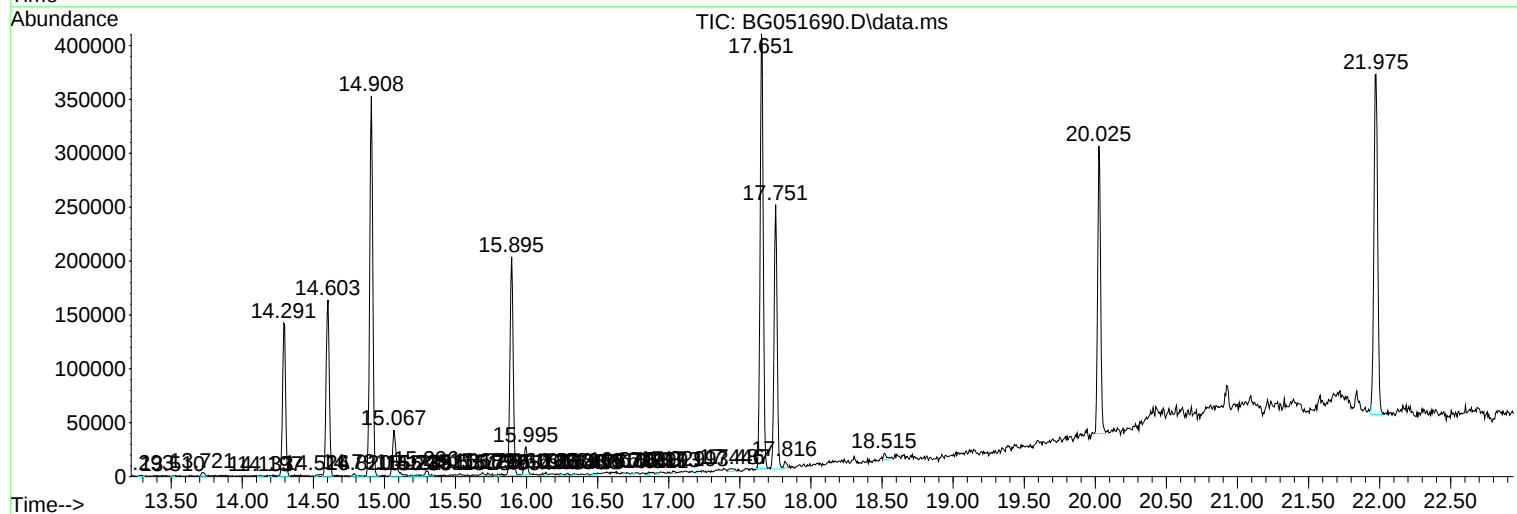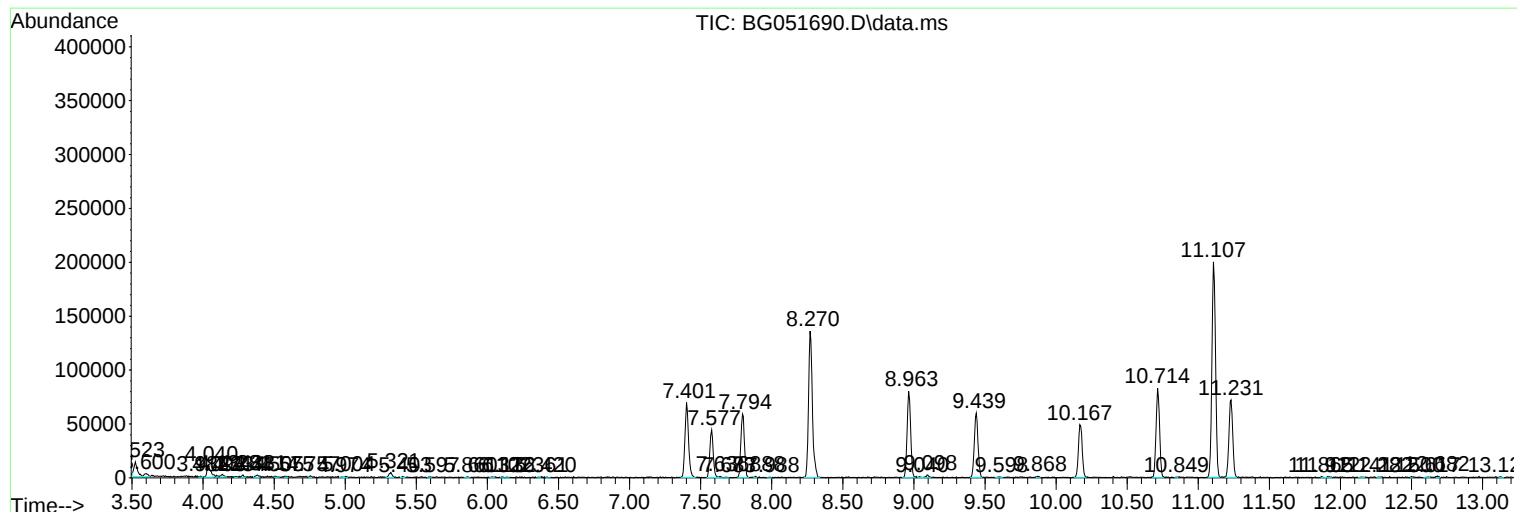

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051690.D
Acq On : 20 Dec 2021 20:49
Operator : CG/JU
Sample : M5171-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051690.D
Acq On : 20 Dec 2021 20:49
Operator : CG/JU
Sample : M5171-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc