

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051694.D
 Acq On : 20 Dec 2021 23:29
 Operator : CG/JU
 Sample : M5171-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051694.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.600	13	19	26	rVB2	11568	19445	1.52%	0.141%
2	3.882	62	67	69	rVB3	2454	2792	0.22%	0.020%
3	4.023	87	91	108	rVV	150953	263144	20.51%	1.913%
4	4.381	145	152	155	rBV3	1975	2820	0.22%	0.021%
5	7.401	659	666	676	rBV	223161	409144	31.89%	2.974%
6	7.577	689	696	703	rBV	154004	255732	19.93%	1.859%
7	7.630	703	705	709	rVB3	3657	4118	0.32%	0.030%
8	7.794	722	733	741	rBV	203937	356105	27.76%	2.589%
9	8.270	804	814	821	rBV	137611	235477	18.36%	1.712%
10	8.317	821	822	828	rVB	1937	2657	0.21%	0.019%
11	8.963	924	932	942	rBV2	248216	451807	35.22%	3.285%
12	9.439	1005	1013	1023	rVB	214319	377158	29.40%	2.742%
13	9.874	1083	1087	1090	rVB	1466	2078	0.16%	0.015%
14	10.173	1131	1138	1148	rVB	180670	328360	25.60%	2.387%
15	10.714	1223	1230	1238	rBV	272569	492996	38.43%	3.584%
16	10.855	1248	1254	1261	rBV3	1995	4396	0.34%	0.032%
17	11.107	1290	1297	1306	rBV	187416	344293	26.84%	2.503%
18	11.231	1309	1318	1327	rBV	263109	478726	37.32%	3.480%
19	12.500	1530	1534	1540	rBV3	2133	2613	0.20%	0.019%
20	12.682	1561	1565	1571	rVB4	4383	6654	0.52%	0.048%
21	13.727	1737	1743	1749	rBV5	6156	9666	0.75%	0.070%
22	14.297	1833	1840	1846	rBV	491950	724965	56.51%	5.271%
23	14.532	1876	1880	1883	rBV3	3161	4375	0.34%	0.032%
24	14.603	1885	1892	1900	rVB	565126	887502	69.18%	6.452%
25	14.791	1918	1924	1929	rBV3	2930	4951	0.39%	0.036%
26	14.908	1936	1944	1951	rVB	323573	499332	38.92%	3.630%
27	15.067	1965	1971	1981	rBV	209736	342482	26.70%	2.490%
28	15.302	2006	2011	2014	rVB3	1867	3555	0.28%	0.026%
29	15.531	2045	2050	2055	rVB2	4294	5378	0.42%	0.039%
30	15.689	2072	2077	2080	rBV2	3040	3714	0.29%	0.027%
31	15.736	2080	2085	2088	rVB	3460	3589	0.28%	0.026%
32	15.895	2101	2112	2120	rBV	710829	1087215	84.75%	7.904%
33	15.995	2123	2129	2137	rVV	167030	239196	18.65%	1.739%
34	16.136	2147	2153	2158	rVB5	3278	4809	0.37%	0.035%
35	16.523	2216	2219	2223	rBV3	1797	2786	0.22%	0.020%
36	16.565	2223	2226	2228	rVV2	3031	3119	0.24%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051694.D
 Acq On : 20 Dec 2021 23:29
 Operator : CG/JU
 Sample : M5171-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	16.594	2230	2231	2235	rVV3	2772	2887	0.23%	0.021%
38	16.776	2256	2262	2265	rBV4	2250	3396	0.26%	0.025%
39	17.105	2313	2318	2324	rVB3	2061	4450	0.35%	0.032%
40	17.246	2339	2342	2348	rVB4	1406	2337	0.18%	0.017%
41	17.381	2362	2365	2367	rVV2	2976	3339	0.26%	0.024%
42	17.440	2371	2375	2377	rVV4	2776	3554	0.28%	0.026%
43	17.540	2390	2392	2397	rVB4	3174	3641	0.28%	0.026%
44	17.651	2402	2411	2419	rVV	390489	616342	48.04%	4.481%
45	17.710	2419	2421	2422	rVV2	2460	2224	0.17%	0.016%
46	17.751	2422	2428	2436	rVV	763643	1157380	90.22%	8.414%
47	17.822	2437	2440	2445	rVB5	4188	5874	0.46%	0.043%
48	18.215	2504	2507	2510	rBV4	1738	1926	0.15%	0.014%
49	18.298	2520	2521	2524	rVV2	3468	2551	0.20%	0.019%
50	18.439	2542	2545	2549	rVB4	2217	3347	0.26%	0.024%
51	18.521	2555	2559	2569	rBV2	37533	57984	4.52%	0.422%
52	18.597	2569	2572	2574	rVV4	3090	3882	0.30%	0.028%
53	19.126	2661	2662	2669	rVB6	2315	2675	0.21%	0.019%
54	19.232	2678	2680	2684	rBV3	2213	3157	0.25%	0.023%
55	19.367	2700	2703	2705	rBV2	3489	4576	0.36%	0.033%
56	19.384	2705	2706	2709	rVB3	4195	3362	0.26%	0.024%
57	19.461	2718	2719	2723	rVB4	3015	3048	0.24%	0.022%
58	19.496	2723	2725	2729	rBV4	2553	3940	0.31%	0.029%
59	19.566	2733	2737	2739	rBV4	2683	3724	0.29%	0.027%
60	19.596	2739	2742	2747	rVV4	10249	14034	1.09%	0.102%
61	19.666	2749	2754	2758	rVB2	10682	13502	1.05%	0.098%
62	19.907	2793	2795	2796	rVB2	3528	2221	0.17%	0.016%
63	19.931	2796	2799	2802	rBV6	4691	6497	0.51%	0.047%
64	20.031	2810	2816	2824	rBV	901064	1282853	100.00%	9.326%
65	20.213	2845	2847	2849	rBV3	2051	2565	0.20%	0.019%
66	20.348	2869	2870	2873	rBV3	2646	2066	0.16%	0.015%
67	20.524	2896	2900	2901	rBV3	3960	4617	0.36%	0.034%
68	20.606	2911	2914	2916	rBV4	3164	2881	0.22%	0.021%
69	20.970	2974	2976	2982	rVB6	2962	3717	0.29%	0.027%
70	21.305	3031	3033	3035	rBV3	3123	2193	0.17%	0.016%
71	21.575	3074	3079	3086	rBV2	58200	108166	8.43%	0.786%
72	21.840	3121	3124	3127	rBV4	5536	6391	0.50%	0.046%
73	21.975	3140	3147	3153	rVB	345610	598660	46.67%	4.352%
74	22.122	3170	3172	3173	rBV2	5893	3483	0.27%	0.025%
75	22.786	3283	3285	3287	rVB3	3910	1986	0.15%	0.014%
76	23.496	3403	3406	3407	rBV3	5522	4110	0.32%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051694.D
 Acq On : 20 Dec 2021 23:29
 Operator : CG/JU
 Sample : M5171-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	23.514	3407	3409	3410	rVV2	4447	2422	0.19%	0.018%
78	23.714	3442	3443	3444	rBV	4011	1913	0.15%	0.014%
79	23.802	3453	3458	3465	rVB3	13712	25417	1.98%	0.185%
80	24.272	3536	3538	3543	rBV6	3481	4263	0.33%	0.031%
81	24.477	3569	3573	3579	rVB8	8686	18575	1.45%	0.135%
82	24.583	3589	3591	3594	rVB4	4725	3446	0.27%	0.025%
83	24.613	3594	3596	3597	rBV2	3212	2071	0.16%	0.015%
84	24.665	3603	3605	3608	rBV4	3656	3359	0.26%	0.024%
85	25.229	3690	3701	3715	rVB2	405100	1202995	93.77%	8.746%
86	25.470	3731	3742	3758	rVB	197970	609678	47.53%	4.432%
87	25.782	3793	3795	3797	rVB3	3923	2300	0.18%	0.017%
88	25.840	3801	3805	3806	rBV4	4412	6338	0.49%	0.046%
89	25.999	3829	3832	3833	rBV3	3985	4953	0.39%	0.036%
90	26.146	3855	3857	3860	rVB4	2915	2023	0.16%	0.015%
91	26.363	3893	3894	3896	rBV2	4583	2489	0.19%	0.018%
92	26.763	3960	3962	3963	rBV2	3951	3379	0.26%	0.025%
93	26.786	3963	3966	3967	rBV3	5757	6193	0.48%	0.045%
94	26.880	3980	3982	3984	rBV2	3834	2544	0.20%	0.018%
95	27.285	4049	4051	4055	rBV4	3623	4512	0.35%	0.033%
96	28.026	4175	4177	4180	rBV4	4988	5074	0.40%	0.037%
97	29.864	4489	4490	4495	rBV4	4908	7005	0.55%	0.051%
98	29.905	4495	4497	4498	rVB2	4035	2219	0.17%	0.016%
99	30.046	4520	4521	4524	rBV3	3605	2451	0.19%	0.018%
100	31.580	4780	4782	4783	rVB2	4212	2755	0.21%	0.020%


Sum of corrected areas: 13755061

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051694.D
Acq On : 20 Dec 2021 23:29
Operator : CG/JU
Sample : M5171-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL99

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

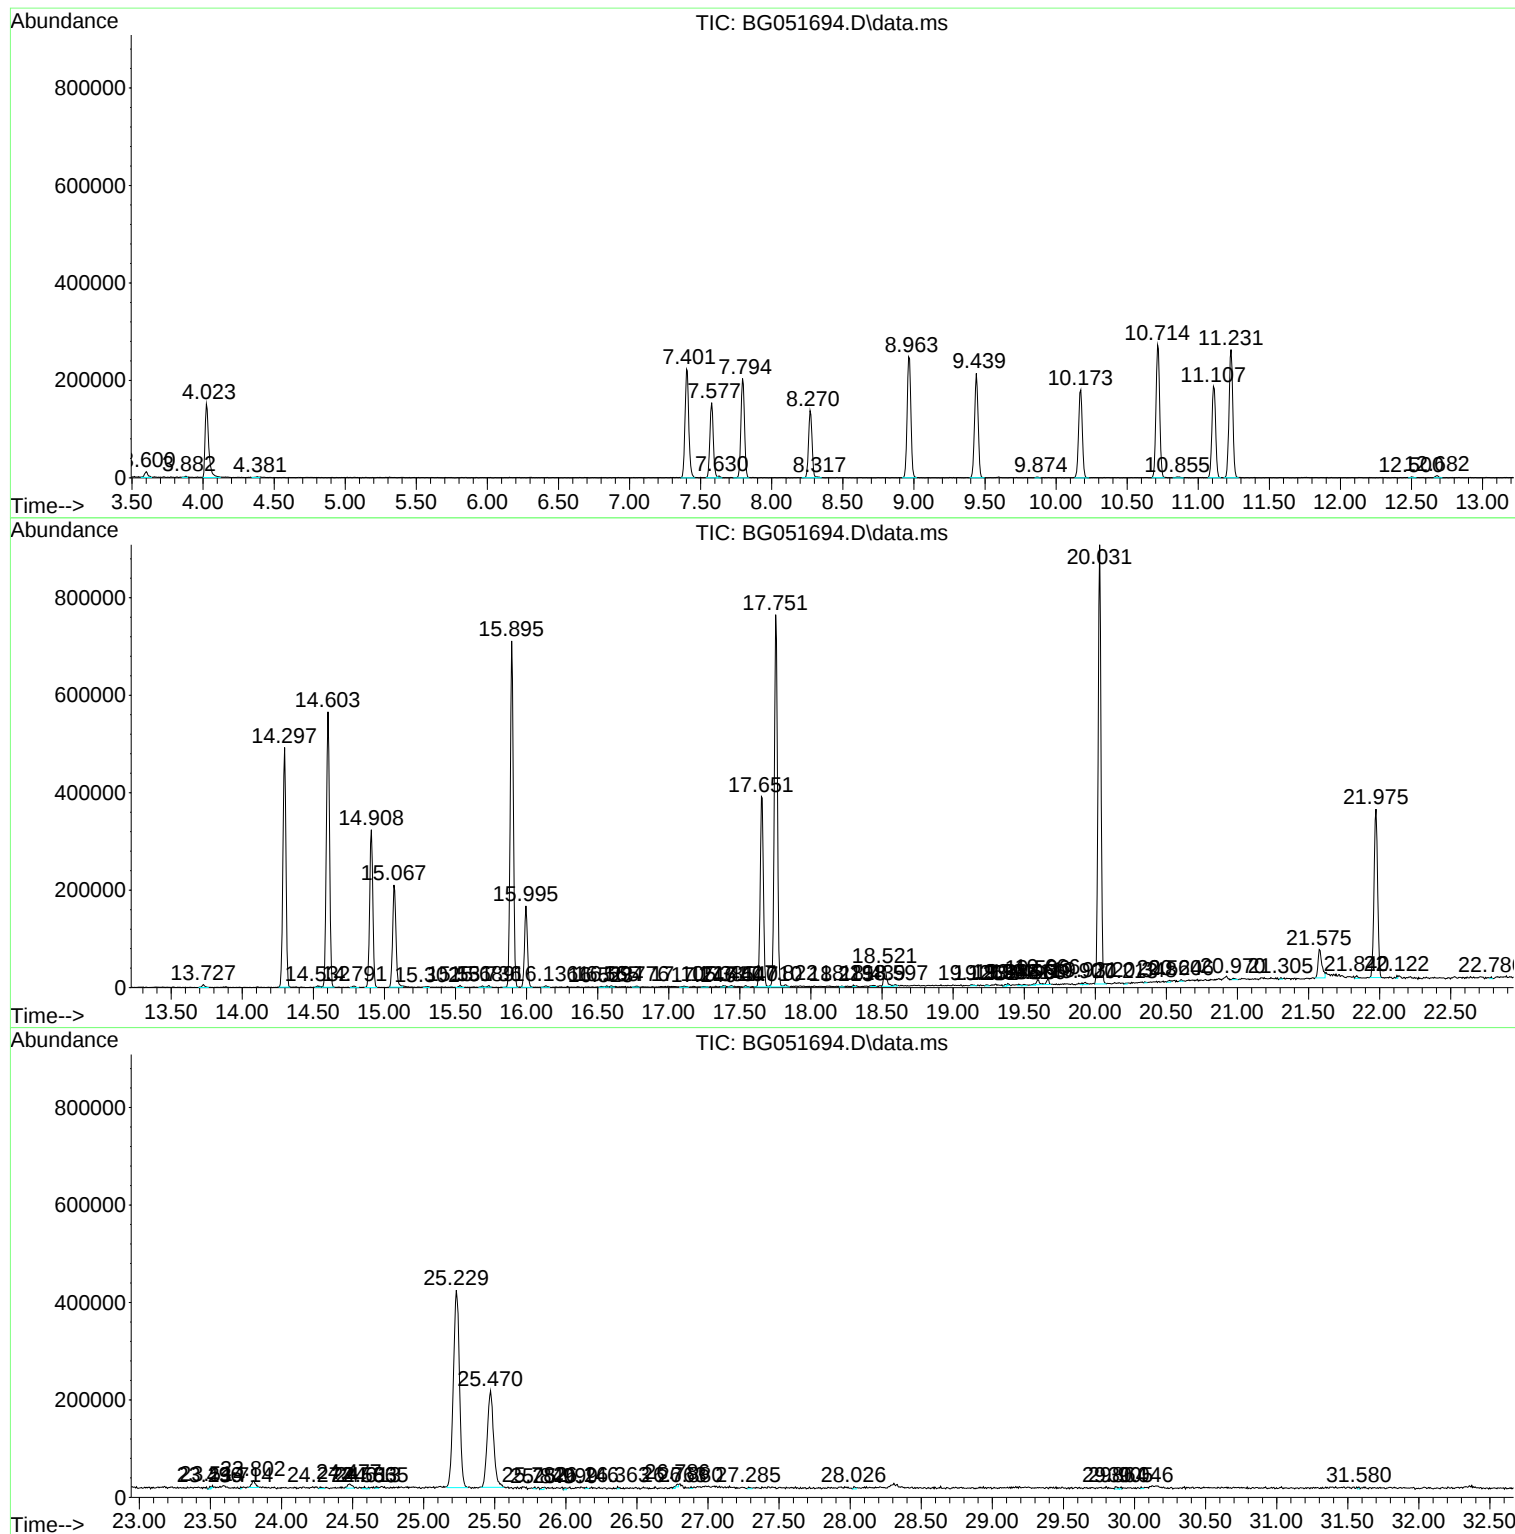

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051694.D
Acq On : 20 Dec 2021 23:29
Operator : CG/JU
Sample : M5171-03
Misc :
ALS Vial : 20 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
BGL99

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.576	3.61 ng/ul	108166	Chrysene-d12		21.975	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	1-Tetracosene		336	C24H48	010192-32-2	87
2	n-Heptadecanol-1		256	C17H36O	001454-85-9	87
3	3-Eicosene, (E)-		280	C20H40	074685-33-9	87
4	Trichloroacetic acid, pentadecyl...		372	C17H31Cl3O2	074339-53-0	83
5	Cyclotetracosane		336	C24H48	000297-03-0	76

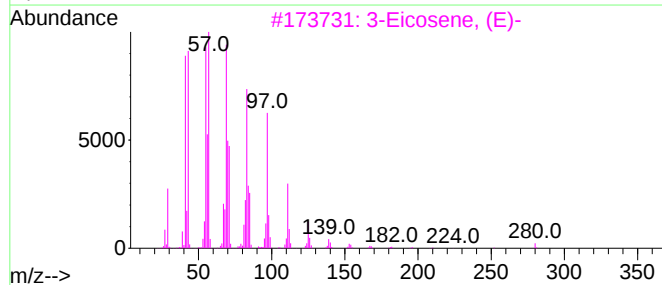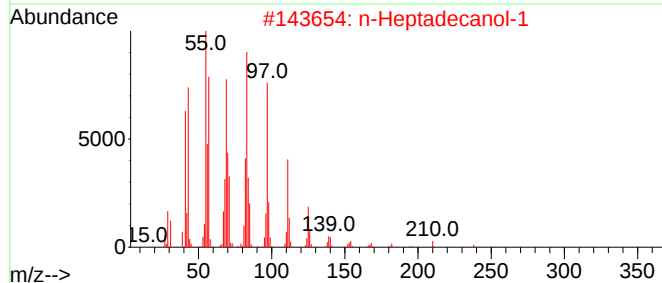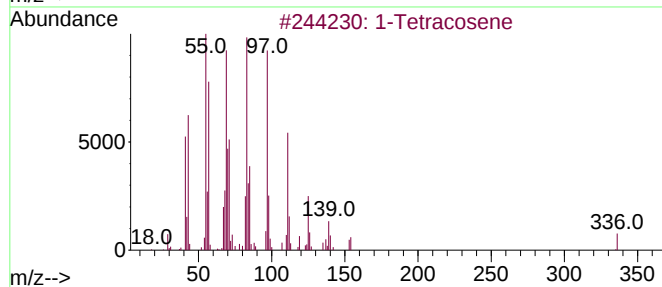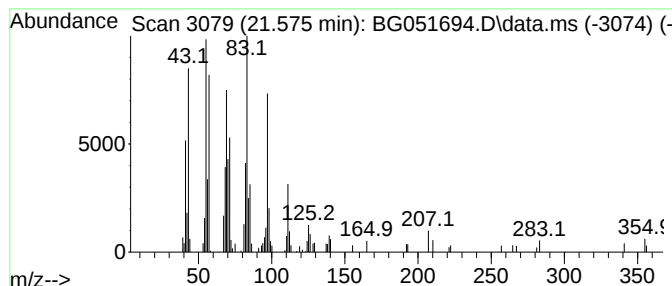

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051694.D
Acq On : 20 Dec 2021 23:29
Operator : CG/JU
Sample : M5171-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL99

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.576	3.6	ng/ul	108166	5	21.975	598660	20.0